

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015111.D
 Acq On : 16 May 2023 16:19
 Operator : CG/JU
 Sample : 02768-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	18	rVB	83688	120629	1.02%	0.117%
2	3.881	82	84	103	rBV	297377	511357	4.31%	0.497%
3	4.117	120	124	133	rVB	37421	63259	0.53%	0.061%
4	4.217	137	141	149	rVB	21109	36891	0.31%	0.036%
5	4.605	202	207	213	rBV6	9945	16770	0.14%	0.016%
6	4.681	215	220	226	rVB	48997	70868	0.60%	0.069%
7	5.170	299	303	308	rBV	7396	12870	0.11%	0.013%
8	5.670	384	388	394	rVB	13620	21518	0.18%	0.021%
9	5.787	404	408	414	rVB	25641	36405	0.31%	0.035%
10	7.240	650	655	657	rBV	39012	57443	0.48%	0.056%
11	7.281	657	662	676	rVB	370026	606988	5.11%	0.590%
12	7.452	684	691	705	rVB	1414254	2204112	18.56%	2.143%
13	7.658	718	726	737	rBV	1295655	2097137	17.66%	2.039%
14	8.134	799	807	815	rBV	1161422	1883645	15.86%	1.831%
15	8.840	920	927	941	rBV	1124815	1880759	15.84%	1.828%
16	9.311	999	1007	1017	rBV	1599517	2704920	22.78%	2.630%
17	9.411	1020	1024	1028	rVB5	9622	14510	0.12%	0.014%
18	9.705	1068	1074	1081	rBV	125920	186041	1.57%	0.181%
19	10.034	1123	1130	1147	rBV	1301551	2158545	18.18%	2.098%
20	10.575	1215	1222	1244	rBV	1880371	3232265	27.22%	3.142%
21	10.963	1280	1288	1296	rBV	1786412	2976675	25.07%	2.894%
22	11.099	1302	1311	1331	rBV	1744764	3050361	25.69%	2.965%
23	11.757	1417	1423	1426	rBV8	5351	12511	0.11%	0.012%
24	12.199	1491	1498	1508	rVB	84016	125621	1.06%	0.122%
25	12.540	1551	1556	1562	rBV	30832	55831	0.47%	0.054%
26	13.657	1741	1746	1753	rBV2	49956	81981	0.69%	0.080%
27	13.740	1756	1760	1769	rVB5	6451	14182	0.12%	0.014%
28	14.175	1827	1834	1848	rBV	4197871	5935787	49.99%	5.770%
29	14.469	1876	1884	1901	rBV	4801298	7031343	59.22%	6.835%
30	14.775	1927	1936	1944	rBV	2892441	4209384	35.45%	4.092%
31	14.863	1948	1951	1957	rVB8	7518	13614	0.11%	0.013%
32	14.957	1961	1967	1984	rBV	347395	646236	5.44%	0.628%
33	15.181	1999	2005	2013	rVB	24603	50543	0.43%	0.049%
34	15.504	2054	2060	2066	rBV	72661	101137	0.85%	0.098%
35	15.722	2091	2097	2098	rBV	61891	72401	0.61%	0.070%
36	15.763	2098	2104	2117	rVV	6184216	8990379	75.71%	8.740%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015111.D
 Acq On : 16 May 2023 16:19
 Operator : CG/JU
 Sample : 02768-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.881	2117	2124	2140	rVV	2238467	3092666	26.05%	3.006%
38	16.004	2140	2145	2151	rVB	29866	51356	0.43%	0.050%
39	16.122	2160	2165	2175	rVB	232962	326668	2.75%	0.318%
40	16.457	2218	2222	2232	rVB6	15921	35221	0.30%	0.034%
41	16.551	2232	2238	2247	rBV6	8523	21362	0.18%	0.021%
42	16.975	2304	2310	2315	rBV	57480	78039	0.66%	0.076%
43	17.198	2344	2348	2354	rBV7	9237	15901	0.13%	0.015%
44	17.528	2397	2404	2413	rBV	3553399	5064895	42.65%	4.924%
45	17.628	2414	2421	2440	rVV	7299219	10364216	87.28%	10.075%
46	17.798	2447	2450	2454	rVB2	9803	13095	0.11%	0.013%
47	18.045	2487	2492	2497	rVB	49165	62279	0.52%	0.061%
48	18.169	2510	2513	2517	rBV6	9636	11907	0.10%	0.012%
49	18.381	2544	2549	2557	rBV	169354	236351	1.99%	0.230%
50	18.457	2558	2562	2573	rVB	48306	66907	0.56%	0.065%
51	18.945	2641	2645	2649	rVB2	41168	52821	0.44%	0.051%
52	19.422	2722	2726	2731	rBV	89214	114265	0.96%	0.111%
53	19.492	2733	2738	2745	rVB2	102657	154958	1.31%	0.151%
54	19.604	2753	2757	2764	rBV4	85858	120638	1.02%	0.117%
55	19.710	2772	2775	2779	rBV	50911	58629	0.49%	0.057%
56	19.845	2792	2798	2813	rBV	8990427	11874100	100.00%	11.543%
57	20.386	2887	2890	2893	rVB	49598	51156	0.43%	0.050%
58	21.280	3039	3042	3050	rBV3	120905	198367	1.67%	0.193%
59	21.604	3092	3097	3108	rVB	3591074	4790376	40.34%	4.657%
60	24.010	3498	3506	3525	rVB2	4909572	10294656	86.70%	10.008%
61	24.174	3527	3534	3545	rVB	2072671	4430261	37.31%	4.307%




Sum of corrected areas: 102866008

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015111.D
Acq On : 16 May 2023 16:19
Operator : CG/JU
Sample : 02768-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

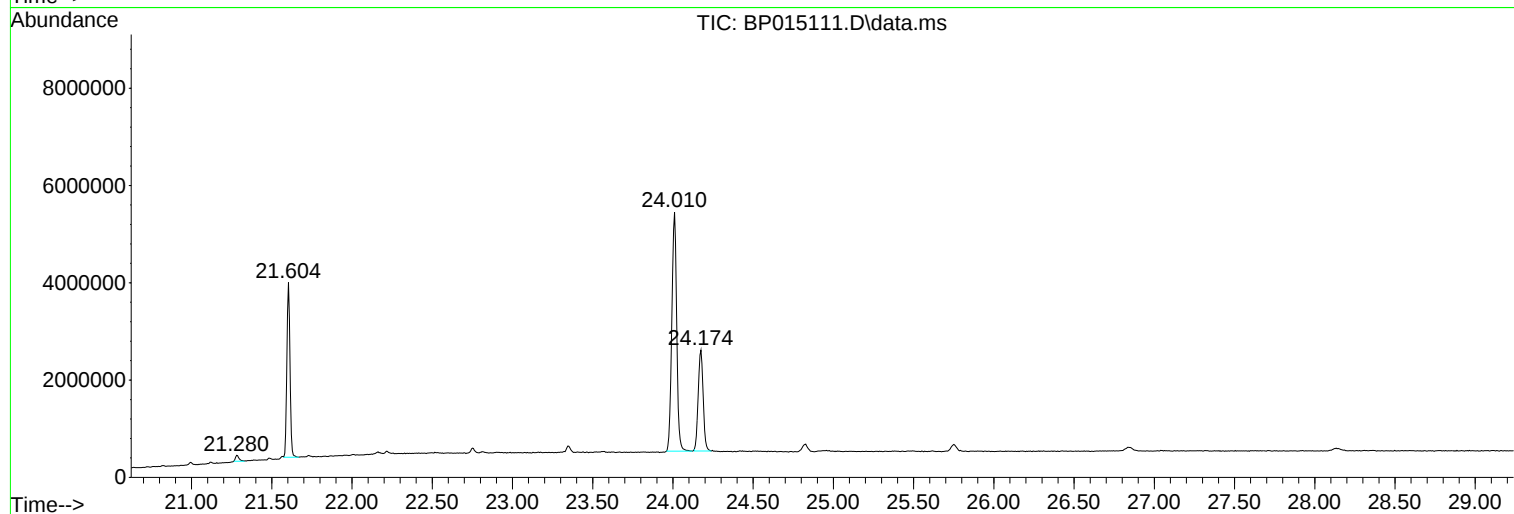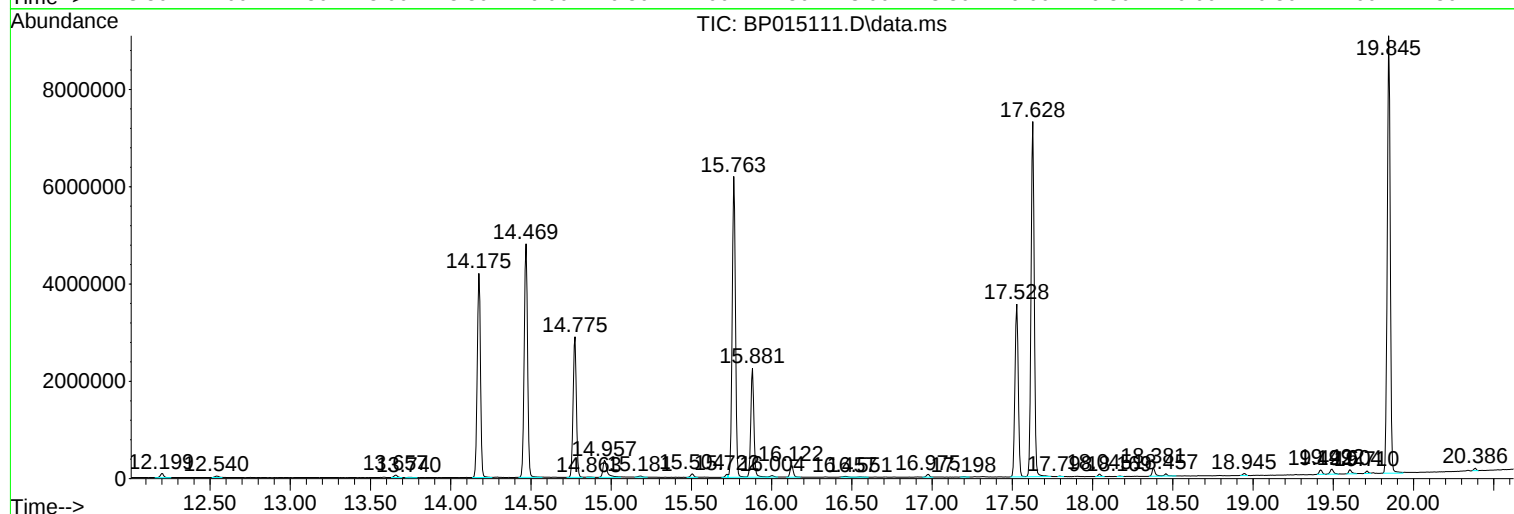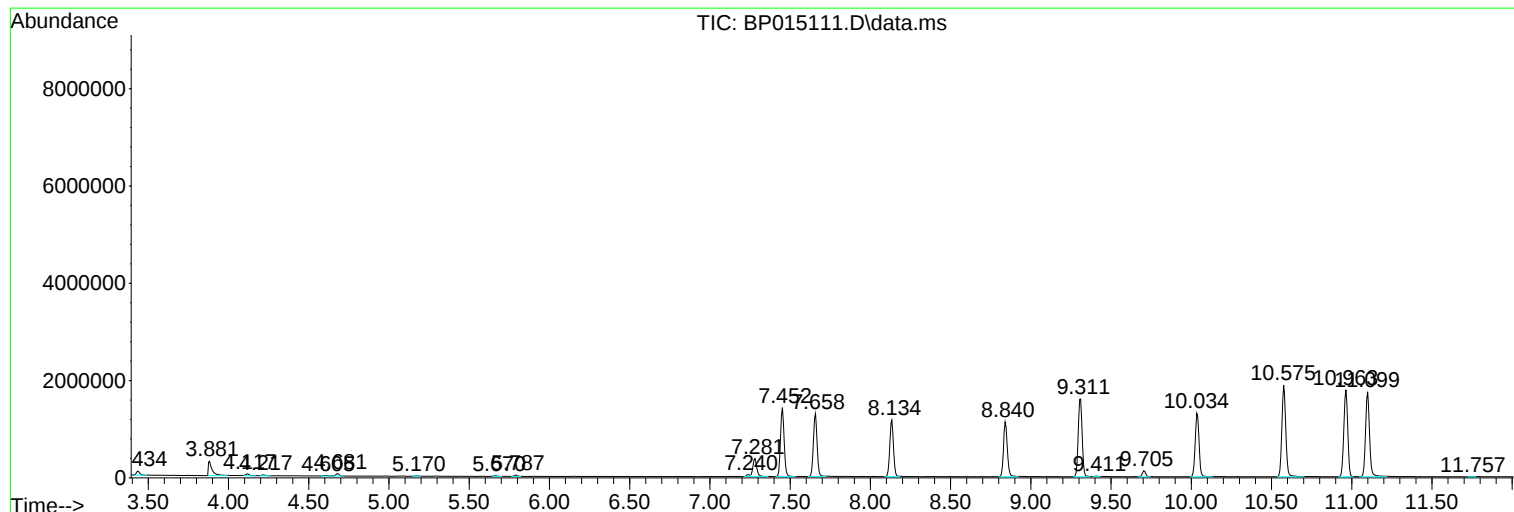

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015111.D
Acq On : 16 May 2023 16:19
Operator : CG/JU
Sample : 02768-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015111.D
Acq On : 16 May 2023 16:19
Operator : CG/JU
Sample : 02768-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
