

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015114.D
 Acq On : 16 May 2023 18:01
 Operator : CG/JU
 Sample : 02768-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	16	rVB	80052	109736	0.93%	0.106%
2	3.875	81	83	103	rBV	296129	494727	4.20%	0.478%
3	4.117	119	124	130	rVB	36409	57029	0.48%	0.055%
4	4.217	137	141	146	rVB2	21846	30462	0.26%	0.029%
5	4.675	215	219	226	rVB	50059	72359	0.62%	0.070%
6	5.664	383	387	393	rVB	14516	20662	0.18%	0.020%
7	5.793	404	409	414	rVB	25491	36690	0.31%	0.035%
8	6.146	465	469	474	rVB2	12016	18937	0.16%	0.018%
9	7.240	649	655	657	rBV	37353	58943	0.50%	0.057%
10	7.281	657	662	675	rVB	365744	597914	5.08%	0.577%
11	7.452	684	691	701	rBV	1421010	2216248	18.84%	2.140%
12	7.658	717	726	737	rBV	1290072	2096698	17.82%	2.025%
13	7.858	755	760	769	rVB6	7821	19406	0.16%	0.019%
14	8.134	799	807	814	rBV	1183741	1919889	16.32%	1.854%
15	8.187	814	816	823	rVB7	9216	12358	0.11%	0.012%
16	8.840	920	927	942	rBV	1154042	1893069	16.09%	1.828%
17	9.310	999	1007	1018	rBV	1641116	2737508	23.27%	2.644%
18	9.410	1019	1024	1030	rBV	43777	69057	0.59%	0.067%
19	9.704	1068	1074	1084	rVB	122087	188830	1.60%	0.182%
20	10.034	1122	1130	1142	rBV	1334793	2213885	18.82%	2.138%
21	10.575	1213	1222	1236	rBV	1961201	3291643	27.98%	3.179%
22	10.963	1278	1288	1297	rBV	1853116	3040440	25.84%	2.936%
23	11.099	1303	1311	1325	rBV	1783843	3091560	26.28%	2.986%
24	11.746	1414	1421	1424	rBV6	13807	26810	0.23%	0.026%
25	12.198	1491	1498	1505	rVB	82670	121669	1.03%	0.118%
26	12.540	1550	1556	1566	rBV2	32858	64612	0.55%	0.062%
27	13.581	1728	1733	1737	rBV6	6678	12637	0.11%	0.012%
28	14.175	1827	1834	1847	rBV	4310879	5845328	49.68%	5.645%
29	14.287	1851	1853	1863	rVB9	6326	13091	0.11%	0.013%
30	14.469	1877	1884	1896	rBV	4803796	7092343	60.28%	6.850%
31	14.775	1929	1936	1945	rBV	2872320	4275854	36.34%	4.130%
32	14.957	1961	1967	1988	rBV	331770	624015	5.30%	0.603%
33	15.175	2000	2004	2012	rVB7	21653	41086	0.35%	0.040%
34	15.504	2055	2060	2064	rBV7	6573	12749	0.11%	0.012%
35	15.581	2070	2073	2080	rVB	8062	12879	0.11%	0.012%
36	15.722	2092	2097	2098	rBV2	63097	74579	0.63%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015114.D
 Acq On : 16 May 2023 18:01
 Operator : CG/JU
 Sample : 02768-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.763	2098	2104	2117	rVV	6108262	8804895	74.84%	8.504%
38	15.881	2117	2124	2137	rVV	2258017	3070234	26.09%	2.965%
39	15.998	2141	2144	2150	rVB2	28392	46603	0.40%	0.045%
40	16.122	2159	2165	2177	rBV	191379	286015	2.43%	0.276%
41	16.469	2219	2224	2230	rVB8	8967	18399	0.16%	0.018%
42	16.975	2305	2310	2315	rBV	53030	68185	0.58%	0.066%
43	17.310	2364	2367	2375	rVB6	9262	18521	0.16%	0.018%
44	17.528	2397	2404	2414	rBV	3595050	5153377	43.80%	4.977%
45	17.628	2414	2421	2445	rVV	7185650	10317611	87.69%	9.965%
46	17.792	2447	2449	2455	rVB2	11089	16438	0.14%	0.016%
47	17.904	2462	2468	2471	rBV5	10027	20979	0.18%	0.020%
48	18.039	2488	2491	2495	rVB	44948	56557	0.48%	0.055%
49	18.169	2510	2513	2520	rVB8	10628	14873	0.13%	0.014%
50	18.380	2544	2549	2558	rBV	122061	183611	1.56%	0.177%
51	18.457	2558	2562	2570	rVB	37722	53565	0.46%	0.052%
52	18.945	2641	2645	2649	rVB	44002	49924	0.42%	0.048%
53	19.422	2721	2726	2730	rBV	93129	126133	1.07%	0.122%
54	19.486	2733	2737	2747	rVB	97762	163609	1.39%	0.158%
55	19.604	2753	2757	2768	rBV3	84290	131784	1.12%	0.127%
56	19.710	2771	2775	2778	rBV	46993	60245	0.51%	0.058%
57	19.845	2792	2798	2806	rBV	8876159	11765637	100.00%	11.363%
58	20.380	2887	2889	2894	rVB2	46857	48511	0.41%	0.047%
59	21.280	3039	3042	3047	rBV4	85818	132557	1.13%	0.128%
60	21.604	3092	3097	3105	rVB	3583023	4847486	41.20%	4.682%
61	23.345	3390	3393	3401	rVB	167394	259301	2.20%	0.250%
62	24.010	3497	3506	3524	rBV2	4830476	10617049	90.24%	10.254%
63	24.168	3526	3533	3548	rVB	2188151	4702526	39.97%	4.542%




Sum of corrected areas: 103540327

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP05114.D
Acq On : 16 May 2023 18:01
Operator : CG/JU
Sample : 02768-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

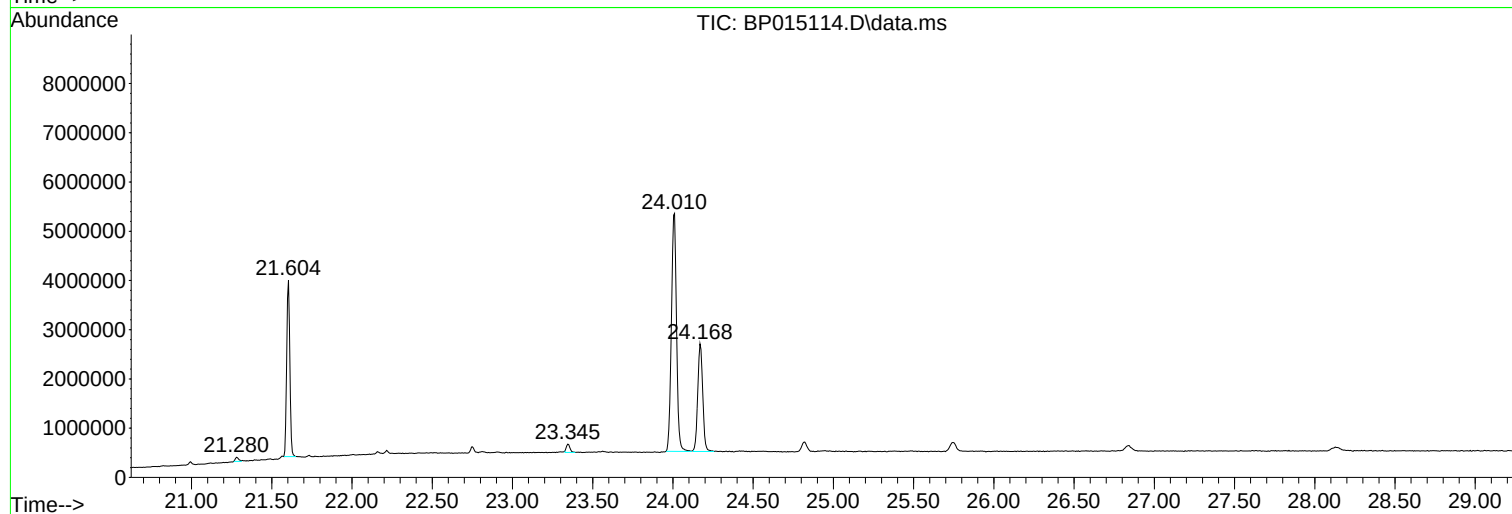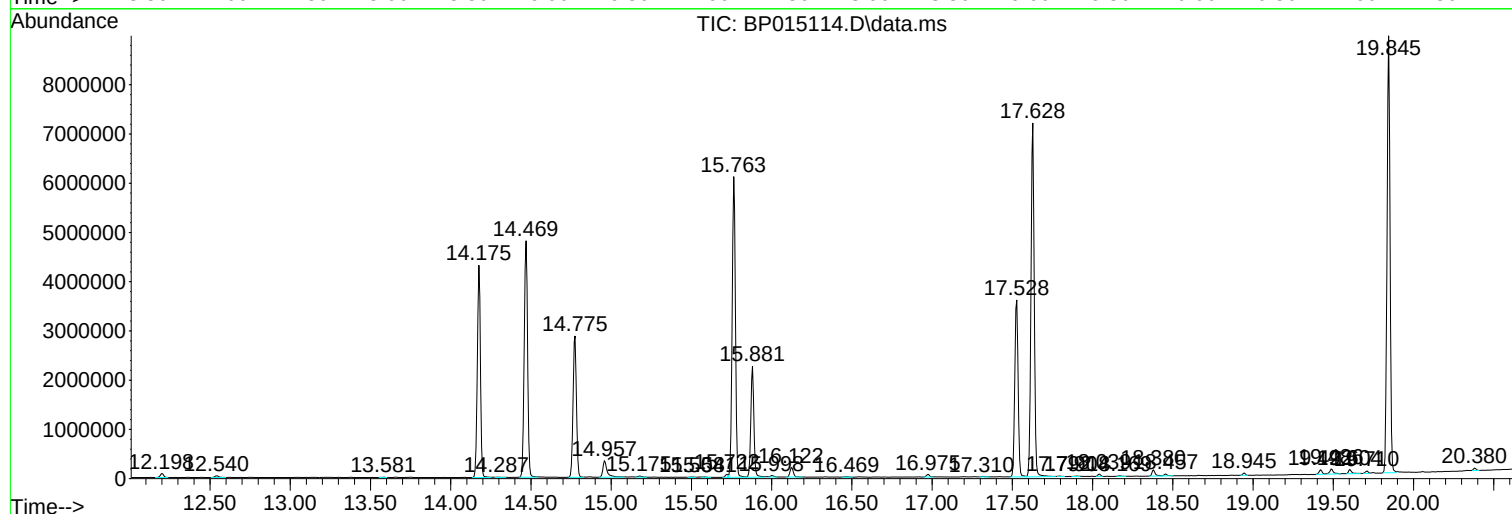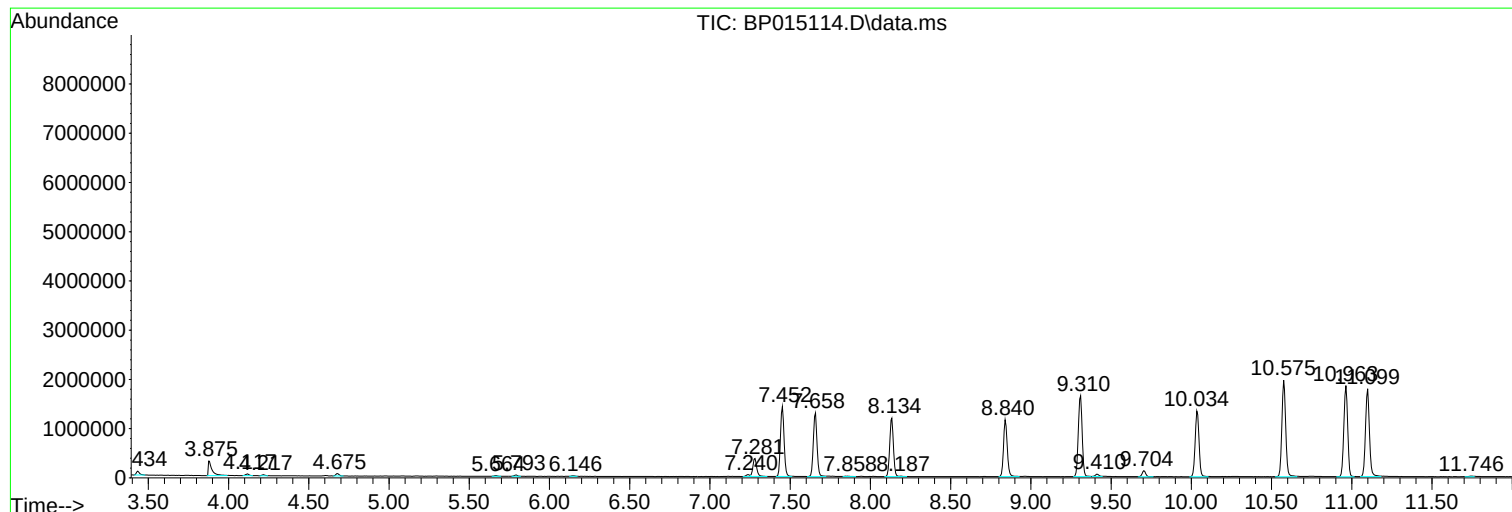

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015114.D
Acq On : 16 May 2023 18:01
Operator : CG/JU
Sample : 02768-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015114.D
Acq On : 16 May 2023 18:01
Operator : CG/JU
Sample : 02768-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc