

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015117.D
 Acq On : 16 May 2023 20:16
 Operator : CG/JU
 Sample : PB152800BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK800

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rVB	121964	159962	1.39%	0.134%
2	3.870	80	82	103	rBV	1578864	2453763	21.39%	2.053%
3	4.217	137	141	146	rVB	22112	30208	0.26%	0.025%
4	7.281	654	662	676	rBV	1801646	2947763	25.70%	2.466%
5	7.452	684	691	703	rVB	1629352	2550411	22.23%	2.134%
6	7.652	718	725	740	rBV	1852671	3065243	26.72%	2.565%
7	8.128	799	806	820	rVB	1370092	2244965	19.57%	1.878%
8	8.840	916	927	944	rBV	2420847	3967582	34.59%	3.320%
9	9.305	999	1006	1021	rBV	1838704	3091663	26.95%	2.587%
10	10.034	1122	1130	1146	rBV	1585713	2578323	22.48%	2.157%
11	10.575	1213	1222	1241	rBV	2317828	3950442	34.44%	3.305%
12	10.963	1279	1288	1296	rBV	2099808	3517086	30.66%	2.943%
13	11.099	1303	1311	1332	rBV	2523427	4413295	38.48%	3.692%
14	12.546	1550	1557	1571	rBV4	31074	73505	0.64%	0.061%
15	13.657	1740	1746	1752	rBV2	39941	64721	0.56%	0.054%
16	13.745	1756	1761	1767	rVB9	6924	11494	0.10%	0.010%
17	14.175	1826	1834	1849	rBV	4472356	6213202	54.17%	5.198%
18	14.287	1849	1853	1861	rVB	7112	16005	0.14%	0.013%
19	14.469	1876	1884	1898	rBV	5175577	7635028	66.56%	6.388%
20	14.769	1928	1935	1946	rBV	3277797	4926983	42.95%	4.122%
21	14.869	1948	1952	1958	rVB8	6266	12439	0.11%	0.010%
22	14.957	1960	1967	1993	rBV	2014024	3204200	27.93%	2.681%
23	15.763	2096	2104	2117	rBV	6420535	9166147	79.91%	7.669%
24	15.881	2117	2124	2140	rVV	2065499	2983574	26.01%	2.496%
25	16.004	2140	2145	2153	rVB3	33972	61218	0.53%	0.051%
26	17.198	2345	2348	2353	rVB3	9595	13116	0.11%	0.011%
27	17.316	2362	2368	2373	rBV6	8896	17832	0.16%	0.015%
28	17.528	2397	2404	2414	rBV	4199791	5923055	51.64%	4.956%
29	17.628	2414	2421	2442	rVB	6756950	9992797	87.12%	8.361%
30	19.422	2722	2726	2731	rBV	82512	115006	1.00%	0.096%
31	19.486	2733	2737	2748	rVB	74580	118140	1.03%	0.099%
32	19.845	2792	2798	2812	rBV	8379578	11470300	100.00%	9.597%
33	21.604	3091	3097	3107	rBV	4132435	5833247	50.86%	4.881%
34	22.751	3289	3292	3299	rVB2	146281	203153	1.77%	0.170%
35	23.345	3390	3393	3402	rVB	210787	352152	3.07%	0.295%
36	24.004	3497	3505	3525	rBV2	4725286	10341369	90.16%	8.652%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015117.D
Acq On : 16 May 2023 20:16
Operator : CG/JU
Sample : PB152800BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	24.174	3526	3534	3545	rVB	2475861	5286057	46.08%	4.423%
38	24.821	3640	3644	3650	rVB2	278675	515382	4.49%	0.431%




Sum of corrected areas: 119520828

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015117.D
Acq On : 16 May 2023 20:16
Operator : CG/JU
Sample : PB152800BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

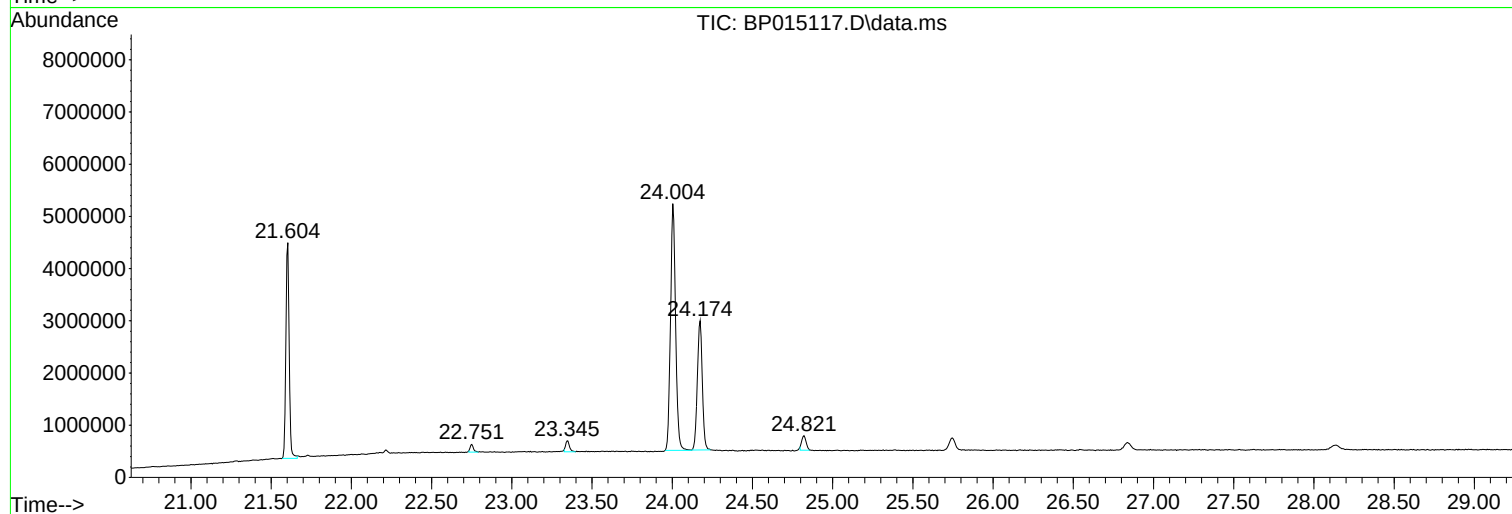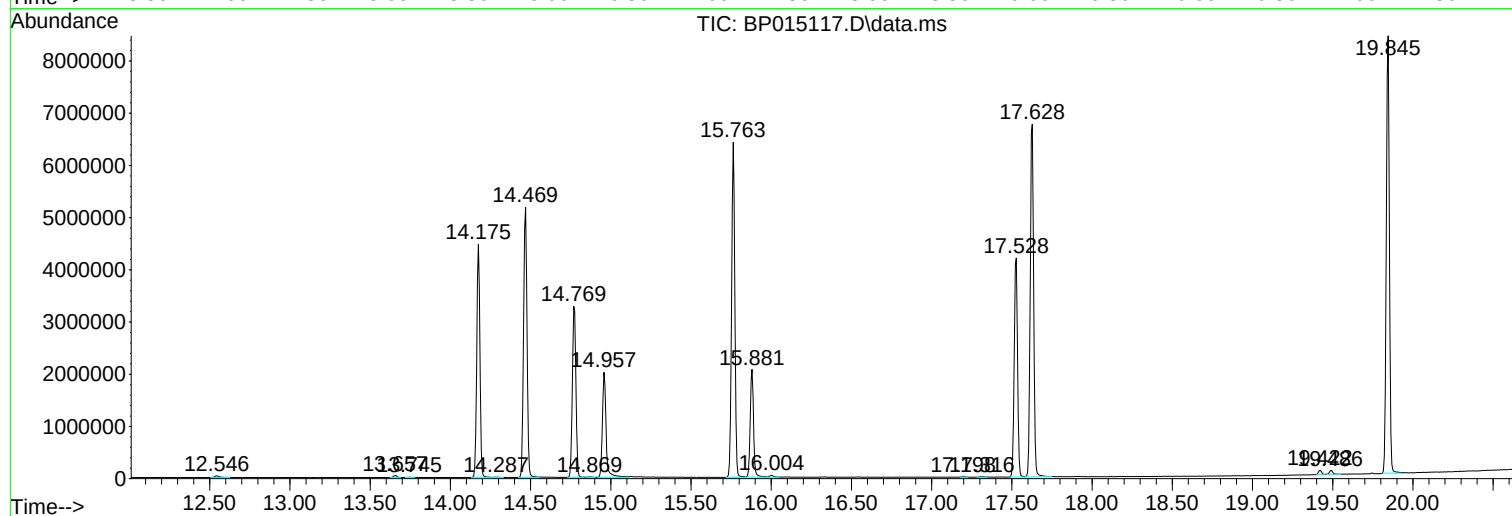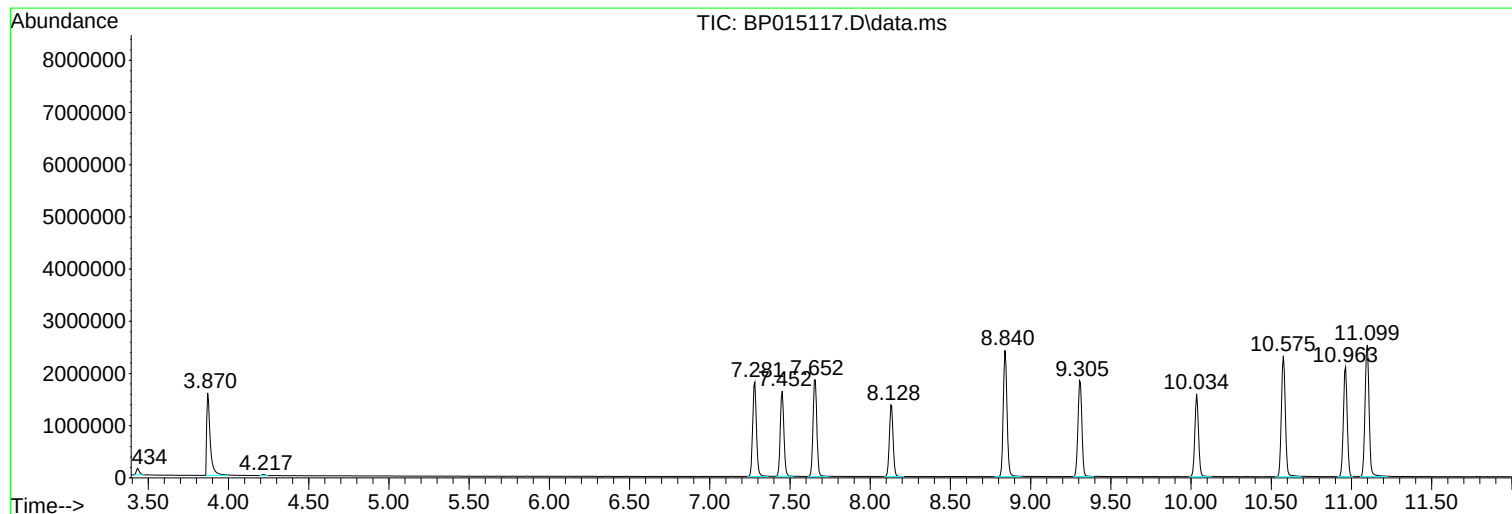

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015117.D
Acq On : 16 May 2023 20:16
Operator : CG/JU
Sample : PB152800BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015117.D
Acq On : 16 May 2023 20:16
Operator : CG/JU
Sample : PB152800BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------