

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051624\
 Data File : BP020412.D
 Acq On : 16 May 2024 15:40
 Operator : MA/JU
 Sample : PB160897BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	14	18	23	rVB	19059	23512	1.22%	0.124%
2	3.599	83	87	106	rBV	148139	323912	16.79%	1.707%
3	3.887	132	136	143	rVB3	6156	12634	0.65%	0.067%
4	4.299	204	206	210	rBV5	2292	2920	0.15%	0.015%
5	6.787	623	629	650	rBV	147391	413740	21.45%	2.180%
6	6.946	650	656	672	rVB	154352	302119	15.66%	1.592%
7	7.134	681	688	704	rBV	208707	424210	21.99%	2.235%
8	7.587	759	765	788	rBV	231062	444700	23.05%	2.343%
9	8.305	881	887	913	rBV	213112	527554	27.35%	2.780%
10	8.499	918	920	926	rVB7	1617	2847	0.15%	0.015%
11	8.758	955	964	980	rBV	198249	417143	21.62%	2.198%
12	9.469	1077	1085	1113	rBV	169039	373933	19.38%	1.970%
13	10.016	1172	1178	1208	rBV	158973	519533	26.93%	2.737%
14	10.363	1229	1237	1252	rBV	320690	605384	31.38%	3.190%
15	10.540	1259	1267	1299	rBV	140442	508055	26.34%	2.677%
16	12.022	1513	1519	1522	rBV8	3019	6178	0.32%	0.033%
17	13.693	1796	1803	1820	rBV	555781	918326	47.60%	4.839%
18	13.957	1839	1848	1865	rBV	558729	989644	51.30%	5.215%
19	14.269	1892	1901	1915	rBV	488739	874778	45.35%	4.609%
20	14.404	1921	1924	1930	rVB7	1149	2108	0.11%	0.011%
21	14.587	1947	1955	1968	rBV3	65245	266665	13.82%	1.405%
22	15.304	2068	2077	2093	rBV	730503	1292962	67.02%	6.813%
23	15.469	2098	2105	2116	rBV	152841	368650	19.11%	1.942%
24	16.116	2212	2215	2220	rBV7	1651	2819	0.15%	0.015%
25	16.910	2346	2350	2352	rBV5	1605	2485	0.13%	0.013%
26	17.116	2378	2385	2397	rBV	709622	1181404	61.24%	6.225%
27	17.234	2397	2405	2421	rVV	829222	1516573	78.61%	7.991%
28	19.175	2731	2735	2739	rBV6	9511	16699	0.87%	0.088%
29	19.622	2805	2811	2827	rBV	1200605	1893335	98.14%	9.976%
30	21.610	3143	3149	3161	rBV	705063	1389829	72.04%	7.323%
31	24.733	3670	3680	3698	rBV	687329	1929139	100.00%	10.165%
32	24.963	3709	3719	3736	rVB	425041	1424782	73.86%	7.507%




Sum of corrected areas: 18978572

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051624\
Data File : BP020412.D
Acq On : 16 May 2024 15:40
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

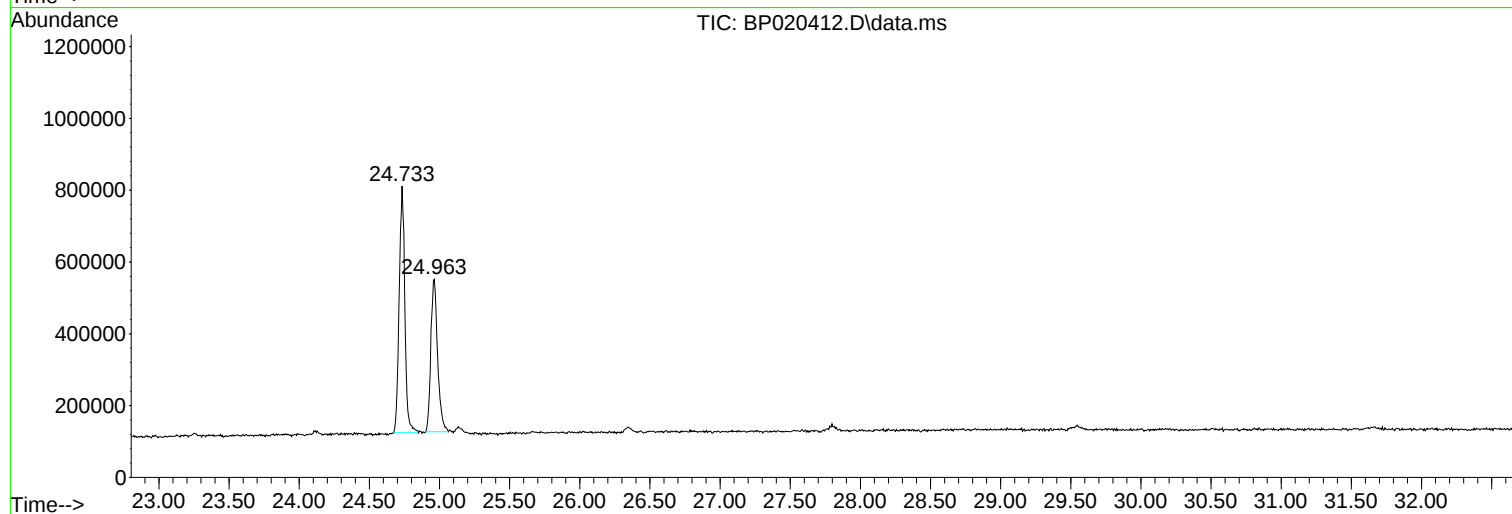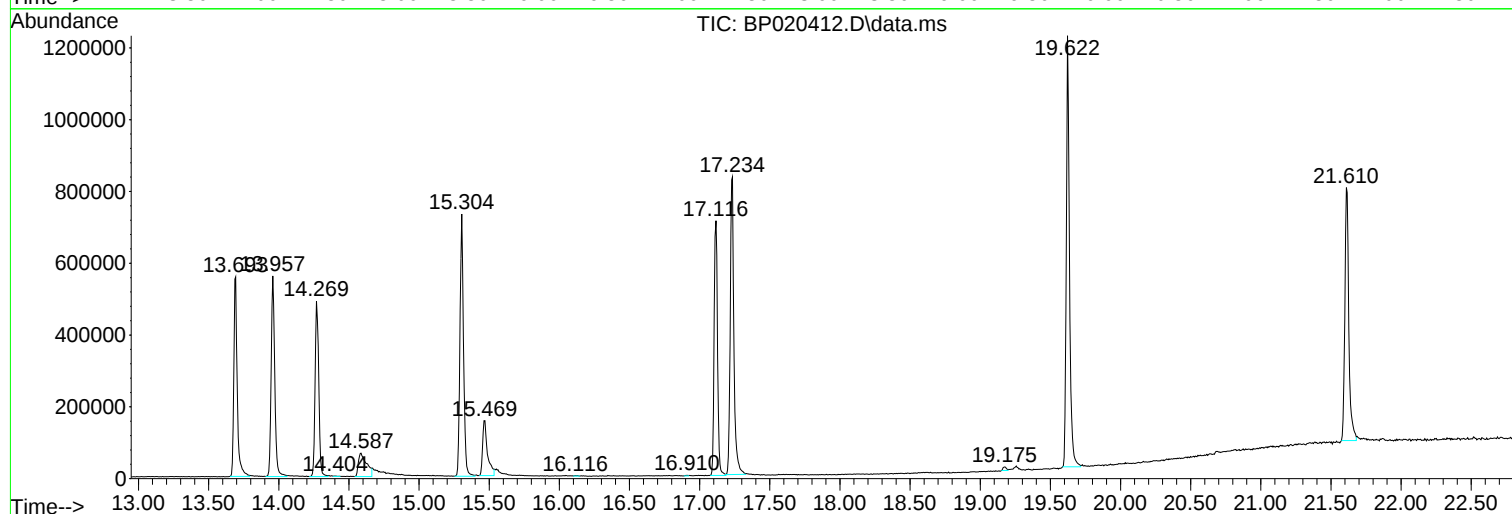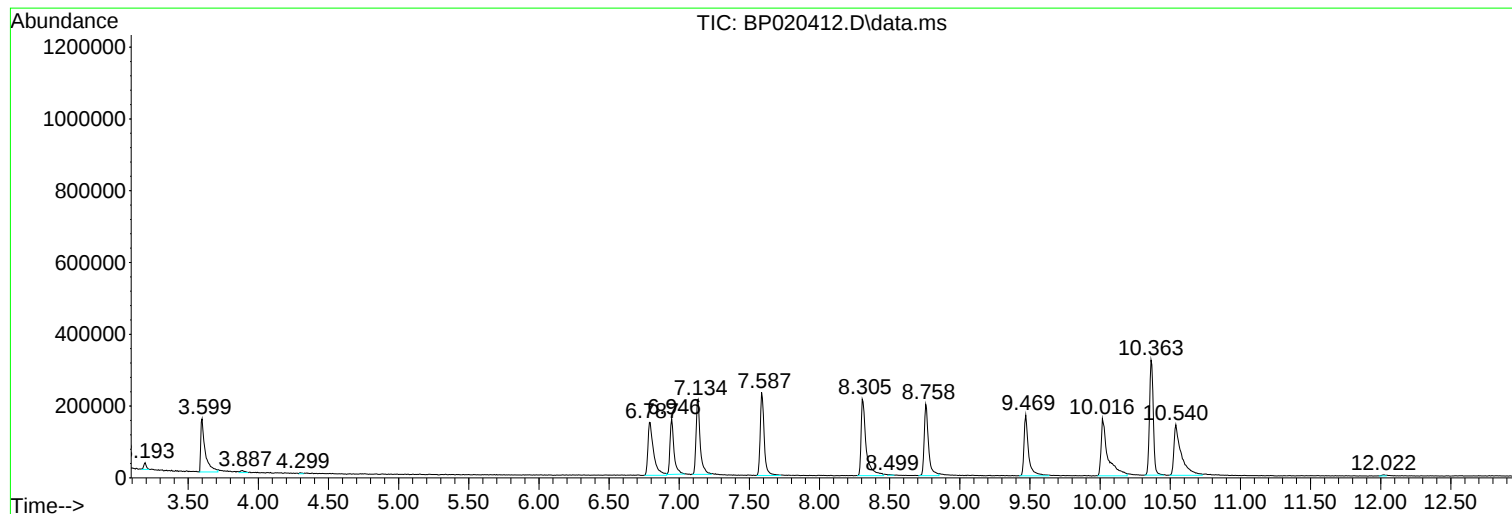

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051624\
Data File : BP020412.D
Acq On : 16 May 2024 15:40
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051624\
Data File : BP020412.D
Acq On : 16 May 2024 15:40
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc