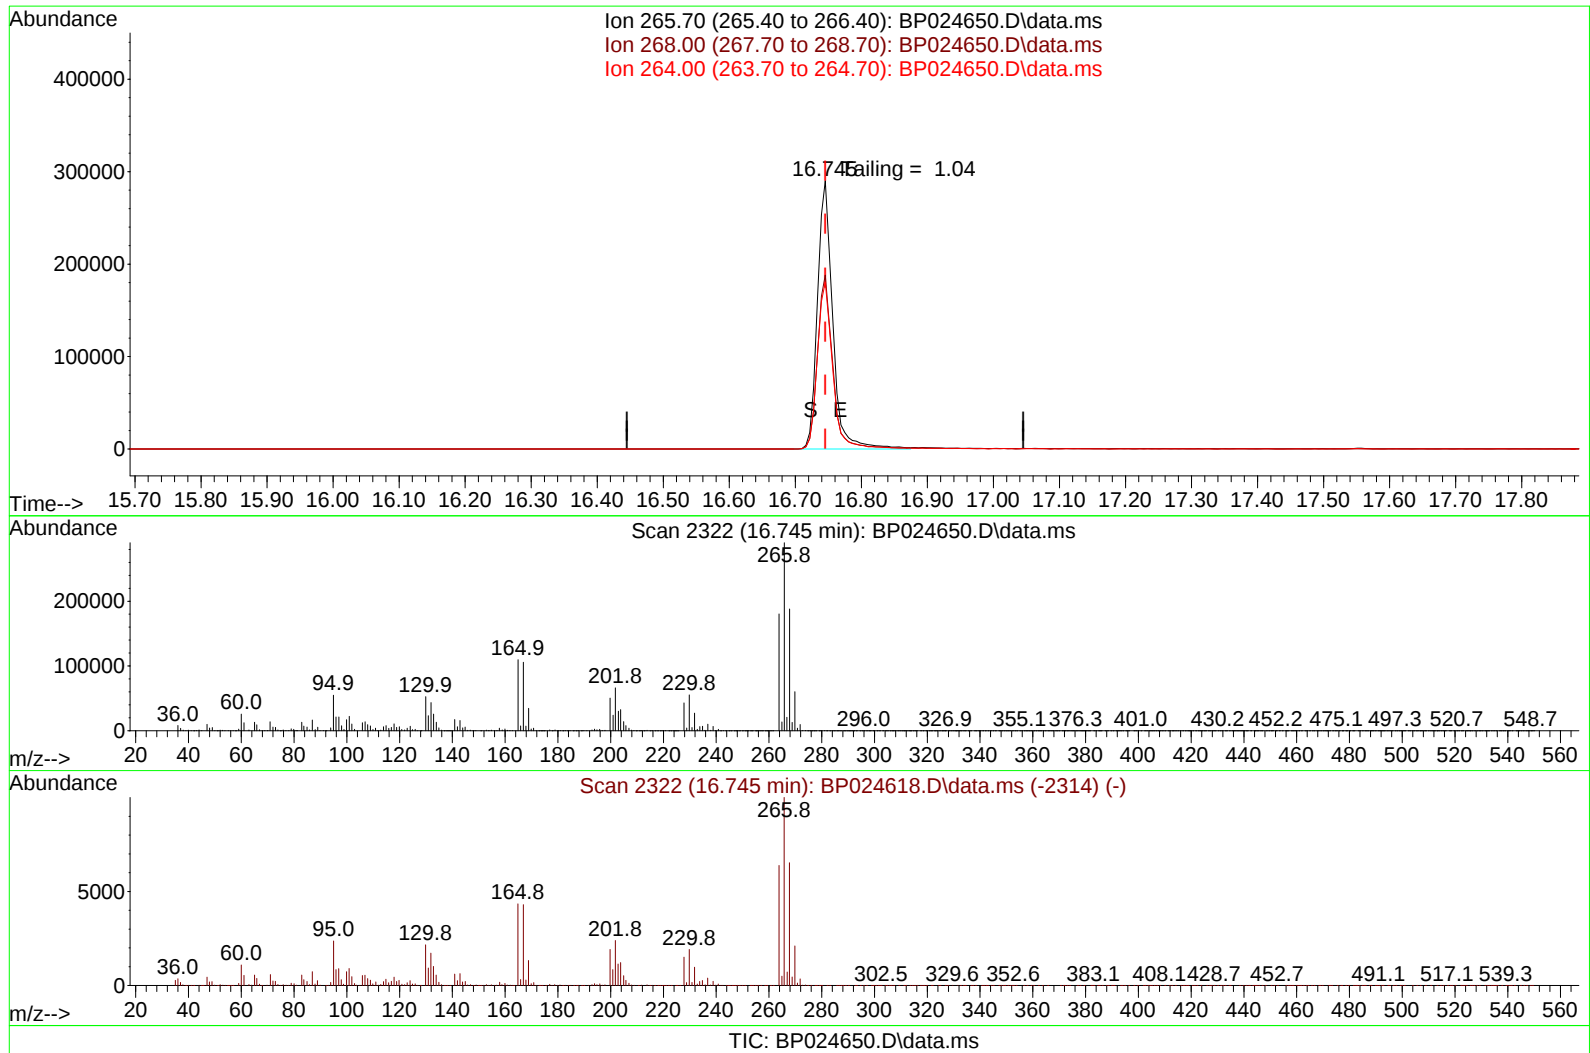


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024650.D
Acq On : 16 May 2025 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: May 16 11:41:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****16.745min (+ 0.000) 55883.60 ng****response 469236**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.79
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024650.D
Acq On : 16 May 2025 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 11:41:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

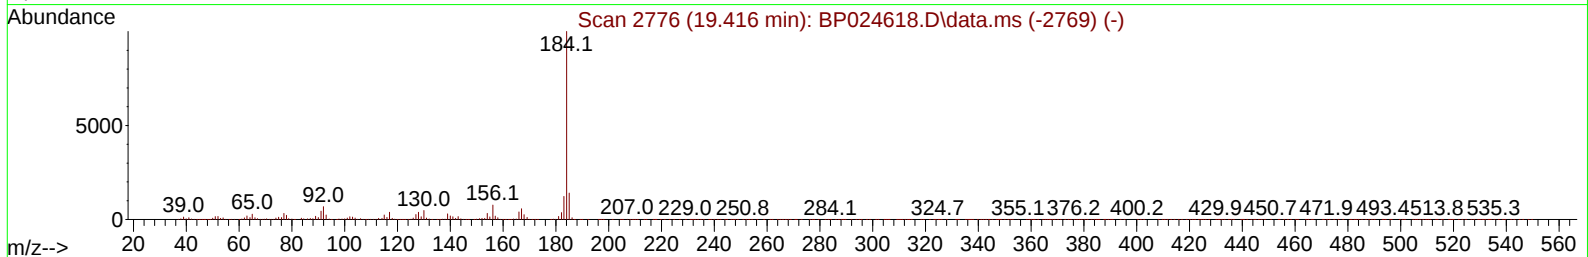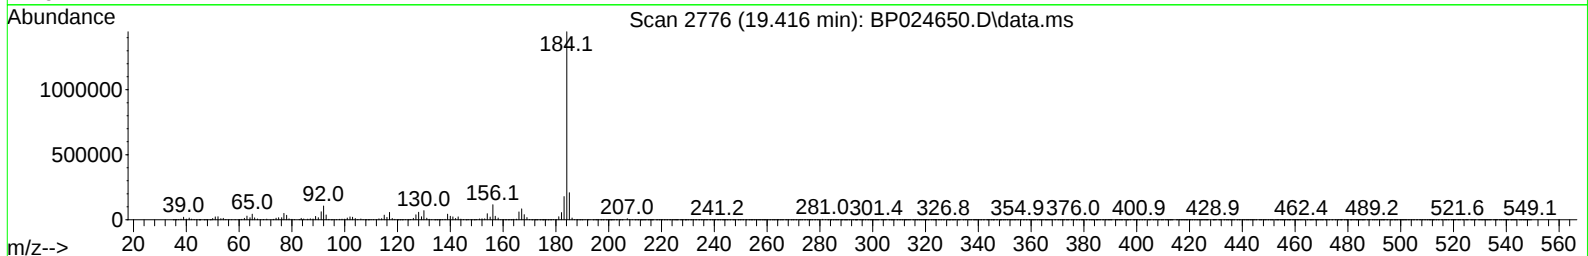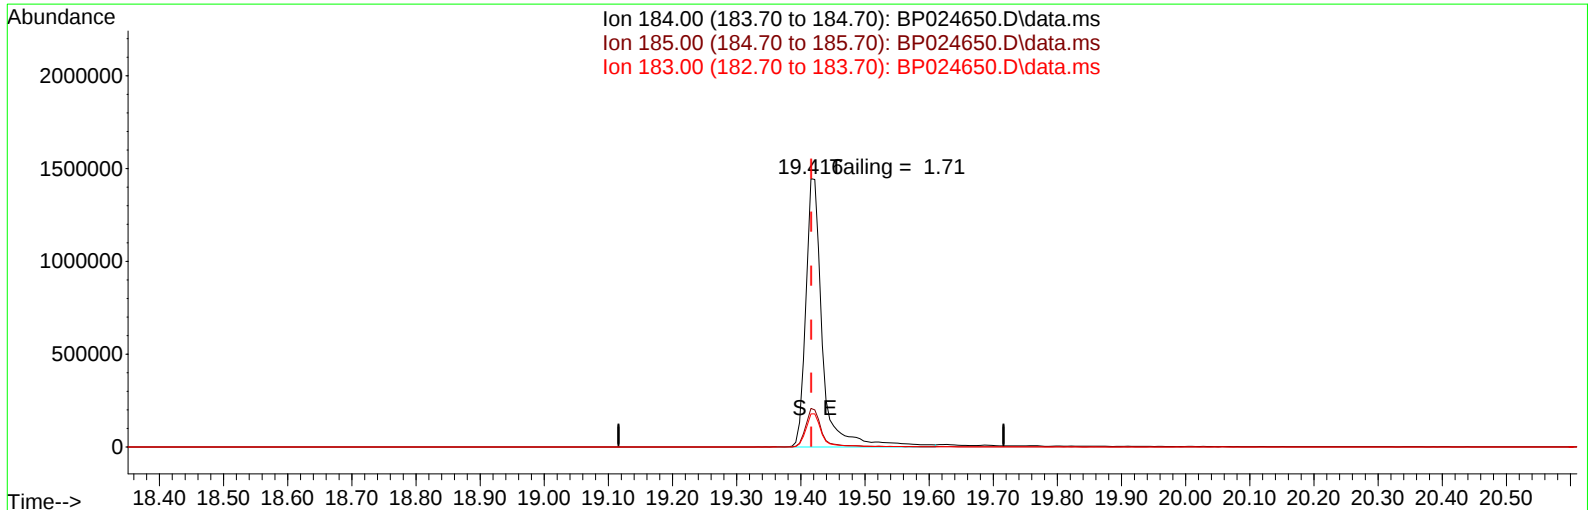

TIC: BP024650.D\data.ms

(77) Benzidine

19.416min (-0.000) 43939.06 ng

response 2620821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	12.30	12.37
0.00	0.00	0.00