
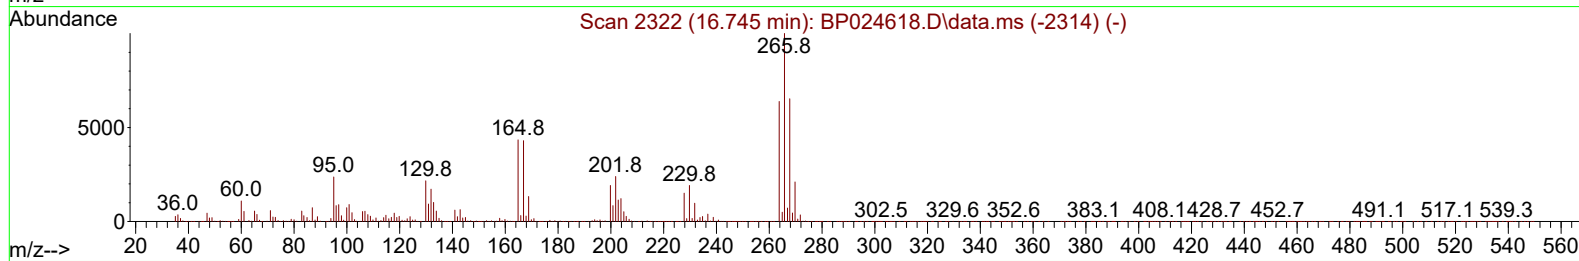
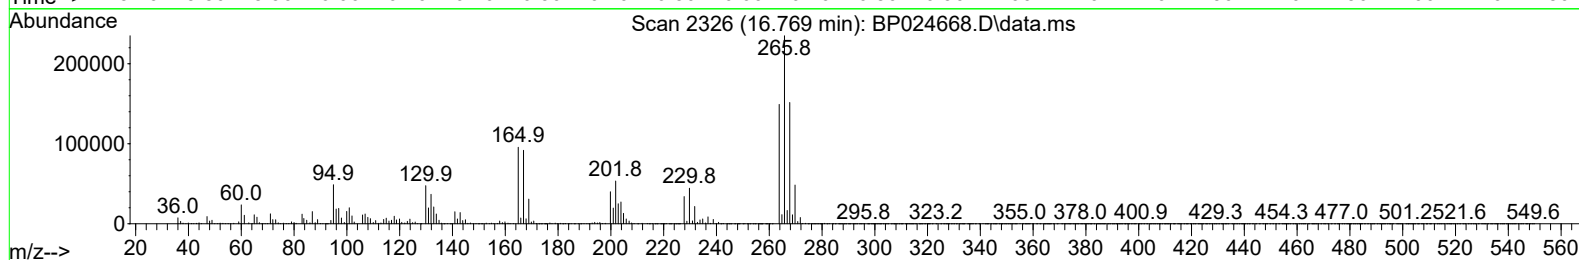


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024668.D
Acq On : 16 May 2025 22:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 06:36:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

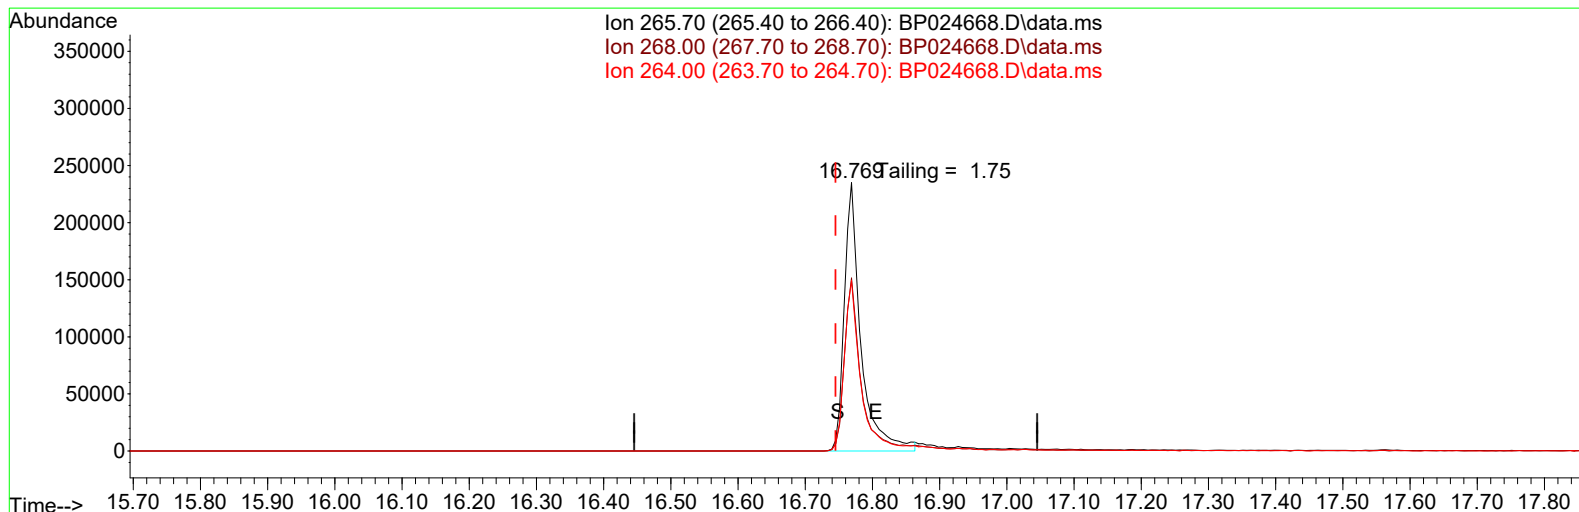

TIC: BP024668.D\data.ms

(70) Pentachlorophenol (C)




16.769min (+ 0.024) 376790.59 ng

response 399036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.52
264.00	63.90	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024668.D
Acq On : 16 May 2025 22:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 06:36:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

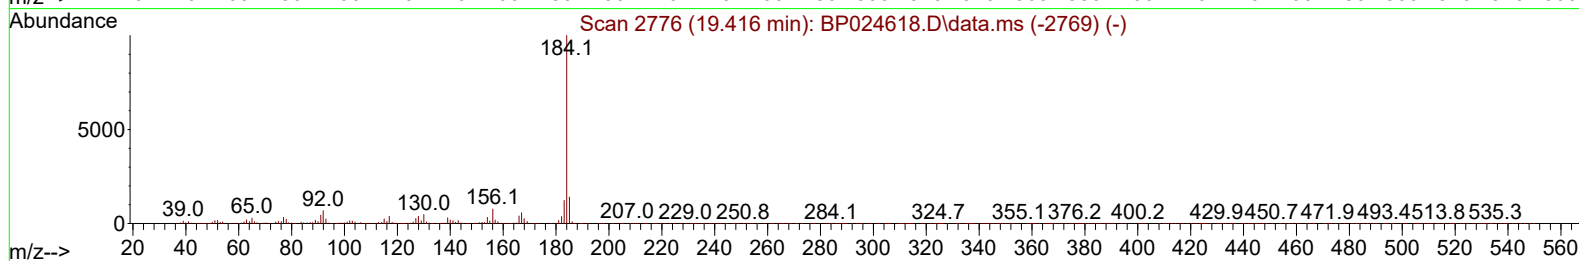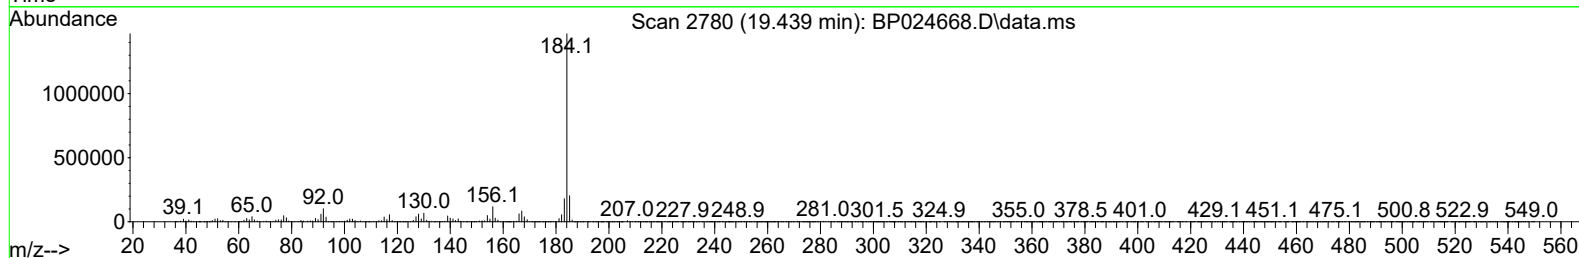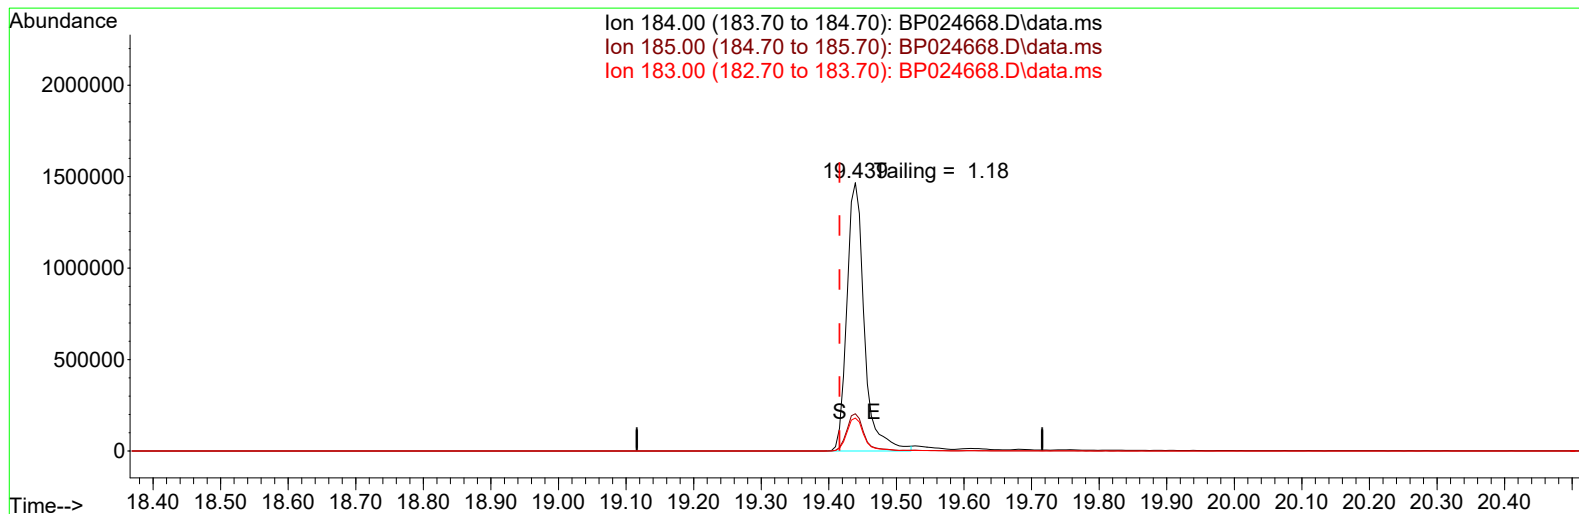

TIC: BP024668.D\data.ms

(77) Benzidine

19.439min (+ 0.023) 577599.08 ng

response 2611422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	12.30	12.30
0.00	0.00	0.00