
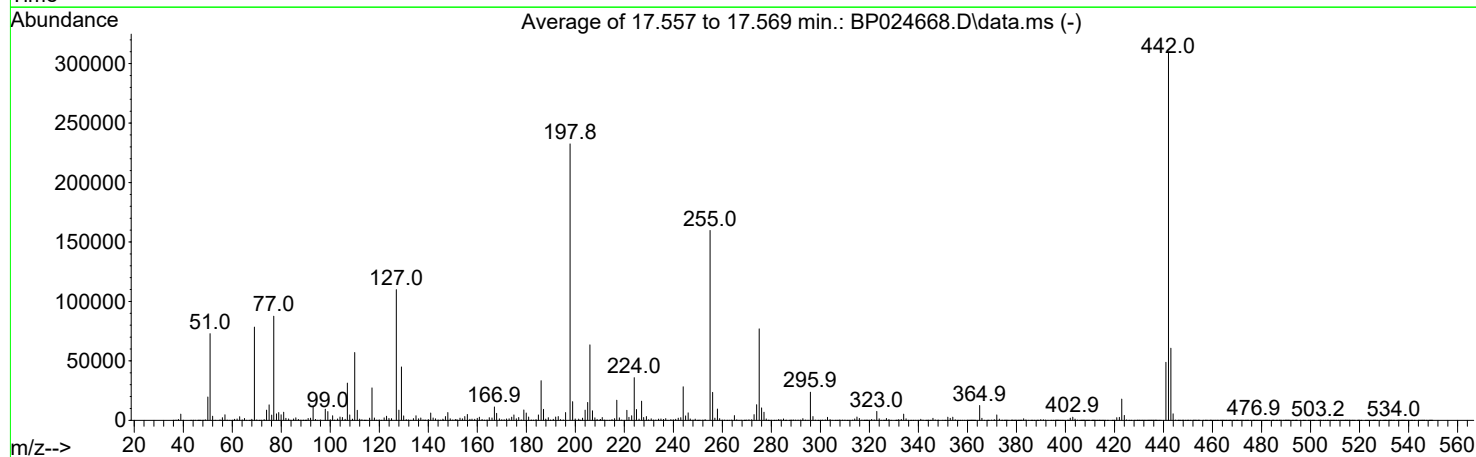


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024668.D
Acq On : 16 May 2025 22:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

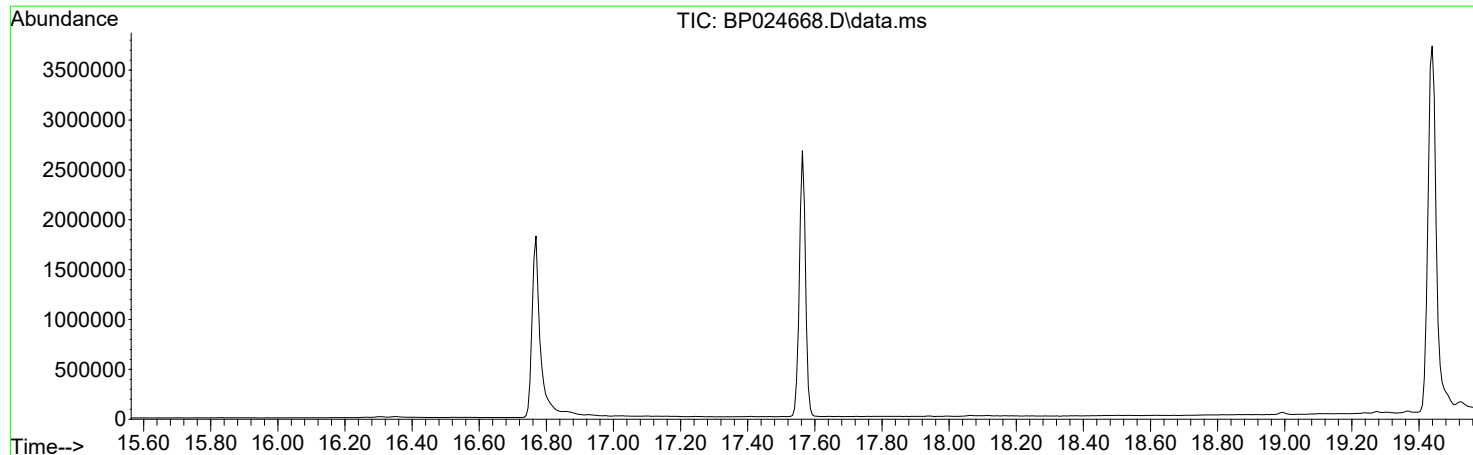

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	72876	PASS
68	69	0.00	2	1.3	1020	PASS
69	198	0.00	100	33.8	78491	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	47.3	109917	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	232491	PASS
199	198	5	9	6.8	15755	PASS
275	198	10	60	33.1	77025	PASS
365	198	1	100	5.4	12518	PASS
441	198	0.01	100	21.0	48785	PASS
442	442	100	100	100.0	309333	PASS
443	442	15	24	19.6	60728	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2025	BNA_P	<u>BP024668.D</u>
Compound Name	Response	Retention Time
DDT	886992	20.722
DDD	45854	20.257
DDE	18409	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
64263	951255	6.76

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024668.D
Acq On : 16 May 2025 22:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 19 06:36:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

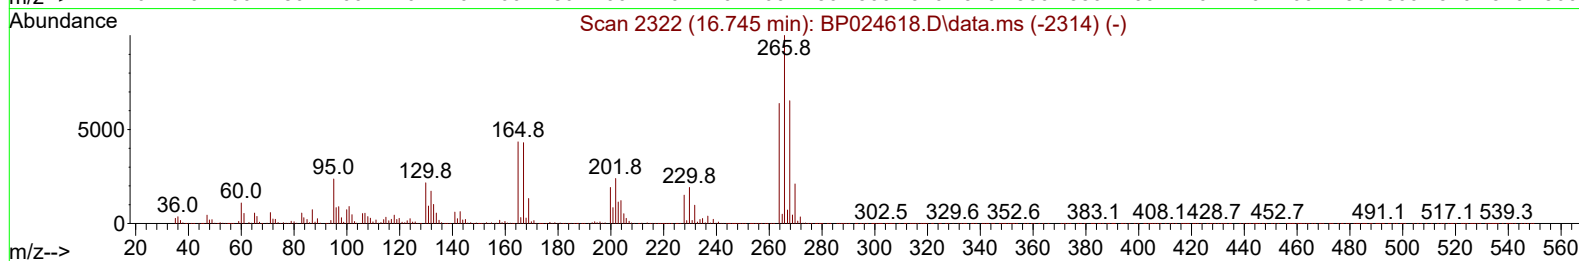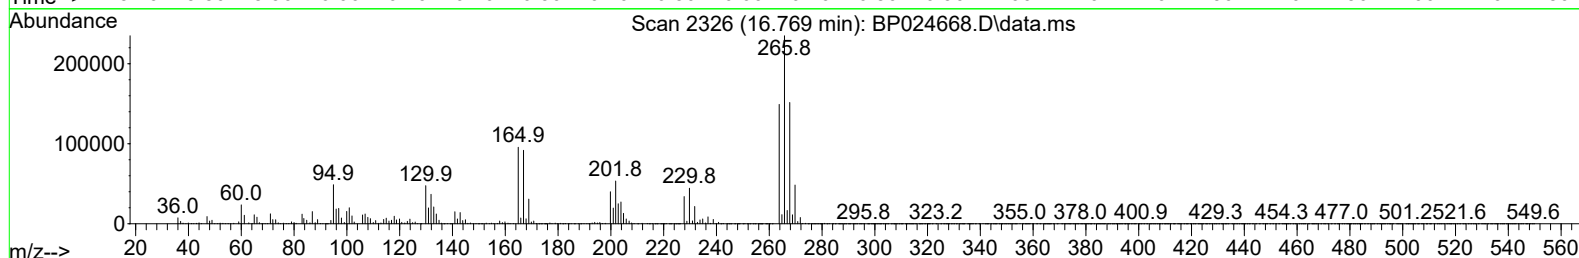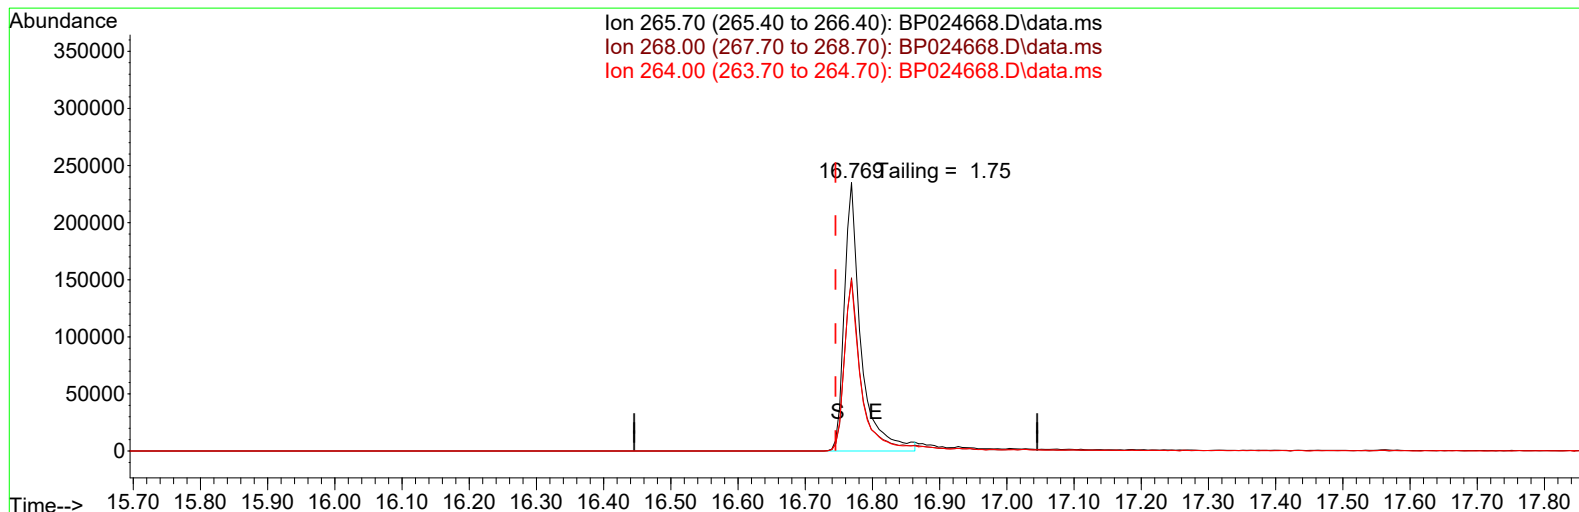

TIC: BP024668.D\data.ms

(70) Pentachlorophenol (C)

16.769min (+ 0.024) 376790.59 ng




response 399036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.52
264.00	63.90	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024668.D
Acq On : 16 May 2025 22:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 19 06:36:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

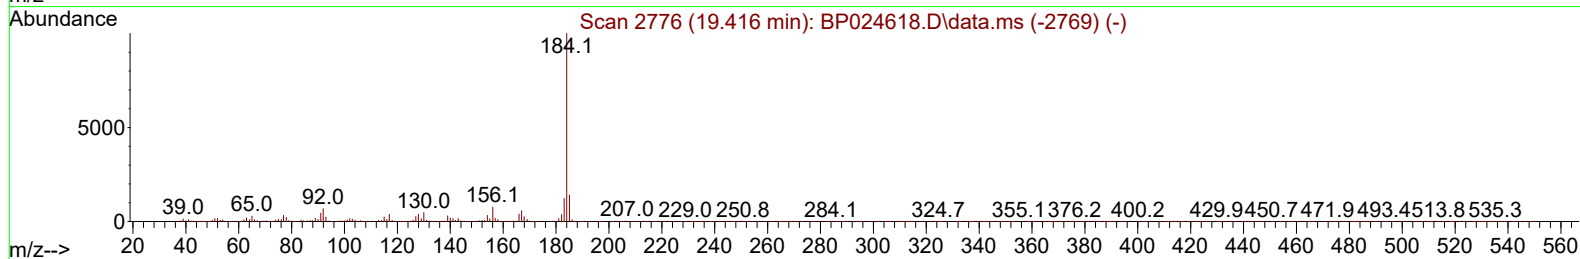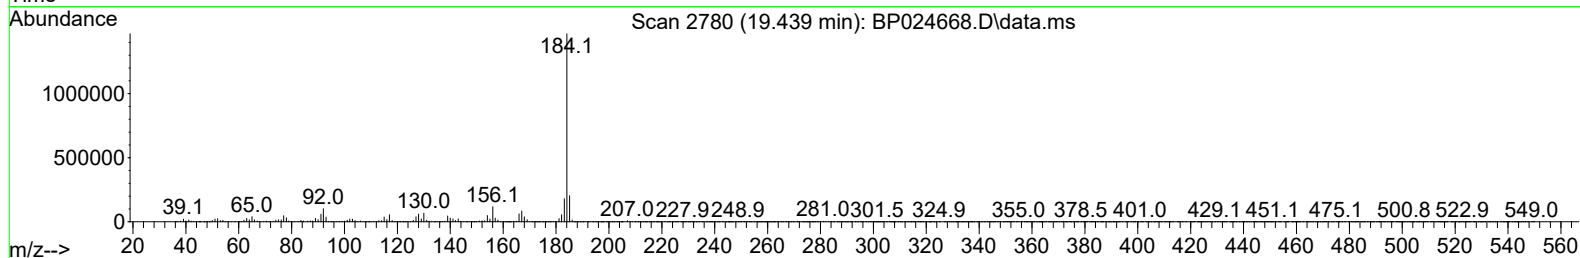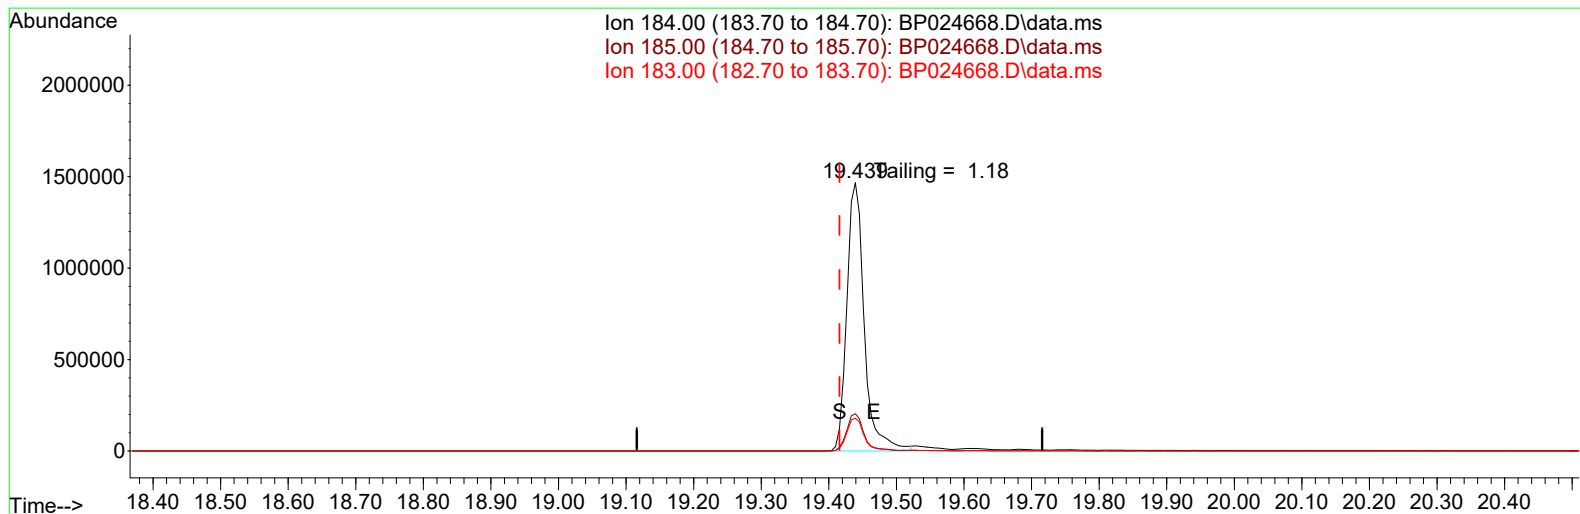

TIC: BP024668.D\data.ms

(77) Benzidine

19.439min (+ 0.023) 577599.08 ng

response 2611422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	12.30	12.30
0.00	0.00	0.00