

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
 Data File : BP051723.D
 Acq On : 17 May 2023 10:10
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714

Quant Time: May 18 00:48:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	312326	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.957	136	1479077	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.769	164	927904	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.528	188	1985313	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	1755935	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1831339	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	67676	8.419	ng/uL	0.00
4) Pyridine-d5	3.870	84	501763	22.021	ng/ul	0.00
7) Phenol-d5	7.275	99	632147	21.799	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.446	67	392248	23.420	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.652	132	448235	21.023	ng/ul	-0.01
15) 4-Methylphenol-d8	8.840	113	470417	20.358	ng/ul	-0.01
21) Nitrobenzene-d5	9.305	128	241422	20.772	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.034	143	261959	20.256	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.575	165	493139	21.132	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.093	131	757013	21.925	ng/ul	-0.01
46) Dimethylphthalate-d6	14.175	166	1489530	21.243	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	1745964	21.772	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.957	143	283160	20.797	ng/ul	-0.01
60) Fluorene-d10	15.763	176	1225567	20.714	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	238753	19.083	ng/ul	0.00
73) Anthracene-d10	17.622	188	1997344	21.971	ng/ul	-0.01
81) Pyrene-d10	19.845	212	2193683	21.540	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.004	264	1891062	20.802	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.470	88	73736	8.537	ng/uL	98
5) Pyridine	3.893	79	527855	22.274	ng/ul	98
6) Benzaldehyde	7.258	77	163852	20.557	ng/ul	97
8) Phenol	7.305	94	667416	22.445	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.540	93	544179	22.874	ng/ul	98
12) 2-Chlorophenol	7.687	128	484640	21.490	ng/ul	99
13) 2-Methylphenol	8.569	108	456528	19.864	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.663	45	657519	22.060	ng/ul	99
16) Acetophenone	8.963	105	806151	22.353	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.946	70	409854	21.669	ng/ul	100
18) 4-Methylphenol	8.905	108	527940	20.871	ng/ul	99
19) Hexachloroethane	9.222	117	204595	22.218	ng/ul	98
22) Nitrobenzene	9.346	77	635201	22.129	ng/ul	98
23) Isophorone	9.875	82	1248233	21.156	ng/ul	99
25) 2-Nitrophenol	10.063	139	298179	21.026	ng/ul	96
26) 2,4-Dimethylphenol	10.116	107	623845	22.045	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.357	93	786373	21.905	ng/ul	98
29) 2,4-Dichlorophenol	10.599	162	503499	21.360	ng/ul	98
30) Naphthalene	11.010	128	1749329	21.755	ng/ul	100
32) 4-Chloroaniline	11.122	127	791473	22.304	ng/ul	98
33) Hexachlorobutadiene	11.293	225	294823	20.753	ng/ul	98
34) Caprolactam	11.893	113	164172	18.474	ng/ul	89
35) 4-Chloro-3-methylphenol	12.228	107	567301	21.314	ng/ul	99
36) 2-Methylnaphthalene	12.610	142	1174067	21.670	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
 Data File : BP015123.D
 Acq On : 17 May 2023 10:10
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714


Quant Time: May 18 00:48:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.828	142	1191232	21.894	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.969	216	602205	21.700	ng/ul	98
40) Hexachlorocyclopentadiene	12.946	237	322163	17.917	ng/ul	97
41) 2,4,6-Trichlorophenol	13.210	196	399166	20.369	ng/ul	99
42) 2,4,5-Trichlorophenol	13.281	196	442684	20.835	ng/ul	99
43) 1,1'-Biphenyl	13.604	154	1601087	22.239	ng/ul	99
44) 2-Chloronaphthalene	13.651	162	1248228	22.201	ng/ul	99
45) 2-Nitroaniline	13.851	65	358074	22.259	ng/ul	90
47) Dimethylphthalate	14.222	163	1570438	21.506	ng/ul	99
48) 2,6-Dinitrotoluene	14.345	165	303858	21.003	ng/ul	98
50) Acenaphthylene	14.493	152	1986685	22.203	ng/ul	99
51) 3-Nitroaniline	14.675	138	230657	17.706	ng/ul	100
52) Acenaphthene	14.834	153	1355940	22.187	ng/ul	99
53) 2,4-Dinitrophenol	14.881	184	153298	15.959	ng/ul	92
55) 4-Nitrophenol	14.975	109	222647	22.233	ng/ul	96
56) Dibenzofuran	15.169	168	1880632	22.124	ng/ul	100
57) 2,4-Dinitrotoluene	15.128	165	444502	21.233	ng/ul	93
58) 2,3,4,6-Tetrachlorophenol	15.393	232	371271	20.704	ng/ul	99
59) Diethylphthalate	15.581	149	1540636	21.153	ng/ul	99
61) Fluorene	15.816	166	1454707	21.295	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.804	204	701271	21.011	ng/ul	98
63) 4-Nitroaniline	15.834	138	193246	17.178	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.892	198	250613	19.408	ng/ul	100
67) N-Nitrosodiphenylamine	16.022	169	1238905	21.223	ng/ul	98
68) 4-Bromophenyl-phenylether	16.704	248	441237	21.577	ng/ul	99
69) Hexachlorobenzene	16.822	284	521754	21.591	ng/ul	97
70) Atrazine	16.975	200	448880	20.804	ng/ul	99
71) Pentachlorophenol	17.169	266	293845	19.439	ng/ul	99
72) Phenanthrene	17.569	178	2396723	22.170	ng/ul	99
74) Anthracene	17.657	178	2441158	22.330	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.575	216	616976	21.918	ng/ul	99
76) Pentachlorobenzene	15.087	250	609471	21.564	ng/ul	99
77) Carbazole	17.922	167	2184853	22.792	ng/ul	100
78) Di-n-butylphthalate	18.457	149	2584958	20.940	ng/ul	100
80) Fluoranthene	19.522	202	2680478	21.595	ng/ul	100
82) Pyrene	19.869	202	2836847	22.131	ng/ul	97
83) Butylbenzylphthalate	20.727	149	1118285	19.679	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.510	252	800466	20.756	ng/ul	98
85) Benzo(a)anthracene	21.586	228	2628946	21.653	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.486	149	1604557	19.613	ng/ul	99
87) Chrysene	21.645	228	2540492	21.889	ng/ul	98
89) Di-n-octyl phthalate	22.463	149	2693097	21.472	ng/ul	100
90) Benzo(b)fluoranthene	23.380	252	2585316	22.268	ng/ul	99
91) Benzo(k)fluoranthene	23.433	252	2467684	22.136	ng/ul	99
93) Benzo(a)pyrene	24.057	252	2192927	21.370	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.892	276	2467319	18.569	ng/ul	100
95) Dibenzo(a,h)anthracene	26.910	278	2060709	18.893	ng/ul	99
96) Benzo(g,h,i)perylene	27.733	276	1932325	17.834	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 18 00:48:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration







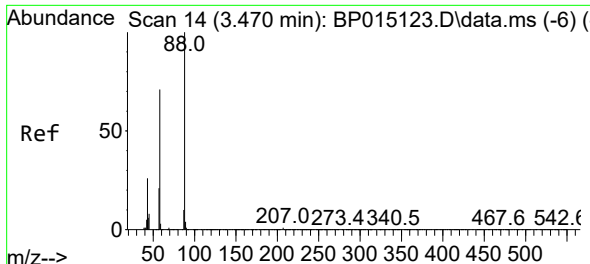

#2
1,4-Dioxane
Concen: 8.537 ng/uL
RT: 3.470 min Scan# 14
Delta R.T. 0.000 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion: 88 Resp: 73736
Ion Ratio Lower Upper
88 100
43 26.4 20.4 30.6
58 70.8 55.4 83.2

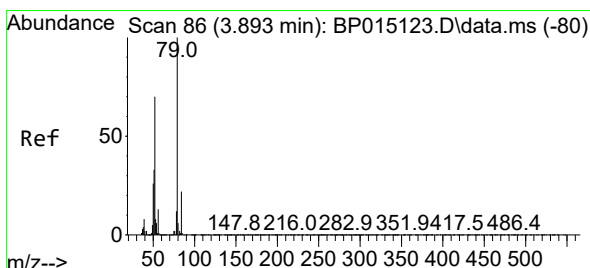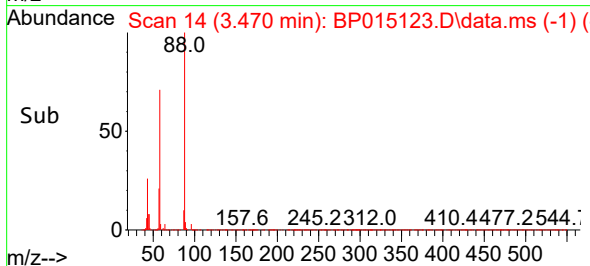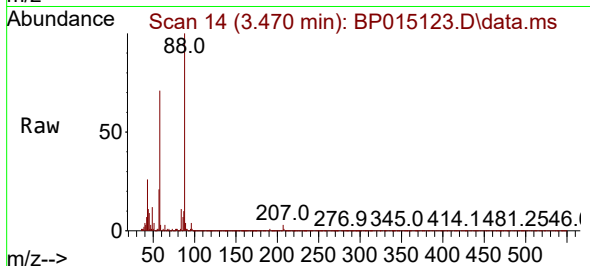

#5
Pyridine
Concen: 22.274 ng/uL
RT: 3.893 min Scan# 86
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion: 79 Resp: 527855
Ion Ratio Lower Upper
79 100
52 70.0 55.4 83.2
51 33.9 25.4 38.2


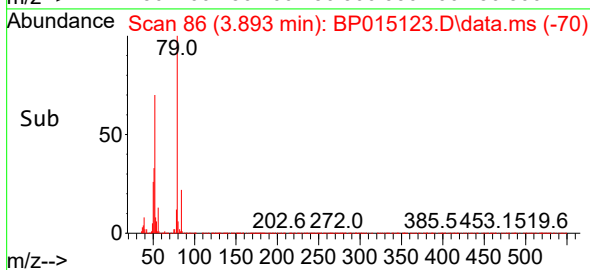

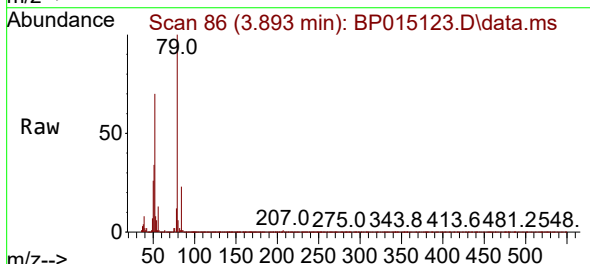




#6
Benzaldehyde
Concen: 20.557 ng/ul
RT: 7.258 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion: 77 Resp: 163852
Ion Ratio Lower Upper
77 100
105 100.3 76.9 115.3
106 94.6 75.0 112.6



#8
Phenol
Concen: 22.445 ng/ul
RT: 7.305 min Scan# 666
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion: 94 Resp: 667416
Ion Ratio Lower Upper
94 100
65 26.8 20.6 31.0
66 34.1 26.1 39.1

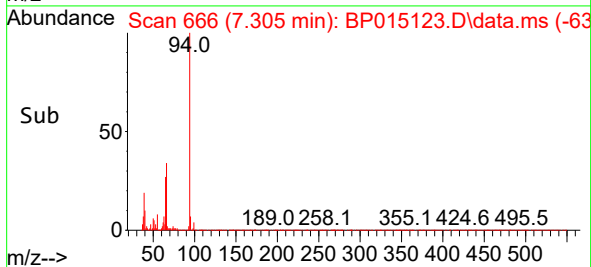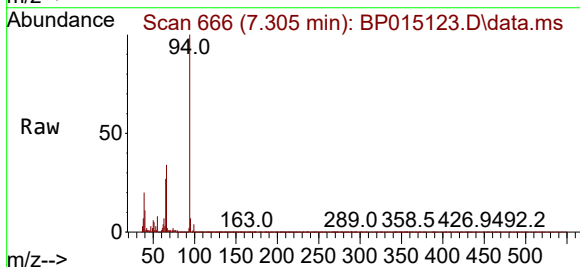







#10
 Bis(2-Chloroethyl)ether
 Concen: 22.874 ng/ul
 RT: 7.540 min Scan# 706
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714

Tgt Ion: 93 Resp: 544179




Ion	Ratio	Lower	Upper
93	100		
63	74.5	58.0	87.0
95	32.0	26.4	39.6




#12
 2-Chlorophenol
 Concen: 21.490 ng/ul
 RT: 7.687 min Scan# 731
 Delta R.T. -0.006 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Tgt Ion: 128 Resp: 484640

Ion	Ratio	Lower	Upper
128	100		
64	45.4	36.2	54.2
130	32.2	26.3	39.5





#13

2-Methylphenol

Concen: 19.864 ng/ul

RT: 8.569 min Scan# 881

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :





SSTD020714

Tgt Ion:108 Resp: 456528

Ion Ratio Lower Upper

108 100

107 87.3 71.8 107.6



#14

2,2'-oxybis(1-Chloropropane)

Concen: 22.060 ng/ul

RT: 8.663 min Scan# 897

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion: 45 Resp: 657519


Ion Ratio Lower Upper

45 100

77 15.2 12.8 19.2

79 11.6 9.5 14.3









#16
Acetophenone
Concen: 22.353 ng/ul
RT: 8.963 min Scan# 948
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:105 Resp: 806151
Ion Ratio Lower Upper
105 100
77 75.9 59.4 89.2
51 25.2 19.2 28.8



#17
N-Nitroso-di-n-propylamine
Concen: 21.669 ng/ul
RT: 8.946 min Scan# 945
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion: 70 Resp: 409854
Ion Ratio Lower Upper
70 100
42 51.5 41.0 61.6
101 9.4 7.9 11.9
130 20.0 16.1 24.1



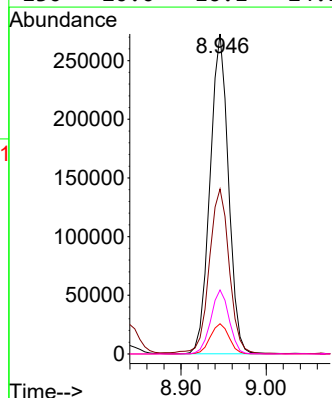





#18
4-Methylphenol
Concen: 20.871 ng/ul
RT: 8.905 min Scan# 911
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:108 Resp: 527940
Ion Ratio Lower Upper
108 100
107 111.8 88.5 132.7



#19
Hexachloroethane
Concen: 22.218 ng/ul
RT: 9.222 min Scan# 992
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:117 Resp: 204595
Ion Ratio Lower Upper
117 100
201 94.3 75.8 113.8
199 60.7 46.5 69.7









#22
Nitrobenzene
Concen: 22.129 ng/ul
RT: 9.346 min Scan# 1013
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion: 77 Resp: 635201
Ion Ratio Lower Upper
77 100
123 44.2 36.2 54.2
65 13.3 10.1 15.1

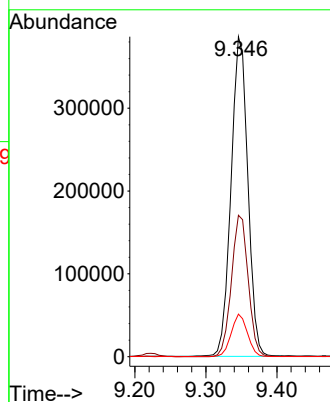

#23
Isophorone
Concen: 21.156 ng/ul
RT: 9.875 min Scan# 1103
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion: 82 Resp: 1248233
Ion Ratio Lower Upper
82 100
95 6.4 5.4 8.0
138 16.5 13.6 20.4






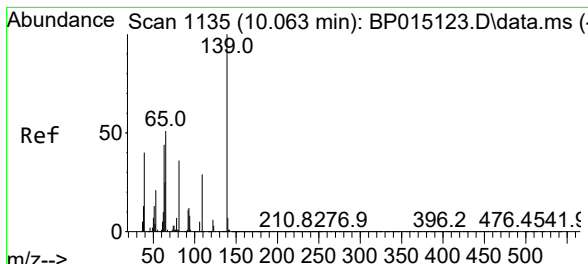


#25
 2-Nitrophenol
 Concen: 21.026 ng/ul
 RT: 10.063 min Scan# 1135
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714

Tgt Ion:139 Resp: 298179




Ion	Ratio	Lower	Upper
139	100		
65	51.7	38.4	57.6
109	28.5	22.2	33.2

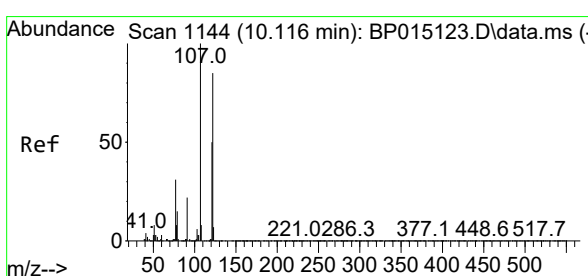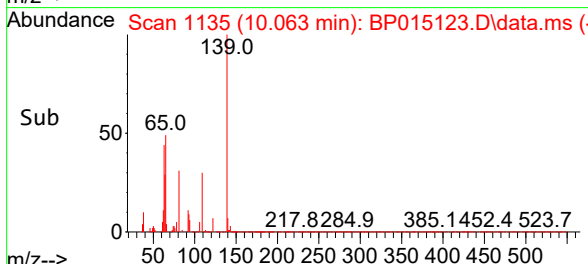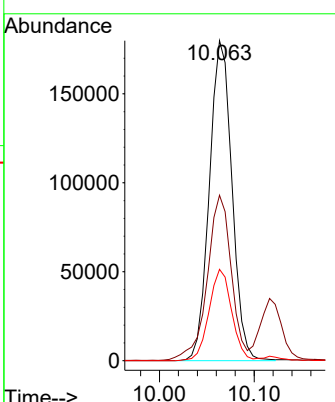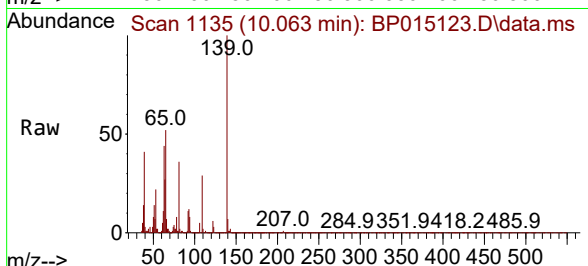


#26
 2,4-Dimethylphenol
 Concen: 22.045 ng/ul
 RT: 10.116 min Scan# 1144
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Tgt Ion:107 Resp: 623845

Ion	Ratio	Lower	Upper
107	100		
121	50.3	41.0	61.6
122	86.4	69.5	104.3


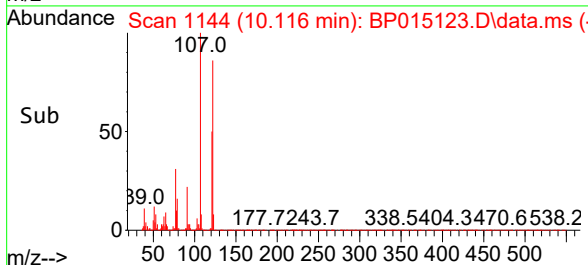
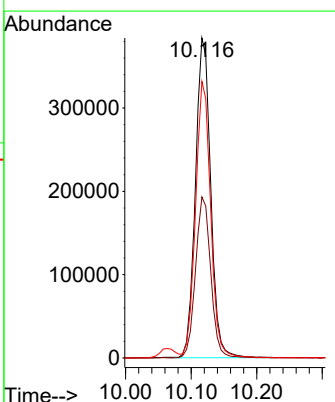
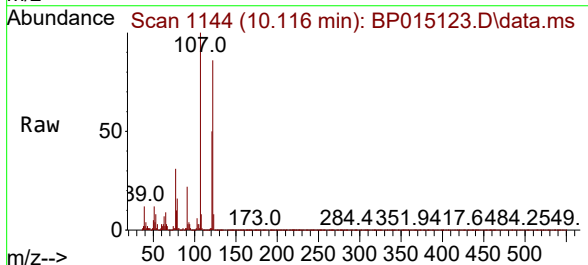




#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.905 ng/ul
 RT: 10.357 min Scan# 1185
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714


Tgt Ion: 93 Resp: 786373
 Ion Ratio Lower Upper
 93 100
 95 32.3 26.7 40.1
 123 11.2 9.1 13.7

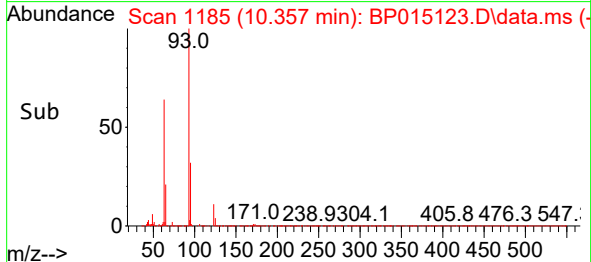

#29
 2,4-Dichlorophenol
 Concen: 21.360 ng/ul
 RT: 10.599 min Scan# 1226
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Tgt Ion: 162 Resp: 503499
 Ion Ratio Lower Upper
 162 100
 164 66.2 52.0 78.0
 98 37.4 28.9 43.3


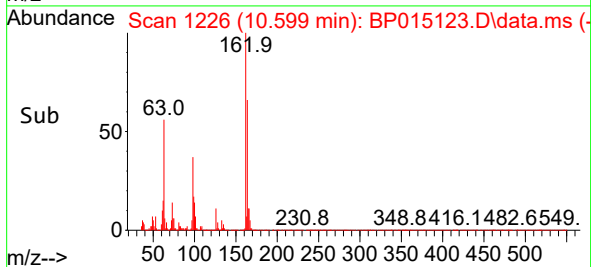

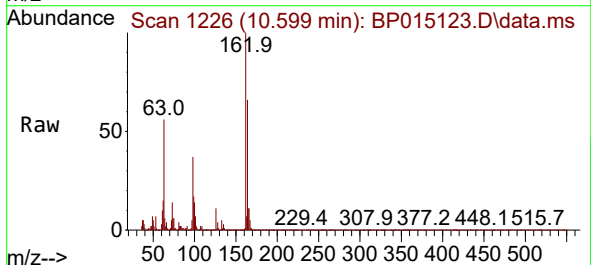




#30
Naphthalene
Concen: 21.755 ng/ul
RT: 11.010 min Scan# 1296
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:128 Resp: 1749329
Ion Ratio Lower Upper
128 100
129 10.8 8.9 13.3
127 13.2 10.6 15.8

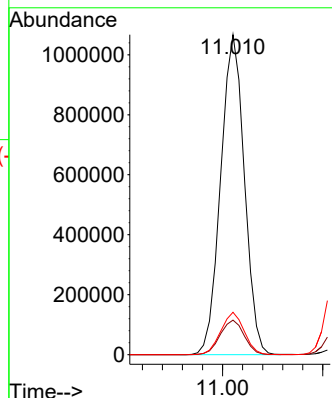

#32
4-Chloroaniline
Concen: 22.304 ng/ul
RT: 11.122 min Scan# 1315
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:127 Resp: 791473
Ion Ratio Lower Upper
127 100
129 31.4 25.8 38.8




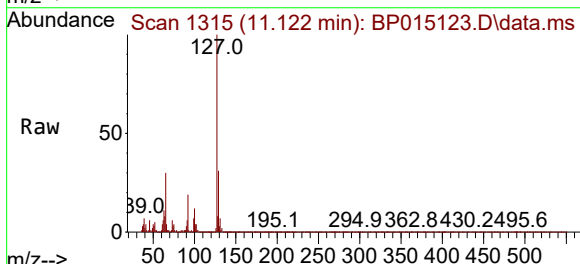




#33
Hexachlorobutadiene
Concen: 20.753 ng/ul
RT: 11.293 min Scan# 11
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:225 Resp: 294823
Ion Ratio Lower Upper
225 100
223 62.8 51.0 76.6
227 63.8 52.2 78.4



#34
Caprolactam
Concen: 18.474 ng/ul
RT: 11.893 min Scan# 1446
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:113 Resp: 164172
Ion Ratio Lower Upper
113 100
55 168.4 121.2 181.8
56 121.5 90.2 135.4




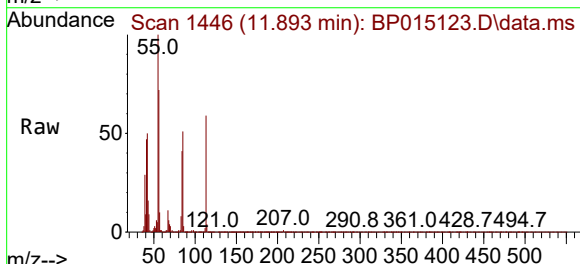




#35
4-Chloro-3-methylphenol
Concen: 21.314 ng/ul
RT: 12.228 min Scan# 1503
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:107 Resp: 567301
Ion Ratio Lower Upper
107 100
144 26.0 20.3 30.5
142 79.6 63.2 94.8

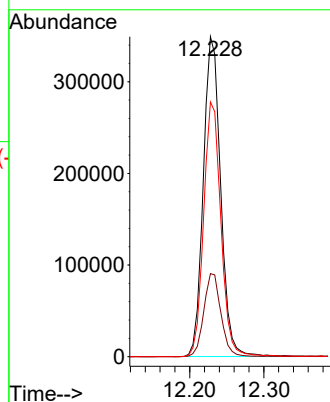

#36
2-Methylnaphthalene
Concen: 21.670 ng/ul
RT: 12.610 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:142 Resp: 1174067
Ion Ratio Lower Upper
142 100
141 87.7 71.0 106.6





#37

1-Methylnaphthalene

Concen: 21.894 ng/ul

RT: 12.828 min Scan# 1605

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:142 Resp: 1191232

Ion Ratio Lower Upper

142 100

141 92.6 74.6 112.0

116 3.8 2.9 4.3



#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.700 ng/ul

RT: 12.969 min Scan# 1629

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Tgt Ion:216 Resp: 602205




Ion Ratio Lower Upper


216 100

214 78.4 61.4 92.0

179 21.5 15.9 23.9

108 18.3 13.7 20.5


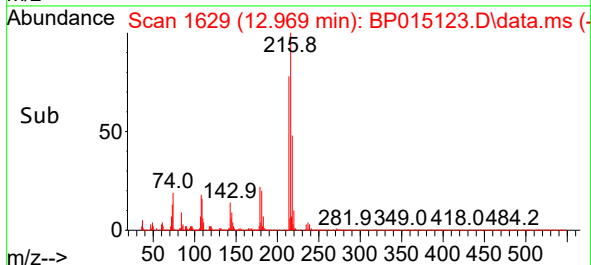
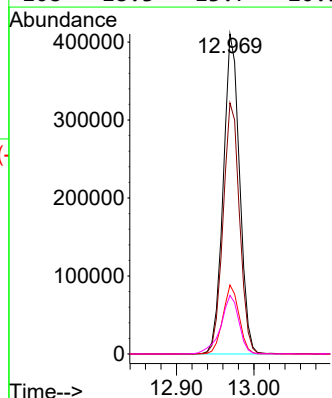
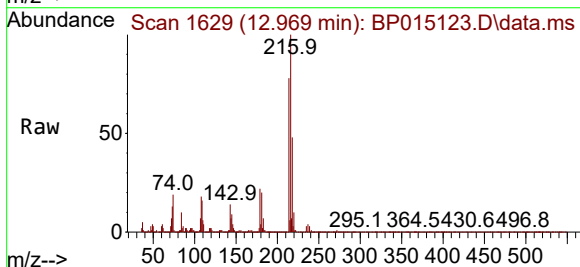




#40
Hexachlorocyclopentadiene
Concen: 17.917 ng/ul
RT: 12.946 min Scan# 1625
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:237 Resp: 322163
Ion Ratio Lower Upper
237 100
235 64.7 49.4 74.0
272 13.2 10.4 15.6



#41
2,4,6-Trichlorophenol
Concen: 20.369 ng/ul
RT: 13.210 min Scan# 1670
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:196 Resp: 399166
Ion Ratio Lower Upper
196 100
198 94.6 75.5 113.3
200 30.6 23.6 35.4

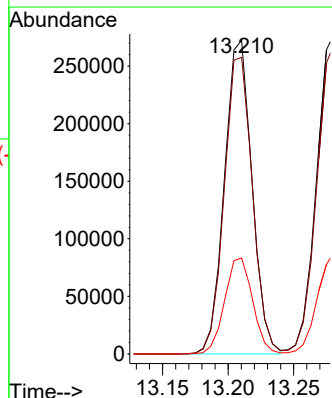



#42

2,4,5-Trichlorophenol

Concen: 20.835 ng/ul

RT: 13.281 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:196 Resp: 442684

Ion Ratio Lower Upper

196 100

198 97.1 77.0 115.4

200 31.8 24.3 36.5

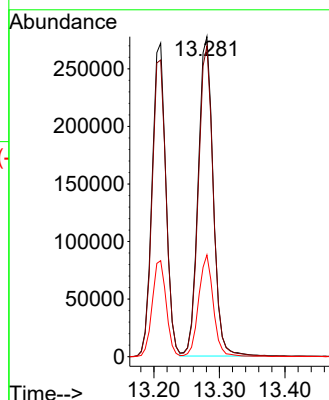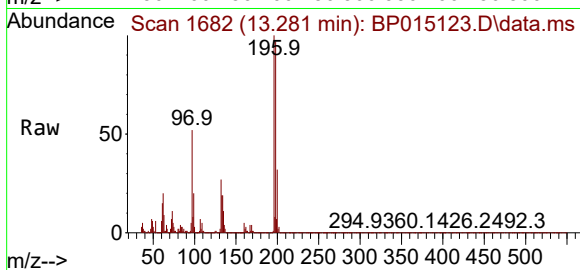

#43

1,1'-Biphenyl

Concen: 22.239 ng/ul

RT: 13.604 min Scan# 1737

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:154 Resp: 1601087


Ion Ratio Lower Upper

154 100

153 40.1 32.7 49.1

76 14.0 10.7 16.1



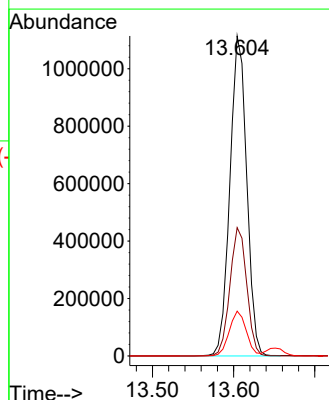





#44
2-Chloronaphthalene
Concen: 22.201 ng/ul
RT: 13.651 min Scan# 1745
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:162 Resp: 1248228
Ion Ratio Lower Upper
162 100
164 33.1 25.9 38.9
127 38.1 30.8 46.2

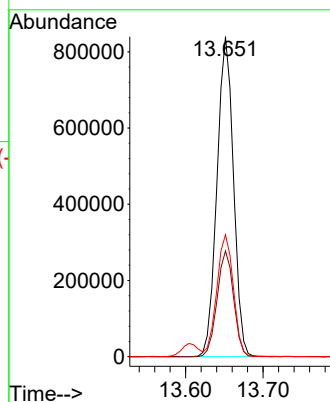

#45
2-Nitroaniline
Concen: 22.259 ng/ul
RT: 13.851 min Scan# 1779
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion: 65 Resp: 358074
Ion Ratio Lower Upper
65 100
92 71.1 59.8 89.8
138 100.4 92.3 138.5









#47
Dimethylphthalate
Concen: 21.506 ng/ul
RT: 14.222 min Scan# 1842
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:163 Resp: 1570438
Ion Ratio Lower Upper
163 100
194 3.9 3.1 4.7
164 10.0 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 21.003 ng/ul
RT: 14.345 min Scan# 1863
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:165 Resp: 303858
Ion Ratio Lower Upper
165 100
89 61.6 48.0 72.0
121 22.7 17.5 26.3









#50
Acenaphthylene
Concen: 22.203 ng/ul
RT: 14.493 min Scan# 1888
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:152 Resp: 1986685
Ion Ratio Lower Upper
152 100
151 19.7 16.1 24.1
153 13.7 10.3 15.5



#51
3-Nitroaniline
Concen: 17.706 ng/ul
RT: 14.675 min Scan# 1919
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:138 Resp: 230657
Ion Ratio Lower Upper
138 100
108 10.8 8.8 13.2
92 116.6 93.4 140.0

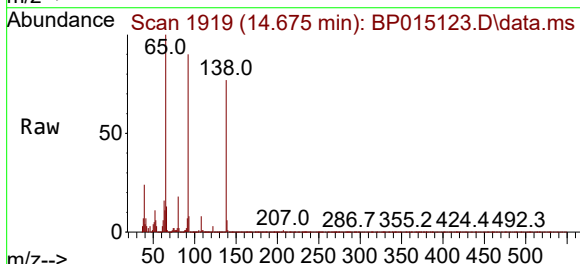



#52

Acenaphthene

Concen: 22.187 ng/ul

RT: 14.834 min Scan# 1946

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:153 Resp: 1355940

Ion Ratio Lower Upper

153 100

152 47.9 38.0 57.0

154 87.5 71.0 106.4



#53

2,4-Dinitrophenol

Concen: 15.959 ng/ul

RT: 14.881 min Scan# 1954

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:184 Resp: 153298


Ion Ratio Lower Upper

184 100

63 72.3 49.7 74.5

154 60.9 47.5 71.3









#55
4-Nitrophenol
Concen: 22.233 ng/ul
RT: 14.975 min Scan# 1970
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:109 Resp: 222647
Ion Ratio Lower Upper
109 100
139 139.7 115.3 172.9
65 139.0 107.9 161.9



#56
Dibenzofuran
Concen: 22.124 ng/ul
RT: 15.169 min Scan# 2003
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:168 Resp: 1880632
Ion Ratio Lower Upper
168 100
139 36.6 29.4 44.0









#57
2,4-Dinitrotoluene
Concen: 21.233 ng/ul
RT: 15.128 min Scan# 1996
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:165 Resp: 444502
Ion Ratio Lower Upper
165 100
63 45.8 33.1 49.7
182 2.5 2.1 3.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 20.704 ng/ul
RT: 15.393 min Scan# 2041
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:232 Resp: 371271
Ion Ratio Lower Upper
232 100
131 44.9 36.8 55.2
130 2.4 1.9 2.9
166 31.2 24.6 37.0


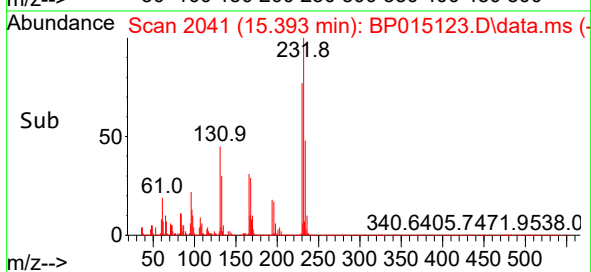






#59
Diethylphthalate
Concen: 21.153 ng/ul
RT: 15.581 min Scan# 2073
Delta R.T. -0.006 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:149 Resp: 1540636
Ion Ratio Lower Upper
149 100
177 22.2 17.5 26.3
150 11.9 9.8 14.8



#61
Fluorene
Concen: 21.295 ng/ul
RT: 15.816 min Scan# 2113
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:166 Resp: 1454707
Ion Ratio Lower Upper
166 100
165 97.9 77.8 116.6
167 13.4 10.6 15.8




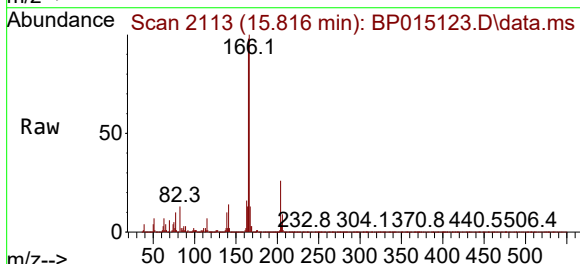




#62
4-Chlorophenyl-phenylether
Concen: 21.011 ng/ul
RT: 15.804 min Scan# 2111
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:204 Resp: 701271
Ion Ratio Lower Upper
204 100
206 32.5 26.1 39.1
141 57.9 44.5 66.7



#63
4-Nitroaniline
Concen: 17.178 ng/ul
RT: 15.834 min Scan# 2116
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:138 Resp: 193246
Ion Ratio Lower Upper
138 100
92 51.5 41.2 61.8
108 75.1 60.1 90.1









#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.408 ng/ul
 RT: 15.892 min Scan# 2126
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714


Tgt Ion:198 Resp: 250613
 Ion Ratio Lower Upper
 198 100
 182 4.5 3.7 5.5
 77 26.7 21.2 31.8



#67
 N-Nitrosodiphenylamine
 Concen: 21.223 ng/ul
 RT: 16.022 min Scan# 2148
 Delta R.T. -0.006 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Tgt Ion:169 Resp: 1238905
 Ion Ratio Lower Upper
 169 100
 168 68.5 53.5 80.3
 167 37.0 28.9 43.3









#68
4-Bromophenyl-phenylether
Concen: 21.577 ng/ul
RT: 16.704 min Scan# 21
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:248 Resp: 441237
Ion Ratio Lower Upper
248 100
250 97.7 79.0 118.4
141 73.6 58.6 87.8



#69
Hexachlorobenzene
Concen: 21.591 ng/ul
RT: 16.822 min Scan# 2284
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:284 Resp: 521754
Ion Ratio Lower Upper
284 100
142 36.7 27.3 40.9
249 31.9 24.6 36.8





#70

Atrazine

Concen: 20.804 ng/ul

RT: 16.975 min Scan# 2310

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:200 Resp: 448880

Ion Ratio Lower Upper

200 100

173 27.1 21.4 32.2

215 48.9 38.1 57.1

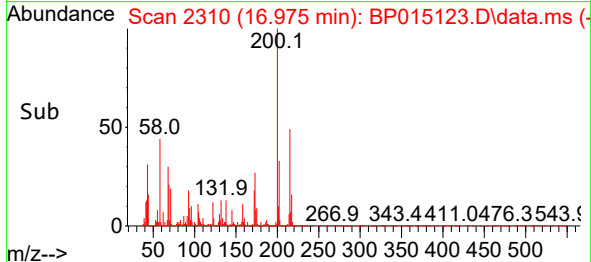

#71

Pentachlorophenol

Concen: 19.439 ng/ul

RT: 17.169 min Scan# 2343

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:266 Resp: 293845


Ion Ratio Lower Upper

266 100

264 64.4 51.0 76.4

268 65.3 51.8 77.6

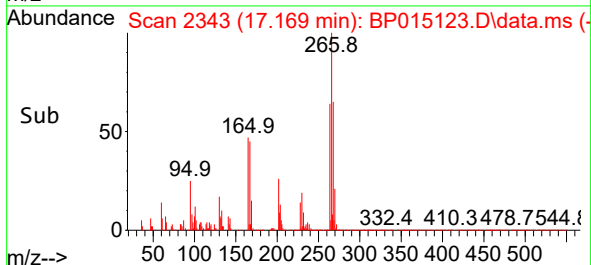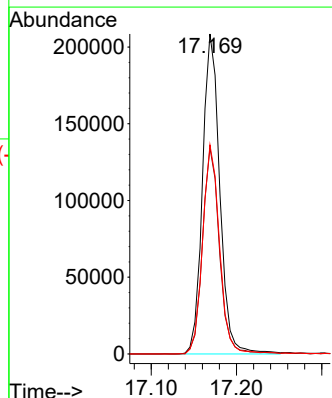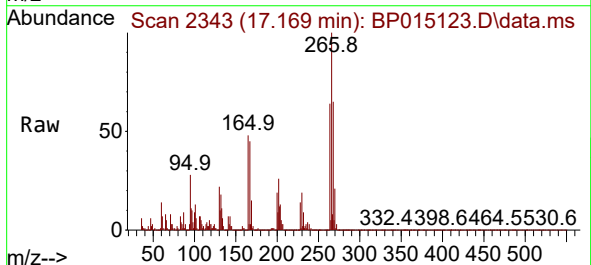



#72

Phenanthrene

Concen: 22.170 ng/ul

RT: 17.569 min Scan# 2411

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:178 Resp: 2396723

Ion Ratio Lower Upper

178 100

179 15.7 12.2 18.2

176 19.4 15.6 23.4



#74

Anthracene

Concen: 22.330 ng/ul

RT: 17.657 min Scan# 2426

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:178 Resp: 2441158


Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.2

176 18.7 15.2 22.8





#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.918 ng/uL

RT: 13.575 min Scan# 1732

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:216 Resp: 616976

Ion Ratio Lower Upper

216 100

214 76.7 62.2 93.4

218 47.4 38.2 57.2



#76

Pentachlorobenzene

Concen: 21.564 ng/uL

RT: 15.087 min Scan# 1989

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:250 Resp: 609471


Ion Ratio Lower Upper

250 100

248 61.9 49.8 74.6

252 63.6 51.6 77.4

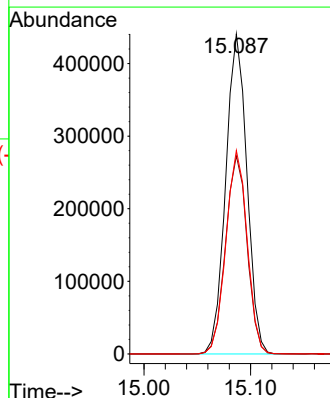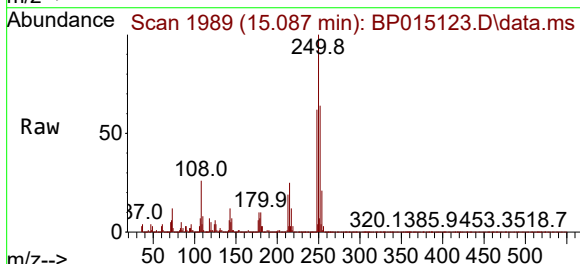







#77
 Carbazole
 Concen: 22.792 ng/ul
 RT: 17.922 min Scan# 2471
 Delta R.T. -0.011 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020714

Tgt Ion:167 Resp: 2184853




Ion	Ratio	Lower	Upper
167	100		
166	22.0	17.4	26.2
139	13.1	10.2	15.4




#78
 Di-n-butylphthalate
 Concen: 20.940 ng/ul
 RT: 18.457 min Scan# 2562
 Delta R.T. -0.006 min
 Lab File: BP015123.D
 Acq: 17 May 2023 10:10

Tgt Ion:149 Resp: 2584958

Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.3	10.9
104	5.0	3.9	5.9

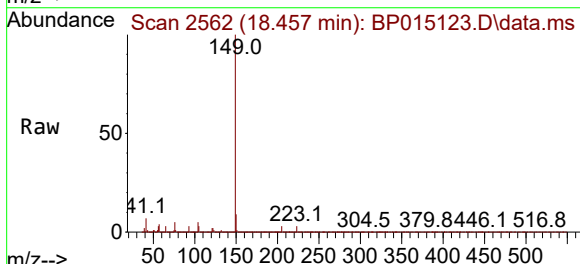



#80

Fluoranthene

Concen: 21.595 ng/ul

RT: 19.522 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:202 Resp: 2680478

Ion Ratio Lower Upper

202 100

101 12.0 9.5 14.3

100 9.1 7.3 10.9

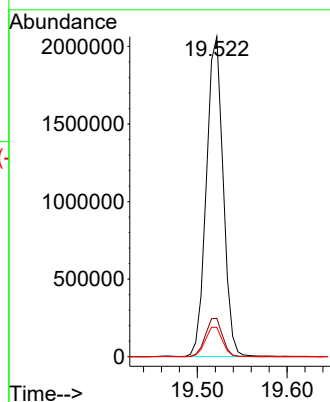

#82

Pyrene

Concen: 22.131 ng/ul

RT: 19.869 min Scan# 2802

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:202 Resp: 2836847


Ion Ratio Lower Upper

202 100

101 15.2 11.2 16.8

100 12.7 9.0 13.6





#83

Butylbenzylphthalate

Concen: 19.679 ng/ul

RT: 20.727 min Scan# 2948

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:149 Resp: 1118285

Ion Ratio Lower Upper

149 100

91 75.0 57.4 86.2

206 19.8 16.6 25.0



#84

3,3'-Dichlorobenzidine

Concen: 20.756 ng/ul

RT: 21.510 min Scan# 3081

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:252 Resp: 800466


Ion Ratio Lower Upper

252 100

254 65.3 50.8 76.2

126 12.7 9.8 14.8





#85

Benzo(a)anthracene

Concen: 21.653 ng/ul

RT: 21.586 min Scan# 3094

Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:228 Resp: 2628946

Ion Ratio Lower Upper

228 100

229 20.0 16.1 24.1

226 27.6 21.9 32.9



#86

Bis(2-ethylhexyl)phthalate

Concen: 19.613 ng/ul

RT: 21.486 min Scan# 3077

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:149 Resp: 1604557


Ion Ratio Lower Upper

149 100

167 26.8 21.8 32.6

279 3.8 3.2 4.8





#87

Chrysene

Concen: 21.889 ng/ul

RT: 21.645 min Scan# 3104

Delta R.T. -0.006 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:228 Resp: 2540492

Ion Ratio Lower Upper

228 100

226 30.4 25.0 37.6

229 19.5 16.1 24.1



#89

Di-n-octyl phthalate

Concen: 21.472 ng/ul




RT: 22.463 min Scan# 3243


Delta R.T. -0.011 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Tgt Ion:149 Resp: 2693097









#90
Benzo(b)fluoranthene
Concen: 22.268 ng/ul
RT: 23.380 min Scan# 3399
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10




Instrument :
BNA_P
ClientSampleId :
SSTD020714


Tgt Ion:252 Resp: 2585316
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.2
125 10.9 8.3 12.5



#91
Benzo(k)fluoranthene
Concen: 22.136 ng/ul
RT: 23.433 min Scan# 3408
Delta R.T. -0.011 min
Lab File: BP015123.D
Acq: 17 May 2023 10:10

Tgt Ion:252 Resp: 2467684
Ion Ratio Lower Upper
252 100
253 22.1 17.5 26.3
125 10.8 8.5 12.7





#93

Benzo(a)pyrene

Concen: 21.370 ng/ul

RT: 24.057 min Scan# 3514

Delta R.T. -0.017 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:252 Resp: 2192927

Ion Ratio Lower Upper

252 100

253 22.3 17.2 25.8

125 12.0 9.1 13.7



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.569 ng/ul

RT: 26.892 min Scan# 3996

Delta R.T. -0.023 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10




Tgt Ion:276 Resp: 2467319


Ion Ratio Lower Upper

276 100

138 25.2 20.1 30.1

277 24.5 19.8 29.8

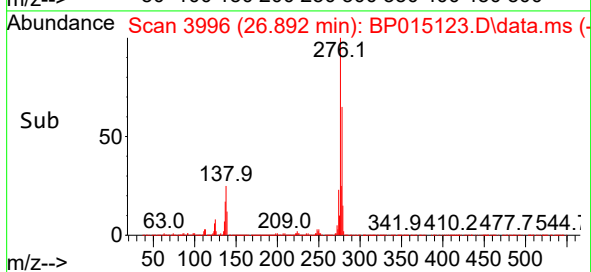

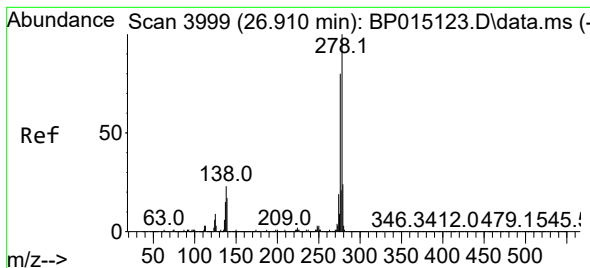

#95

Dibenzo(a,h)anthracene

Concen: 18.893 ng/ul

RT: 26.910 min Scan# 3999

Delta R.T. -0.023 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Instrument :

BNA_P

ClientSampleId :

SSTD020714





Tgt Ion:278 Resp: 2060709

Ion Ratio Lower Upper

278 100

139 17.3 13.3 19.9

279 24.0 19.1 28.7

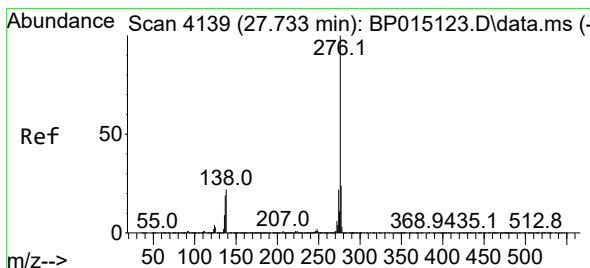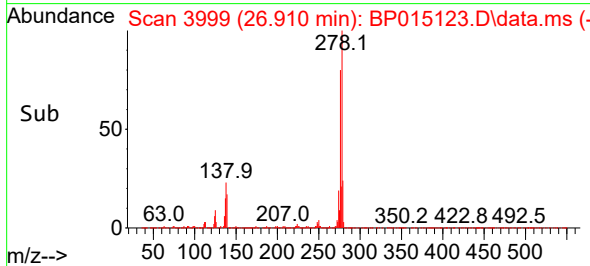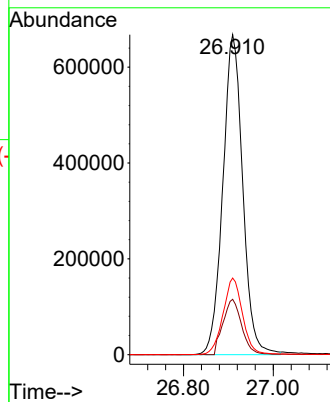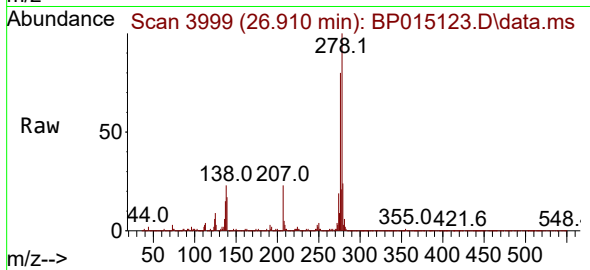

#96

Benzo(g,h,i)perylene

Concen: 17.834 ng/ul

RT: 27.733 min Scan# 4139

Delta R.T. -0.023 min

Lab File: BP015123.D

Acq: 17 May 2023 10:10

Tgt Ion:276 Resp: 1932325

Ion Ratio Lower Upper

276 100

138 21.7 17.7 26.5

277 23.5 18.8 28.2

