

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
 Data File : BP015124.D
 Acq On : 17 May 2023 10:45
 Operator : CG/JU
 Sample : PB152822BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK822

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	17	rVB	101654	138621	1.36%	0.143%
2	3.870	79	82	103	rBV	1262997	2001426	19.64%	2.070%
3	4.217	136	141	149	rVB	41119	66146	0.65%	0.068%
4	7.275	654	661	678	rBV	1499152	2390502	23.46%	2.472%
5	7.446	684	690	704	rVB	1309195	2102095	20.63%	2.174%
6	7.652	718	725	738	rBV	1557092	2490674	24.44%	2.576%
7	8.128	799	806	816	rVB	1002499	1614263	15.84%	1.669%
8	8.840	919	927	941	rBV	1927925	3231805	31.72%	3.342%
9	9.305	999	1006	1022	rBV	1569500	2557835	25.10%	2.645%
10	10.034	1122	1130	1142	rBV	1253407	2086089	20.47%	2.157%
11	10.575	1213	1222	1244	rBV	1730783	3034354	29.78%	3.138%
12	10.957	1279	1287	1301	rBV	1314903	2241798	22.00%	2.318%
13	11.093	1303	1310	1327	rBV	1758551	3179989	31.21%	3.288%
14	12.546	1549	1557	1566	rBV2	23935	57297	0.56%	0.059%
15	13.657	1741	1746	1751	rBV2	15125	24374	0.24%	0.025%
16	14.175	1827	1834	1847	rBV	3889079	5431696	53.31%	5.617%
17	14.469	1875	1884	1898	rBV	4305433	6478276	63.58%	6.699%
18	14.769	1927	1935	1943	rBV	2482700	3569413	35.03%	3.691%
19	14.957	1960	1967	1988	rBV	1734993	2701073	26.51%	2.793%
20	15.181	2001	2005	2016	rVB	11909	22634	0.22%	0.023%
21	15.763	2097	2104	2117	rBV	5586324	7941790	77.94%	8.212%
22	15.881	2117	2124	2136	rVV	1712663	2482258	24.36%	2.567%
23	15.998	2141	2144	2150	rVB2	26570	42904	0.42%	0.044%
24	17.310	2363	2367	2375	rVB4	8002	13228	0.13%	0.014%
25	17.522	2397	2403	2413	rBV	2943107	4316909	42.37%	4.464%
26	17.622	2414	2420	2441	rVB2	6238282	8883908	87.18%	9.187%
27	19.422	2721	2726	2732	rBV2	74447	111570	1.09%	0.115%
28	19.486	2733	2737	2745	rVV	62376	98263	0.96%	0.102%
29	19.845	2792	2798	2812	rBV	7633996	10189737	100.00%	10.537%
30	21.604	3092	3097	3110	rBV	2993244	4174865	40.97%	4.317%
31	24.004	3497	3505	3523	rBV2	4308186	9106469	89.37%	9.417%
32	24.168	3526	3533	3544	rVB	1809883	3921602	38.49%	4.055%




Sum of corrected areas: 96703863

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
Data File : BP015124.D
Acq On : 17 May 2023 10:45
Operator : CG/JU
Sample : PB152822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

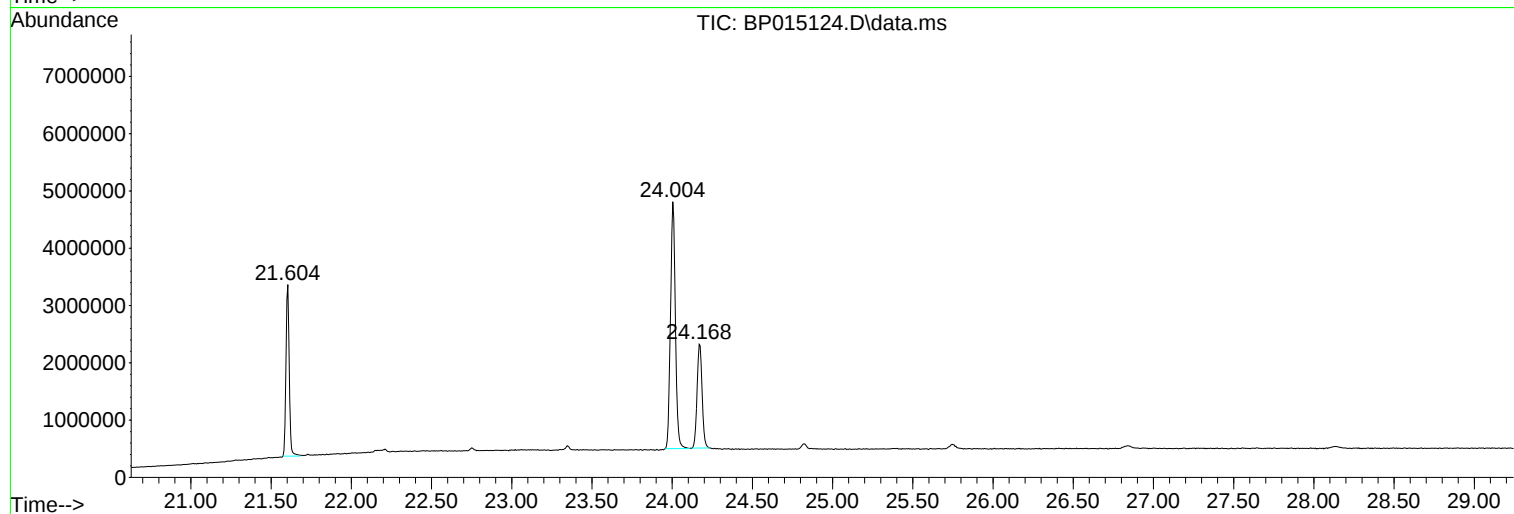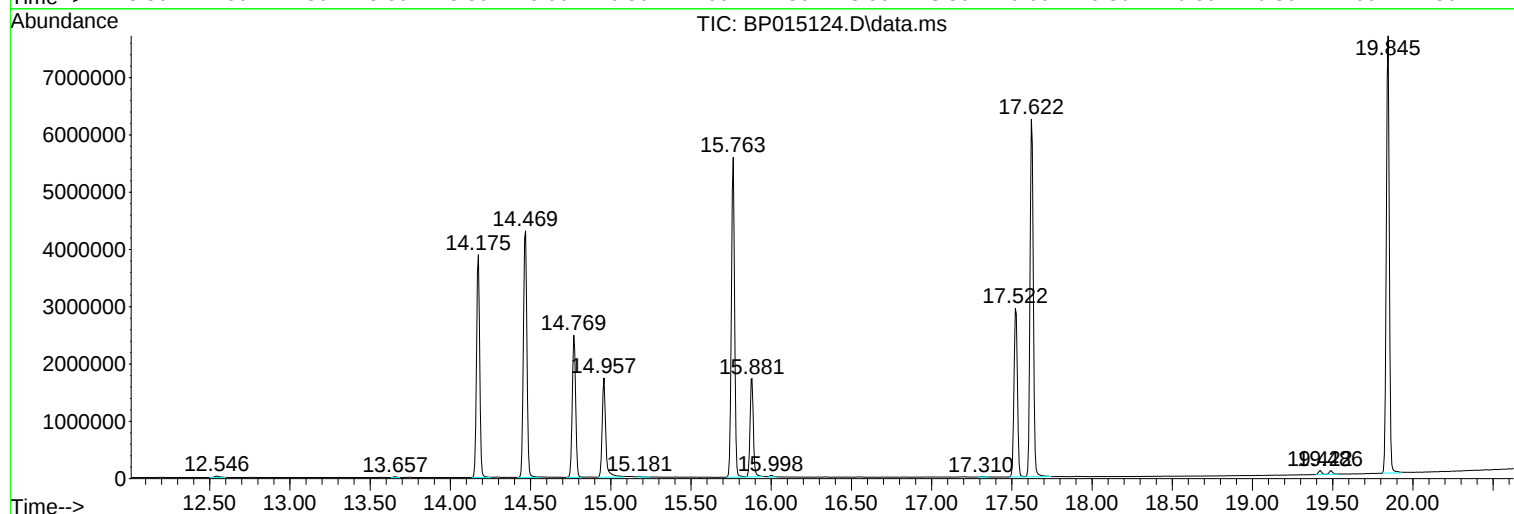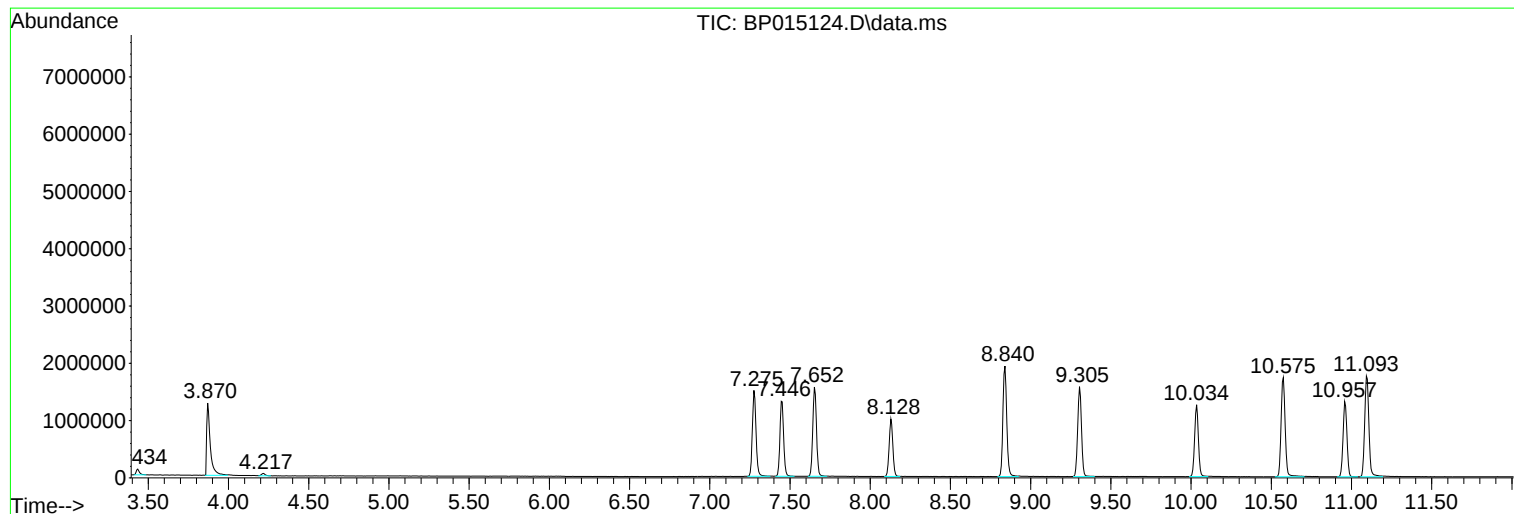

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
Data File : BP015124.D
Acq On : 17 May 2023 10:45
Operator : CG/JU
Sample : PB152822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051723\
Data File : BP015124.D
Acq On : 17 May 2023 10:45
Operator : CG/JU
Sample : PB152822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------