
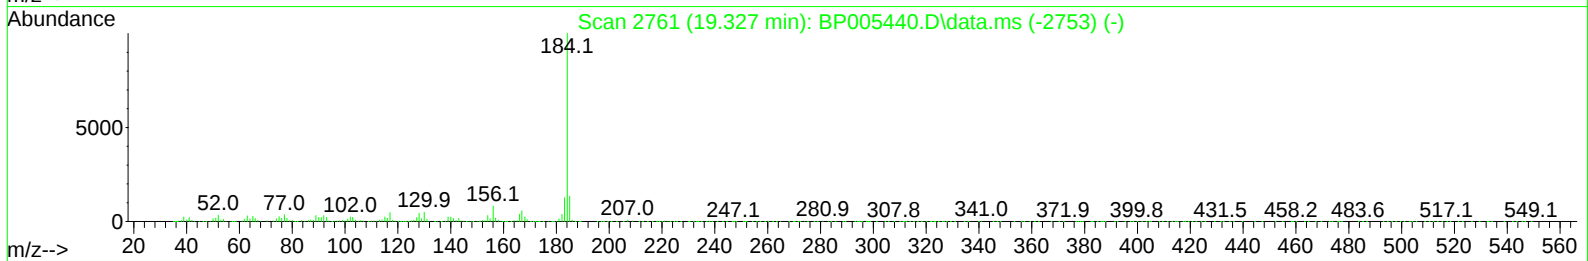
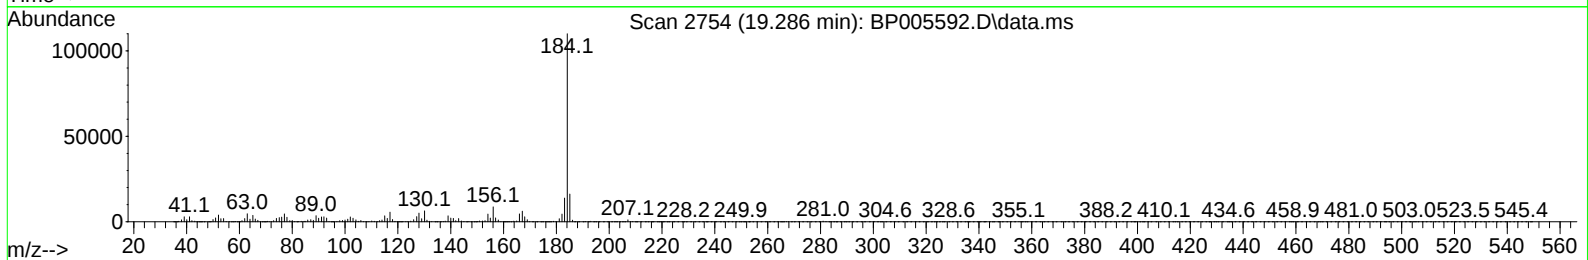


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005592.D
Acq On : 18 May 2021 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 15:37:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 17 15:35:47 2021
Response via : Initial Calibration

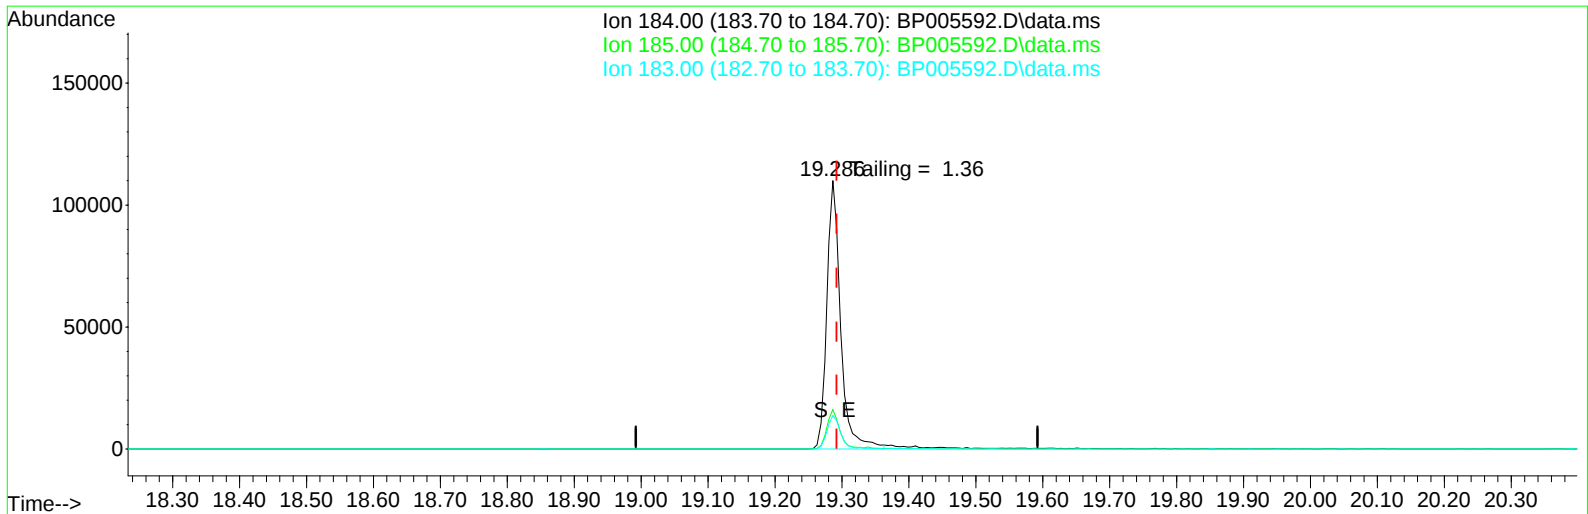




TIC: BP005592.D\data.ms

(77) Benzidine**19.286min (-0.006) 791907.58 ng****response 159351**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.75
183.00	12.30	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005592.D
Acq On : 18 May 2021 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 15:37:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 17 15:35:47 2021
Response via : Initial Calibration

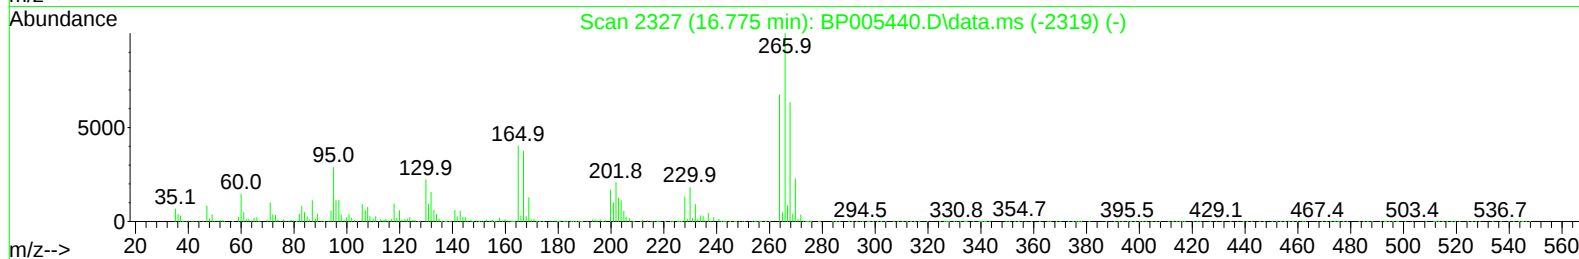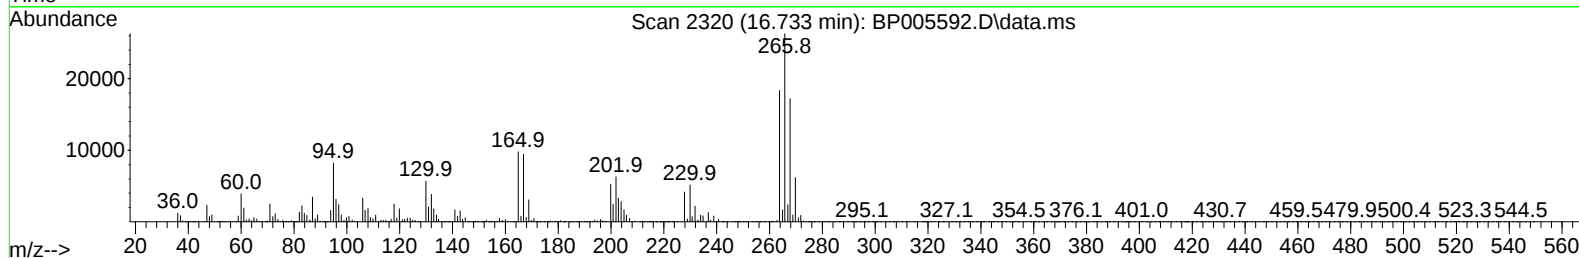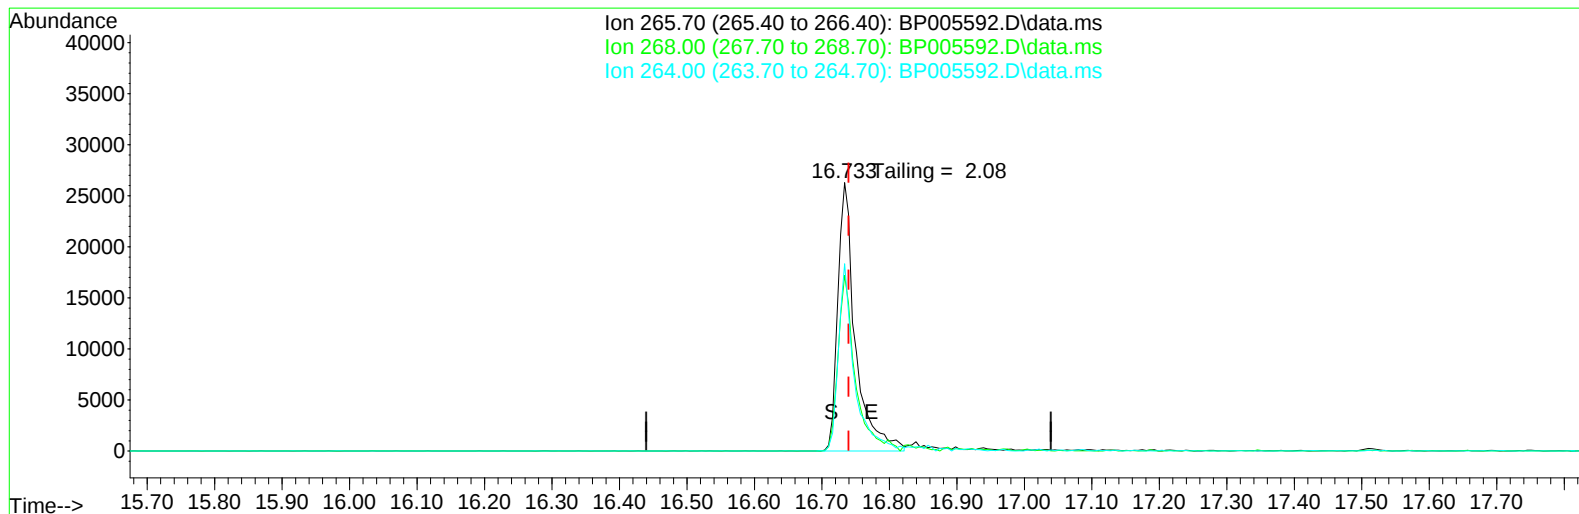

TIC: BP005592.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.006) 378491.12 ng

response 47706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.43
264.00	67.10	69.78
0.00	0.00	0.00