

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
 Data File : BP005594.D
 Acq On : 18 May 2021 11:03
 Operator : CG/JU
 Sample : PB136376BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136376BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.258	363	369	385	rBV	245238	372233	30.56%	9.128%
2	6.863	635	642	661	rBV	192552	340222	27.93%	8.343%
3	7.663	771	778	790	rBV	47365	73851	6.06%	1.811%
4	8.834	968	977	995	rBV	120808	227112	18.64%	5.569%
5	10.457	1246	1253	1270	rBV	38020	77353	6.35%	1.897%
6	12.934	1667	1674	1685	rBV	376419	565007	46.38%	13.855%
7	14.316	1902	1909	1921	rBV2	60195	102906	8.45%	2.523%
8	15.816	2157	2164	2182	rBV	356655	567764	46.61%	13.923%
9	17.075	2372	2378	2392	rBV	75304	130954	10.75%	3.211%
10	19.645	2809	2815	2826	rBV	1071674	1218132	100.00%	29.871%
11	21.174	3070	3075	3087	rBV2	131240	203384	16.70%	4.987%
12	23.468	3459	3465	3475	rVB	99063	199024	16.34%	4.881%




Sum of corrected areas: 4077942

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005594.D
Acq On : 18 May 2021 11:03
Operator : CG/JU
Sample : PB136376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

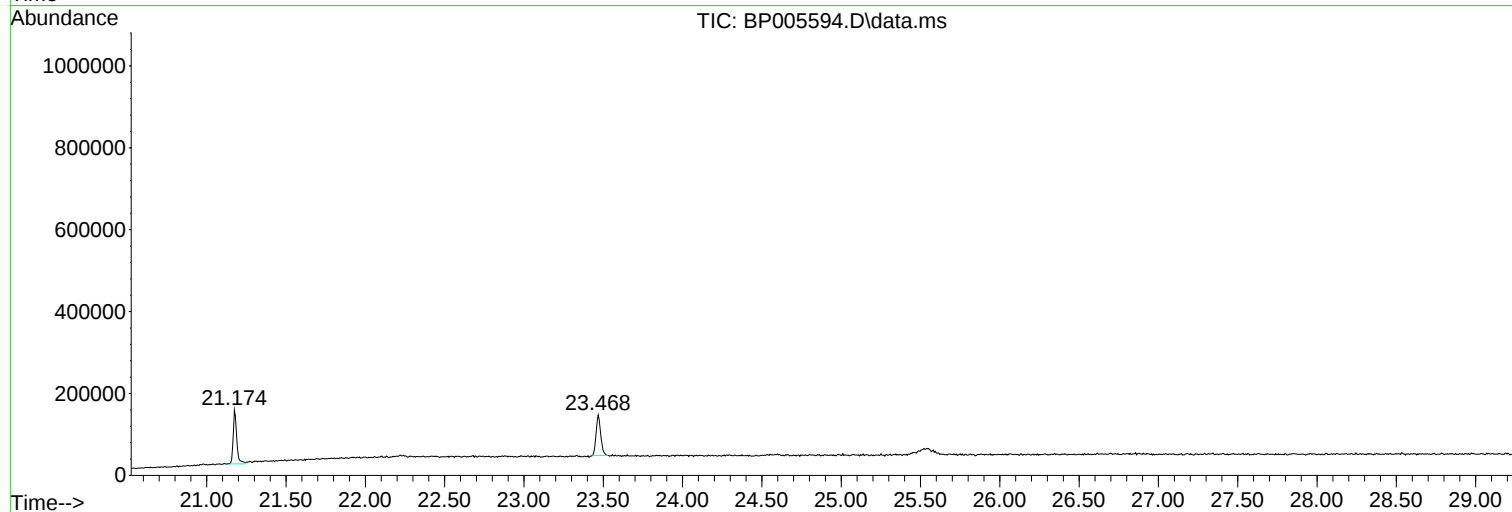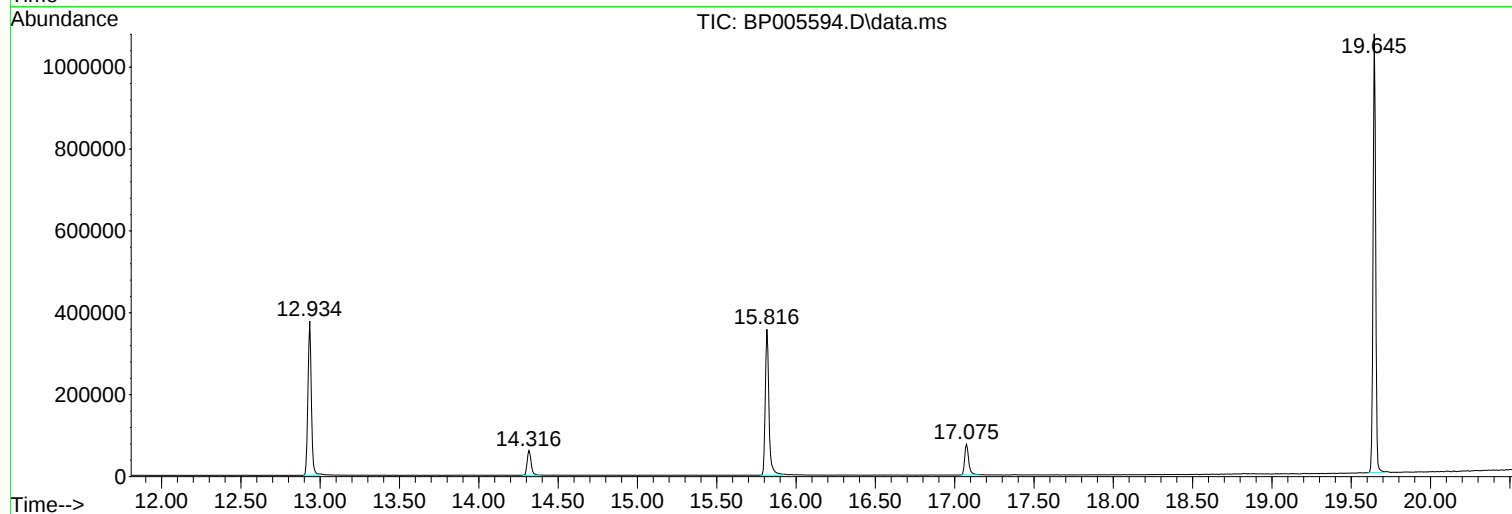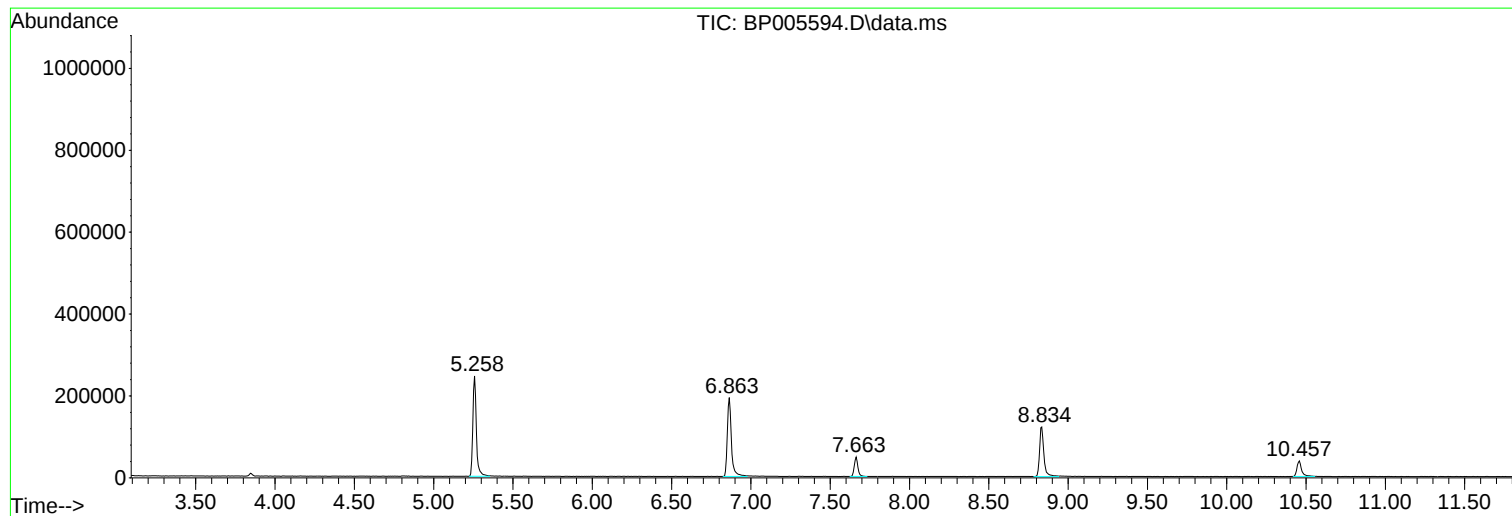

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005594.D
Acq On : 18 May 2021 11:03
Operator : CG/JU
Sample : PB136376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005594.D
Acq On : 18 May 2021 11:03
Operator : CG/JU
Sample : PB136376BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136376BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------