
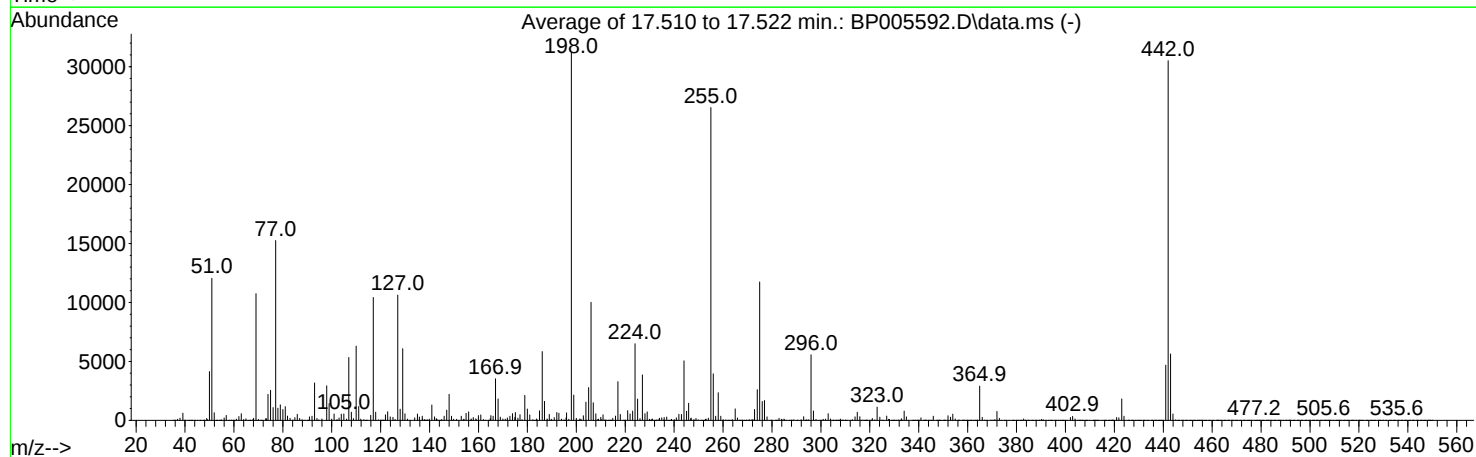


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
 Data File : BP005592.D
 Acq On : 18 May 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 17 15:35:47 2021

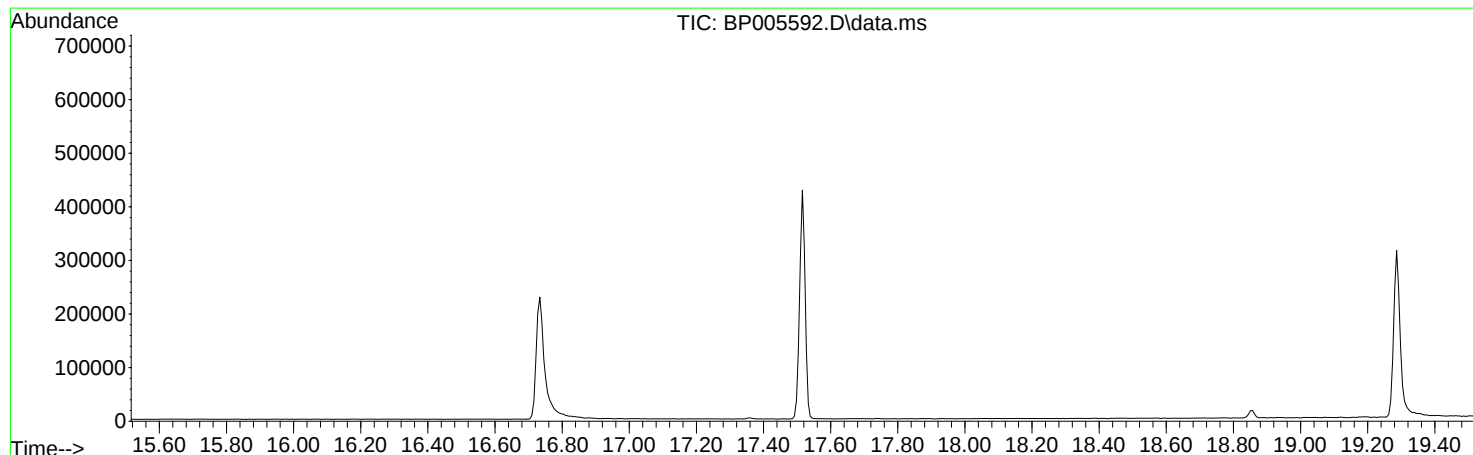

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	12046	PASS
68	69	0.00	2	1.6	175	PASS
69	198	0.00	100	34.4	10745	PASS
70	69	0.00	2	0.8	84	PASS
127	198	10	80	34.0	10621	PASS
197	198	0.00	2	0.3	102	PASS
198	198	100	100	100.0	31203	PASS
199	198	5	9	6.9	2150	PASS
275	198	10	60	37.6	11738	PASS
365	198	1	100	9.3	2903	PASS
441	198	0.01	100	15.0	4681	PASS
442	442	100	100	100.0	30517	PASS
443	442	15	24	18.5	5634	PASS

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/18/2021	BNA_P	<u>BP005592.D</u>
Compound Name	Response	Retention Time
DDT	123905	20.47
DDD	4118	20.05
DDE	408	19.54
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4526	128431	3.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
 Data File : BP005592.D
 Acq On : 18 May 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 18 15:37:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 17 15:35:47 2021
 Response via : Initial Calibration

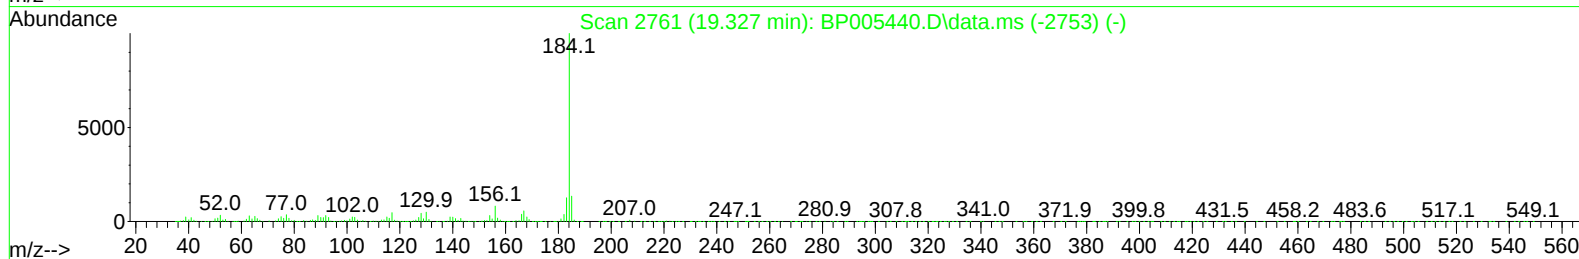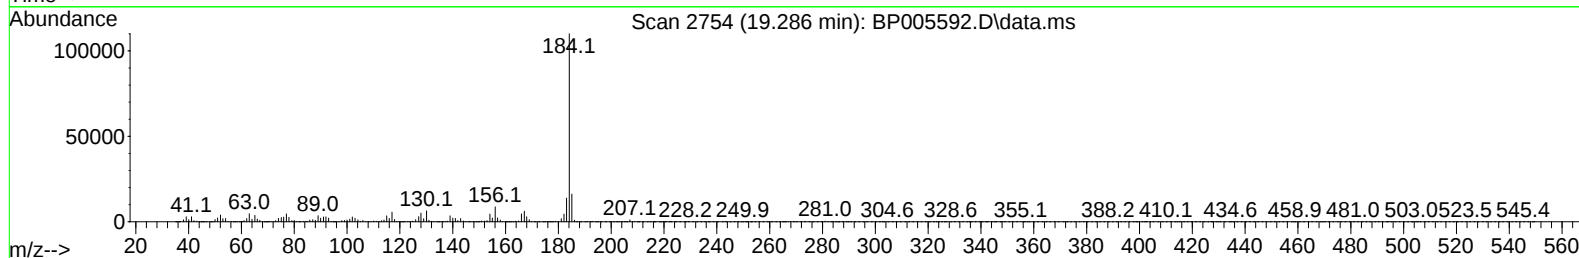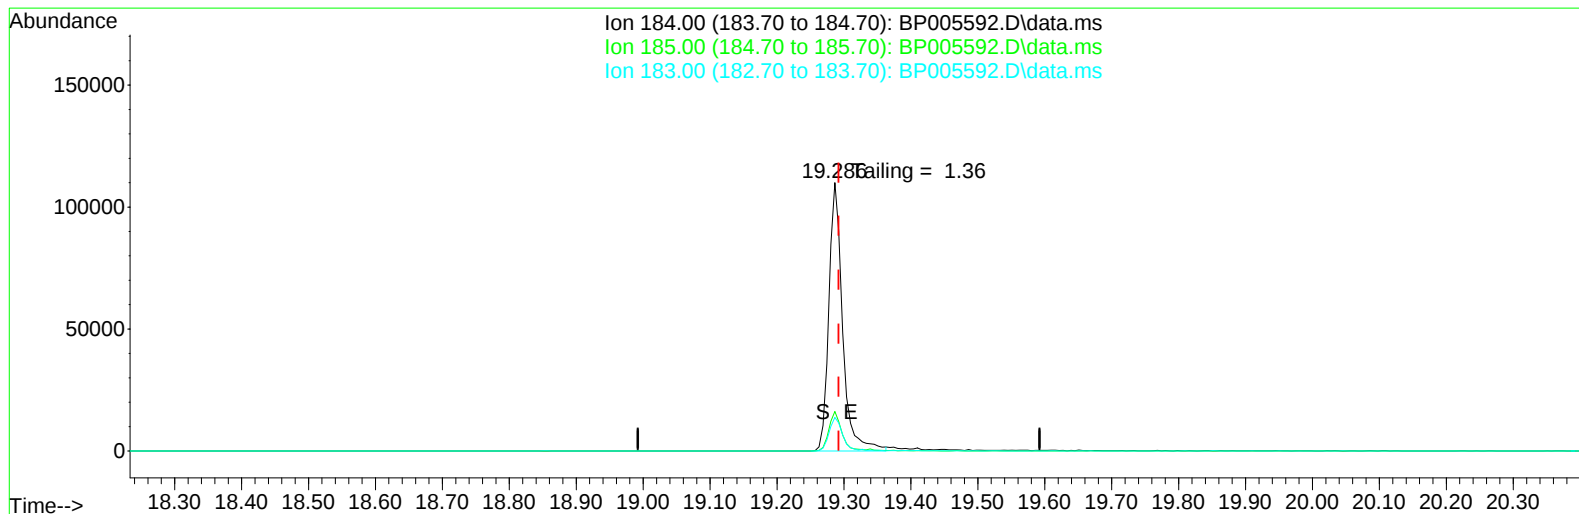

TIC: BP005592.D\data.ms

(77) Benzidine

19.286min (-0.006) 791907.58 ng




response 159351

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.75
183.00	12.30	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051821\
Data File : BP005592.D
Acq On : 18 May 2021 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 18 15:37:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 17 15:35:47 2021
Response via : Initial Calibration

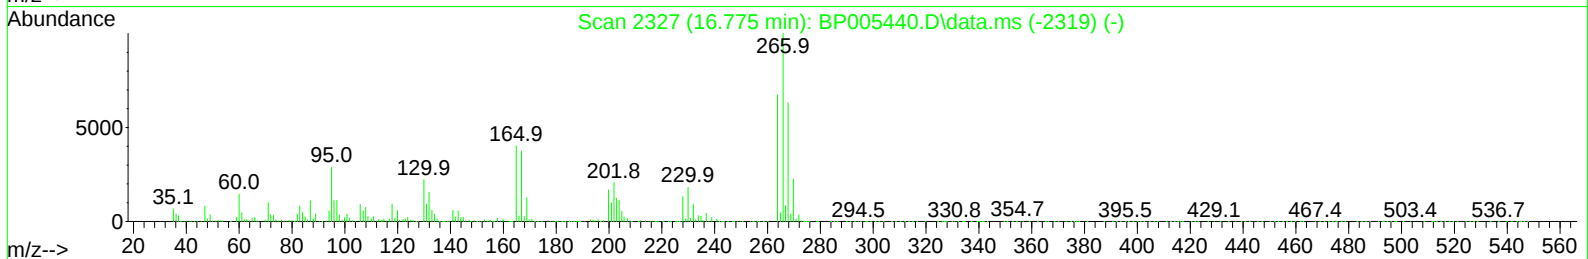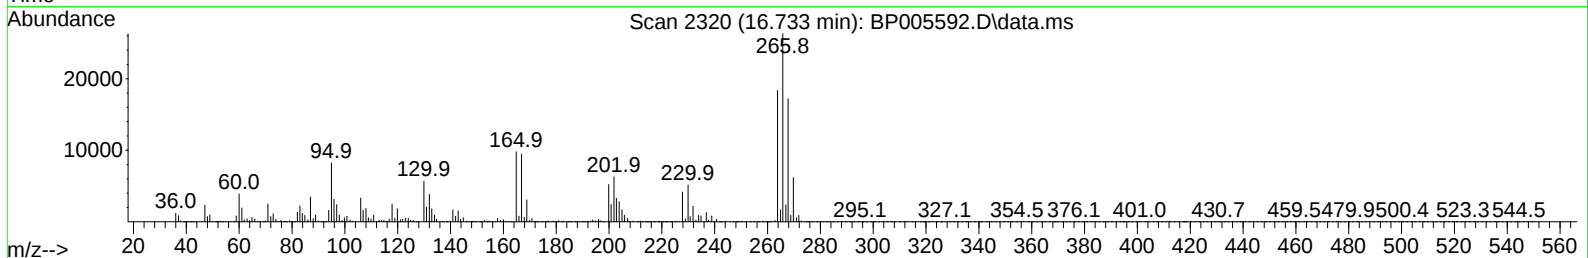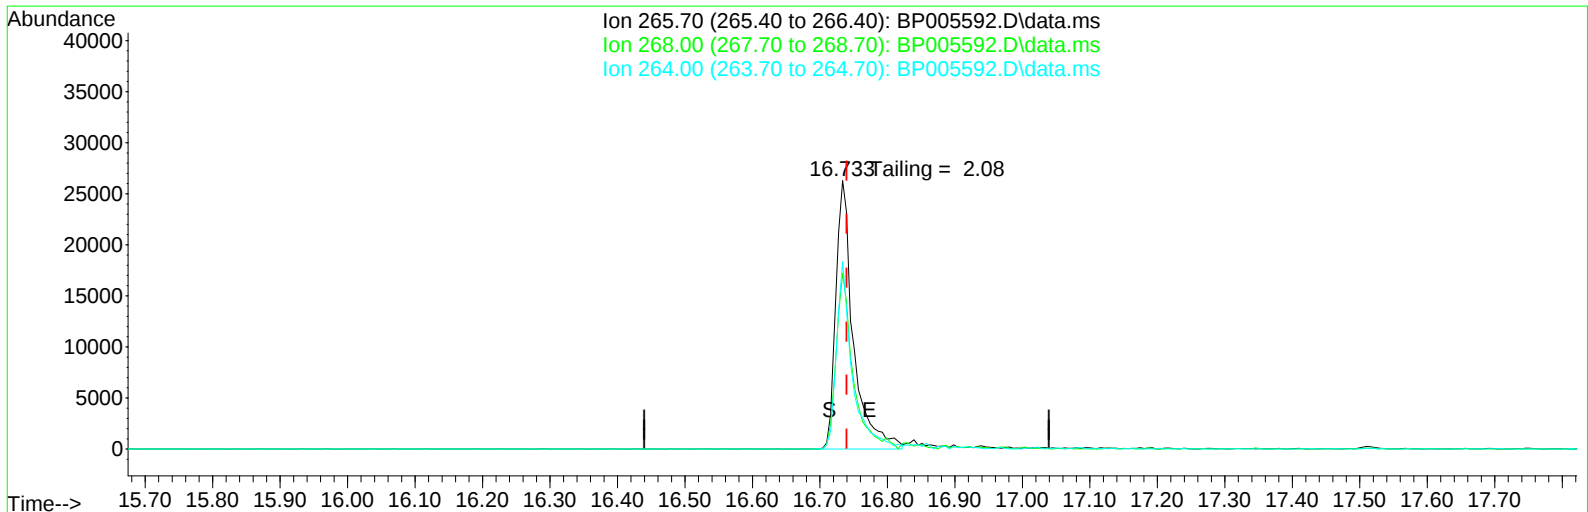

TIC: BP005592.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.006) 378491.12 ng

response 47706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.43
264.00	67.10	69.78
0.00	0.00	0.00