

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015151.D
 Acq On : 18 May 2023 18:22
 Operator : CG/JU
 Sample : 02612-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH7

Quant Time: May 19 01:09:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	351364	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1590501	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	1001793	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	2181013	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1853423	20.000	ng/ul	0.00
88) Perylene-d12	24.157	264	1698989	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	27380	3.028	ng/uL	0.00
4) Pyridine-d5	3.875	84	379211	14.793	ng/ul	0.00
7) Phenol-d5	7.275	99	775947	23.785	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	510970	27.119	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	605682	25.251	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	605804	23.304	ng/ul	0.00
21) Nitrobenzene-d5	9.304	128	315957	25.280	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	362073	26.036	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	605509	24.130	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	875370	23.577	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	2230645	29.467	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	2471450	28.545	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	317992	21.633	ng/ul	0.00
60) Fluorene-d10	15.757	176	1866284	29.217	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	260832	18.977	ng/ul	0.00
73) Anthracene-d10	17.616	188	2964433	29.683	ng/ul	0.00
81) Pyrene-d10	19.833	212	3400431	31.633	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	2620951	31.076	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.963	105	106041	2.614	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015151.D
Acq On : 18 May 2023 18:22
Operator : CG/JU
Sample : 02612-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH7


Quant Time: May 19 01:09:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

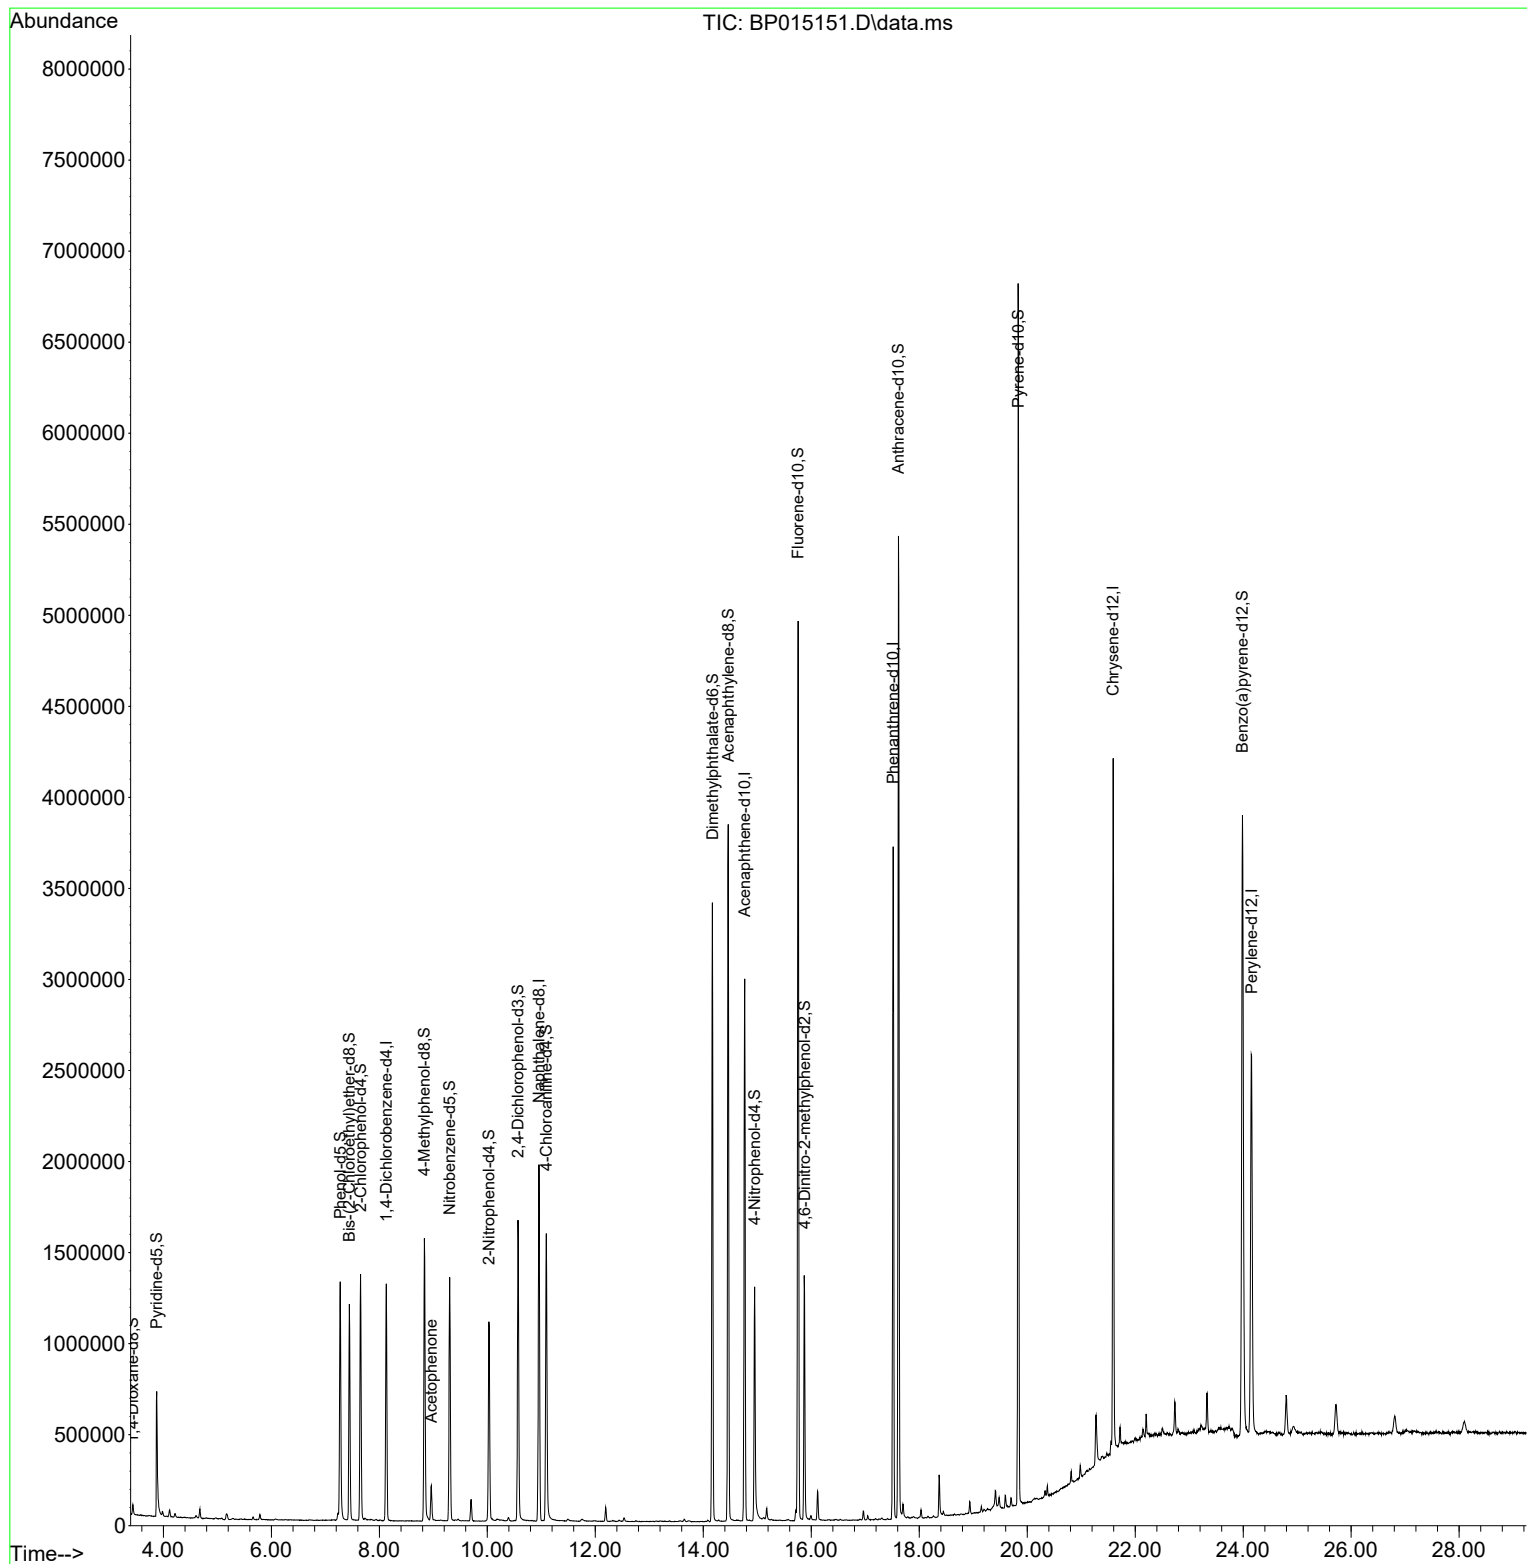

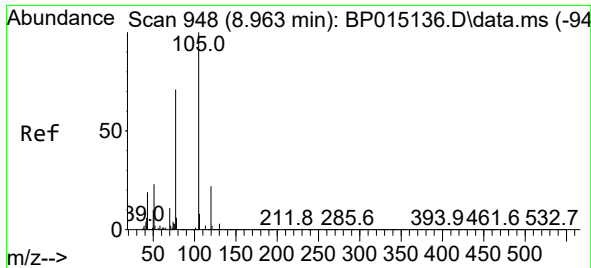

#16
Acetophenone
Concen: 2.614 ng/ul
RT: 8.963 min Scan# 94
Delta R.T. -0.000 min
Lab File: BP015151.D
Acq: 18 May 2023 18:22

Instrument :
BNA_P
ClientSampleId :
JREH7

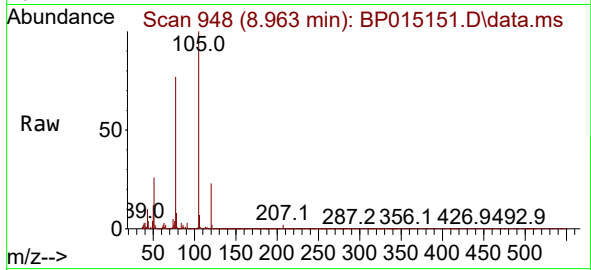

Tgt Ion:105 Resp: 106041
Ion Ratio Lower Upper
105 100
77 77.3 59.4 89.2
51 25.5 19.2 28.8

