

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015154.D
 Acq On : 18 May 2023 20:02
 Operator : CG/JU
 Sample : 02612-17
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREJ1

Quant Time: May 19 01:10:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	299399	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1373906	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	747217	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1769909	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1656764	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1686013	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	13126	1.703	ng/uL	0.00
4) Pyridine-d5	3.881	84	668	0.031	ng/ul	0.01
7) Phenol-d5	7.275	99	366117	13.170	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	253850	15.811	ng/ul	0.00
11) 2-Chlorophenol-d4	7.651	132	297408	14.551	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	313050	14.133	ng/ul	0.00
21) Nitrobenzene-d5	9.304	128	155672	14.419	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	166117	13.829	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	311720	14.381	ng/ul	0.00
31) 4-Chloroaniline-d4	11.092	131	449875	14.027	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1064776	18.858	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1129507	17.491	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	125053	11.406	ng/ul	0.00
60) Fluorene-d10	15.757	176	892314	18.728	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	117972	10.577	ng/ul	0.00
73) Anthracene-d10	17.616	188	1551082	19.138	ng/ul	0.00
81) Pyrene-d10	19.833	212	2106883	21.926	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	1762604	21.060	ng/ul	0.00
Target Compounds						Qvalue
16) Acetophenone	8.963	105	122244	3.536	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015154.D
Acq On : 18 May 2023 20:02
Operator : CG/JU
Sample : 02612-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREJ1


Quant Time: May 19 01:10:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

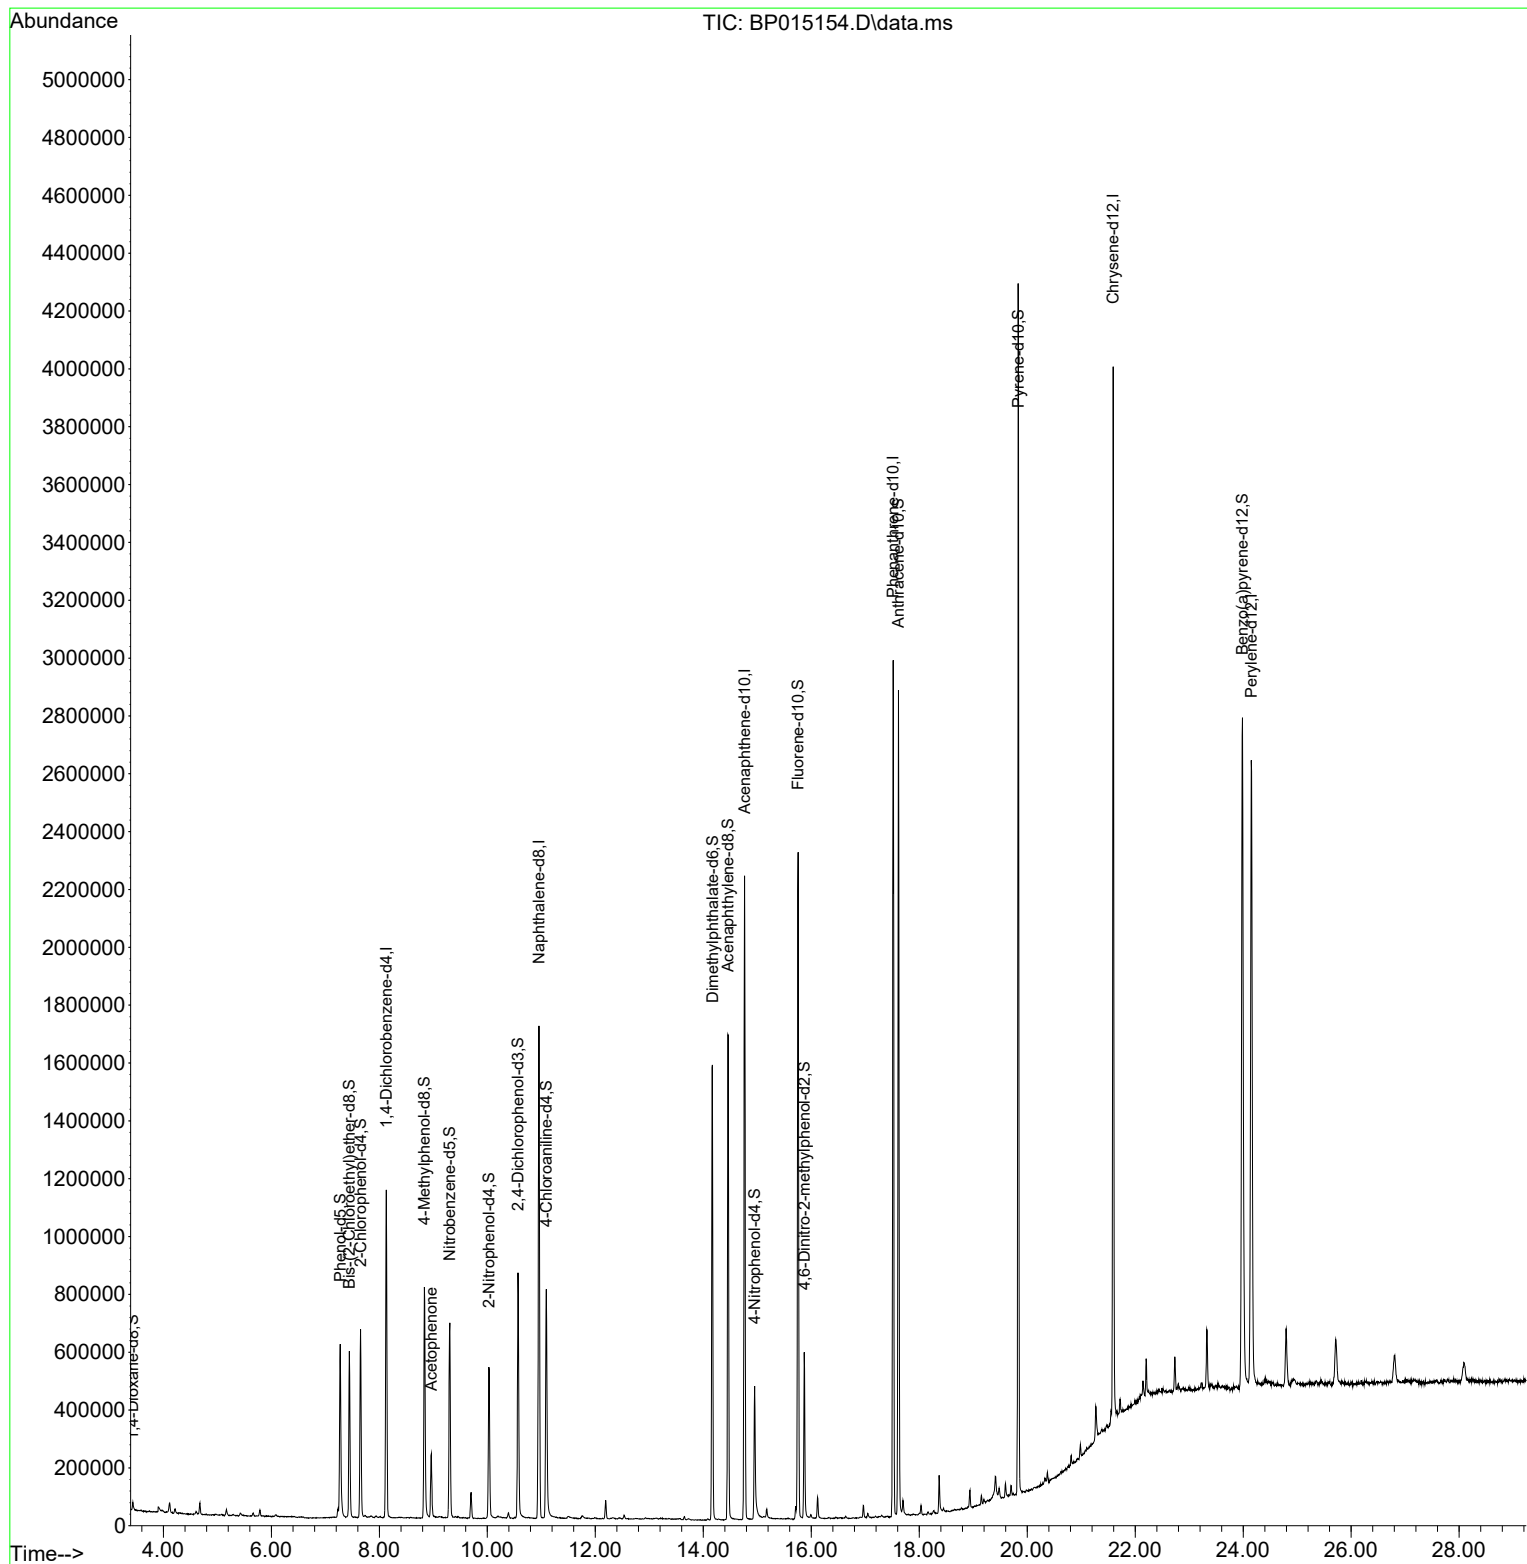

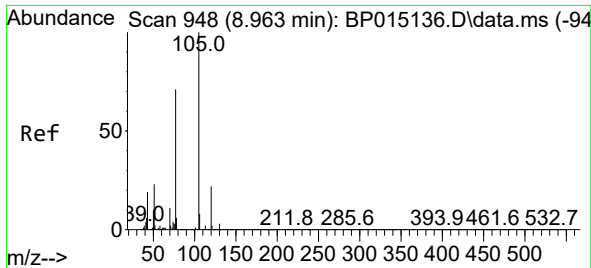

#16
Acetophenone
Concen: 3.536 ng/ul
RT: 8.963 min Scan# 94
Delta R.T. -0.000 min
Lab File: BP015154.D
Acq: 18 May 2023 20:02

Instrument :
BNA_P
ClientSampleId :
JREJ1

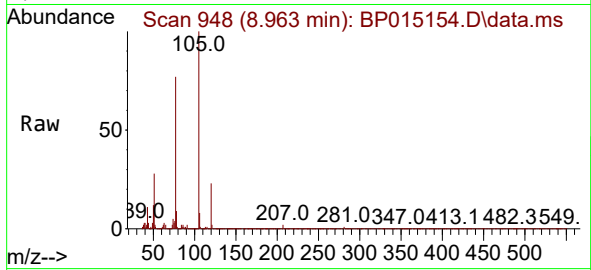

Tgt Ion:	105	Resp:	122244
Ion	Ratio	Lower	Upper
105	100		
77	77.0	59.4	89.2
51	27.9	19.2	28.8

