

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP05159.D
 Acq On : 18 May 2023 22:49
 Operator : CG/JU
 Sample : 02612-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH8

Quant Time: May 19 01:11:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	269038	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1180662	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	750087	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.515	188	1672784	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1605046	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	1624538	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	17616	2.544	ng/uL	0.00
4) Pyridine-d5	3.887	84	1177	0.060	ng/ul	0.02
7) Phenol-d5	7.275	99	511657	20.483	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.445	67	347380	24.079	ng/ul	0.00
11) 2-Chlorophenol-d4	7.651	132	399195	21.735	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	387504	19.468	ng/ul	0.00
21) Nitrobenzene-d5	9.298	128	210526	22.692	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	233814	22.650	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	396950	21.310	ng/ul	0.00
31) 4-Chloroaniline-d4	11.092	131	546246	19.820	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1560197	27.526	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1710763	26.390	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	190907	17.345	ng/ul	0.00
60) Fluorene-d10	15.757	176	1332989	27.871	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.868	200	168196	15.955	ng/ul	0.00
73) Anthracene-d10	17.615	188	2216951	28.943	ng/ul	0.00
81) Pyrene-d10	19.833	212	2793324	30.007	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	2471670	30.649	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.963	105	117007	3.766	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015159.D
Acq On : 18 May 2023 22:49
Operator : CG/JU
Sample : 02612-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH8


Quant Time: May 19 01:11:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

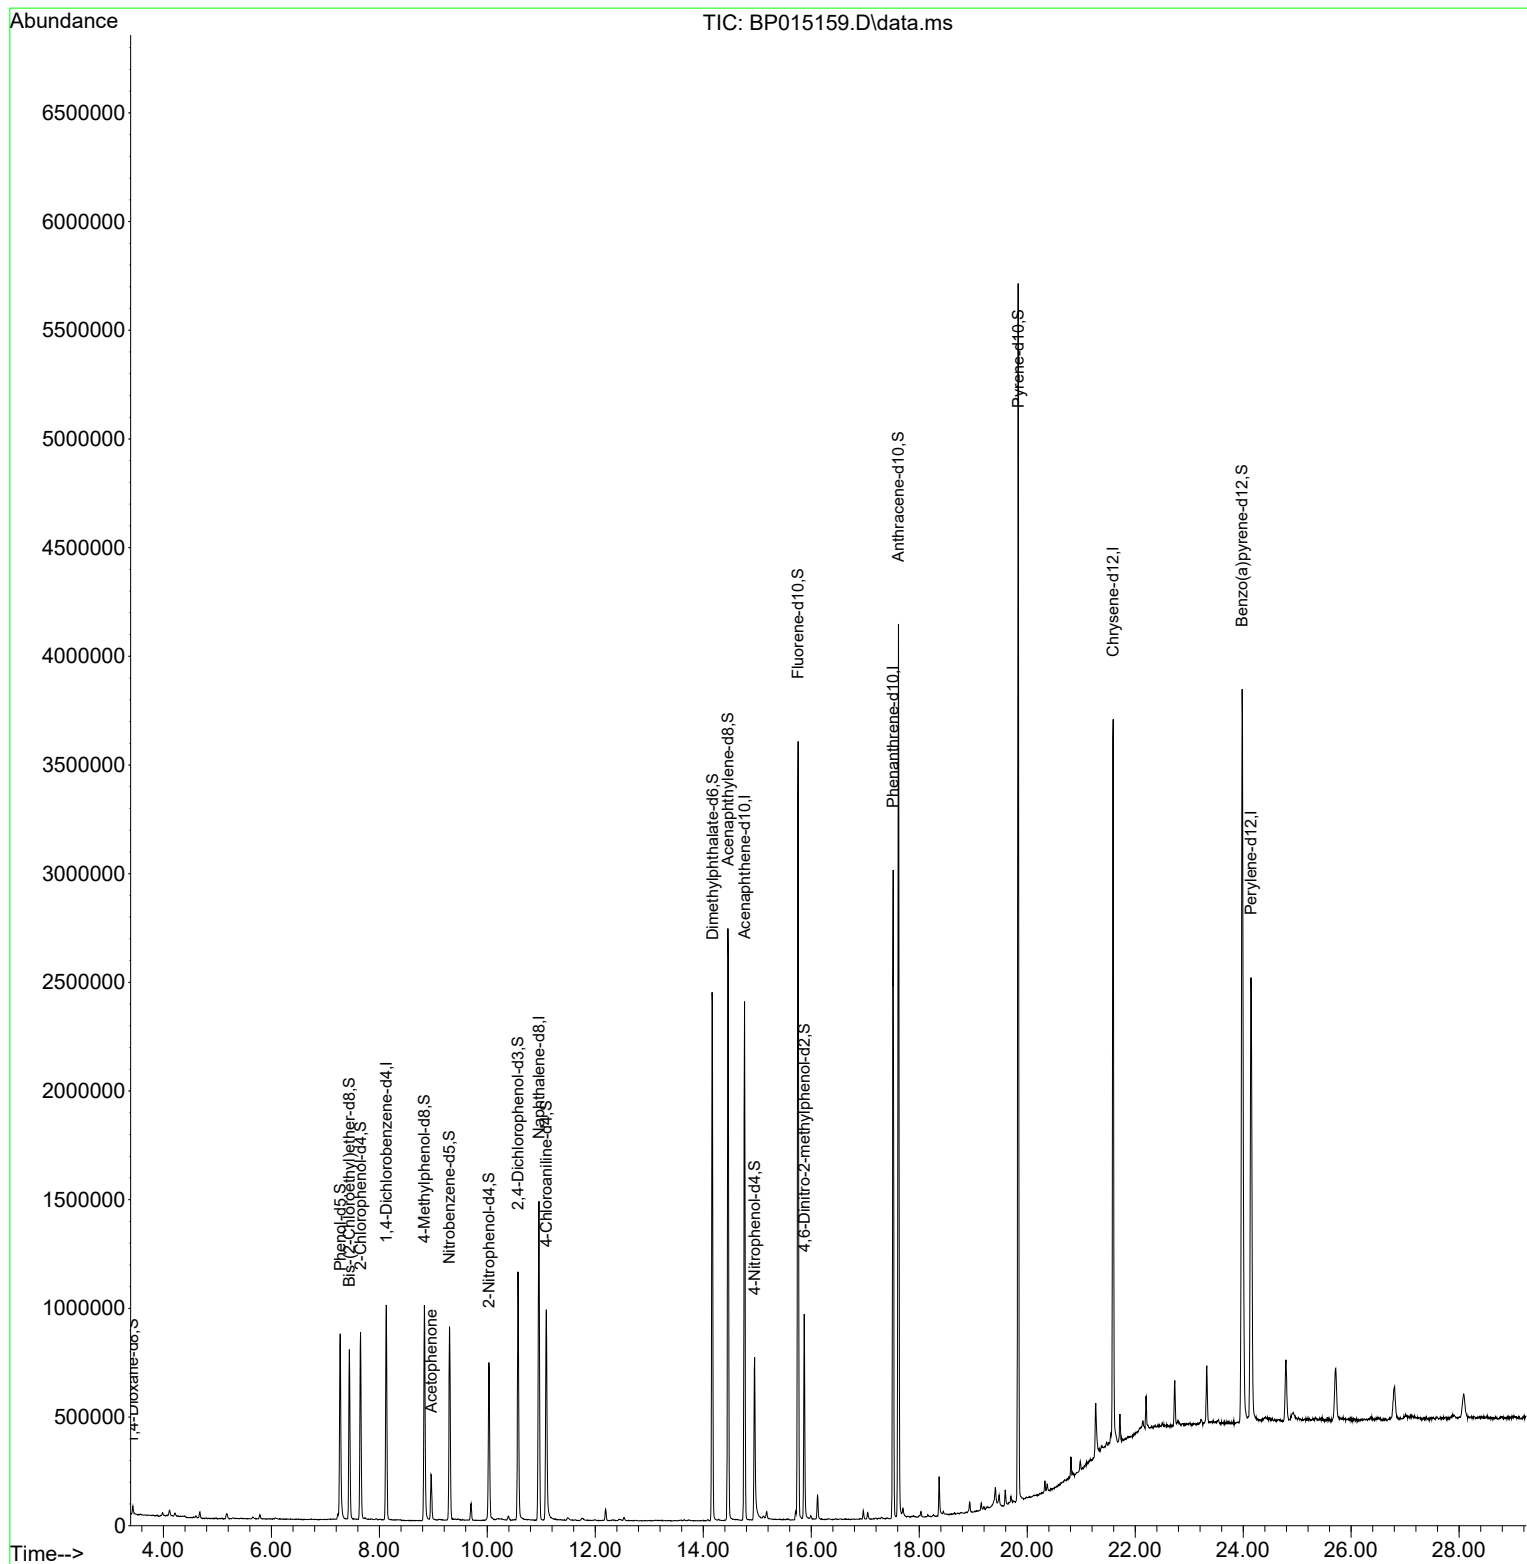

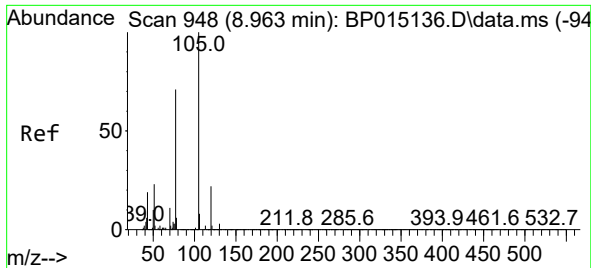

#16
 Acetophenone
 Concen: 3.766 ng/ul
 RT: 8.963 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: BP015159.D
 Acq: 18 May 2023 22:49

Instrument :
 BNA_P
 ClientSampleId :
 JREH8

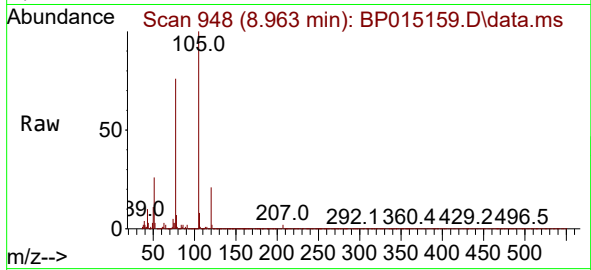

Tgt Ion:105 Resp: 117007
 Ion Ratio Lower Upper
 105 100
 77 75.6 59.4 89.2
 51 26.2 19.2 28.8

