

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015160.D
 Acq On : 18 May 2023 23:22
 Operator : CG/JU
 Sample : 02612-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH9

Quant Time: May 19 01:11:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	296297	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1307923	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	631483	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1651757	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1595017	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	1653630	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	22608	2.965	ng/uL	0.00
4) Pyridine-d5	3.887	84	361	0.017	ng/ul	0.02
7) Phenol-d5	7.275	99	532061	19.340	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	369560	23.259	ng/ul	0.00
11) 2-Chlorophenol-d4	7.651	132	452287	22.360	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	450683	20.559	ng/ul	0.00
21) Nitrobenzene-d5	9.304	128	236123	22.975	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	251634	22.004	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	435440	21.101	ng/ul	0.00
31) 4-Chloroaniline-d4	11.092	131	628631	20.589	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1311545	27.485	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1406867	25.778	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	165331	17.843	ng/ul	0.00
60) Fluorene-d10	15.757	176	1117105	27.744	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	159166	15.290	ng/ul	0.00
73) Anthracene-d10	17.616	188	2125133	28.097	ng/ul	0.00
81) Pyrene-d10	19.833	212	2707270	29.265	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	2582617	31.462	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.957	105	136955	4.003	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015160.D
Acq On : 18 May 2023 23:22
Operator : CG/JU
Sample : 02612-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH9


Quant Time: May 19 01:11:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

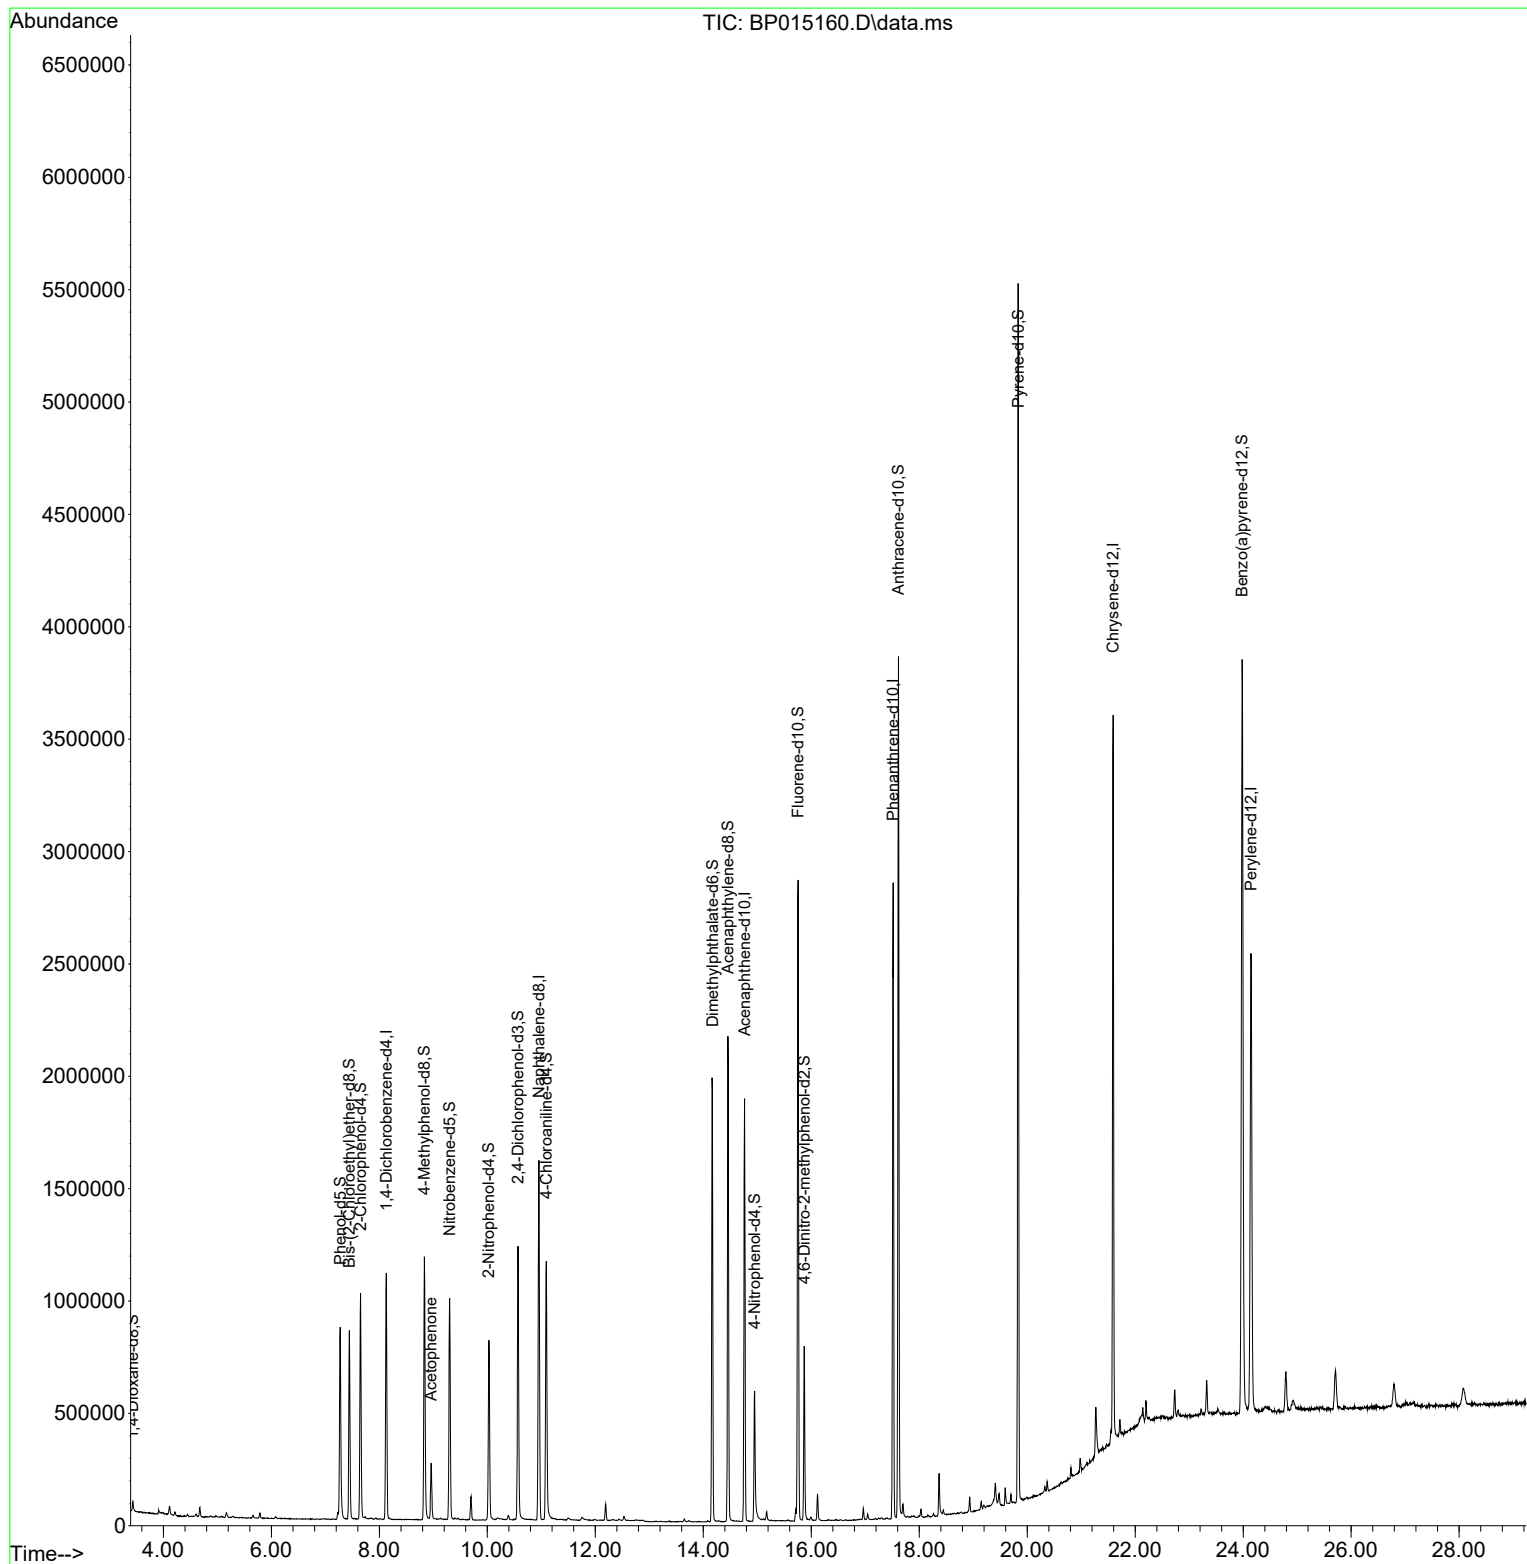

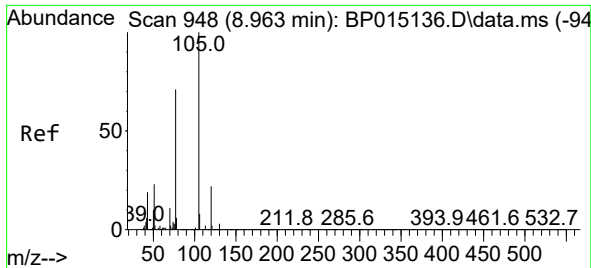

#16
Acetophenone
Concen: 4.003 ng/ul
RT: 8.957 min Scan# 94
Delta R.T. -0.006 min
Lab File: BP015160.D
Acq: 18 May 2023 23:22

Instrument :
BNA_P
ClientSampleId :
JREH9

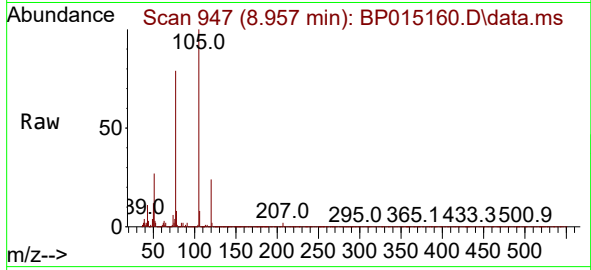

Tgt Ion:105 Resp: 136955
Ion Ratio Lower Upper
105 100
77 78.5 59.4 89.2
51 27.5 19.2 28.8

