




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015141.D
 Acq On : 18 May 2023 12:46
 Operator : CG/JU
 Sample : 02612-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH4

Manual IntegrationsAPPROVED

Quant Time: May 19 00:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 18 01:09:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/19/2023
 Supervised By :Jagrut Upadhyay 05/19/2023

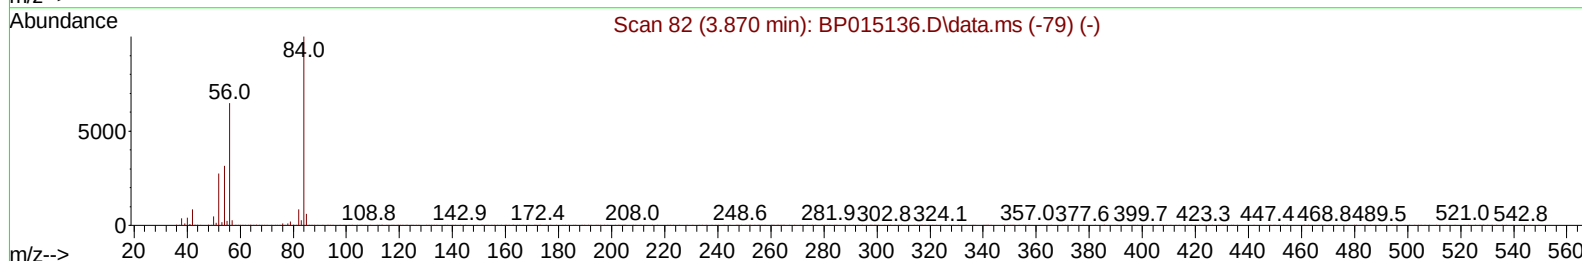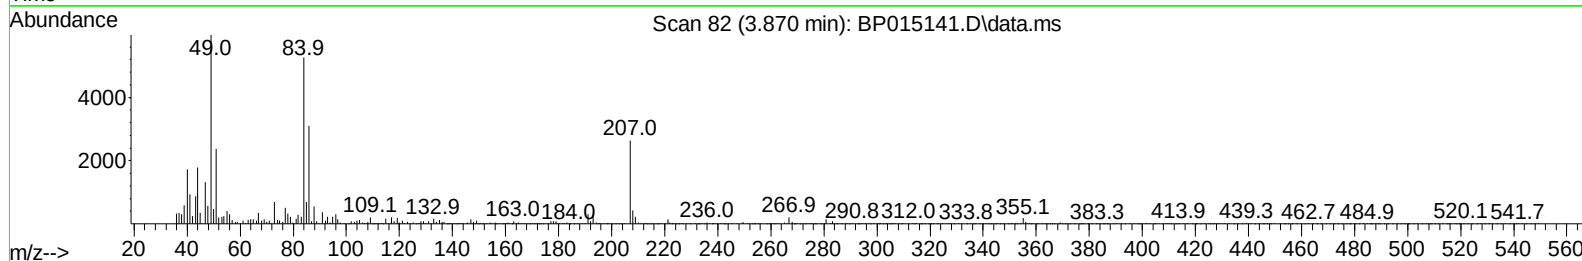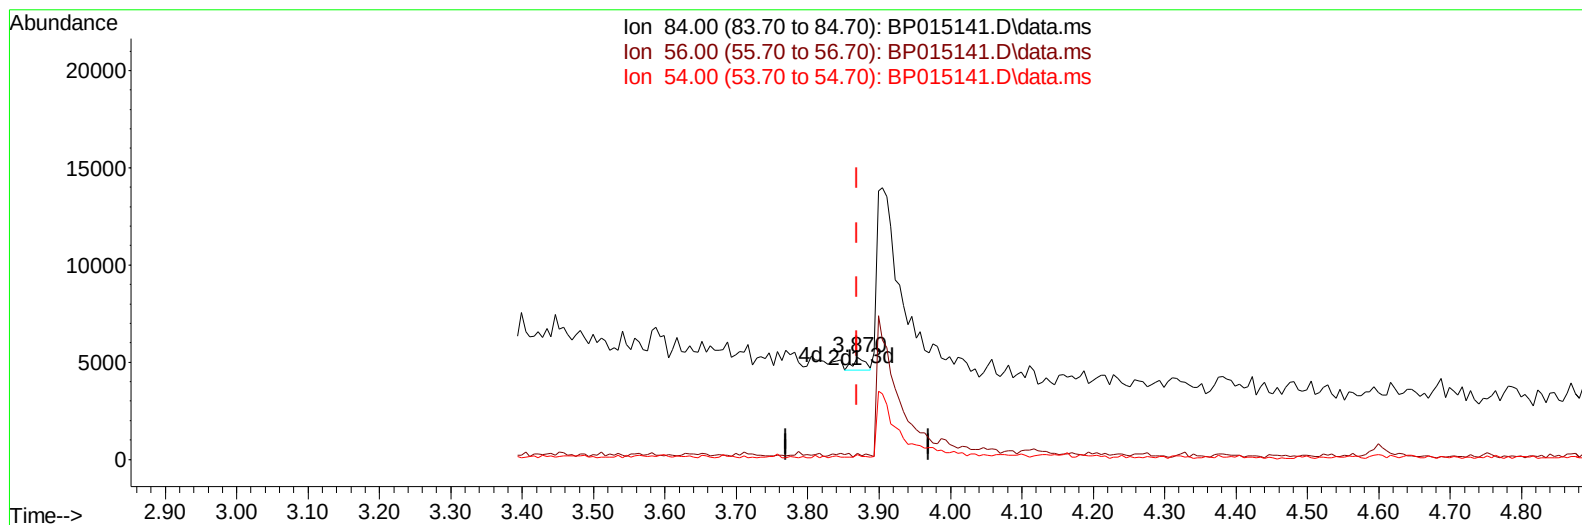

TIC: BP015141.D\data.ms

(4) Pyridine-d5 (S)

3.870min (+ 0.000) 0.03 ng/u1

response 776

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	60.60	5.81#
54.00	29.10	4.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015141.D
 Acq On : 18 May 2023 12:46
 Operator : CG/JU
 Sample : 02612-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH4

Manual IntegrationsAPPROVED

Quant Time: May 19 00:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 18 01:09:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/19/2023
 Supervised By :Jagrut Upadhyay 05/19/2023

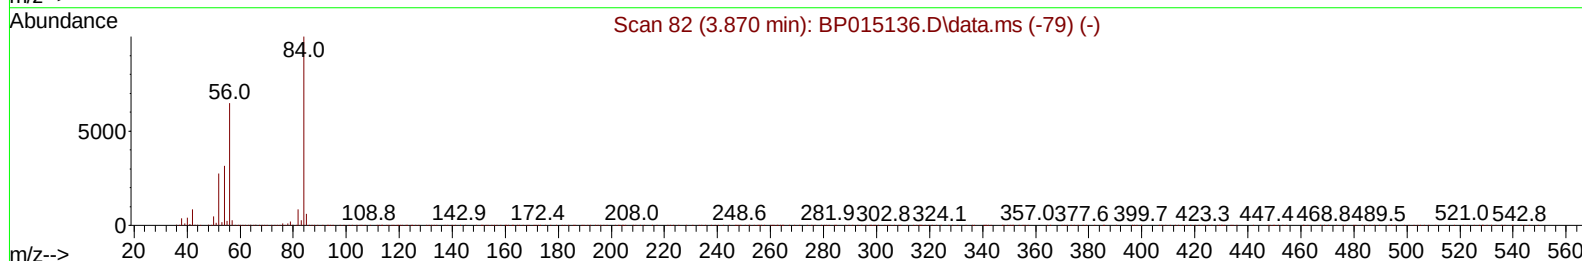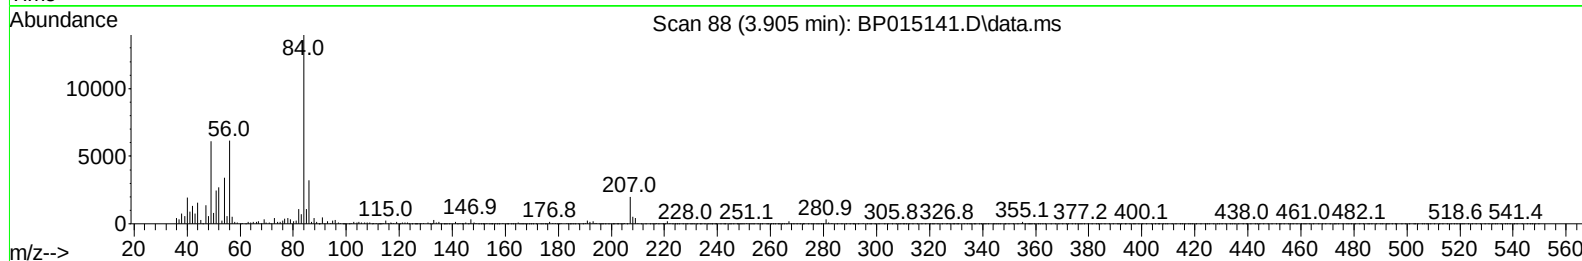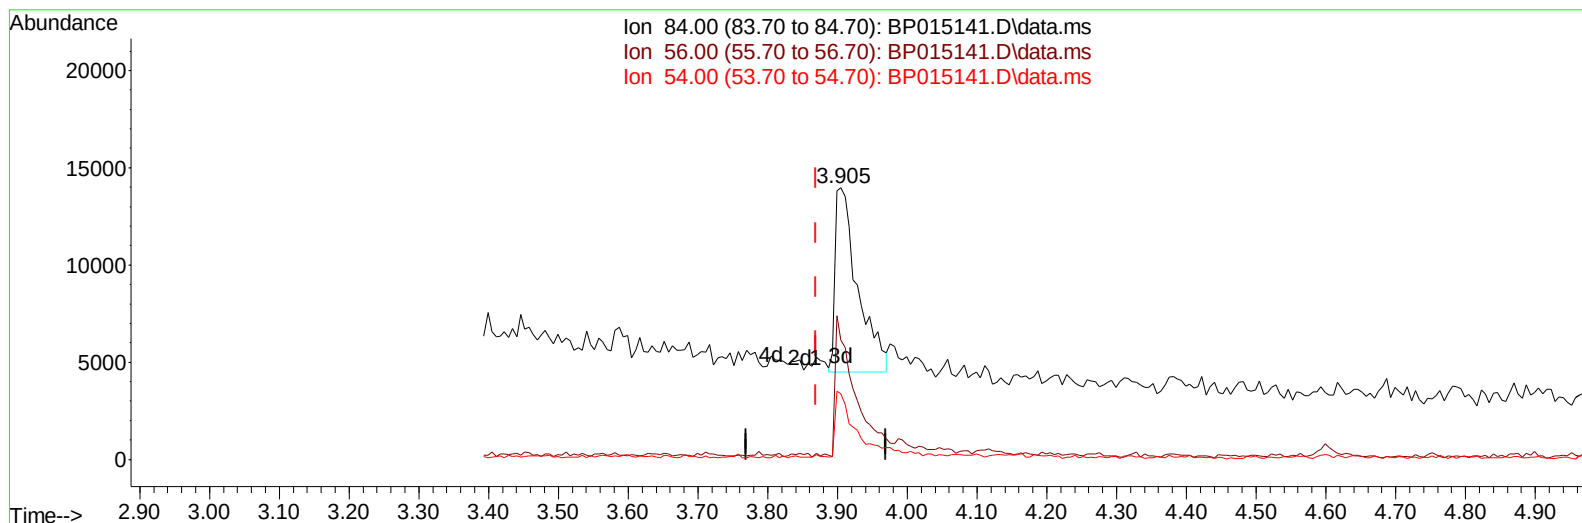

TIC: BP015141.D\data.ms

(4) Pyridine-d5 (S)

3.905min (+ 0.035) 0.91 ng/ul m

response 21238

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	60.60	44.04#
54.00	29.10	24.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015141.D
 Acq On : 18 May 2023 12:46
 Operator : CG/JU
 Sample : 02612-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/19/2023
 Supervised By :Jagrut Upadhyay 05/19/2023

Quant Time: May 19 00:58:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 18 01:09:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	318998	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1461787	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	907590	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.522	188	2016694	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1681023	20.000	ng/ul	-0.01
88) Perylene-d12	24.157	264	1784561	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	13232	1.612	ng/uL	0.00
4) Pyridine-d5	3.905	84	21238m	0.913	ng/ul	0.04
7) Phenol-d5	7.275	99	393613	13.290	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	263375	15.397	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	302022	13.869	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	258617	10.958	ng/ul	0.00
21) Nitrobenzene-d5	9.305	128	157554	13.716	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	169168	13.236	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	309844	13.435	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	408210	11.963	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1209582	17.637	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	1318660	16.811	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	140526	10.552	ng/ul	0.00
60) Fluorene-d10	15.757	176	1054958	18.230	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	118059	9.289	ng/ul	0.00
73) Anthracene-d10	17.616	188	1617857	17.520	ng/ul	0.00
81) Pyrene-d10	19.833	212	1962690	20.131	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	1651469	18.642	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.963	105	96962	2.632	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015141.D
Acq On : 18 May 2023 12:46
Operator : CG/JU
Sample : 02612-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH4

Manual IntegrationsAPPROVED

Quant Time: May 19 00:58:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 18 01:09:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/19/2023
Supervised By :Jagrut Upadhyay 05/19/2023

