

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015142.D
 Acq On : 18 May 2023 13:20
 Operator : CG/JU
 Sample : 02612-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH6

Quant Time: May 19 00:43:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 18 01:09:56 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	322548	20.000	ng/u1	0.00
20) Naphthalene-d8	10.957	136	1326238	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	918518	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.522	188	2023919	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1702212	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	1808304	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	18510	2.230	ng/uL	0.00
4) Pyridine-d5	3.875	84	279433	11.875	ng/u1	0.00
7) Phenol-d5	7.275	99	494007	16.496	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	320456	18.527	ng/u1	0.00
11) 2-Chlorophenol-d4	7.652	132	380042	17.259	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	400632	16.788	ng/u1	0.00
21) Nitrobenzene-d5	9.305	128	194344	18.648	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	208218	17.956	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	382862	18.297	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	495276	15.998	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	1396705	20.123	ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	1544939	19.462	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	181616	13.475	ng/u1	0.00
60) Fluorene-d10	15.757	176	1203991	20.557	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	130356	10.220	ng/u1	0.00
73) Anthracene-d10	17.616	188	1935505	20.885	ng/u1	0.00
81) Pyrene-d10	19.839	212	2377900	24.086	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	2074772	23.113	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.963	105	88696	2.381	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015142.D
Acq On : 18 May 2023 13:20
Operator : CG/JU
Sample : 02612-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH6

Quant Time: May 19 00:43:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 18 01:09:56 2023
Response via : Initial Calibration

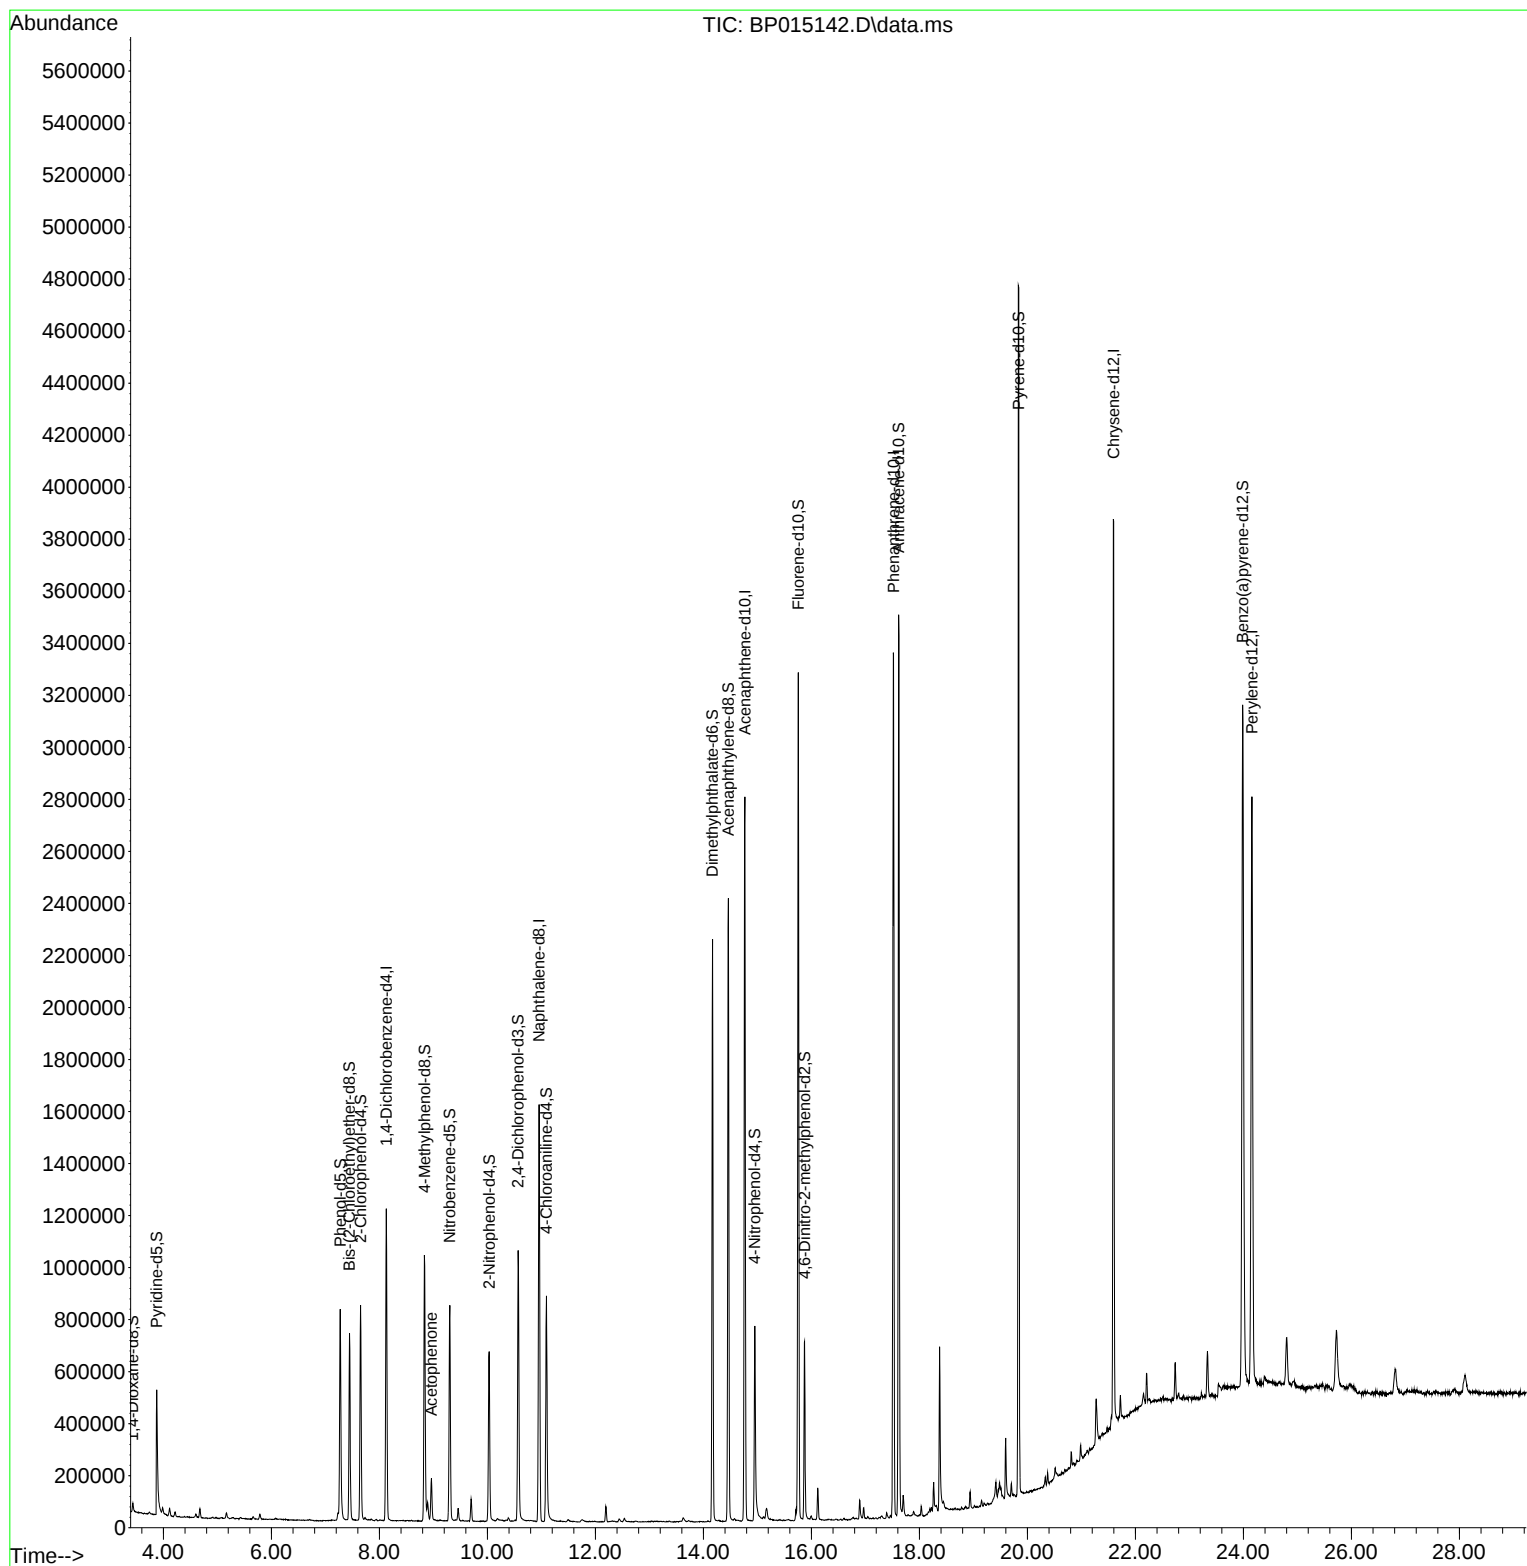

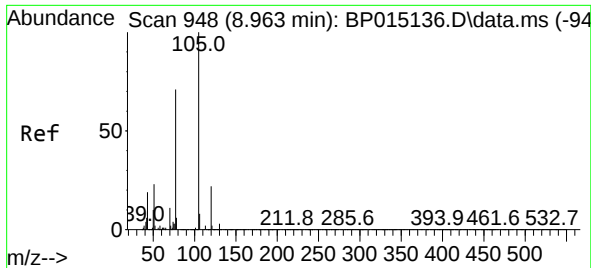

#16
 Acetophenone
 Concen: 2.381 ng/ul
 RT: 8.963 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP015142.D
 Acq: 18 May 2023 13:20

Instrument :
 BNA_P
 ClientSampleId :
 JREH6

Tgt Ion:	105	Resp:	88696
Ion	Ratio	Lower	Upper
105	100		
77	74.8	59.4	89.2
51	26.4	19.2	28.8

