

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015153.D
 Acq On : 18 May 2023 19:29
 Operator : CG/JU
 Sample : 02612-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG9

Quant Time: May 19 01:10:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	278767	20.000	ng/ul	0.00
20) Naphthalene-d8	10.958	136	1407864	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	891764	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1943056	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1631723	20.000	ng/ul	0.00
88) Perylene-d12	24.157	264	1633826	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	47135	6.570	ng/uL	0.00
4) Pyridine-d5	3.876	84	332325	16.341	ng/ul	0.00
7) Phenol-d5	7.275	99	914848	35.346	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	592047	39.605	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	718758	37.769	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	813319	39.435	ng/ul	0.00
21) Nitrobenzene-d5	9.305	128	423740	38.303	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	486438	39.517	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	830424	37.386	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	1179386	35.886	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	2974860	44.146	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	3307774	42.919	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	468462	35.801	ng/ul	0.00
60) Fluorene-d10	15.757	176	2498159	43.934	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	383823	31.345	ng/ul	0.00
73) Anthracene-d10	17.616	188	3970690	44.628	ng/ul	0.00
81) Pyrene-d10	19.834	212	4716191	49.835	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.992	264	3992573	49.227	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.963	105	99887	3.103	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015153.D
Acq On : 18 May 2023 19:29
Operator : CG/JU
Sample : 02612-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG9

Quant Time: May 19 01:10:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

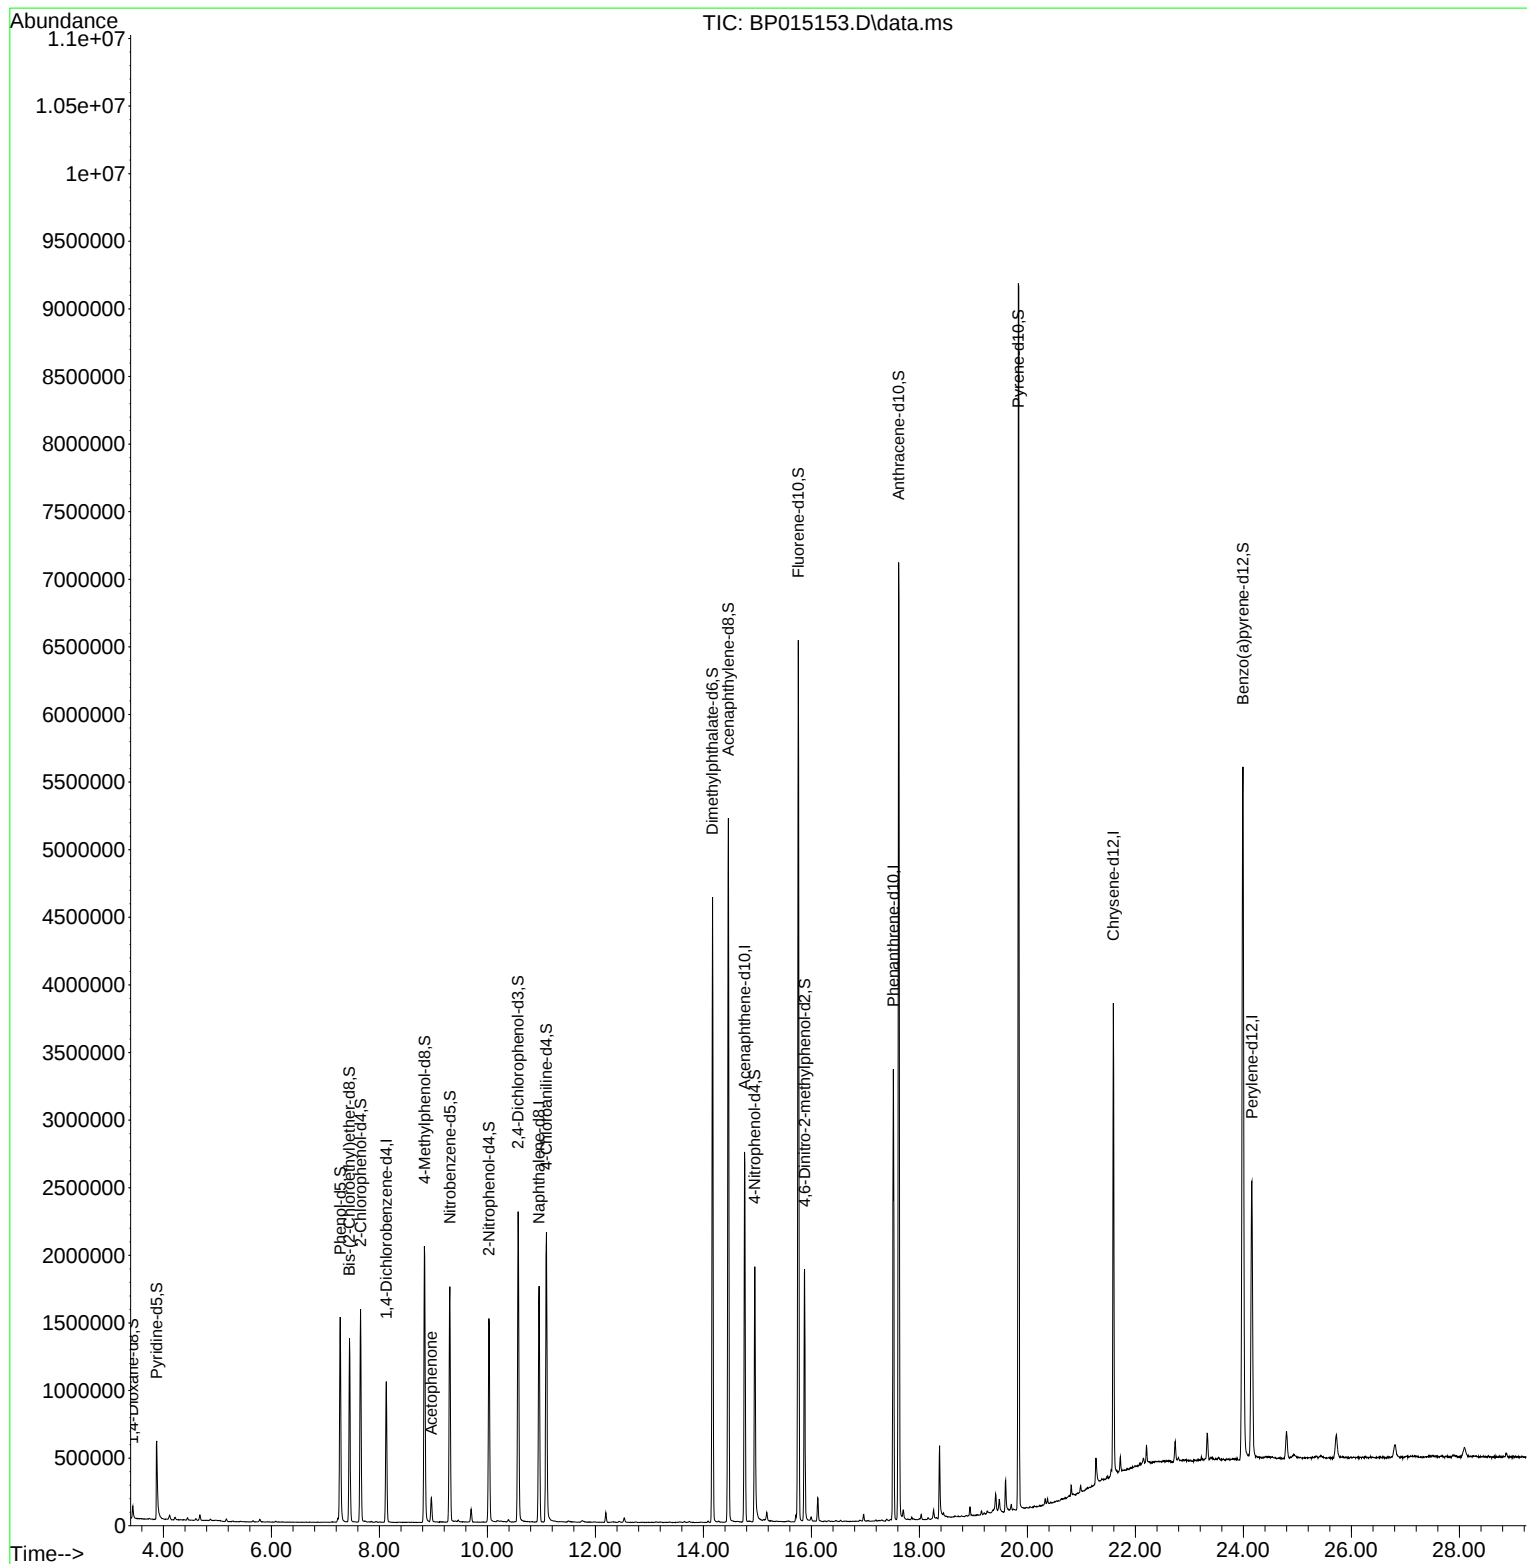

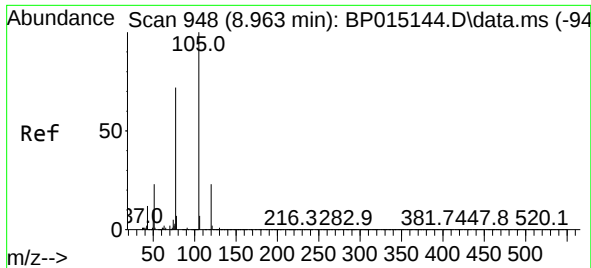

#16
Acetophenone
Concen: 3.103 ng/ul
RT: 8.963 min Scan# 94
Delta R.T. 0.000 min
Lab File: BP015153.D
Acq: 18 May 2023 19:29

Instrument :
BNA_P
ClientSampleId :
JREG9

Tgt Ion:105 Resp: 99887
Ion Ratio Lower Upper
105 100
77 74.4 59.4 89.2
51 26.2 19.2 28.8

