

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015156.D
 Acq On : 18 May 2023 21:09
 Operator : CG/JU
 Sample : 02612-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG7

Quant Time: May 19 01:32:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	270822	20.000	ng/u1	0.00
20) Naphthalene-d8	10.957	136	1349505	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.763	164	853396	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.516	188	1893074	20.000	ng/u1	0.00
79) Chrysene-d12	21.592	240	1662889	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	1729267	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	18710	2.684	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.275	99	531210	21.126	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	359569	24.759	ng/u1	0.00
11) 2-Chlorophenol-d4	7.652	132	415671	22.483	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	394674	19.698	ng/u1	0.00
21) Nitrobenzene-d5	9.305	128	192282	18.132	ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	223490	18.941	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	413724	19.431	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	586859	18.629	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	1539773	23.877	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	1693438	22.960	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	196777	15.714	ng/u1	0.00
60) Fluorene-d10	15.757	176	1311643	24.104	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	162758	13.642	ng/u1	0.00
73) Anthracene-d10	17.616	188	2068202	23.859	ng/u1	0.00
81) Pyrene-d10	19.833	212	2529749	26.230	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	2206847	25.708	ng/u1	0.00


Target Compounds					Qvalue	
16) Acetophenone	8.958	105	72741	2.326	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015156.D
Acq On : 18 May 2023 21:09
Operator : CG/JU
Sample : 02612-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG7

Quant Time: May 19 01:32:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

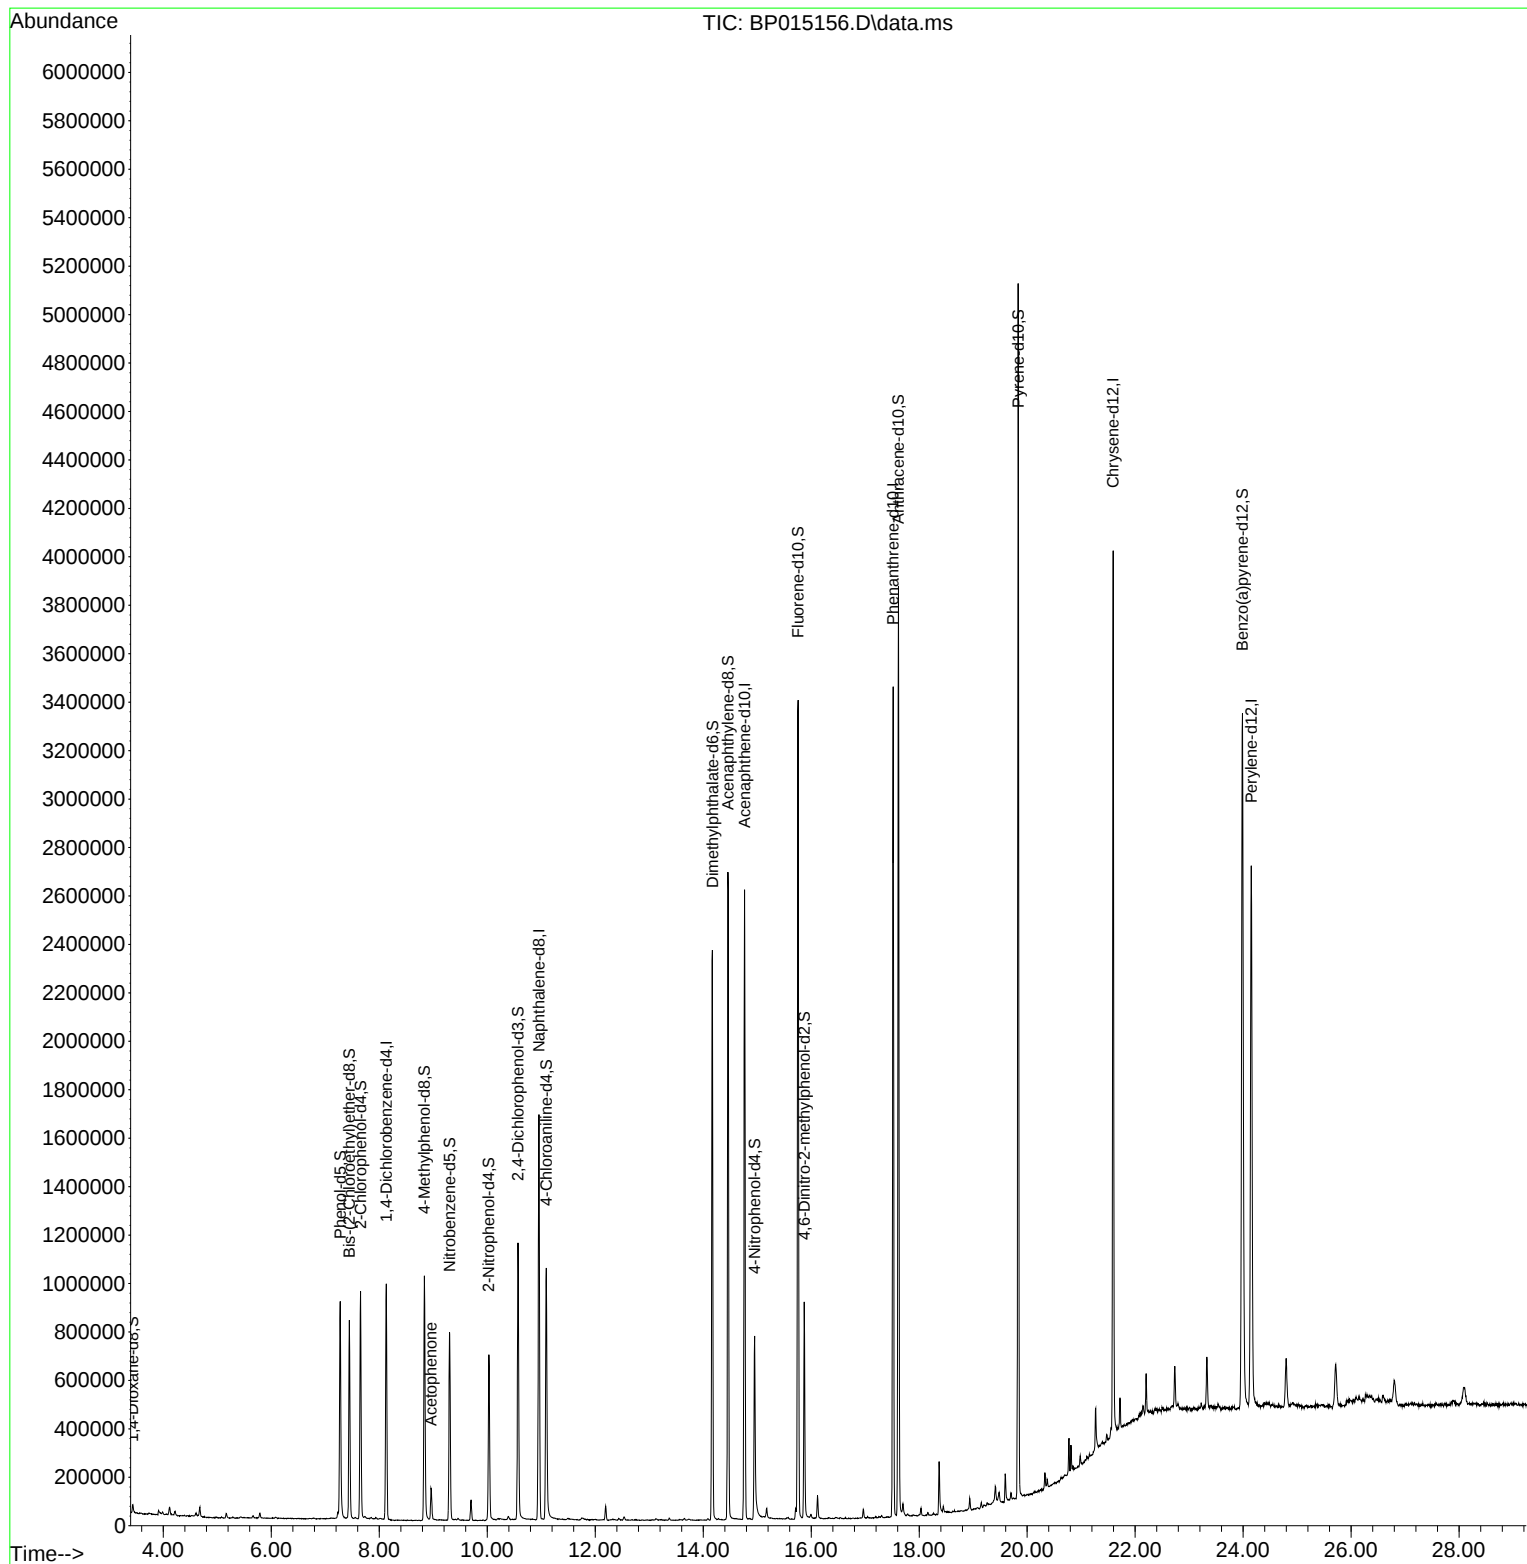

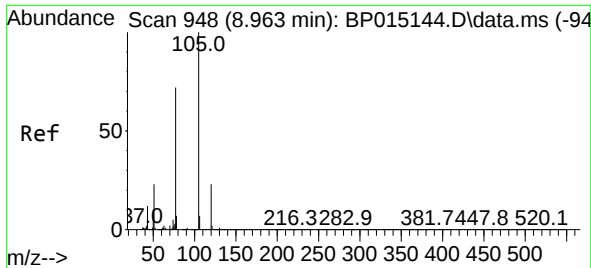

#16
Acetophenone
Concen: 2.326 ng/ul
RT: 8.958 min Scan# 94
Delta R.T. -0.006 min
Lab File: BP015156.D
Acq: 18 May 2023 21:09

Instrument :
BNA_P
ClientSampleId :
JREG7

Tgt Ion:105 Resp: 72741
Ion Ratio Lower Upper
105 100
77 77.1 59.4 89.2
51 26.8 19.2 28.8

