

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP05158.D
 Acq On : 18 May 2023 22:15
 Operator : CG/JU
 Sample : 02612-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG6

Quant Time: May 19 01:35:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	286776	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1263812	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	805291	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1792144	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1590525	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1693695	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	9939	1.347	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.275	99	327450	12.298	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	216919	14.106	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	253564	12.952	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	240012	11.312	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	121874	12.272	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	126984	11.492	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	245949	12.335	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	358047	12.136	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	957945	15.742	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1044763	15.012	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	102528	8.677	ng/ul	0.00
60) Fluorene-d10	15.751	176	817706	15.925	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	81346	7.202	ng/ul	0.00
73) Anthracene-d10	17.616	188	1280999	15.610	ng/ul	0.00
81) Pyrene-d10	19.833	212	1605021	17.399	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1422542	16.920	ng/ul	-0.01


Target Compounds					Qvalue
16) Acetophenone	8.957	105	69174	2.089 ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015158.D
Acq On : 18 May 2023 22:15
Operator : CG/JU
Sample : 02612-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG6

Quant Time: May 19 01:35:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

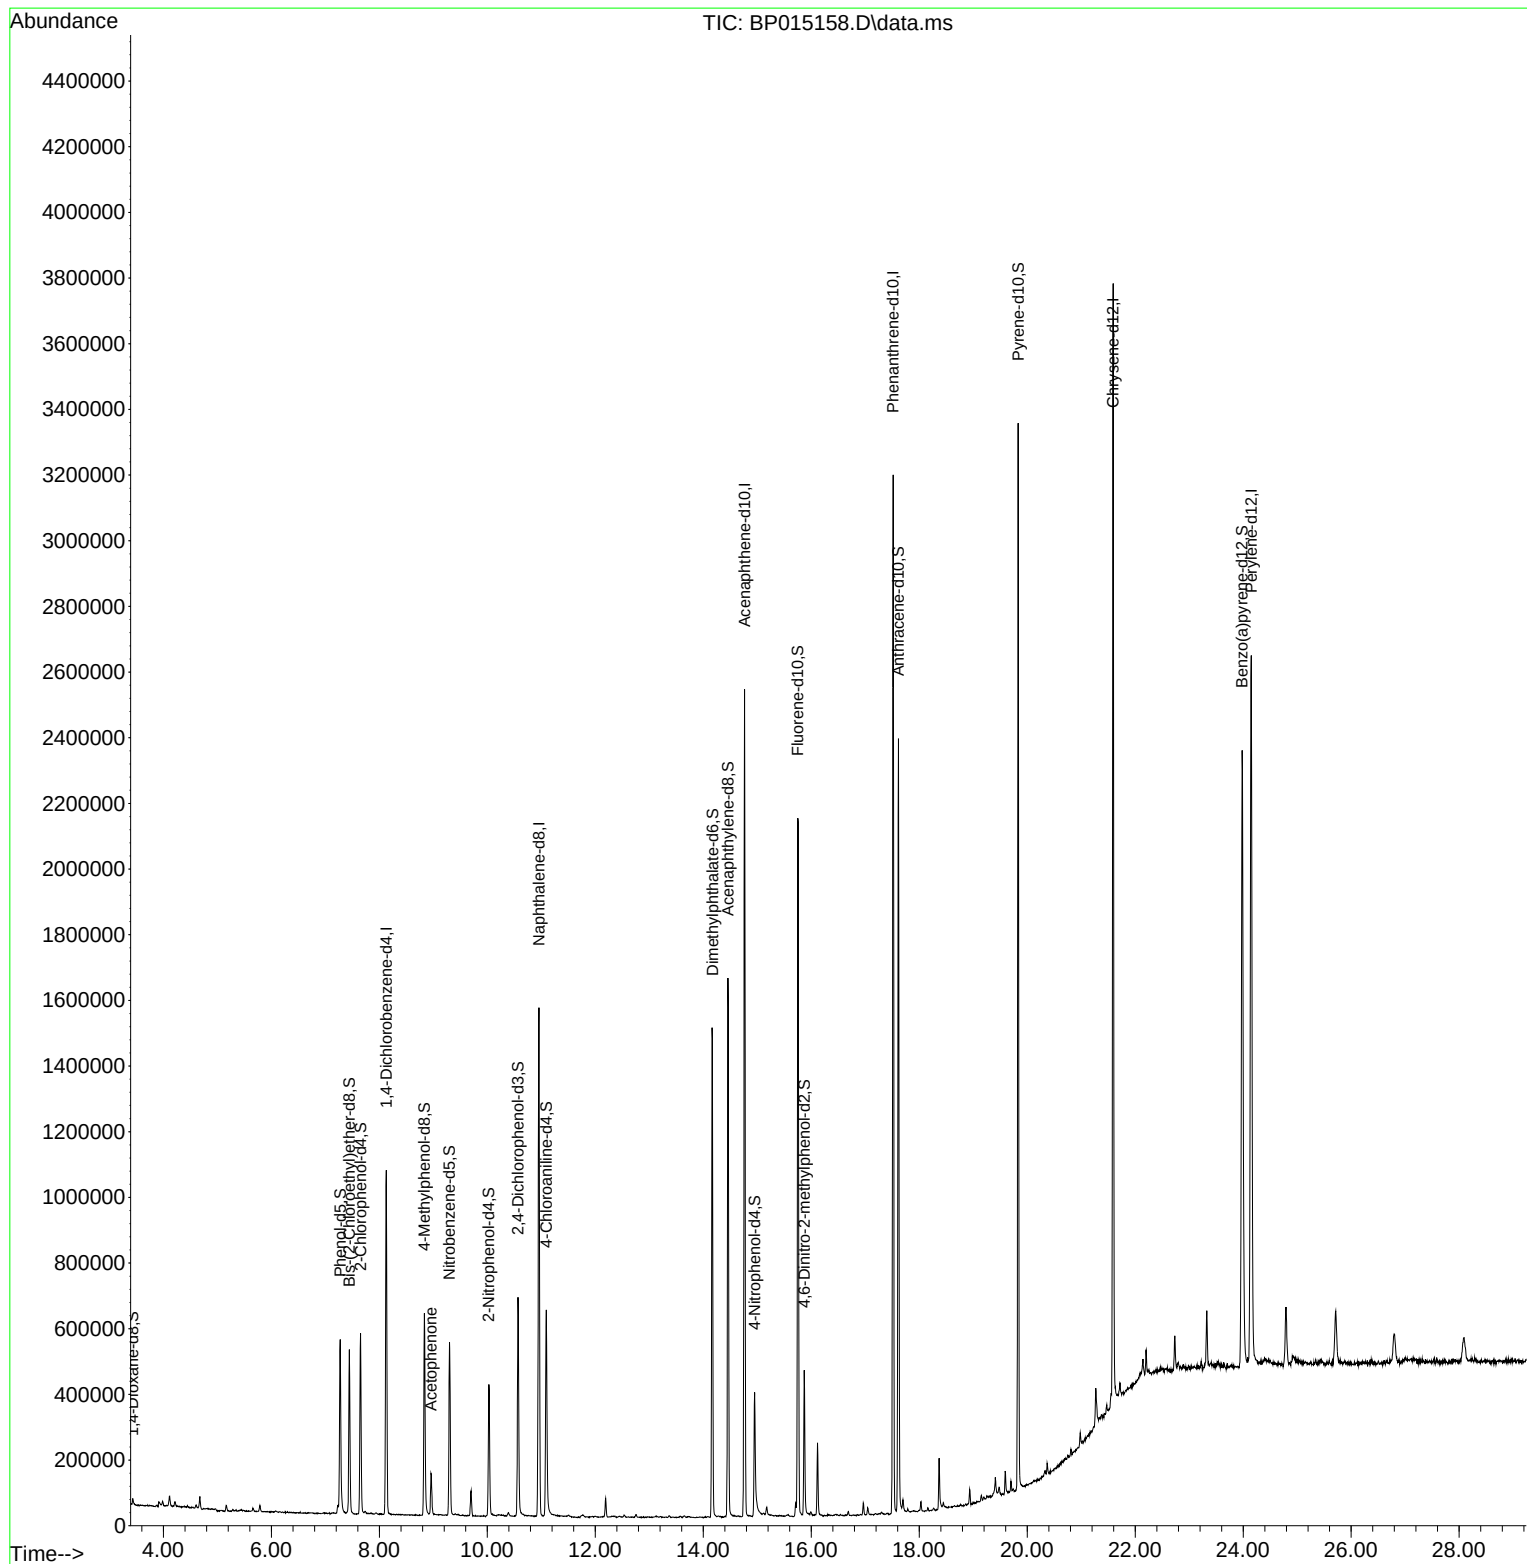

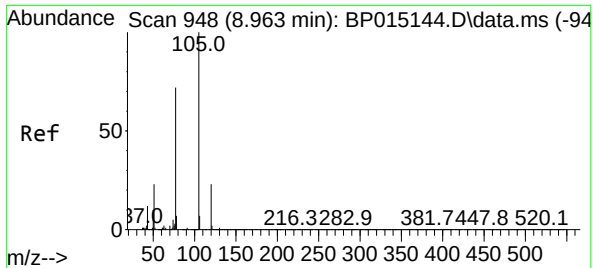

#16
 Acetophenone
 Concen: 2.089 ng/ul
 RT: 8.957 min Scan# 94
 Delta R.T. -0.006 min
 Lab File: BP015158.D
 Acq: 18 May 2023 22:15

Instrument :
 BNA_P
 ClientSampleId :
 JREG6

Tgt Ion:	105	Resp:	69174
Ion	Ratio	Lower	Upper
105	100		
77	76.7	59.4	89.2
51	29.7	19.2	28.8#

