

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015161.D
 Acq On : 18 May 2023 23:56
 Operator : CG/JU
 Sample : 02612-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH1

Quant Time: May 19 01:39:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	304876	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1369664	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	872575	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1916503	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1650916	20.000	ng/ul	-0.01
88) Perylene-d12	24.145	264	1635665	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	17804	2.269	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.275	99	503189	17.776	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	333890	20.423	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	385829	18.538	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	397133	17.606	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	193138	17.945	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	209073	17.458	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	381857	17.671	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	521879	16.323	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	1423653	21.591	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1558672	20.669	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	190033	14.842	ng/ul	0.00
60) Fluorene-d10	15.751	176	1216501	21.865	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	149774	12.401	ng/ul	0.00
73) Anthracene-d10	17.616	188	1995338	22.737	ng/ul	0.00
81) Pyrene-d10	19.833	212	2469893	25.795	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1984531	24.441	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.299	94	32274	1.112	ng/ul#	88
16) Acetophenone	8.958	105	87273	2.479	ng/ul	93
18) 4-Methylphenol	8.893	108	166942	6.761	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP0515161.D
Acq On : 18 May 2023 23:56
Operator : CG/JU
Sample : 02612-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH1

Quant Time: May 19 01:39:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration




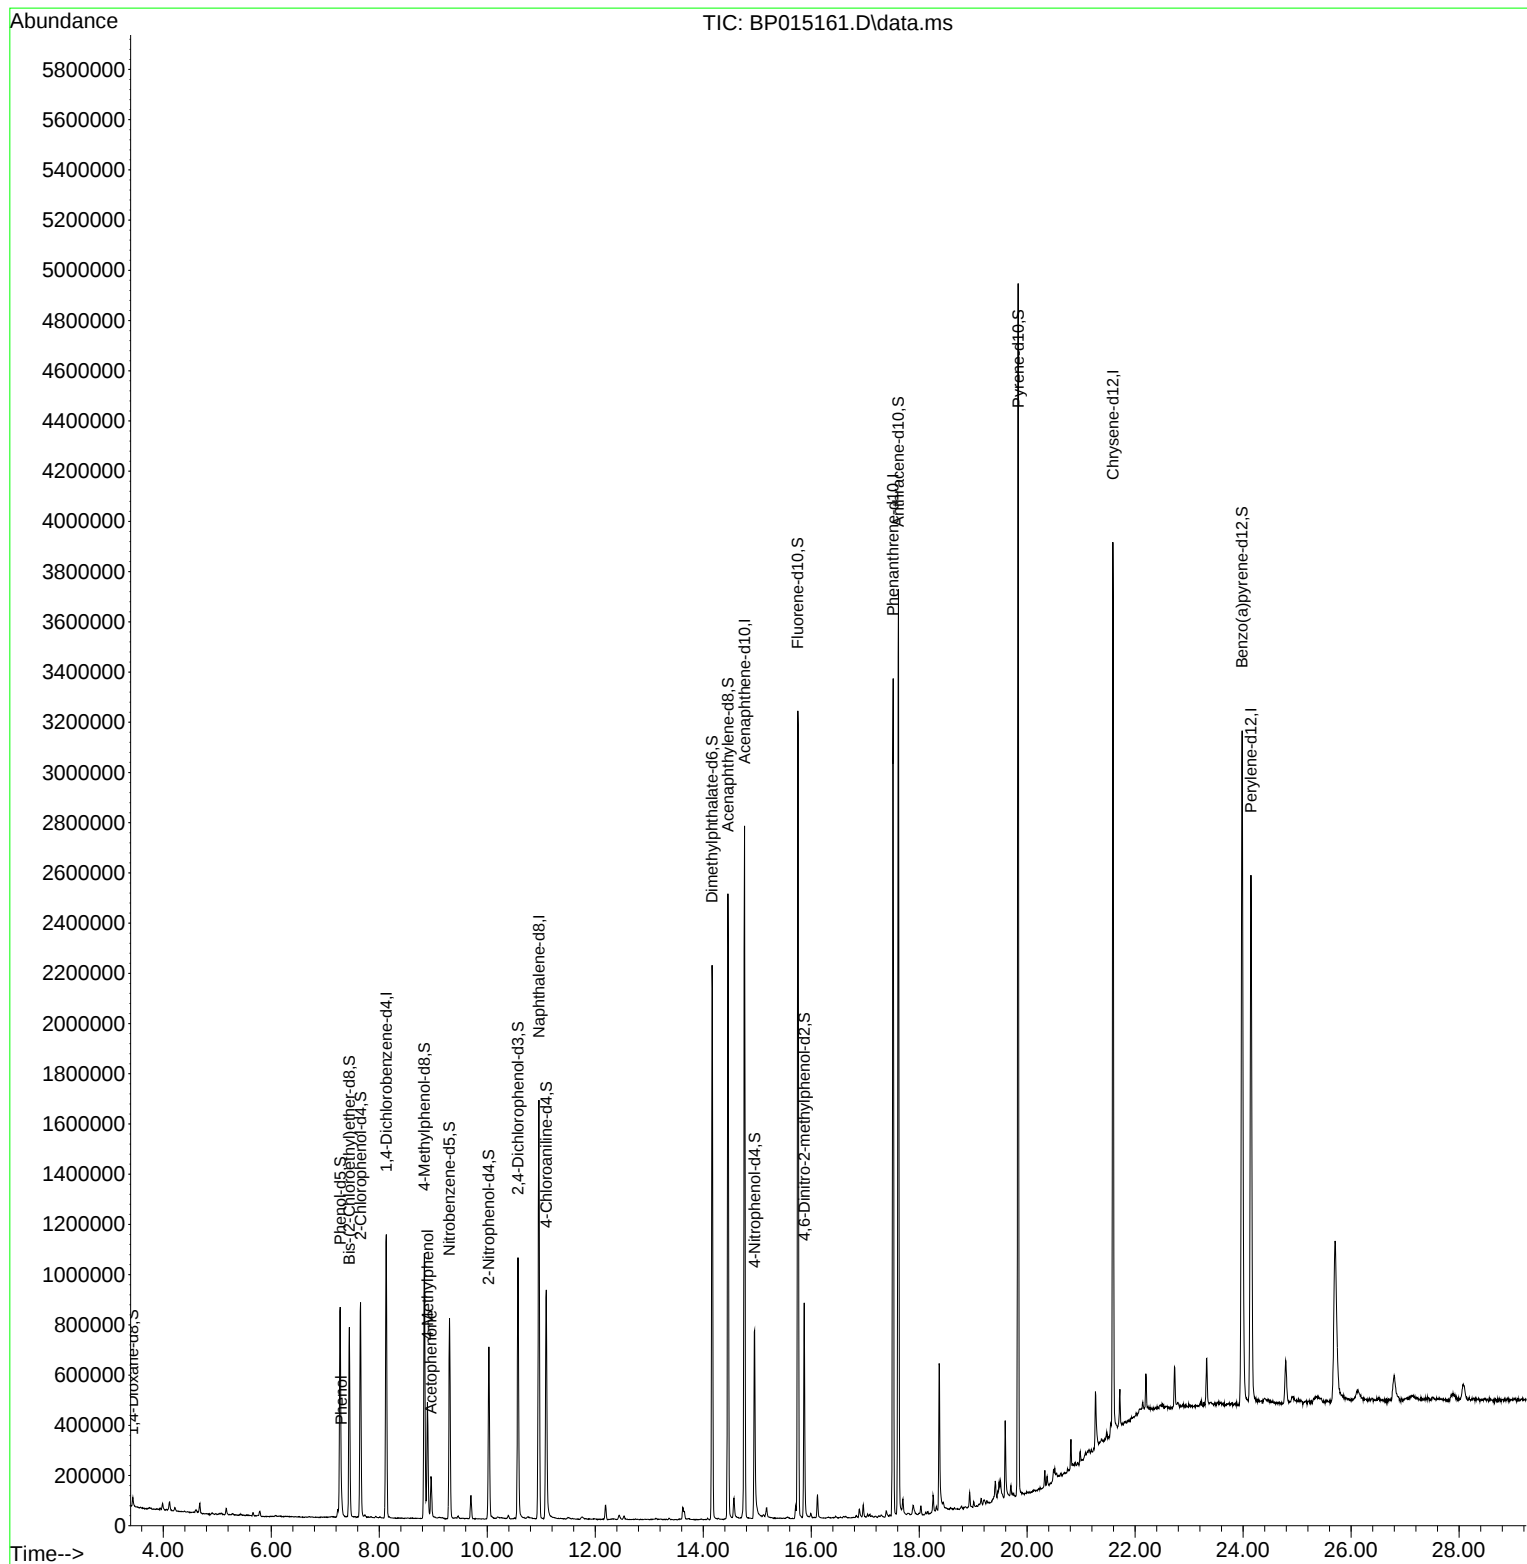


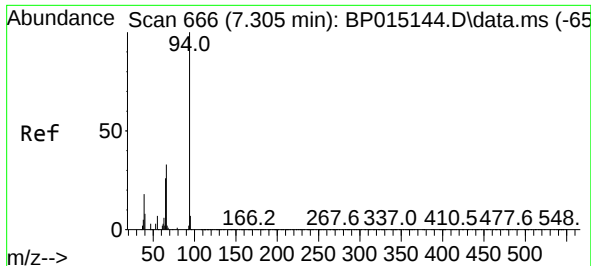

#8
Phenol
Concen: 1.112 ng/ul
RT: 7.299 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP015161.D
Acq: 18 May 2023 23:56




Instrument :
BNA_P
ClientSampleId :
JREH1


Tgt Ion: 94 Resp: 32274
Ion Ratio Lower Upper
94 100
65 29.2 20.6 31.0
66 41.5 26.1 39.1#

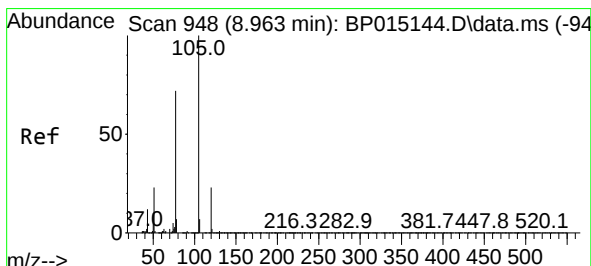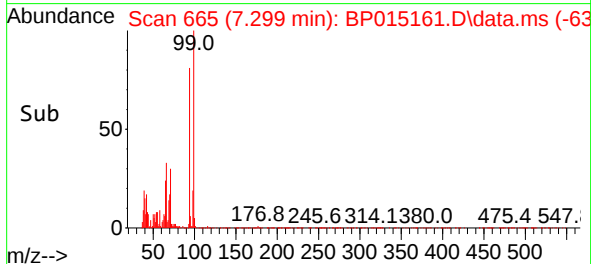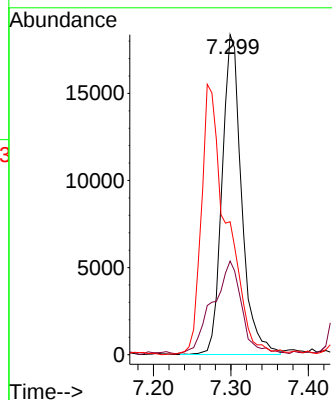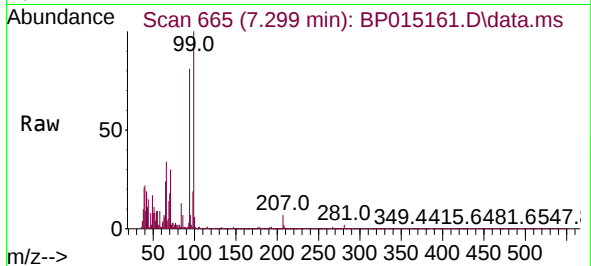

#16
Acetophenone
Concen: 2.479 ng/ul
RT: 8.958 min Scan# 947
Delta R.T. -0.006 min
Lab File: BP015161.D
Acq: 18 May 2023 23:56

Tgt Ion: 105 Resp: 87273
Ion Ratio Lower Upper
105 100
77 81.0 59.4 89.2
51 27.0 19.2 28.8

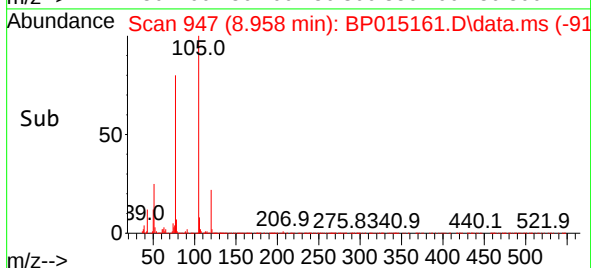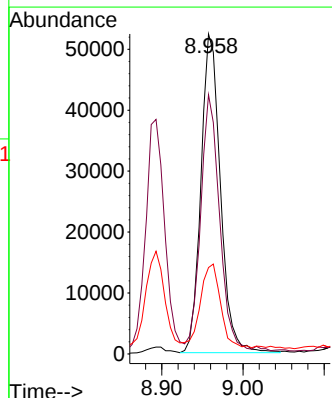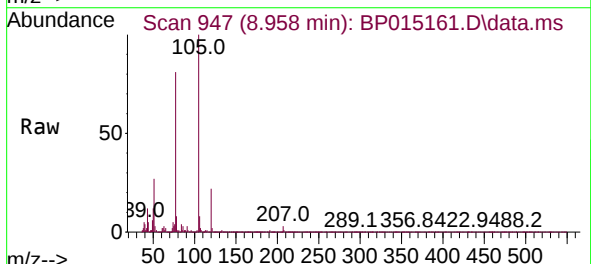

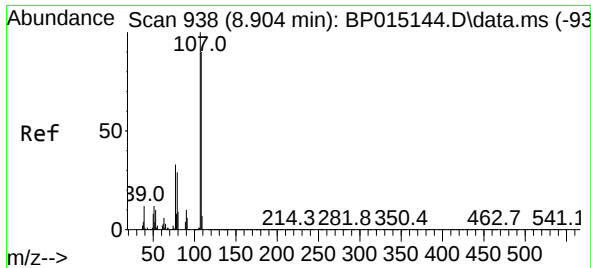

#18
 4-Methylphenol
 Concen: 6.761 ng/ul
 RT: 8.893 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BP015161.D
 Acq: 18 May 2023 23:56

Instrument :
 BNA_P
 ClientSampleId :
 JREH1

Tgt Ion:108 Resp: 166942
 Ion Ratio Lower Upper
 108 100
 107 124.2 88.5 132.7

