

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015137.D
 Acq On : 18 May 2023 10:33
 Operator : CG/JU
 Sample : PB152776BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK776

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	17	rVB	95765	136023	1.43%	0.141%
2	3.870	80	82	105	rBV	1295117	2013451	21.21%	2.095%
3	4.211	137	140	149	rVB	20924	33006	0.35%	0.034%
4	7.275	653	661	677	rBV	1439346	2312364	24.36%	2.405%
5	7.446	684	690	703	rVB	1264677	2041116	21.50%	2.123%
6	7.652	718	725	741	rBV	1544211	2470380	26.02%	2.570%
7	8.128	799	806	814	rBV	1180089	1907217	20.09%	1.984%
8	8.840	919	927	946	rBV	1893058	3221855	33.94%	3.352%
9	9.305	998	1006	1015	rBV	1570497	2520350	26.55%	2.622%
10	10.034	1121	1130	1144	rBV	1237136	2029737	21.38%	2.111%
11	10.575	1214	1222	1241	rBV	1737235	2993992	31.54%	3.115%
12	10.957	1278	1287	1300	rBV	1724182	2901892	30.57%	3.019%
13	11.093	1301	1310	1335	rBV	1931174	3437375	36.21%	3.576%
14	12.546	1549	1557	1566	rBV2	22055	54226	0.57%	0.056%
15	13.657	1739	1746	1751	rBV6	8253	16369	0.17%	0.017%
16	13.751	1756	1762	1768	rVB8	5784	12898	0.14%	0.013%
17	14.169	1824	1833	1848	rBV	3749120	5251711	55.32%	5.463%
18	14.463	1873	1883	1906	rBV	4285062	6367992	67.08%	6.624%
19	14.769	1928	1935	1944	rBV	2810718	4174411	43.97%	4.342%
20	14.957	1959	1967	1989	rBV	1519897	2505486	26.39%	2.606%
21	15.175	2001	2004	2008	rVB5	6936	9722	0.10%	0.010%
22	15.757	2096	2103	2117	rBV	4969580	7449847	78.48%	7.750%
23	15.875	2117	2123	2139	rVV	1582692	2262663	23.84%	2.354%
24	15.998	2140	2144	2150	rVB	26335	43279	0.46%	0.045%
25	16.545	2231	2237	2243	rBV9	6747	16311	0.17%	0.017%
26	17.198	2343	2348	2353	rBV8	7386	13260	0.14%	0.014%
27	17.310	2361	2367	2371	rBV4	8651	14054	0.15%	0.015%
28	17.522	2396	2403	2413	rBV	3625949	4979745	52.46%	5.180%
29	17.622	2413	2420	2432	rBV	5869219	8337121	87.83%	8.673%
30	19.416	2721	2725	2731	rBV2	61317	91243	0.96%	0.095%
31	19.486	2733	2737	2745	rVV	58491	91992	0.97%	0.096%
32	19.839	2791	2797	2812	rBV	7510383	9492762	100.00%	9.875%
33	21.598	3091	3096	3107	rBV	3460272	4754528	50.09%	4.946%
34	23.998	3496	3504	3521	rVB2	3740469	7840416	82.59%	8.156%
35	24.163	3525	3532	3545	rVB	2047873	4330800	45.62%	4.505%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015137.D
Acq On : 18 May 2023 10:33
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 96129594

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015137.D
Acq On : 18 May 2023 10:33
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

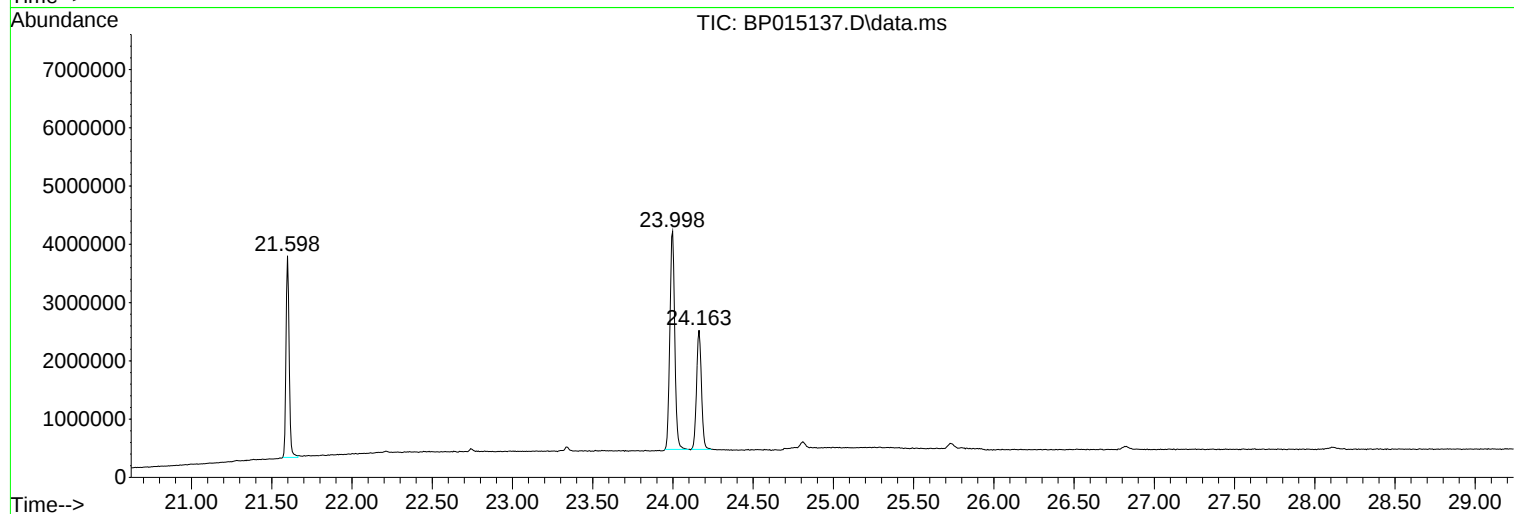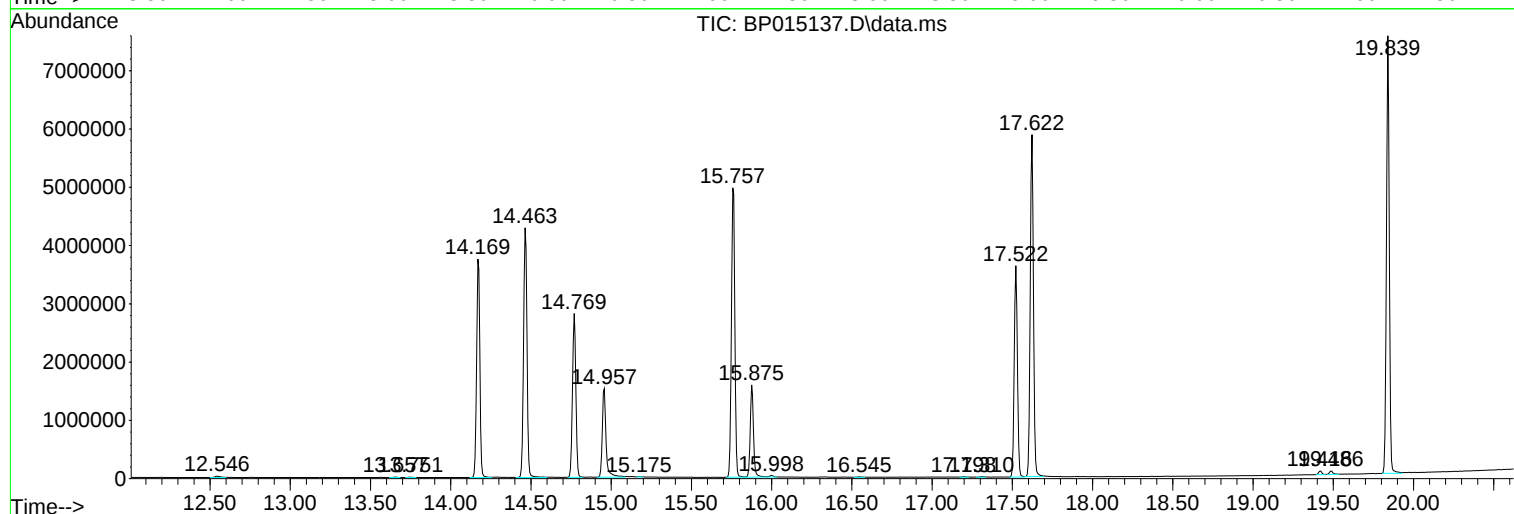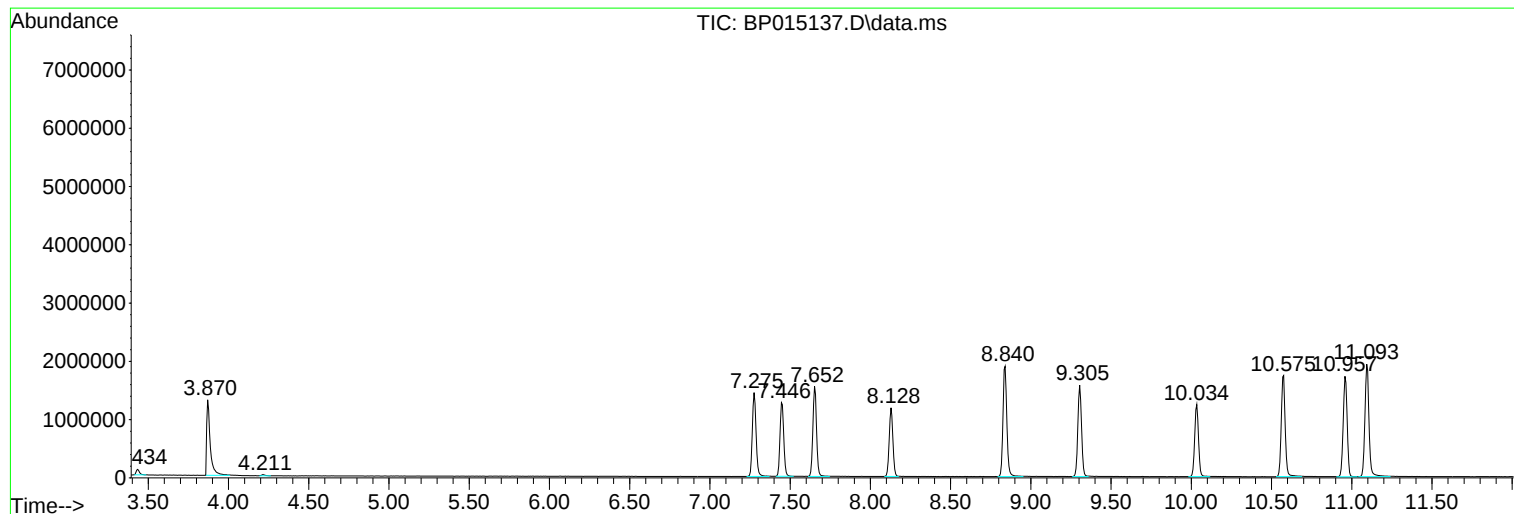

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015137.D
Acq On : 18 May 2023 10:33
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015137.D
Acq On : 18 May 2023 10:33
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------