

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015145.D
 Acq On : 18 May 2023 15:00
 Operator : CG/JU
 Sample : PB152776BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK776

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rVB	91819	130188	1.39%	0.137%
2	3.869	79	82	106	rBV	1226483	1956092	20.96%	2.059%
3	4.216	137	141	148	rVB	21244	32761	0.35%	0.034%
4	7.275	654	661	681	rBV	1481212	2338620	25.06%	2.462%
5	7.446	684	690	703	rVB	1292268	2029715	21.75%	2.137%
6	7.651	717	725	737	rBV	1488819	2388552	25.59%	2.515%
7	8.128	798	806	814	rBV	991822	1571248	16.83%	1.654%
8	8.834	918	926	941	rBV	1595886	2693872	28.86%	2.836%
9	9.304	998	1006	1018	rBV	1375137	2239008	23.99%	2.357%
10	10.034	1120	1130	1140	rBV	1179454	1987631	21.30%	2.093%
11	10.569	1213	1221	1238	rBV	1784971	3094752	33.16%	3.258%
12	10.957	1278	1287	1297	rBV	1764604	2912259	31.20%	3.066%
13	11.092	1301	1310	1323	rBV	1921290	3356604	35.96%	3.534%
14	12.539	1550	1556	1569	rVB	22603	51007	0.55%	0.054%
15	13.651	1738	1745	1751	rBV10	8788	17153	0.18%	0.018%
16	14.169	1827	1833	1844	rBV	3718914	5085578	54.49%	5.354%
17	14.463	1876	1883	1897	rBV	4053732	6031311	64.62%	6.350%
18	14.769	1928	1935	1944	rBV	2735693	4033684	43.22%	4.247%
19	14.951	1959	1966	1993	rBV	1552263	2482404	26.60%	2.613%
20	15.757	2096	2103	2116	rBV	5190930	7484649	80.19%	7.880%
21	15.875	2116	2123	2135	rVV	1754443	2310656	24.76%	2.433%
22	15.998	2139	2144	2152	rVB3	26700	45478	0.49%	0.048%
23	16.539	2232	2236	2242	rBV8	6012	10071	0.11%	0.011%
24	17.310	2362	2367	2370	rBV2	7569	11842	0.13%	0.012%
25	17.522	2396	2403	2412	rBV	3515422	4891158	52.40%	5.149%
26	17.621	2413	2420	2436	rVV2	5530895	8109163	86.88%	8.537%
27	19.416	2721	2725	2730	rBV2	66069	83765	0.90%	0.088%
28	19.480	2733	2736	2742	rVV	52630	75571	0.81%	0.080%
29	19.839	2791	2797	2811	rBV	7015778	9333599	100.00%	9.826%
30	21.592	3090	3095	3104	rBV	3340705	4781818	51.23%	5.034%
31	23.333	3388	3391	3399	rVB	165377	256072	2.74%	0.270%
32	23.992	3495	3503	3519	rVB2	3878934	8537465	91.47%	8.988%
33	24.156	3524	3531	3546	rVB	2213209	4624553	49.55%	4.869%




Sum of corrected areas: 94988299

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015145.D
Acq On : 18 May 2023 15:00
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

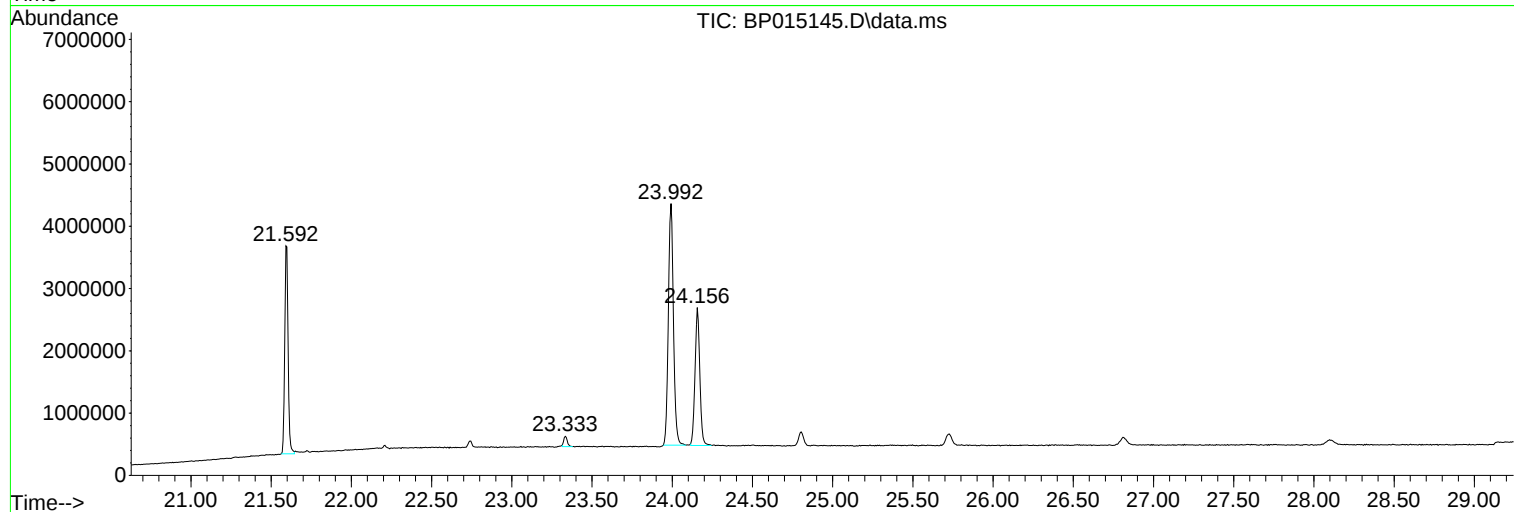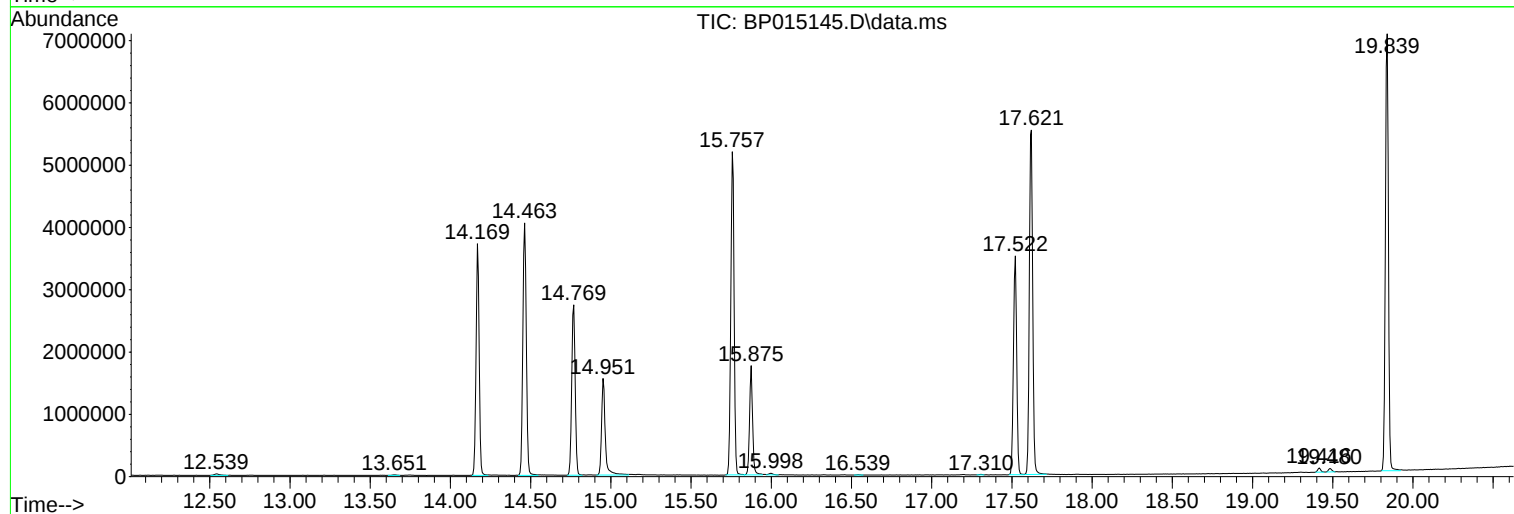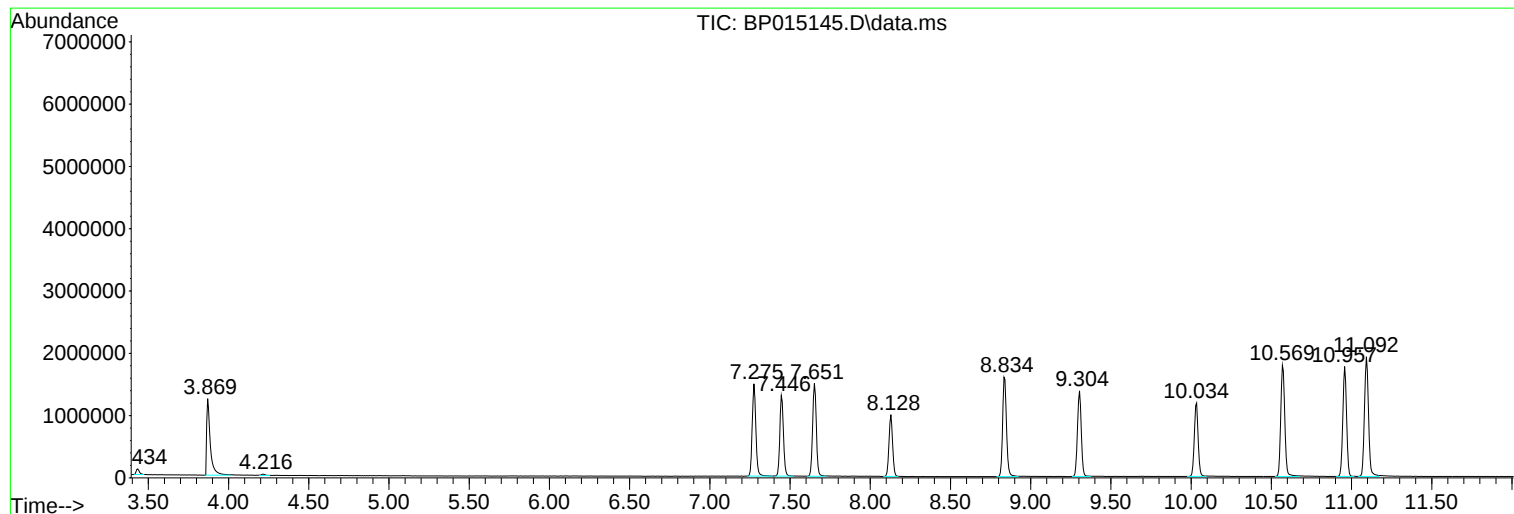

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015145.D
Acq On : 18 May 2023 15:00
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015145.D
Acq On : 18 May 2023 15:00
Operator : CG/JU
Sample : PB152776BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK776

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------