

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015151.D
 Acq On : 18 May 2023 18:22
 Operator : CG/JU
 Sample : 02612-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rVB	54044	73343	0.82%	0.078%
2	3.875	80	83	99	rBV	685235	1064196	11.84%	1.127%
3	3.981	99	101	110	rVB2	27204	39886	0.44%	0.042%
4	4.116	119	124	128	rVB2	37574	55838	0.62%	0.059%
5	4.216	137	141	147	rVB	21222	33538	0.37%	0.036%
6	4.605	203	207	213	rVV5	12943	22281	0.25%	0.024%
7	4.675	214	219	226	rVB	51465	72665	0.81%	0.077%
8	4.975	265	270	276	rVB6	6993	14580	0.16%	0.015%
9	5.169	298	303	311	rBV2	30992	65707	0.73%	0.070%
10	5.663	382	387	394	rBV	16145	23457	0.26%	0.025%
11	5.787	403	408	413	rBV	28593	41304	0.46%	0.044%
12	7.234	646	654	655	rBV	39027	53933	0.60%	0.057%
13	7.275	655	661	680	rVV	1309606	2171307	24.16%	2.300%
14	7.446	684	690	701	rVB	1184309	1808317	20.12%	1.915%
15	7.652	717	725	736	rBV	1351608	2139342	23.80%	2.266%
16	7.734	736	739	744	rVB5	9117	15399	0.17%	0.016%
17	7.940	769	774	780	rVB3	5949	12436	0.14%	0.013%
18	8.128	797	806	815	rBV	1301573	2069768	23.03%	2.192%
19	8.834	919	926	942	rBV	1554214	2595685	28.88%	2.749%
20	8.963	942	948	955	rVV	191065	313317	3.49%	0.332%
21	9.304	998	1006	1016	rBV	1337328	2170362	24.15%	2.299%
22	9.463	1028	1033	1037	rVB6	7625	13198	0.15%	0.014%
23	9.699	1064	1073	1080	rVB	119547	185726	2.07%	0.197%
24	10.028	1117	1129	1147	rBV	1095151	1888069	21.01%	2.000%
25	10.181	1149	1155	1156	rBV6	8166	9677	0.11%	0.010%
26	10.393	1185	1191	1196	rBV2	17318	28378	0.32%	0.030%
27	10.569	1214	1221	1238	rBV	1650497	2810531	31.27%	2.977%
28	10.957	1279	1287	1295	rBV	1957680	3275896	36.44%	3.470%
29	11.093	1303	1310	1329	rBV	1575015	2806335	31.22%	2.972%
30	11.493	1373	1378	1388	rBV	10143	25205	0.28%	0.027%
31	11.757	1416	1423	1431	rBV5	11668	35620	0.40%	0.038%
32	12.193	1492	1497	1504	rVB	77263	111595	1.24%	0.118%
33	12.440	1536	1539	1547	rVB5	6842	11479	0.13%	0.012%
34	12.534	1550	1555	1564	rVB4	18942	33398	0.37%	0.035%
35	13.645	1738	1744	1752	rVB4	13664	25692	0.29%	0.027%
36	13.734	1752	1759	1766	rVB10	5477	14780	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015151.D
 Acq On : 18 May 2023 18:22
 Operator : CG/JU
 Sample : 02612-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.081	1814	1818	1824	rVB6	9222	17094	0.19%	0.018%
38	14.169	1824	1833	1847	rBV	3400761	4801068	53.41%	5.085%
39	14.287	1849	1853	1857	rVB6	6783	10060	0.11%	0.011%
40	14.463	1873	1883	1894	rBV	3826043	5708288	63.51%	6.046%
41	14.769	1927	1935	1942	rBV	2976644	4472890	49.76%	4.738%
42	14.951	1959	1966	1983	rBV	1284593	2079544	23.14%	2.203%
43	15.122	1991	1995	1999	rVV6	7136	11711	0.13%	0.012%
44	15.175	1999	2004	2013	rVB3	63433	104278	1.16%	0.110%
45	15.575	2070	2072	2078	rVB6	6509	10332	0.11%	0.011%
46	15.716	2090	2096	2097	rBV	61019	76290	0.85%	0.081%
47	15.757	2097	2103	2116	rVV	4939052	7031021	78.22%	7.447%
48	15.869	2116	2122	2133	rVV	1340229	1855612	20.64%	1.965%
49	15.992	2139	2143	2149	rVB4	23311	36619	0.41%	0.039%
50	16.116	2159	2164	2174	rBV	159440	233786	2.60%	0.248%
51	16.451	2217	2221	2229	rVB	5294	13009	0.14%	0.014%
52	16.904	2294	2298	2303	rBV8	6380	11720	0.13%	0.012%
53	16.963	2303	2308	2316	rVB2	49993	74016	0.82%	0.078%
54	17.045	2316	2322	2328	rBV2	24182	35927	0.40%	0.038%
55	17.192	2342	2347	2352	rBV9	6897	10143	0.11%	0.011%
56	17.310	2363	2367	2373	rVB4	9533	17503	0.19%	0.019%
57	17.416	2379	2385	2389	rBV9	6548	11965	0.13%	0.013%
58	17.516	2396	2402	2412	rBV	3693041	5355814	59.58%	5.673%
59	17.616	2412	2419	2429	rVV2	5397024	7679575	85.44%	8.134%
60	17.698	2429	2433	2444	rVV4	78509	141471	1.57%	0.150%
61	18.033	2486	2490	2494	rVB	44754	56033	0.62%	0.059%
62	18.163	2508	2512	2516	rVB7	9404	14259	0.16%	0.015%
63	18.369	2543	2547	2557	rBV	230038	346499	3.85%	0.367%
64	18.445	2558	2560	2566	rVB	22813	30142	0.34%	0.032%
65	18.933	2639	2643	2649	rVB	67180	90206	1.00%	0.096%
66	19.151	2676	2680	2684	rBV	32358	39797	0.44%	0.042%
67	19.410	2721	2724	2729	rVB2	83367	116611	1.30%	0.124%
68	19.480	2733	2736	2741	rVB	54522	71193	0.79%	0.075%
69	19.592	2752	2755	2761	rBV3	70892	104236	1.16%	0.110%
70	19.698	2770	2773	2778	rBV2	46328	58059	0.65%	0.061%
71	19.833	2790	2796	2806	rBV	6708174	8988642	100.00%	9.521%
72	20.374	2885	2888	2891	rVB	55103	56392	0.63%	0.060%
73	20.816	2960	2963	2966	rBV	59803	62812	0.70%	0.067%
74	20.980	2989	2991	2997	rVB	60433	70054	0.78%	0.074%
75	21.274	3036	3041	3052	rBV2	275564	612606	6.82%	0.649%
76	21.592	3090	3095	3104	rVB	3773812	5122011	56.98%	5.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015151.D
Acq On : 18 May 2023 18:22
Operator : CG/JU
Sample : 02612-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

77	22.733	3287	3289	3295	rVB	172476	221223	2.46%	0.234%
78	23.333	3388	3391	3396	rVB	217550	304524	3.39%	0.323%
79	23.986	3494	3502	3516	rBV2	3395422	7550304	84.00%	7.997%
80	24.151	3523	3530	3543	rVB	2071279	4563095	50.77%	4.833%




Sum of corrected areas: 94410674

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015151.D
Acq On : 18 May 2023 18:22
Operator : CG/JU
Sample : 02612-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

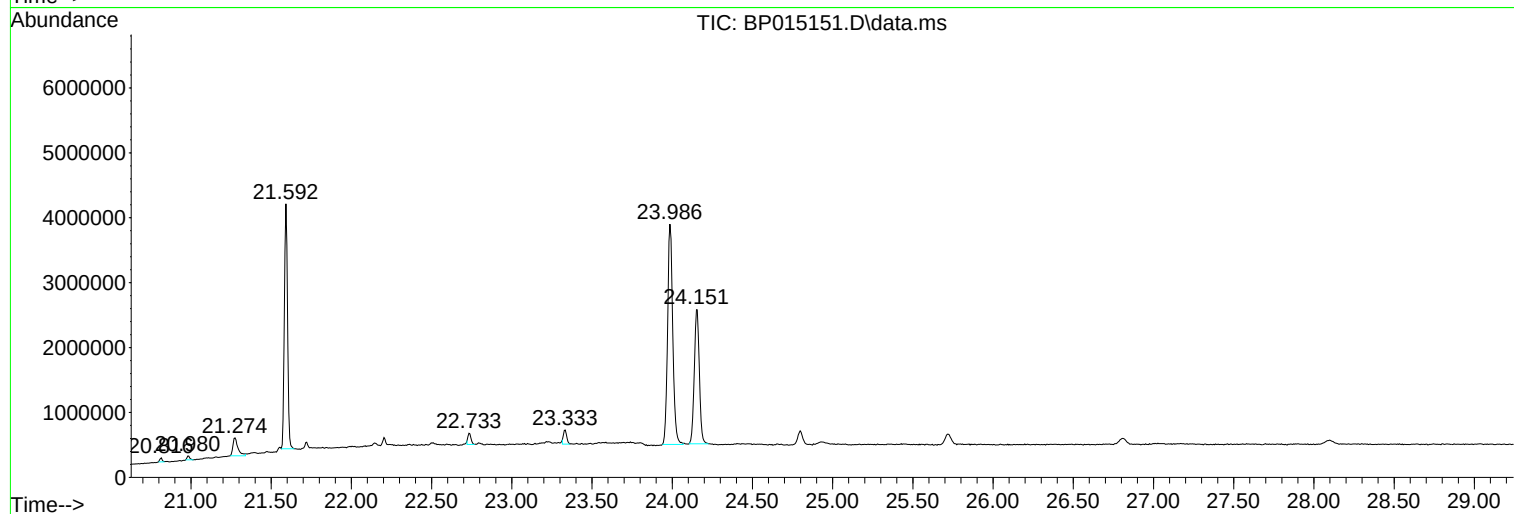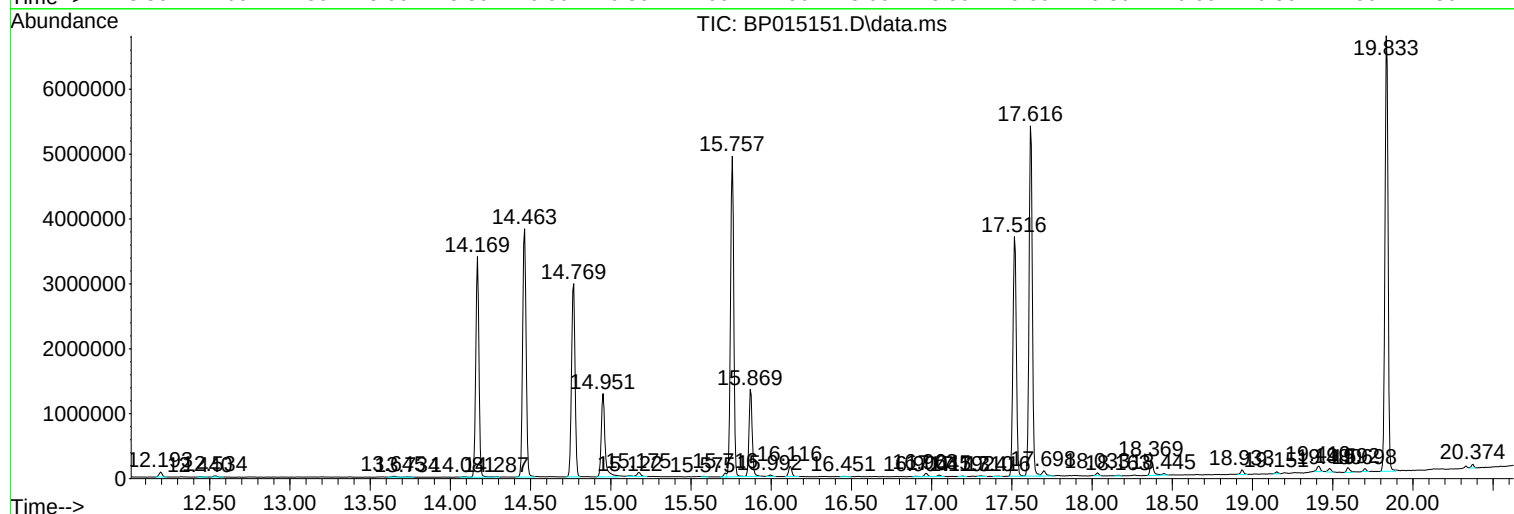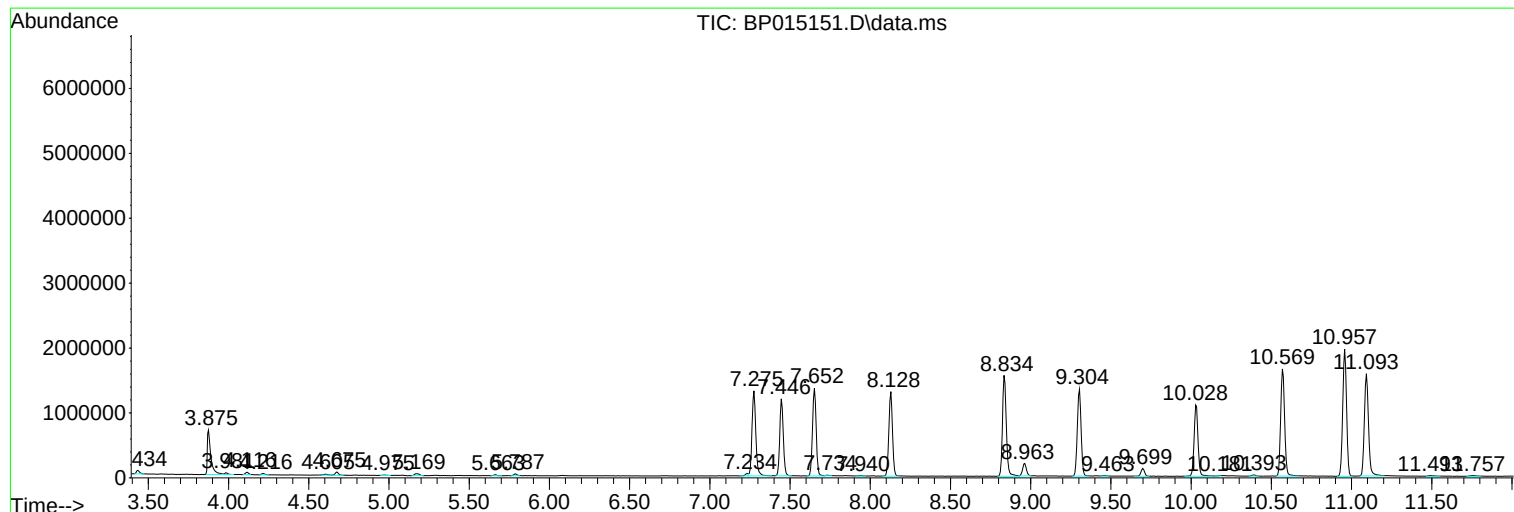

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP05151.D
Acq On : 18 May 2023 18:22
Operator : CG/JU
Sample : 02612-14
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
JREH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.274	2.39 ng/ul	612606	Chrysene-d12	21.592	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Heptadecene	238	C17H34	006765-39-5	94
2	Cyclotetracosane	336	C24H48	000297-03-0	94
3	9-Eicosene, (E)-	280	C20H40	074685-29-3	93
4	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	93
5	Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	93

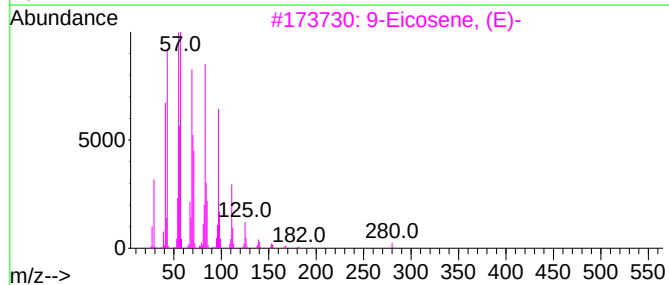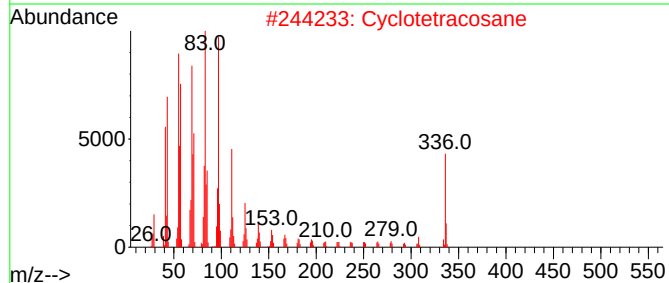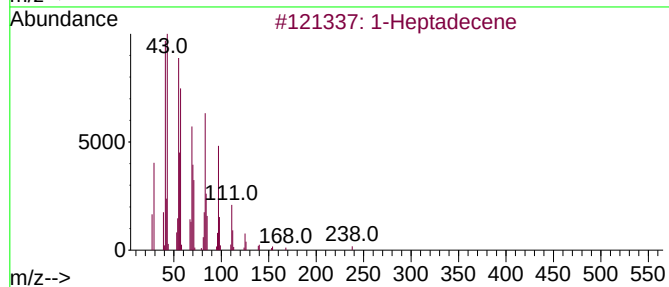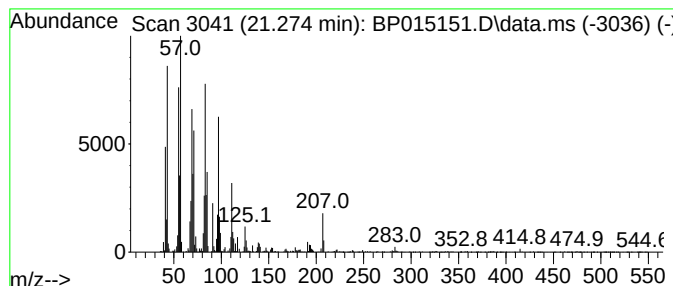

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015151.D
Acq On : 18 May 2023 18:22
Operator : CG/JU
Sample : 02612-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.274	2.4	ng/u1	612606	5	21.592	5122010	20.0