

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015156.D
 Acq On : 18 May 2023 21:09
 Operator : CG/JU
 Sample : 02612-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	13	rVB	32218	45100	0.66%	0.063%
2	3.911	87	89	99	rBV2	17839	42037	0.62%	0.059%
3	4.117	119	124	130	rVB	30832	52288	0.77%	0.073%
4	4.217	137	141	145	rVB	16314	23260	0.34%	0.032%
5	4.605	202	207	211	rBV5	12826	18274	0.27%	0.025%
6	4.675	214	219	224	rVB	39059	57487	0.85%	0.080%
7	5.164	298	302	309	rVB	19063	28612	0.42%	0.040%
8	5.287	321	323	327	rVB5	5393	6882	0.10%	0.010%
9	5.664	382	387	391	rBV	9202	12790	0.19%	0.018%
10	5.787	402	408	413	rBV	19838	29911	0.44%	0.042%
11	7.234	649	654	655	rBV	25825	32432	0.48%	0.045%
12	7.275	655	661	673	rVB	893241	1469078	21.61%	2.046%
13	7.446	680	690	702	rVB	818680	1282715	18.87%	1.786%
14	7.652	717	725	734	rBV	939130	1478291	21.75%	2.058%
15	7.728	736	738	747	rVB6	8683	15555	0.23%	0.022%
16	7.852	754	759	768	rVB7	6288	13813	0.20%	0.019%
17	7.934	771	773	781	rVB5	7417	10467	0.15%	0.015%
18	8.128	798	806	814	rVB	972697	1561289	22.97%	2.174%
19	8.834	918	926	940	rBV	1009936	1680896	24.73%	2.341%
20	8.958	940	947	957	rVB	129941	221992	3.27%	0.309%
21	9.299	998	1005	1016	rBV	776706	1315676	19.36%	1.832%
22	9.458	1027	1032	1038	rVB10	6903	11600	0.17%	0.016%
23	9.699	1066	1073	1079	rBV	85333	122782	1.81%	0.171%
24	10.028	1119	1129	1144	rBV	684659	1160557	17.07%	1.616%
25	10.205	1152	1159	1162	rBV8	5573	12974	0.19%	0.018%
26	10.387	1185	1190	1195	rBV4	12466	22076	0.32%	0.031%
27	10.569	1213	1221	1237	rBV	1142455	1951757	28.71%	2.718%
28	10.957	1279	1287	1296	rBV	1672325	2783604	40.95%	3.876%
29	11.093	1302	1310	1328	rBV	1037591	1897557	27.92%	2.642%
30	11.757	1416	1423	1425	rBV8	8047	16237	0.24%	0.023%
31	12.193	1492	1497	1503	rVB	57587	85075	1.25%	0.118%
32	12.434	1534	1538	1543	rBV4	8015	12856	0.19%	0.018%
33	12.534	1550	1555	1561	rBV3	13616	26494	0.39%	0.037%
34	13.369	1692	1697	1704	rVB7	9126	14466	0.21%	0.020%
35	13.651	1739	1745	1750	rBV6	7919	13825	0.20%	0.019%
36	13.734	1753	1759	1765	rVB9	4046	9780	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015156.D
 Acq On : 18 May 2023 21:09
 Operator : CG/JU
 Sample : 02612-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.087	1815	1819	1826	rBV9	6431	10753	0.16%	0.015%
38	14.169	1826	1833	1847	rVV	2353104	3378522	49.70%	4.705%
39	14.457	1873	1882	1893	rBV	2673179	3930377	57.82%	5.473%
40	14.763	1927	1934	1944	rBV	2599652	3834835	56.42%	5.340%
41	14.951	1958	1966	1985	rBV	758204	1338245	19.69%	1.863%
42	15.175	1998	2004	2014	rVB4	40521	72457	1.07%	0.101%
43	15.710	2091	2095	2097	rBV	45023	57939	0.85%	0.081%
44	15.757	2097	2103	2115	rVV	3381561	4964925	73.04%	6.914%
45	15.869	2116	2122	2135	rVV	895225	1241502	18.26%	1.729%
46	15.998	2139	2144	2150	rVB3	16176	29408	0.43%	0.041%
47	16.116	2159	2164	2174	rVB	94706	133356	1.96%	0.186%
48	16.451	2218	2221	2229	rBV10	4714	10155	0.15%	0.014%
49	16.534	2233	2235	2241	rVB6	4349	7231	0.11%	0.010%
50	16.963	2304	2308	2314	rVB2	36058	47296	0.70%	0.066%
51	17.045	2319	2322	2326	rVB6	6948	8909	0.13%	0.012%
52	17.192	2341	2347	2350	rBV8	7552	12341	0.18%	0.017%
53	17.251	2355	2357	2362	rVV6	6314	10286	0.15%	0.014%
54	17.304	2362	2366	2372	rVB5	9669	16246	0.24%	0.023%
55	17.516	2396	2402	2412	rBV	3424285	4654253	68.47%	6.481%
56	17.616	2412	2419	2428	rVV	3837489	5390324	79.30%	7.506%
57	17.698	2430	2433	2442	rVB4	49956	83303	1.23%	0.116%
58	17.898	2463	2467	2471	rBV7	4286	7149	0.11%	0.010%
59	18.034	2486	2490	2497	rVB3	30810	39061	0.57%	0.054%
60	18.157	2508	2511	2515	rBV5	11833	14856	0.22%	0.021%
61	18.369	2542	2547	2557	rBV2	219965	335385	4.93%	0.467%
62	18.445	2557	2560	2564	rVB	23994	32895	0.48%	0.046%
63	18.934	2640	2643	2649	rVB2	49706	62635	0.92%	0.087%
64	19.151	2676	2680	2684	rBV2	24244	32235	0.47%	0.045%
65	19.410	2720	2724	2730	rVB4	58285	81809	1.20%	0.114%
66	19.592	2751	2755	2763	rBV	119427	176691	2.60%	0.246%
67	19.698	2770	2773	2778	rVB2	26645	30381	0.45%	0.042%
68	19.833	2790	2796	2809	rBV	5014878	6797397	100.00%	9.465%
69	20.328	2877	2880	2883	rBV	63638	70396	1.04%	0.098%
70	20.369	2885	2887	2892	rVB2	32747	35778	0.53%	0.050%
71	20.775	2952	2956	2959	rBV	142179	152612	2.25%	0.213%
72	20.810	2959	2962	2966	rBV	107565	118068	1.74%	0.164%
73	21.269	3036	3040	3048	rBV	167385	249934	3.68%	0.348%
74	21.592	3090	3095	3106	rVB	3626638	4725980	69.53%	6.581%
75	21.722	3114	3117	3121	rVB2	120400	134410	1.98%	0.187%
76	22.204	3196	3199	3205	rVB	157739	182612	2.69%	0.254%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015156.D
Acq On : 18 May 2023 21:09
Operator : CG/JU
Sample : 02612-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

77	22.733	3286	3289	3294	rVB2	164182	219950	3.24%	0.306%
78	23.327	3387	3390	3398	rVB	211546	333207	4.90%	0.464%
79	23.986	3494	3502	3518	rBV2	2852891	6437559	94.71%	8.964%
80	24.151	3523	3530	3548	rVB	2228545	4770309	70.18%	6.643%




Sum of corrected areas: 71814457

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015156.D
Acq On : 18 May 2023 21:09
Operator : CG/JU
Sample : 02612-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

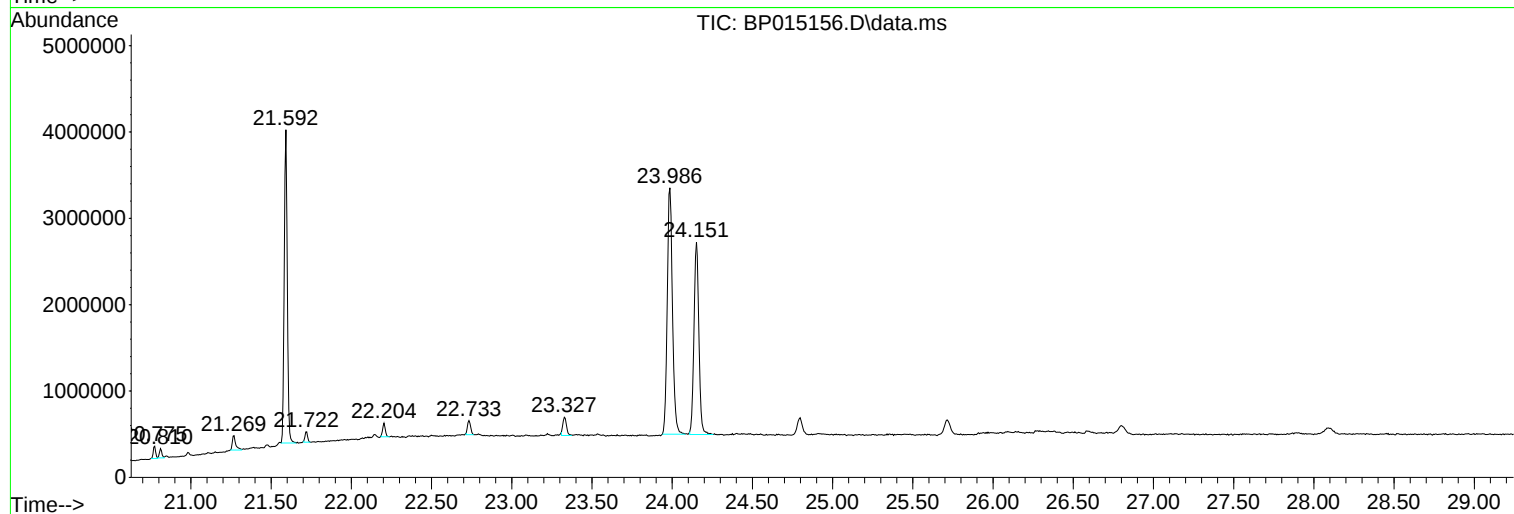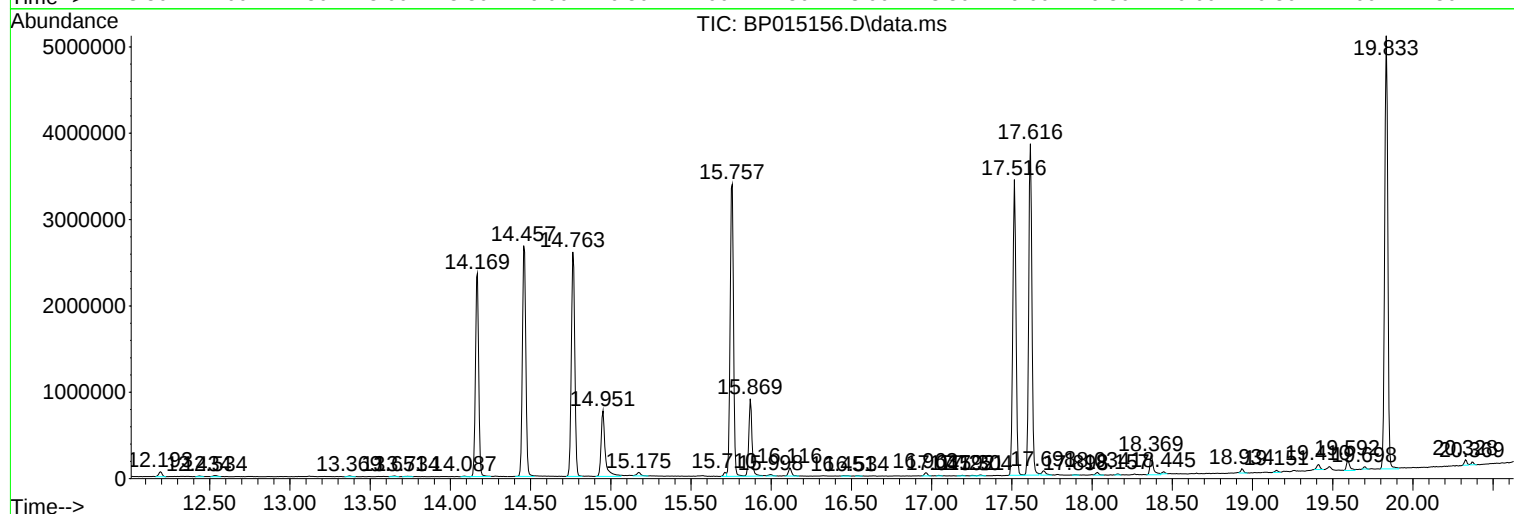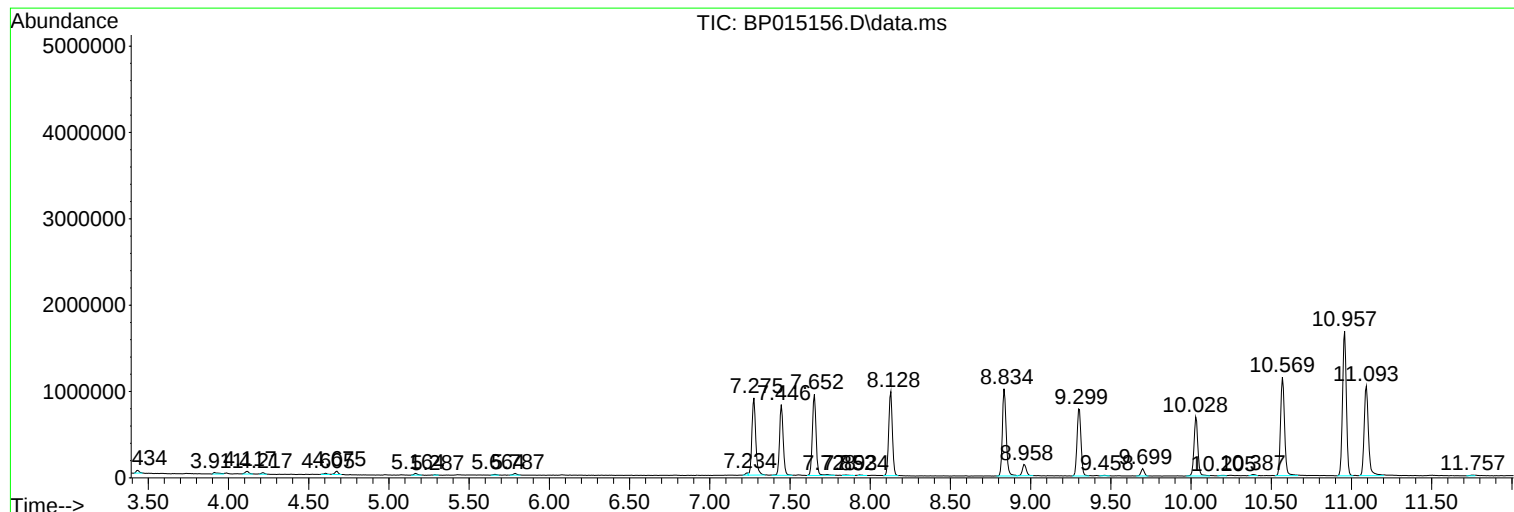

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015156.D
Acq On : 18 May 2023 21:09
Operator : CG/JU
Sample : 02612-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015156.D
Acq On : 18 May 2023 21:09
Operator : CG/JU
Sample : 02612-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc