

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015160.D
 Acq On : 18 May 2023 23:22
 Operator : CG/JU
 Sample : 02612-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	16	rVB	43742	65687	0.90%	0.095%
2	3.910	87	89	94	rBV	16716	21474	0.29%	0.031%
3	4.116	119	124	128	rVB	34168	51984	0.71%	0.075%
4	4.210	137	140	147	rVB2	17316	26611	0.36%	0.039%
5	4.446	178	180	185	rVB5	10566	13082	0.18%	0.019%
6	4.605	203	207	213	rVB7	11588	18678	0.26%	0.027%
7	4.675	215	219	224	rVB	40952	58066	0.79%	0.084%
8	5.169	298	303	309	rVB3	21147	35381	0.48%	0.051%
9	5.663	382	387	395	rVB	12679	19617	0.27%	0.028%
10	5.787	404	408	416	rVB	23672	34723	0.47%	0.050%
11	6.075	453	457	463	rVB5	8975	16220	0.22%	0.024%
12	7.234	649	654	655	rBV	30165	39589	0.54%	0.057%
13	7.275	655	661	675	rVB	852818	1454729	19.89%	2.109%
14	7.446	683	690	701	rBV	838682	1308899	17.90%	1.898%
15	7.651	718	725	736	rBV	1004039	1582239	21.64%	2.294%
16	7.734	737	739	744	rVB5	8368	10185	0.14%	0.015%
17	7.846	756	758	765	rVB6	6029	9560	0.13%	0.014%
18	8.128	799	806	814	rBV	1094574	1756916	24.02%	2.547%
19	8.834	919	926	938	rBV	1170099	1939479	26.52%	2.812%
20	8.957	941	947	960	rVB	246989	422171	5.77%	0.612%
21	9.304	998	1006	1016	rBV	984417	1655320	22.63%	2.400%
22	9.398	1019	1022	1028	rVV7	6794	14449	0.20%	0.021%
23	9.457	1029	1032	1038	rVB8	6843	10640	0.15%	0.015%
24	9.698	1067	1073	1079	rVB	104407	156545	2.14%	0.227%
25	10.028	1118	1129	1145	rBV	800698	1366036	18.68%	1.981%
26	10.198	1152	1158	1162	rBV5	5557	11947	0.16%	0.017%
27	10.393	1185	1191	1197	rVB	19177	34540	0.47%	0.050%
28	10.504	1206	1210	1214	rBV7	4707	9368	0.13%	0.014%
29	10.569	1214	1221	1241	rVV	1217196	2050980	28.05%	2.974%
30	10.957	1280	1287	1295	rBV	1599425	2687109	36.74%	3.896%
31	11.092	1302	1310	1324	rBV	1149040	2052881	28.07%	2.976%
32	11.504	1374	1380	1387	rBV	8258	22190	0.30%	0.032%
33	11.751	1415	1422	1423	rBV3	12260	18188	0.25%	0.026%
34	12.192	1491	1497	1503	rVB2	73076	105319	1.44%	0.153%
35	12.439	1534	1539	1545	rBV7	5471	10983	0.15%	0.016%
36	12.534	1550	1555	1560	rBV2	16631	27733	0.38%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
 Data File : BP015160.D
 Acq On : 18 May 2023 23:22
 Operator : CG/JU
 Sample : 02612-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	13.645	1738	1744	1752	rVB4	12329	21999	0.30%	0.032%
38	14.086	1814	1819	1822	rBV7	5769	7844	0.11%	0.011%
39	14.163	1826	1832	1846	rBV	1976018	2832244	38.73%	4.106%
40	14.457	1875	1882	1894	rBV	2158412	3193893	43.67%	4.631%

41	14.763	1927	1934	1947	rBV	1880438	2790589	38.16%	4.046%
42	14.951	1959	1966	1986	rBV	580094	1016682	13.90%	1.474%
43	15.175	1998	2004	2014	rVB3	39228	68290	0.93%	0.099%
44	15.575	2069	2072	2081	rVB7	5587	9907	0.14%	0.014%
45	15.710	2091	2095	2097	rBV2	51758	64719	0.88%	0.094%

46	15.757	2097	2103	2115	rVB	2851179	4164887	56.95%	6.038%
47	15.869	2115	2122	2131	rBV	773801	1048446	14.34%	1.520%
48	15.992	2139	2143	2149	rVB5	14391	24503	0.34%	0.036%
49	16.116	2158	2164	2174	rBV	116865	164931	2.26%	0.239%
50	16.533	2232	2235	2244	rVB	3959	9000	0.12%	0.013%

51	16.963	2303	2308	2312	rBV2	49882	63349	0.87%	0.092%
52	17.045	2318	2322	2330	rVB2	25074	37686	0.52%	0.055%
53	17.251	2353	2357	2361	rBV7	6691	11115	0.15%	0.016%
54	17.516	2395	2402	2412	rBV	2831213	4027627	55.07%	5.839%
55	17.616	2412	2419	2430	rVV	3833225	5460350	74.67%	7.917%

56	17.698	2430	2433	2444	rVV3	60200	102292	1.40%	0.148%
57	17.780	2445	2447	2452	rVB5	4796	8024	0.11%	0.012%
58	17.998	2480	2484	2486	rBV5	8579	12511	0.17%	0.018%
59	18.033	2486	2490	2497	rVB2	36293	50140	0.69%	0.073%
60	18.157	2509	2511	2515	rBV5	7941	9187	0.13%	0.013%

61	18.269	2526	2530	2534	rVB2	12703	17218	0.24%	0.025%
62	18.369	2542	2547	2556	rBV	189371	280269	3.83%	0.406%
63	18.445	2557	2560	2566	rVB	20065	28279	0.39%	0.041%
64	18.933	2639	2643	2648	rVB	67917	81875	1.12%	0.119%
65	19.151	2676	2680	2684	rBV	35397	46798	0.64%	0.068%

66	19.410	2720	2724	2730	rVB5	88219	138896	1.90%	0.201%
67	19.480	2733	2736	2743	rVB	52938	76077	1.04%	0.110%
68	19.592	2751	2755	2764	rBV2	80618	122848	1.68%	0.178%
69	19.698	2770	2773	2777	rVB2	37457	40526	0.55%	0.059%
70	19.833	2790	2796	2809	rBV	5418677	7096499	97.04%	10.289%

71	20.368	2884	2887	2893	rBV3	43343	53348	0.73%	0.077%
72	20.810	2959	2962	2966	rBV3	48827	61412	0.84%	0.089%
73	21.268	3036	3040	3049	rBV2	217236	430274	5.88%	0.624%
74	21.592	3090	3095	3107	rVB	3209478	4429871	60.57%	6.423%
75	23.980	3493	3501	3516	rBV2	3345057	7313130	100.00%	10.603%

76	24.145	3522	3529	3542	rVB	2032092	4435405	60.65%	6.431%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015160.D
Acq On : 18 May 2023 23:22
Operator : CG/JU
Sample : 02612-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 68972458

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015160.D
Acq On : 18 May 2023 23:22
Operator : CG/JU
Sample : 02612-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

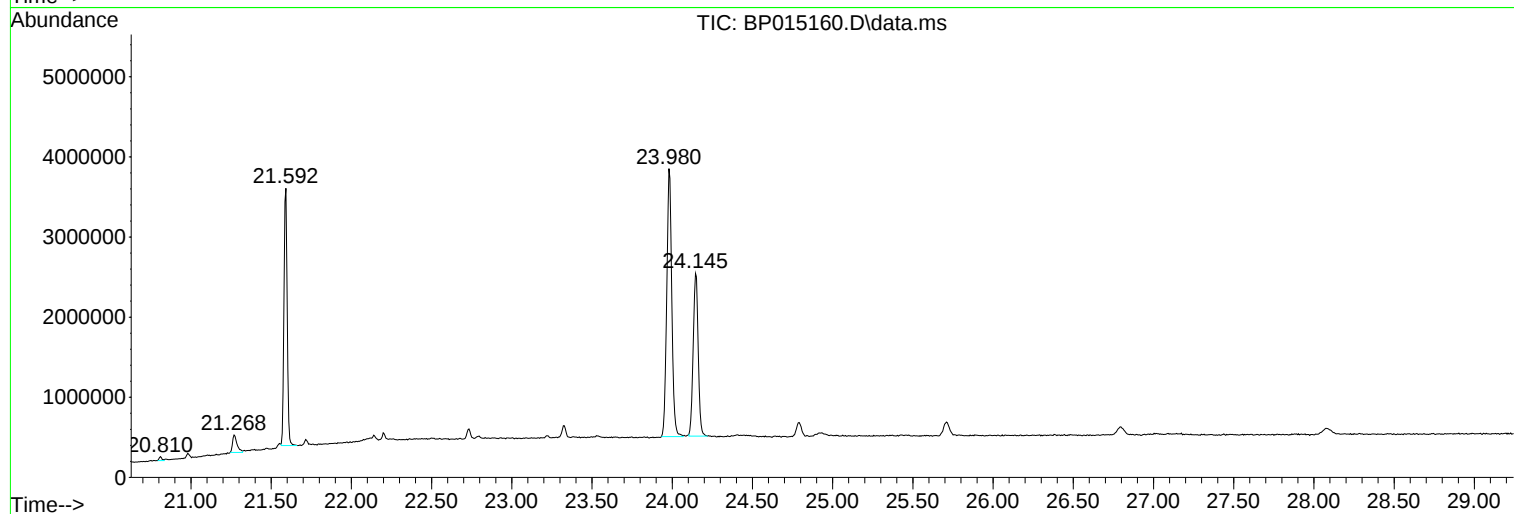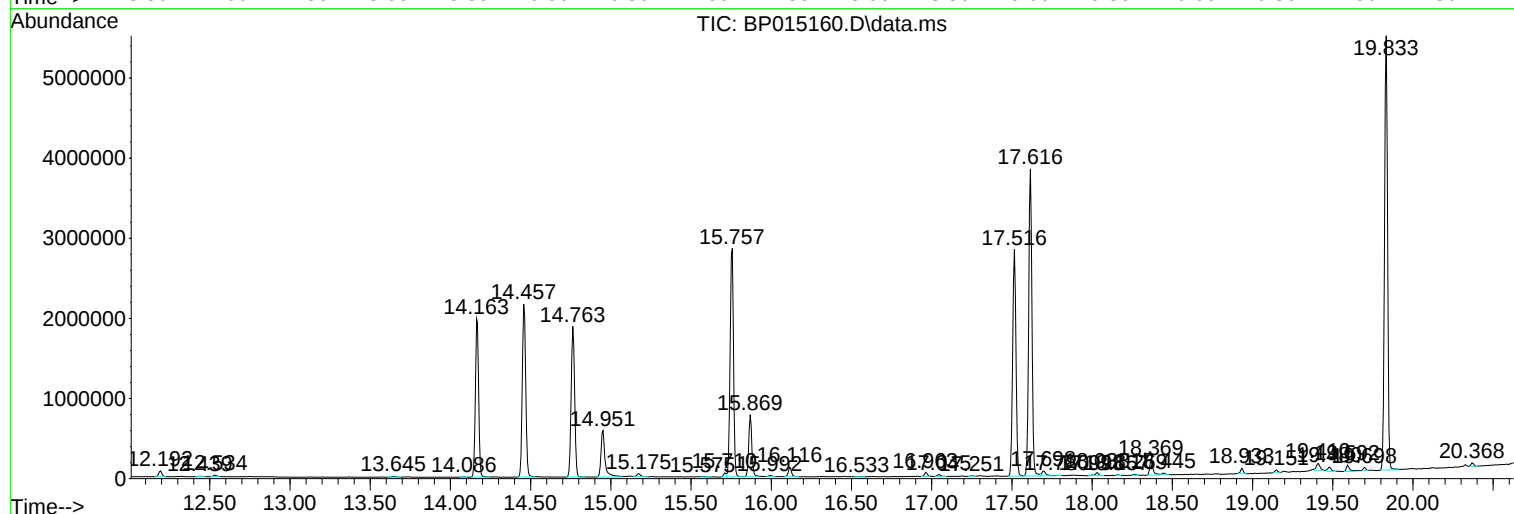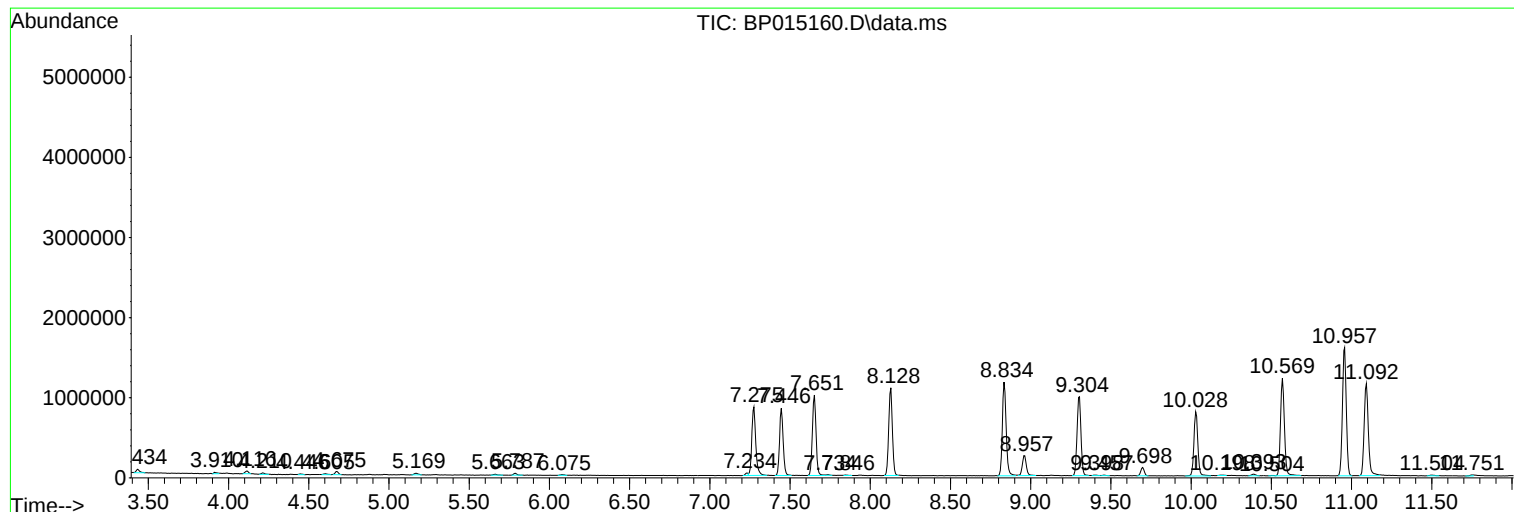

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015160.D
Acq On : 18 May 2023 23:22
Operator : CG/JU
Sample : 02612-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051823\
Data File : BP015160.D
Acq On : 18 May 2023 23:22
Operator : CG/JU
Sample : 02612-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------