

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051921\
 Data File : BP005614.D
 Acq On : 19 May 2021 16:36
 Operator : CG/JU
 Sample : PB136538BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136538BL

Quant Time: May 20 03:24:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 17 15:35:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	7332	20.00	ng	0.00
21) Naphthalene-d8	10.451	136	21156	20.00	ng	# 0.00
39) Acenaphthene-d10	14.310	164	17996	20.00	ng	0.00
64) Phenanthrene-d10	17.075	188	44165	20.00	ng	# 0.00
76) Chrysene-d12	21.174	240	64889	20.00	ng	# 0.00
86) Perylene-d12	23.468	264	73746	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.252	112	55533	145.36	ng	0.00
7) Phenol-d6	6.857	99	55069	115.60	ng	0.00
23) Nitrobenzene-d5	8.828	82	48265	89.79	ng	0.00
42) 2,4,6-Tribromophenol	15.816	330	54943	107.59	ng	0.00
45) 2-Fluorobiphenyl	12.928	172	115708	72.53	ng	0.00
79) Terphenyl-d14	19.645	244	328557	85.99	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051921\
Data File : BP005614.D
Acq On : 19 May 2021 16:36
Operator : CG/JU
Sample : PB136538BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136538BL

Quant Time: May 20 03:24:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 17 15:35:47 2021
Response via : Initial Calibration




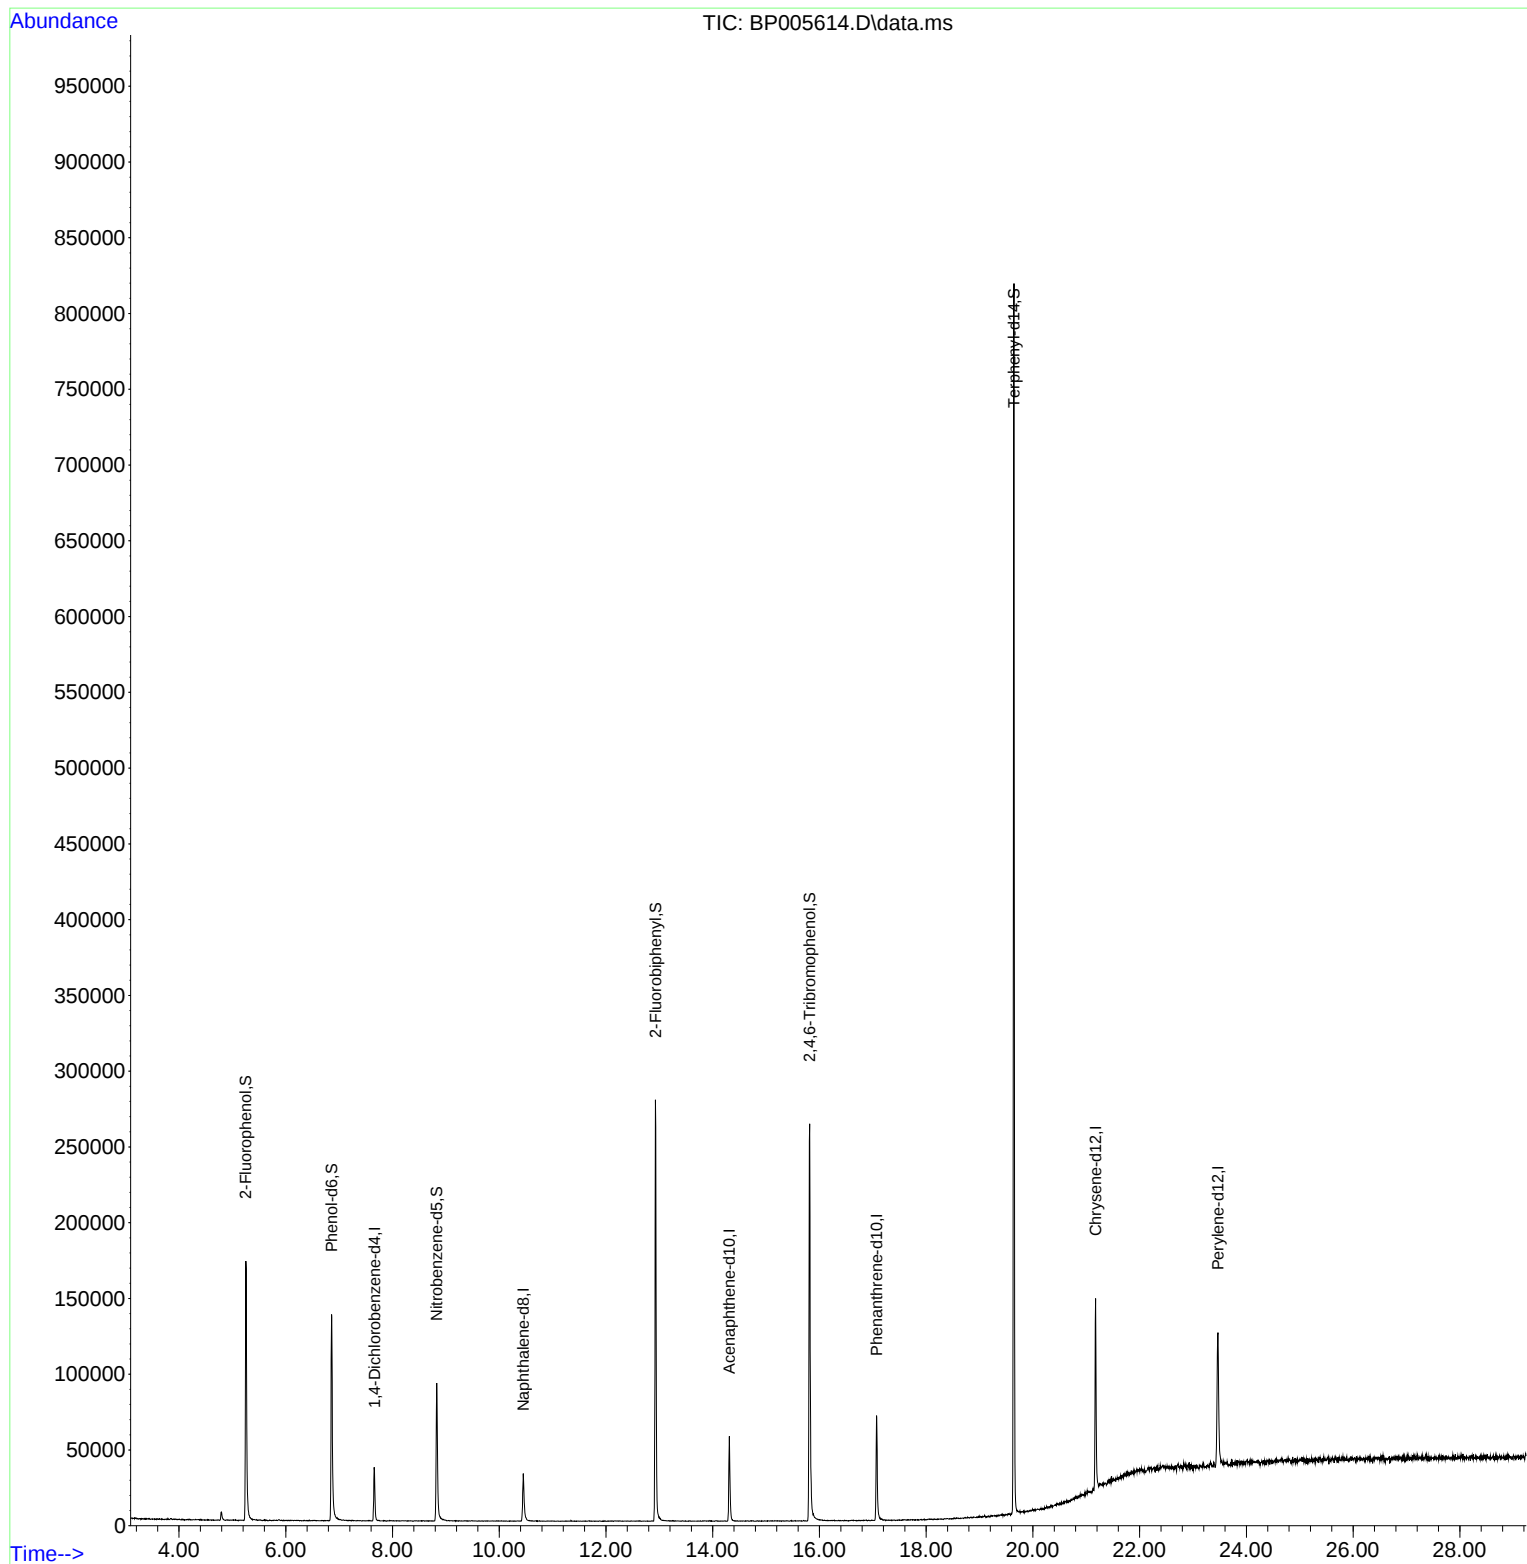


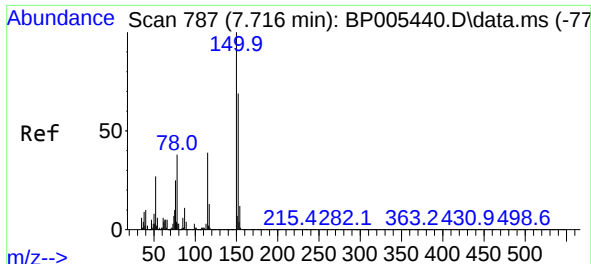

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.663 min Scan# 778
Delta R.T. 0.000 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36




Instrument :
BNA_P
ClientSampleId :
PB136538BL


Tgt Ion:152 Resp: 7332
Ion Ratio Lower Upper
152 100
150 130.6 119.8 179.8
115 62.1 49.0 73.4

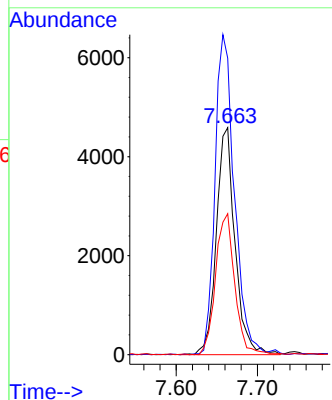

#5
2-Fluorophenol
Concen: 145.36 ng
RT: 5.252 min Scan# 368
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion:112 Resp: 55533
Ion Ratio Lower Upper
112 100
64 58.0 33.6 50.4#
63 49.3 18.6 27.8#


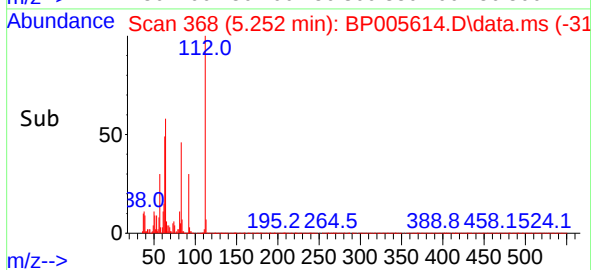
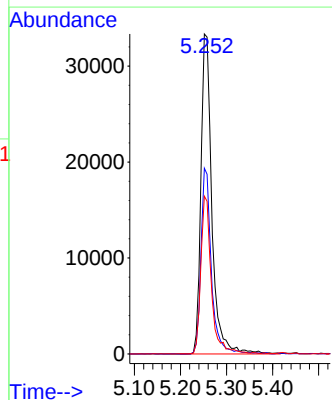
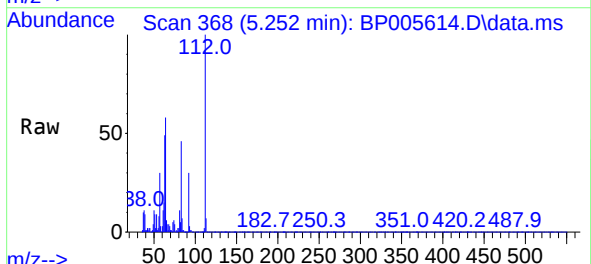


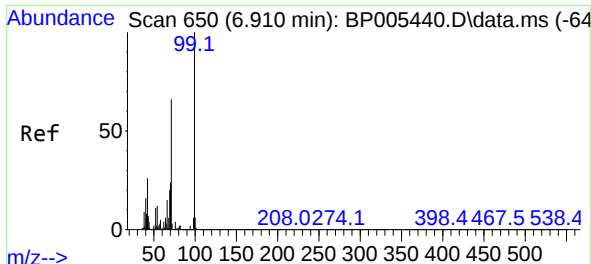

#7
Phenol-d6
Concen: 115.60 ng
RT: 6.857 min Scan# 641
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36




Instrument :
BNA_P
ClientSampleId :
PB136538BL


Tgt Ion:	99	Resp:	55069
Ion	Ratio	Lower	Upper
99	100		
42	32.7	12.9	19.3#
71	74.8	26.7	40.1#

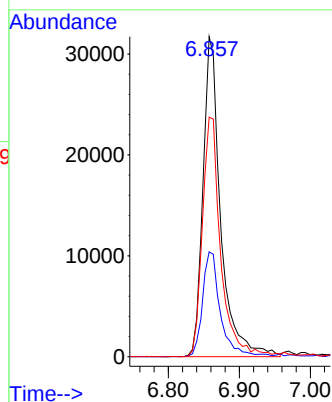

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.451 min Scan# 1252
Delta R.T. -0.000 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion:	136	Resp:	21156
Ion	Ratio	Lower	Upper
136	100		
137	9.2	8.9	13.3
54	9.0	5.0	7.4#
68	3.0	3.7	5.5#


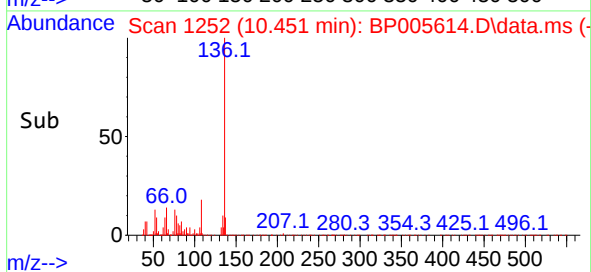
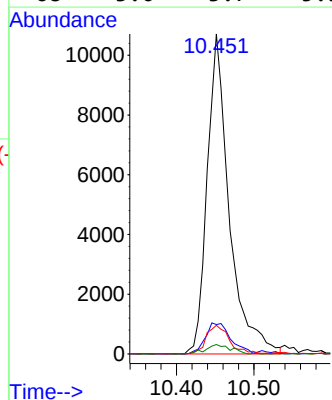
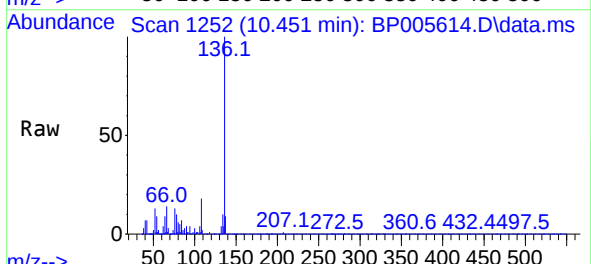


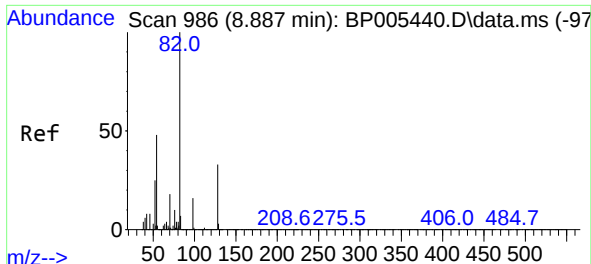

#23
Nitrobenzene-d5
Concen: 89.79 ng
RT: 8.828 min Scan# 976
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36




Instrument :
BNA_P
ClientSampleId :
PB136538BL


Tgt Ion: 82 Resp: 48265
Ion Ratio Lower Upper
82 100
128 27.4 30.5 45.7#
54 51.2 33.9 50.9#

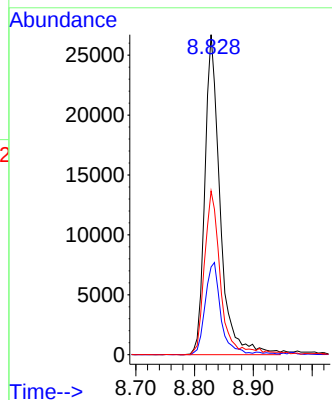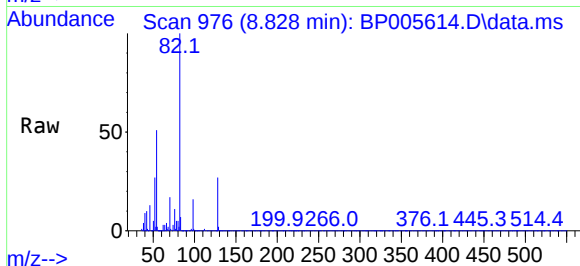

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.310 min Scan# 1908
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion: 164 Resp: 17996
Ion Ratio Lower Upper
164 100
162 102.3 73.5 110.3
160 43.0 40.6 61.0


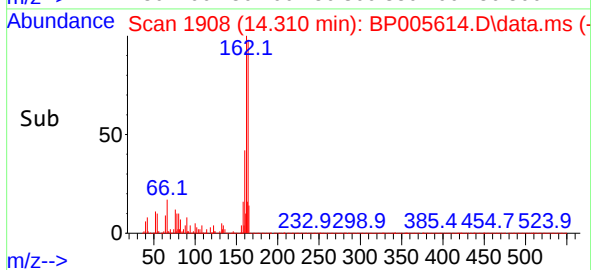
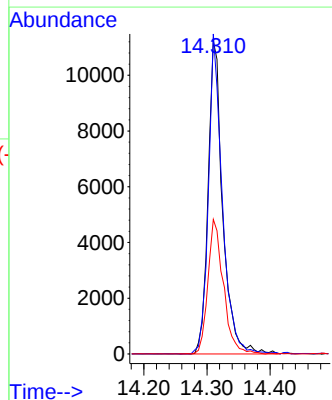
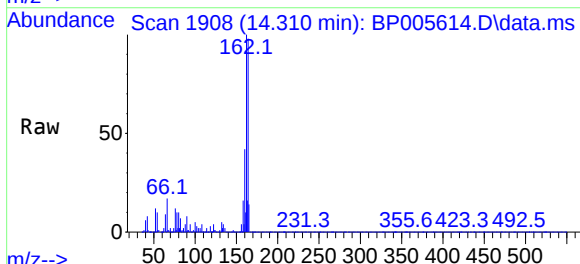


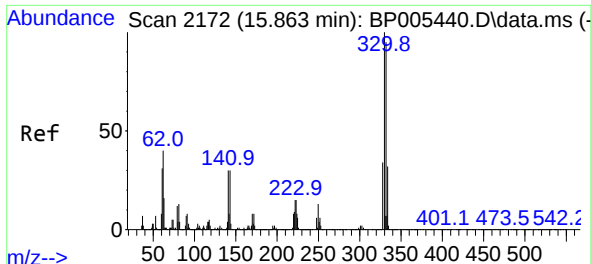

#42
2,4,6-Tribromophenol
Concen: 107.59 ng
RT: 15.816 min Scan# 2164
Delta R.T. -0.000 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36




Instrument :
BNA_P
ClientSampleId :
PB136538BL


Tgt Ion:	330	Resp:	54943
Ion Ratio	Lower	Upper	
330	100		
332	95.4	76.3	114.5
141	33.0	22.8	34.2

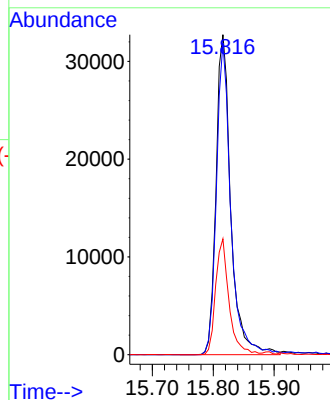

#45
2-Fluorobiphenyl
Concen: 72.53 ng
RT: 12.928 min Scan# 1673
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion:	172	Resp:	115708
Ion Ratio	Lower	Upper	
172	100		
171	36.1	28.1	42.1
170	23.7	19.6	29.4


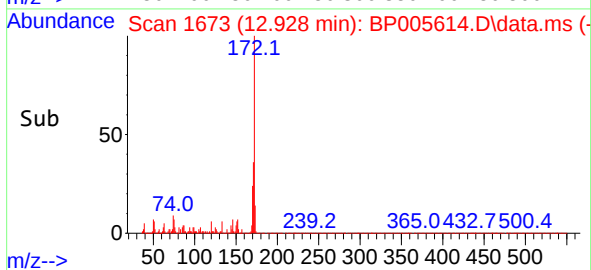
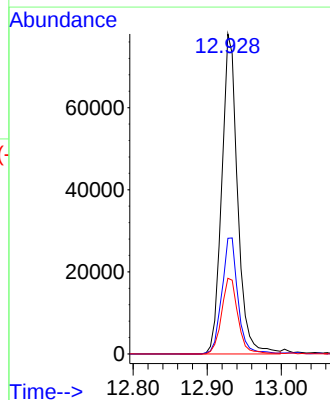
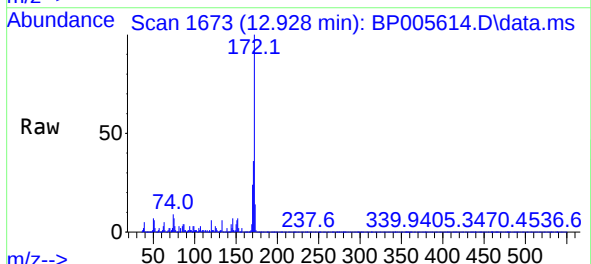




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.075 min Scan# 2378
Delta R.T. -0.000 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36




Instrument :
BNA_P
ClientSampleId :
PB136538BL


Tgt Ion:188	Resp:	44165
Ion Ratio	Lower	Upper
188	100	
94	4.8	5.0 7.6#
80	4.7	5.9 8.9#

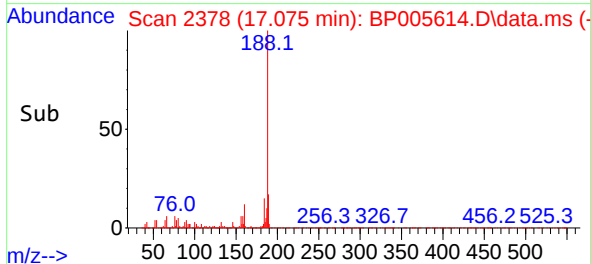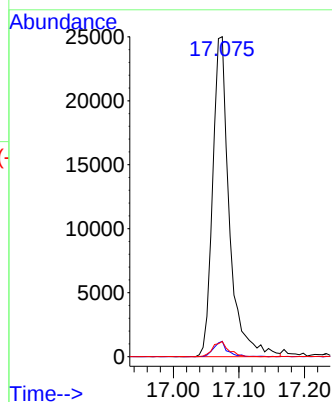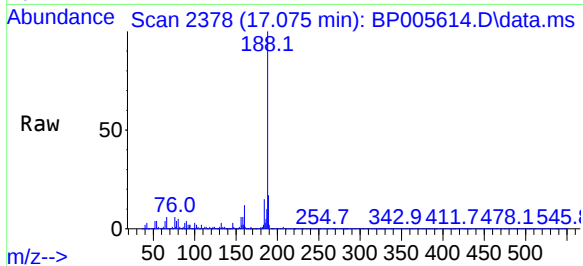

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.174 min Scan# 3075
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion:240	Resp:	64889
Ion Ratio	Lower	Upper
240	100	
120	2.1	4.2 6.2#
236	24.5	20.2 30.2


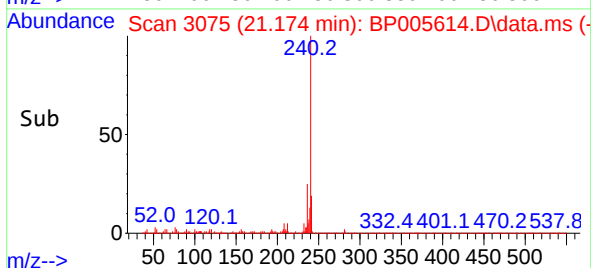
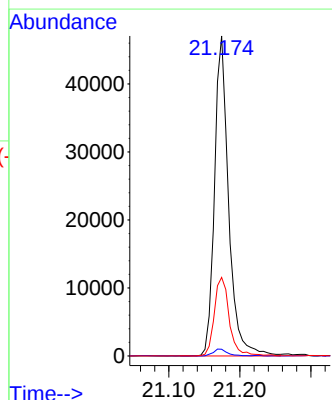
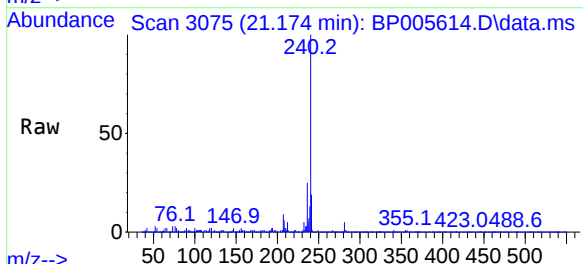




#79
Terphenyl-d14
Concen: 85.99 ng
RT: 19.645 min Scan# 2815
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Instrument :
BNA_P
ClientSampleId :
PB136538BL

Tgt Ion:244 Resp: 328557
Ion Ratio Lower Upper
244 100
212 7.7 5.8 8.6
122 3.8 5.2 7.8#

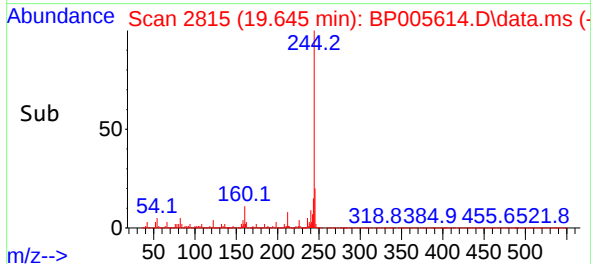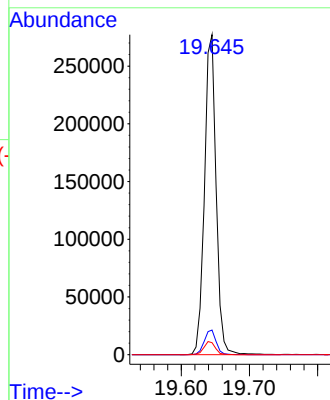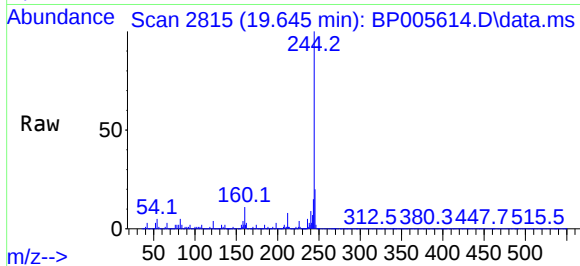

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.468 min Scan# 3465
Delta R.T. -0.006 min
Lab File: BP005614.D
Acq: 19 May 2021 16:36

Tgt Ion:264 Resp: 73746
Ion Ratio Lower Upper
264 100
260 24.4 20.6 30.8
265 21.2 19.0 28.6

