
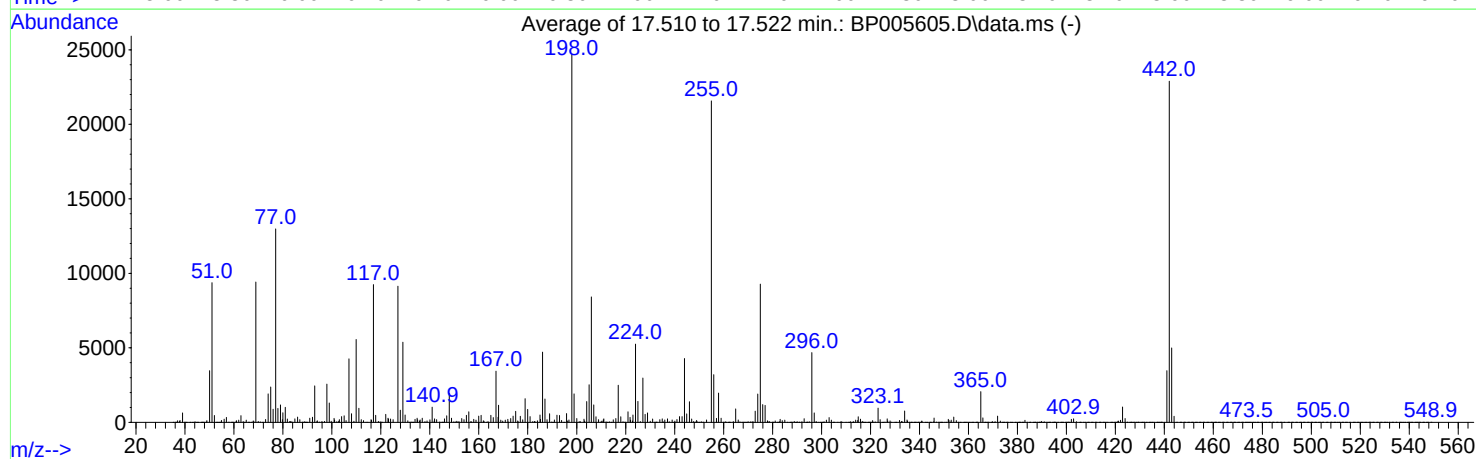


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051921\
 Data File : BP005605.D
 Acq On : 19 May 2021 10:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 17 15:35:47 2021

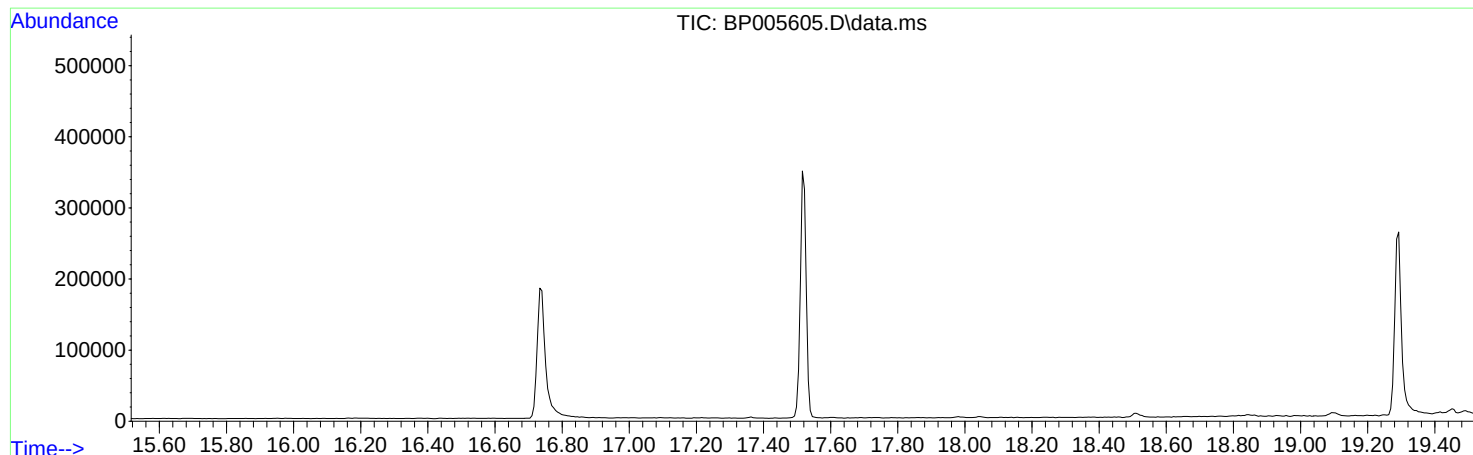




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	9374	PASS
68	69	0.00	2	1.0	91	PASS
69	198	0.00	100	38.1	9415	PASS
70	69	0.00	2	0.6	60	PASS
127	198	10	80	37.0	9138	PASS
197	198	0.00	2	0.7	164	PASS
198	198	100	100	100.0	24684	PASS
199	198	5	9	7.7	1910	PASS
275	198	10	60	37.6	9278	PASS
365	198	1	100	8.3	2057	PASS
441	198	0.01	100	14.0	3466	PASS
442	442	100	100	100.0	22887	PASS
443	442	15	24	21.8	4990	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051921\
 Data File : BP005605.D
 Acq On : 19 May 2021 10:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 19 13:16:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 17 15:35:47 2021
 Response via : Initial Calibration

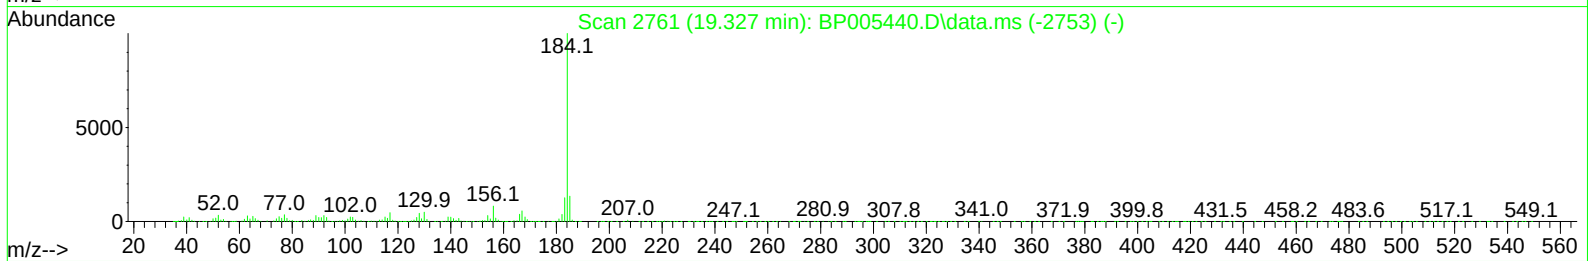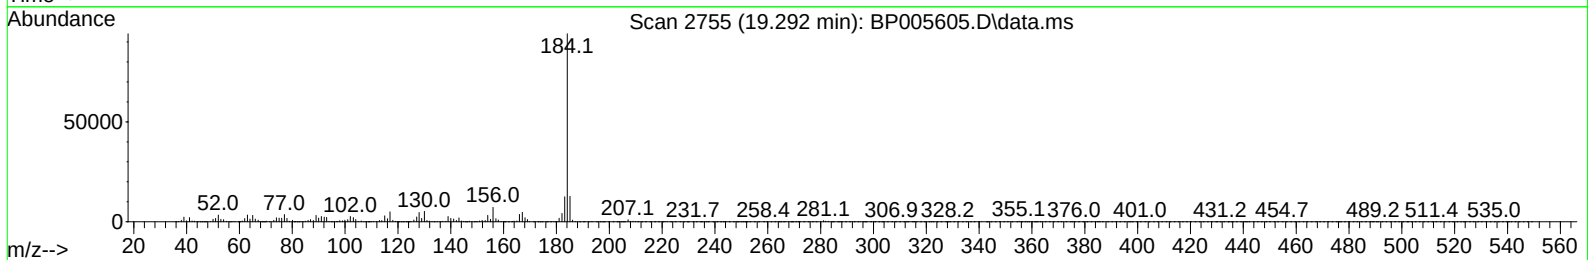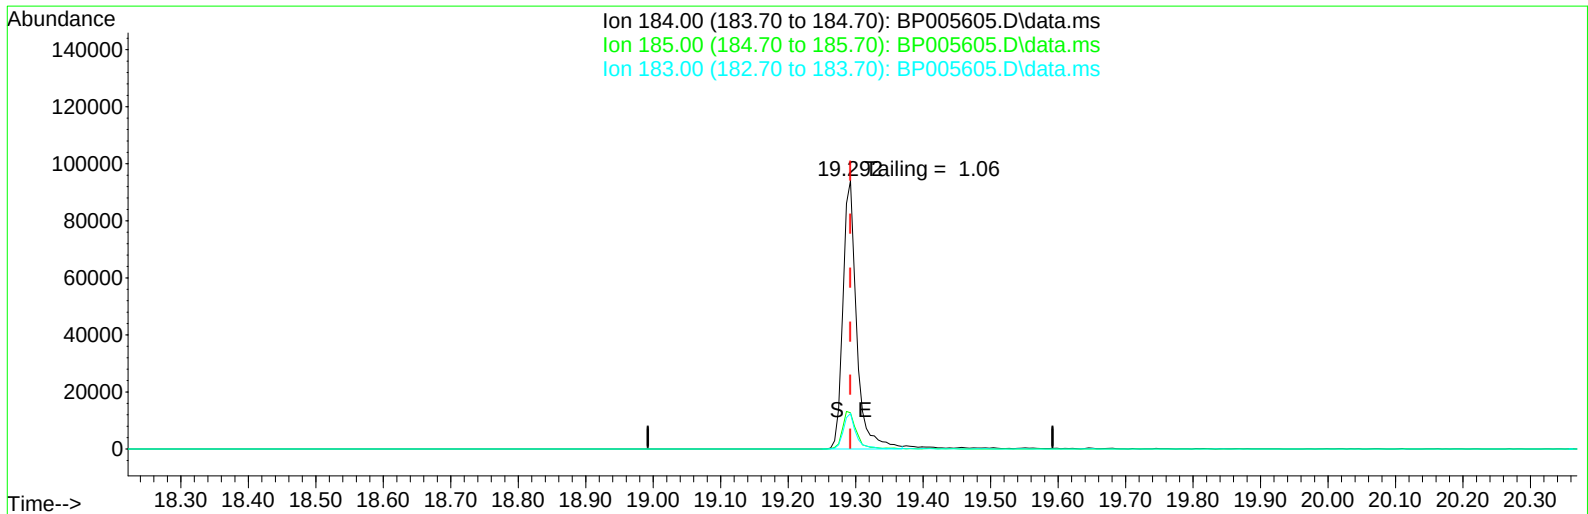

TIC: BP005605.D\data.ms

(77) Benzidine

19.292min (+ 0.000) 2426.25 ng




response 133134

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.50
183.00	12.30	13.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051921\
Data File : BP005605.D
Acq On : 19 May 2021 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 19 13:16:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 17 15:35:47 2021
Response via : Initial Calibration

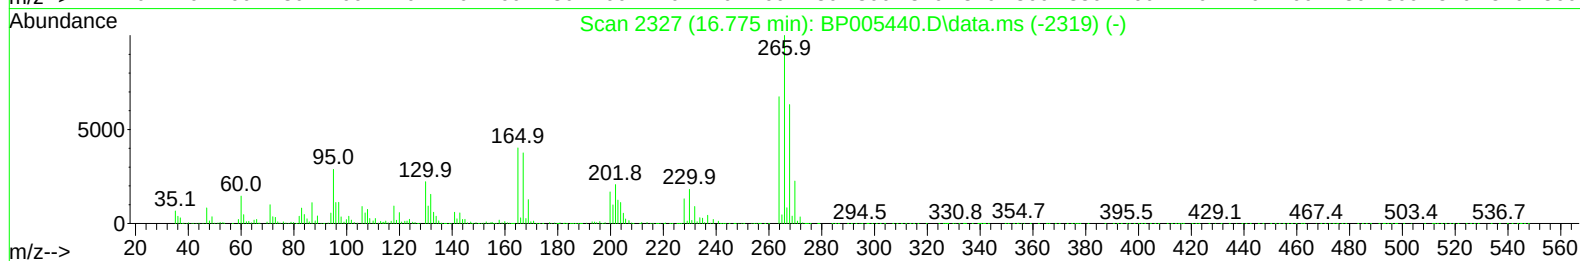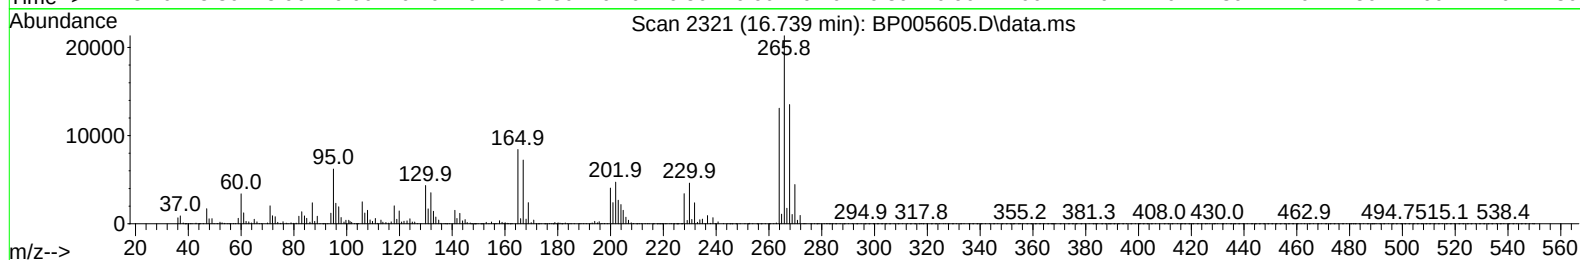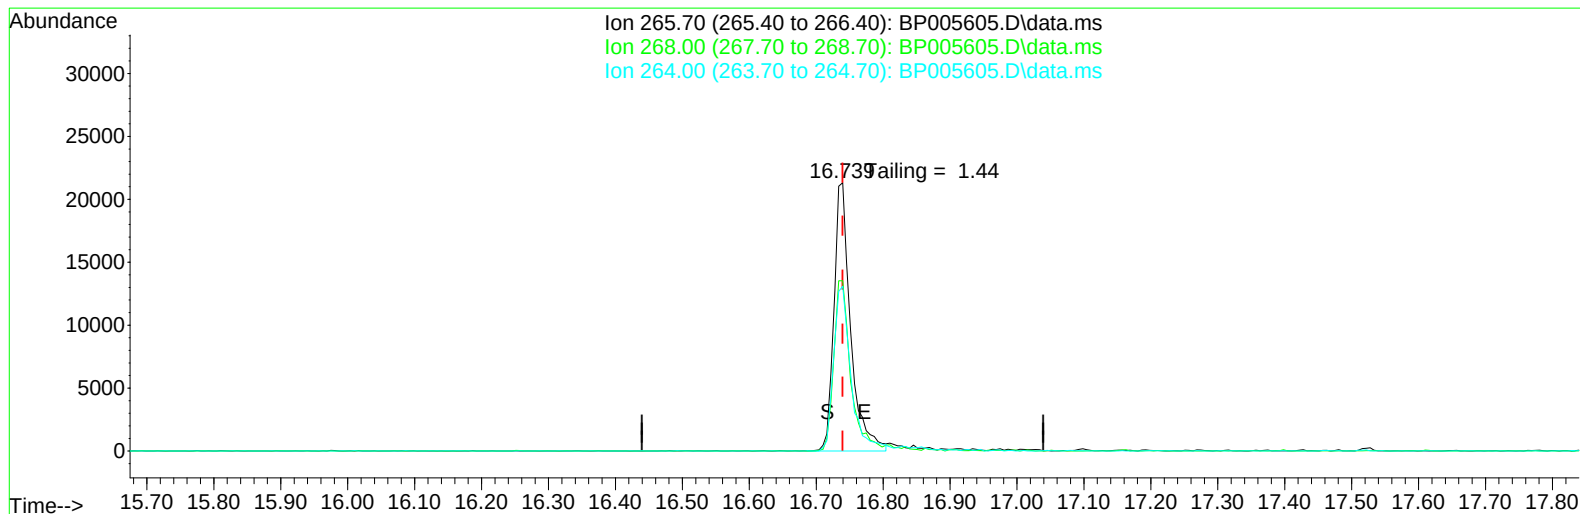

TIC: BP005605.D\data.ms

(70) Pentachlorophenol (C)

16.739min (+ 0.000) 34080.13 ng

response 37944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.44
264.00	67.10	61.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2021	BNA_P	BP005605.D
Compound Name	Response	Retention Time
DDT	93158	20.48
DDD	5941	20.05
DDE	397	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6338	99496	6.37