

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010420.D
 Acq On : 20 May 2022 01:09
 Operator : CG/JU
 Sample : N2918-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTG7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/20/2022
 Supervised By :Yogesh Patel 05/24/2022

Quant Time: May 20 02:29:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	159518	20.000	ng/u1	0.00
20) Naphthalene-d8	10.692	136	694891	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.527	164	481421	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.274	188	1053434	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.362	240	987783	20.000	ng/u1	# 0.00
88) Perylene-d12	23.786	264	877303	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	7952m	2.125	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.063	99	9577	0.715	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	36822m	4.093	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	29317	2.862	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	19158	1.684	ng/u1	0.00
21) Nitrobenzene-d5	9.051	128	20261	3.767	ng/u1	0.00
24) 2-Nitrophenol-d4	9.781	143	19013	3.336	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	32459m	3.012	ng/u1	0.01
31) 4-Chloroaniline-d4	10.839	131	38985	2.433	ng/u1	0.00
46) Dimethylphthalate-d6	13.939	166	152450	4.298	ng/u1	0.00
49) Acenaphthylene-d8	14.216	160	164231m	4.014	ng/u1	0.00
54) 4-Nitrophenol-d4	14.792	143	2283m	0.362	ng/u1	0.06
60) Fluorene-d10	15.522	176	129623	4.201	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	12044m	1.955	ng/u1	0.00
73) Anthracene-d10	17.374	188	220396	4.620	ng/u1	0.00
81) Pyrene-d10	19.610	212	294171	5.608	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.627	264	216612	4.917	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.745	128	37882	1.044	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010420.D
Acq On : 20 May 2022 01:09
Operator : CG/JU
Sample : N2918-09
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
DBTG7

Quant Time: May 20 02:29:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 05/20/2022
Supervised By :Yogesh Patel 05/24/2022

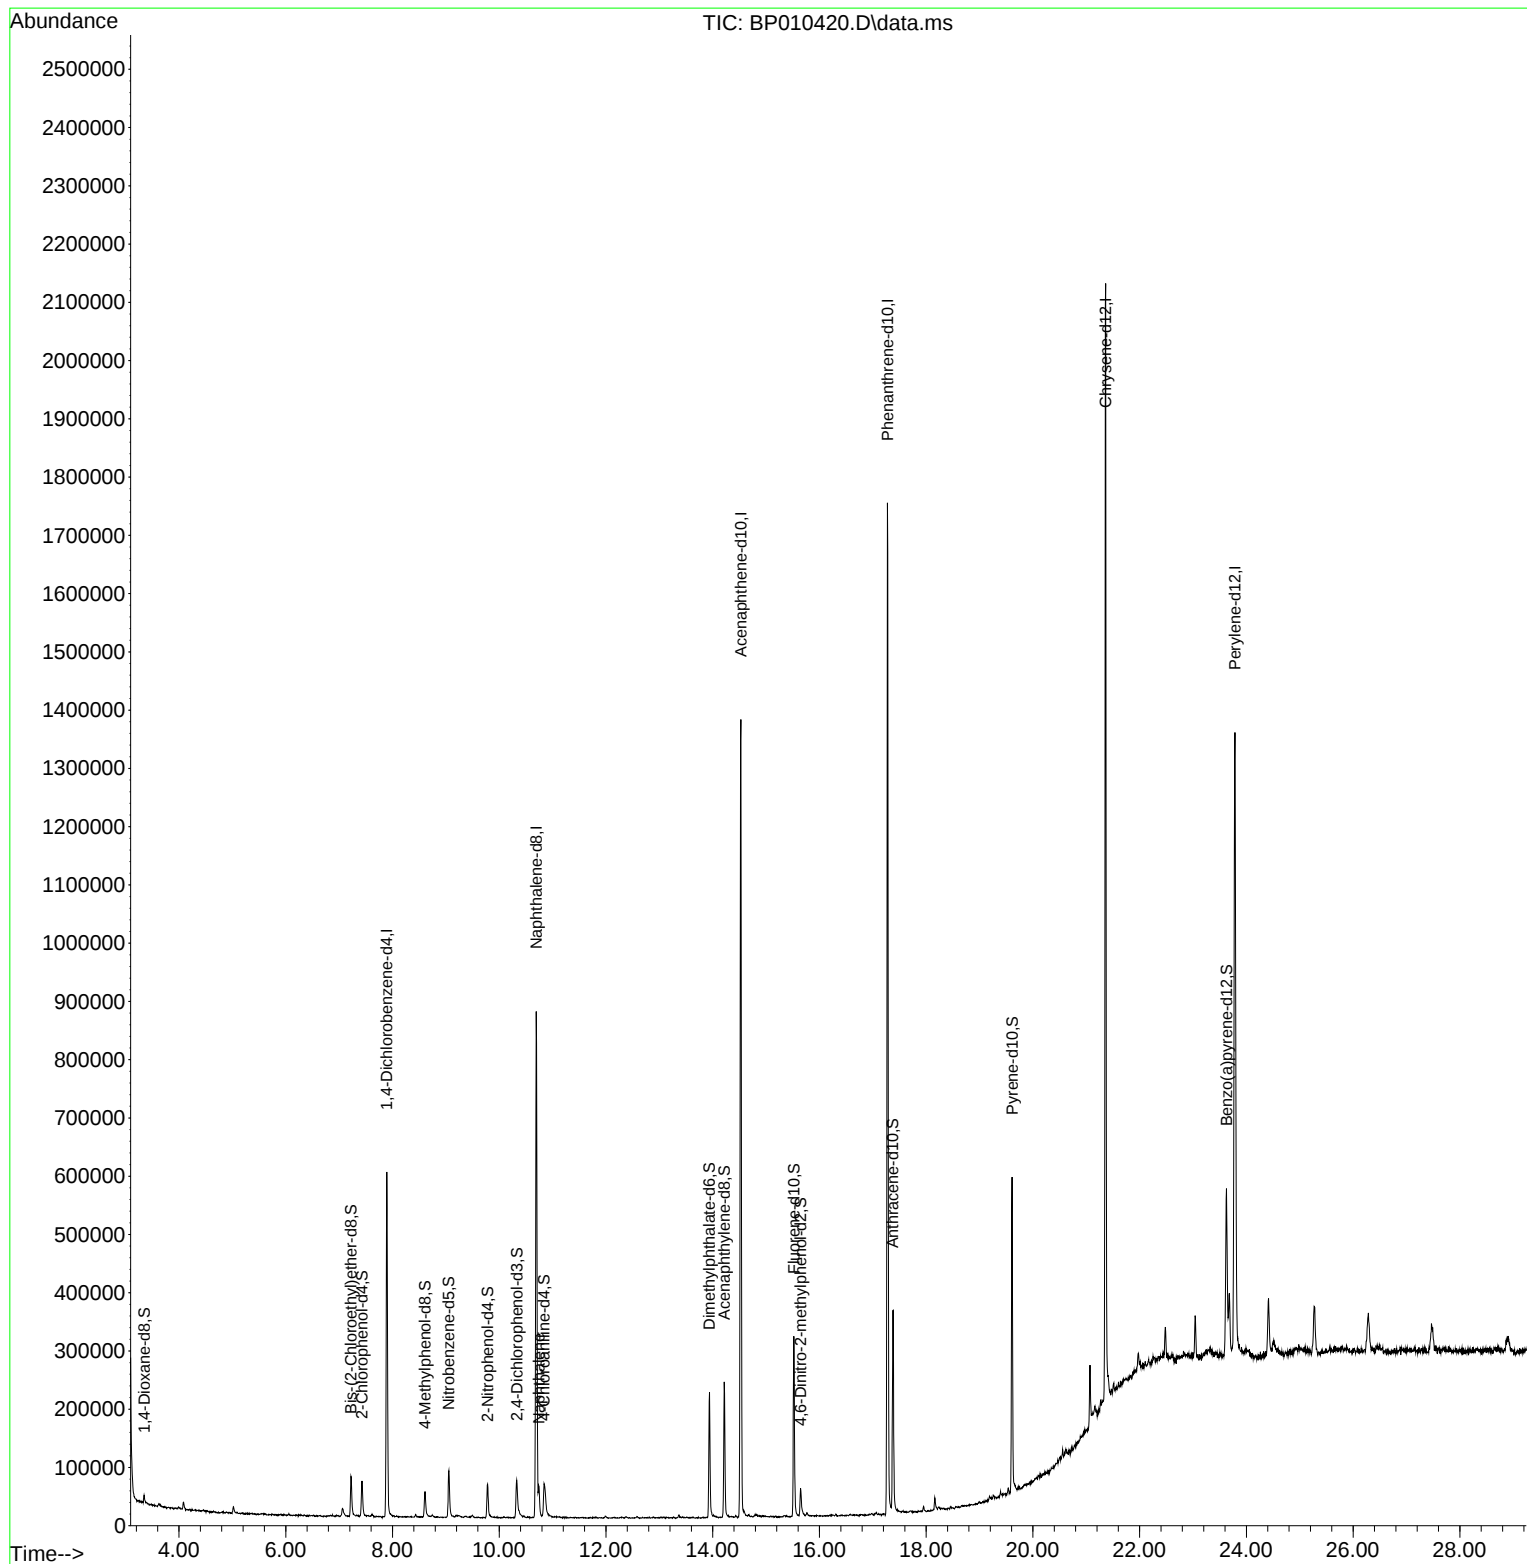

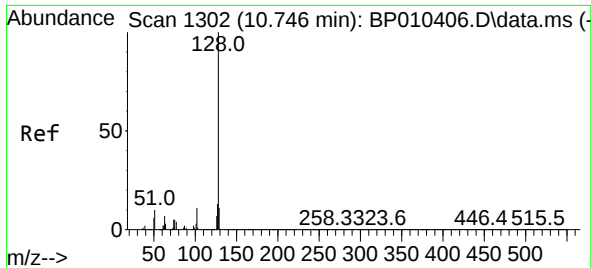

#30
Naphthalene
Concen: 1.044 ng/ul
RT: 10.745 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP010420.D
Acq: 20 May 2022 01:09

Instrument :
BNA_P
ClientSampleId :
DBTG7

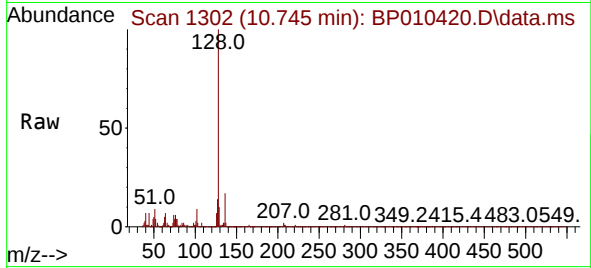

Tgt Ion:128 Resp: 3788
Ion Ratio Lower Upper
128 100
129 10.1 8.6 13.0
127 14.2 12.2 18.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/20/2022
Supervised By :Yogesh Patel 05/24/2022

