

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010408.D
 Acq On : 19 May 2022 17:43
 Operator : CG/JU
 Sample : PB144950BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK950

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	51	rBV	26650	39582	1.11%	0.110%
2	3.758	111	114	138	rBV	341350	714211	19.98%	1.992%
3	4.081	167	169	175	rVB4	6824	8878	0.25%	0.025%
4	7.058	668	675	688	rBV	489226	839457	23.49%	2.341%
5	7.222	696	703	715	rBV	390745	650104	18.19%	1.813%
6	7.428	731	738	750	rBV	482869	842693	23.58%	2.350%
7	7.893	809	817	830	rBV	416115	700802	19.61%	1.955%
8	8.599	928	937	955	rBV	641594	1097838	30.72%	3.062%
9	9.052	1002	1014	1028	rBV	538991	939371	26.28%	2.620%
10	9.610	1105	1109	1113	rBV6	2435	5180	0.14%	0.014%
11	9.775	1128	1137	1155	rBV	431018	761111	21.30%	2.123%
12	10.316	1220	1229	1249	rBV	590922	1106372	30.96%	3.086%
13	10.693	1283	1293	1306	rBV	624529	1076005	30.11%	3.001%
14	10.834	1309	1317	1338	rVV	596806	1161270	32.49%	3.239%
15	12.298	1559	1566	1575	rBV7	7994	19585	0.55%	0.055%
16	13.934	1837	1844	1857	rBV	1283227	1809942	50.64%	5.048%
17	14.040	1860	1862	1869	rVB9	2946	5109	0.14%	0.014%
18	14.222	1885	1893	1905	rBV	1272052	1999133	55.93%	5.576%
19	14.528	1938	1945	1955	rBV	1030550	1512737	42.33%	4.219%
20	14.722	1972	1978	2004	rBV	377549	831938	23.28%	2.320%
21	15.522	2106	2114	2127	rBV	1726656	2619381	73.29%	7.306%
22	15.639	2127	2134	2150	rVV	542300	836089	23.39%	2.332%
23	15.763	2150	2155	2162	rVB2	23509	38564	1.08%	0.108%
24	16.304	2243	2247	2255	rVB6	7782	13793	0.39%	0.038%
25	16.951	2354	2357	2363	rVB7	3782	7409	0.21%	0.021%
26	17.063	2371	2376	2383	rVB8	3752	9210	0.26%	0.026%
27	17.281	2406	2413	2423	rBV	1336452	1942191	54.34%	5.417%
28	17.381	2423	2430	2448	rVB	1984559	2953835	82.65%	8.239%
29	18.286	2580	2584	2587	rBV5	2784	4259	0.12%	0.012%
30	18.657	2643	2647	2649	rBV4	3088	4571	0.13%	0.013%
31	19.192	2734	2738	2742	rBV3	22880	31819	0.89%	0.089%
32	19.257	2746	2749	2756	rVV2	20617	30336	0.85%	0.085%
33	19.610	2803	2809	2822	rBV	2707774	3574040	100.00%	9.969%
34	21.363	3102	3107	3124	rBV	1562817	2239365	62.66%	6.246%
35	23.633	3485	3493	3510	rBV2	1578735	3379904	94.57%	9.427%
36	23.792	3513	3520	3533	rVB2	951131	2046325	57.26%	5.708%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010408.D
Acq On : 19 May 2022 17:43
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 35852409

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010408.D
Acq On : 19 May 2022 17:43
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

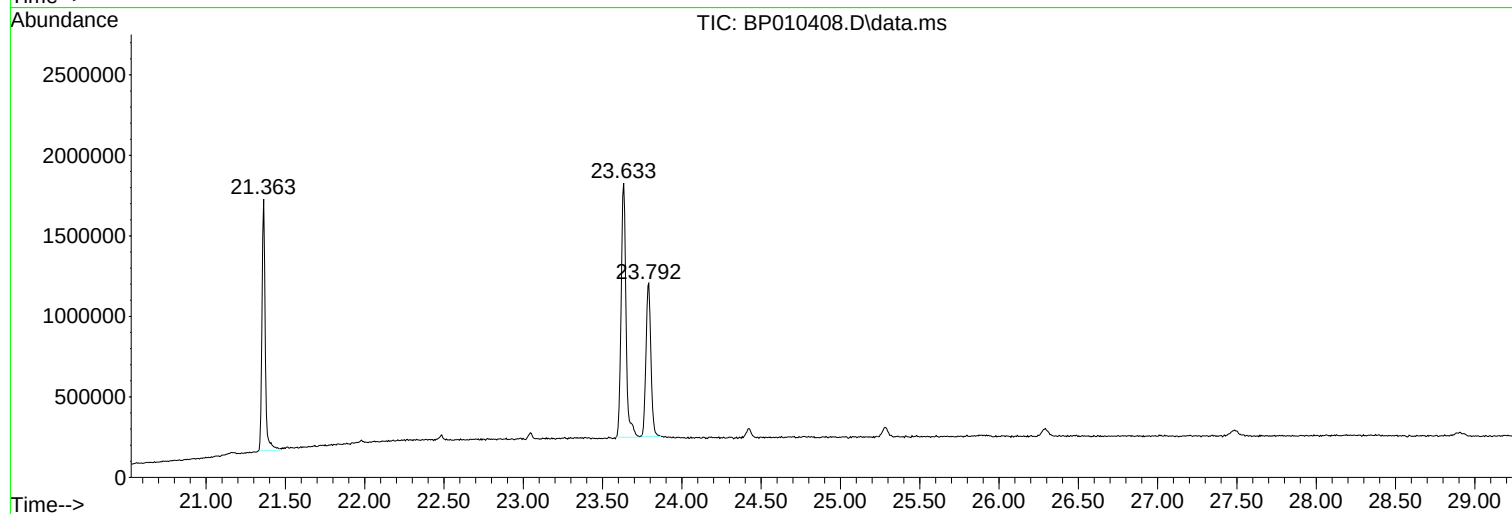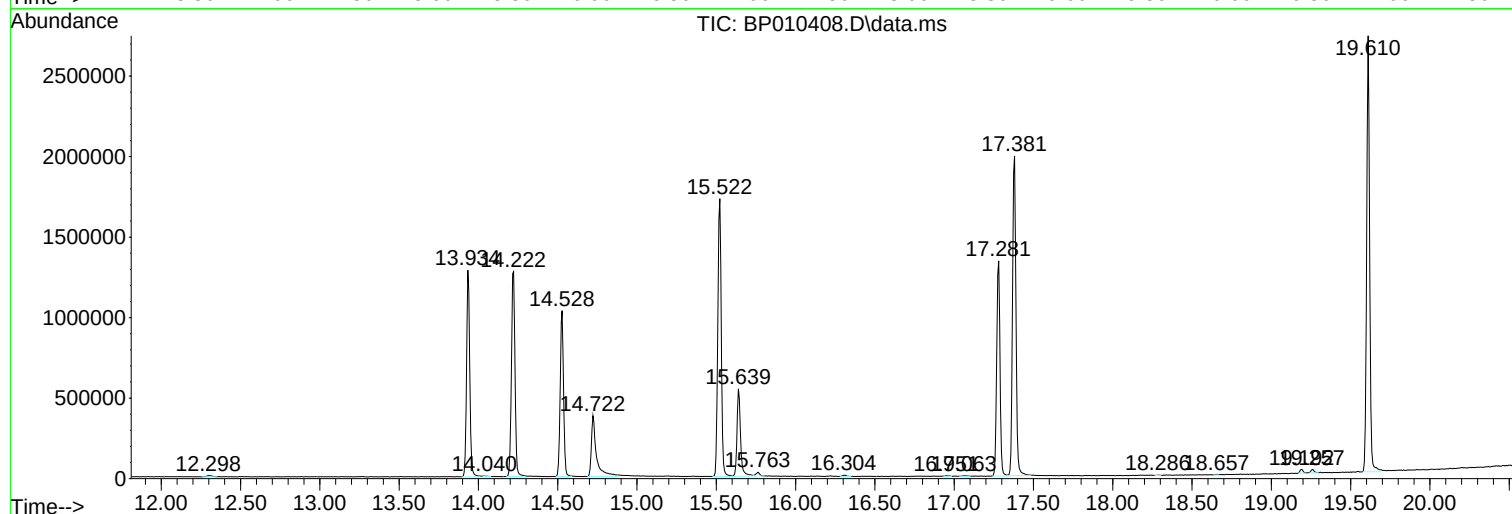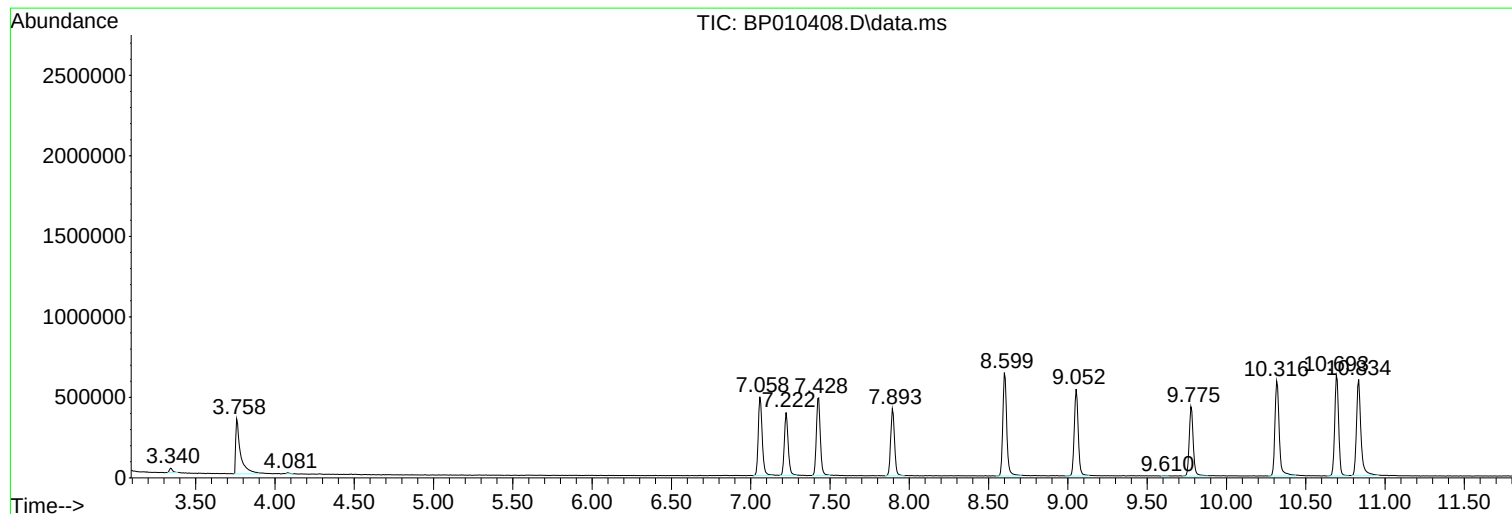

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010408.D
Acq On : 19 May 2022 17:43
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010408.D
Acq On : 19 May 2022 17:43
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc