

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010419.D
 Acq On : 20 May 2022 00:35
 Operator : CG/JU
 Sample : N2918-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	55	rVB	31414	54183	0.89%	0.104%
2	3.770	112	116	138	rBV	147220	322086	5.26%	0.621%
3	3.993	149	154	161	rBV2	19984	33761	0.55%	0.065%
4	4.081	166	169	176	rVB2	11865	18611	0.30%	0.036%
5	5.017	323	328	334	rVB2	28395	48467	0.79%	0.093%
6	5.611	425	429	432	rVB5	5131	7224	0.12%	0.014%
7	6.764	620	625	630	rBV9	3103	7174	0.12%	0.014%
8	7.058	669	675	690	rVB	156608	282508	4.62%	0.545%
9	7.222	696	703	714	rBV	671219	1088281	17.78%	2.098%
10	7.311	716	718	725	rVB2	6674	9778	0.16%	0.019%
11	7.422	730	737	751	rBV	630143	1061478	17.34%	2.047%
12	7.893	809	817	827	rBV	640834	1035392	16.92%	1.996%
13	8.599	930	937	950	rBV	505350	874506	14.29%	1.686%
14	9.052	1006	1014	1027	rBV	893055	1519686	24.83%	2.930%
15	9.493	1082	1089	1096	rBV6	9285	18168	0.30%	0.035%
16	9.775	1129	1137	1151	rBV	711901	1226174	20.04%	2.364%
17	10.316	1221	1229	1252	rBV	920363	1667500	27.25%	3.215%
18	10.693	1284	1293	1302	rBV	944999	1597102	26.10%	3.079%
19	10.828	1309	1316	1334	rBV	765947	1477883	24.15%	2.849%
20	11.534	1428	1436	1437	rBV8	4336	7586	0.12%	0.015%
21	11.993	1510	1514	1518	rVB6	5100	6747	0.11%	0.013%
22	12.252	1554	1558	1559	rBV4	5454	6265	0.10%	0.012%
23	12.287	1559	1564	1573	rVB	16157	33250	0.54%	0.064%
24	12.552	1603	1609	1612	rBV8	3626	7892	0.13%	0.015%
25	12.581	1612	1614	1619	rVB6	4174	6298	0.10%	0.012%
26	12.910	1662	1670	1672	rBV8	3787	10042	0.16%	0.019%
27	13.069	1693	1697	1703	rVB9	4320	9175	0.15%	0.018%
28	13.263	1724	1730	1736	rBV9	3588	7361	0.12%	0.014%
29	13.363	1743	1747	1753	rBV4	12921	21169	0.35%	0.041%
30	13.934	1835	1844	1856	rBV	2176699	2979653	48.69%	5.745%
31	14.046	1861	1863	1869	rVB7	4717	9171	0.15%	0.018%
32	14.216	1883	1892	1908	rBV	2258286	3371884	55.10%	6.501%
33	14.522	1937	1944	1954	rBV	1475387	2234898	36.52%	4.309%
34	14.734	1973	1980	1998	rBV	82719	233955	3.82%	0.451%
35	14.940	2011	2015	2023	rBV	8490	16111	0.26%	0.031%
36	15.169	2050	2054	2061	rVB10	5614	12331	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010419.D
 Acq On : 20 May 2022 00:35
 Operator : CG/JU
 Sample : N2918-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	15.275	2066	2072	2077	rVB8	5806	11536	0.19%	0.022%
38	15.334	2077	2082	2085	rBV4	4903	7285	0.12%	0.014%
39	15.516	2101	2113	2127	rBV	2932965	4515369	73.78%	8.706%
40	15.640	2127	2134	2148	rVV	1020702	1540573	25.17%	2.970%
41	15.763	2150	2155	2164	rVB2	34469	61794	1.01%	0.119%
42	16.022	2193	2199	2206	rVB2	7631	16243	0.27%	0.031%
43	16.210	2226	2231	2235	rBV7	5458	11675	0.19%	0.023%
44	16.304	2243	2247	2253	rVB2	12253	21867	0.36%	0.042%
45	16.416	2262	2266	2269	rBV6	3707	6527	0.11%	0.013%
46	16.493	2274	2279	2283	rVV5	9077	15291	0.25%	0.029%
47	16.545	2287	2288	2294	rVB5	5103	6275	0.10%	0.012%
48	16.781	2324	2328	2333	rBV6	4971	8689	0.14%	0.017%
49	16.957	2356	2358	2362	rVB5	6048	7350	0.12%	0.014%
50	17.275	2406	2412	2422	rBV	1796366	2666280	43.57%	5.141%
51	17.375	2422	2429	2442	rVV	3643592	5250684	85.79%	10.123%
52	17.475	2443	2446	2451	rVB6	14632	22427	0.37%	0.043%
53	17.851	2507	2510	2514	rVB5	6125	7239	0.12%	0.014%
54	17.951	2522	2527	2531	rVB3	28731	38902	0.64%	0.075%
55	18.163	2558	2563	2571	rBV4	42625	72632	1.19%	0.140%
56	18.239	2573	2576	2579	rVB4	8449	9934	0.16%	0.019%
57	18.763	2662	2665	2667	rBV4	8018	9956	0.16%	0.019%
58	19.186	2732	2737	2742	rBV	49852	74922	1.22%	0.144%
59	19.257	2745	2749	2752	rVV	39405	52182	0.85%	0.101%
60	19.392	2769	2772	2781	rBV8	21600	37292	0.61%	0.072%
61	19.534	2793	2796	2802	rVB7	15094	23313	0.38%	0.045%
62	19.610	2803	2809	2826	rVV	4588886	6120035	100.00%	11.799%
63	21.069	3053	3057	3062	rBV	122323	176648	2.89%	0.341%
64	21.363	3102	3107	3121	rVB	1861630	2628080	42.94%	5.067%
65	23.633	3485	3493	3499	rBV2	2299554	4793789	78.33%	9.242%
66	23.786	3512	3519	3529	rVB2	1131517	2328479	38.05%	4.489%




Sum of corrected areas: 51867018

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010419.D
Acq On : 20 May 2022 00:35
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

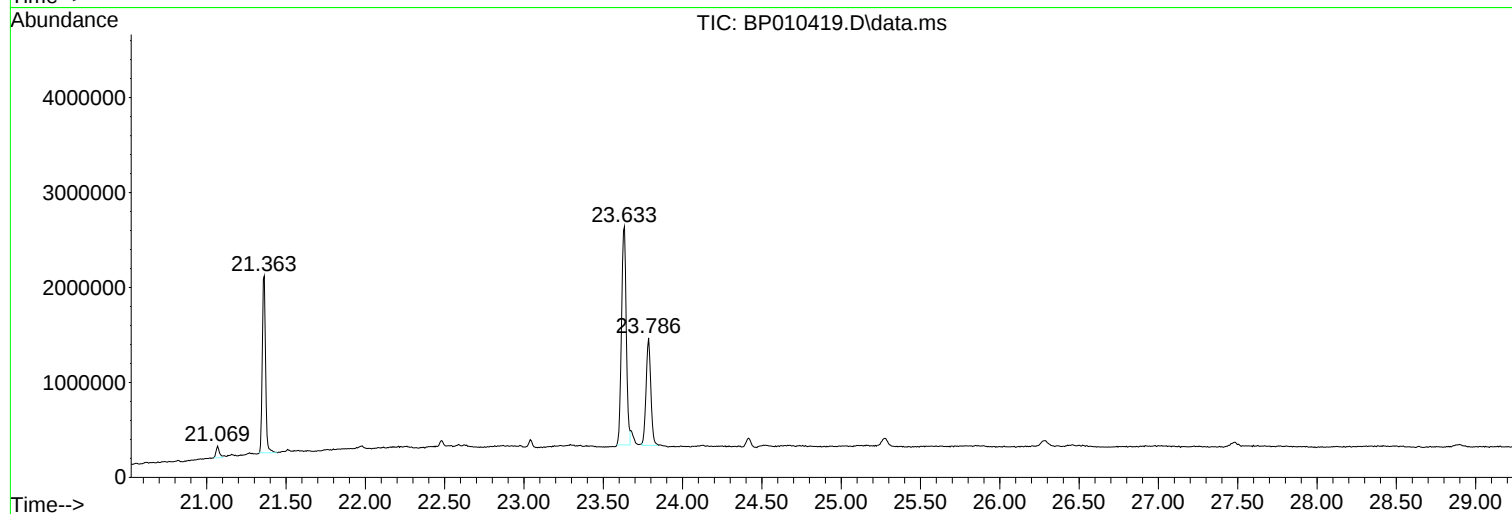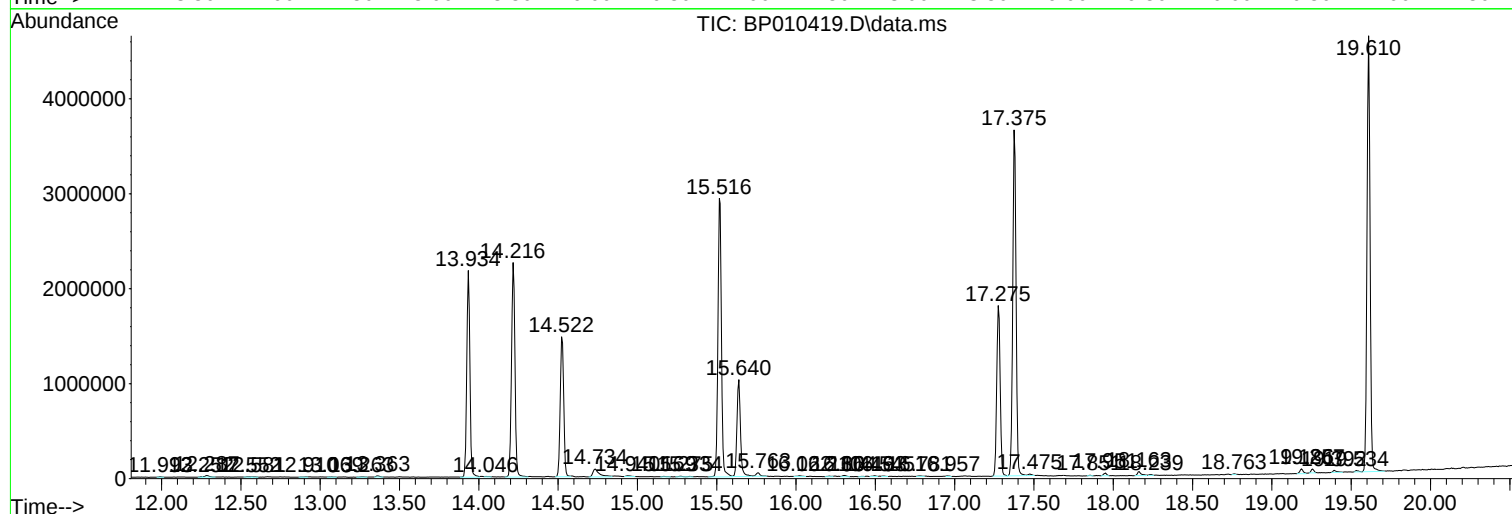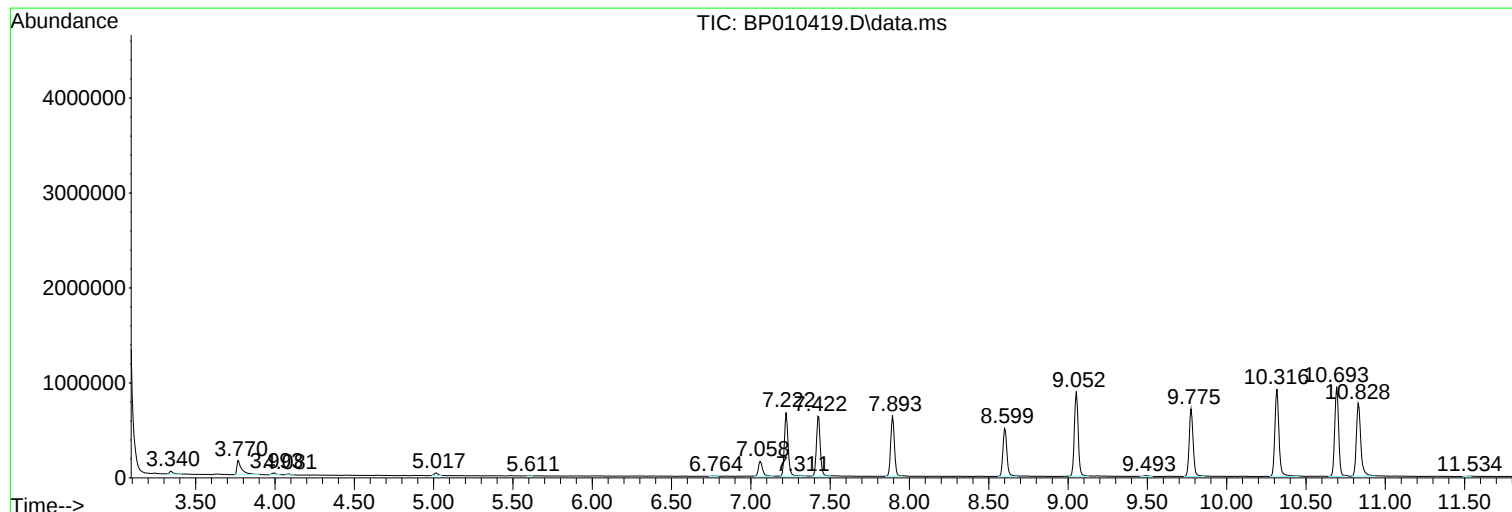

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010419.D
Acq On : 20 May 2022 00:35
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010419.D
Acq On : 20 May 2022 00:35
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc