

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010420.D
 Acq On : 20 May 2022 01:09
 Operator : CG/JU
 Sample : N2918-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	49	rVB3	12847	17161	0.64%	0.102%
2	4.087	166	170	176	rVB	13726	24609	0.91%	0.147%
3	4.516	241	243	245	rBV3	2824	2867	0.11%	0.017%
4	5.016	324	328	337	rBV	11859	23592	0.87%	0.141%
5	5.740	450	451	455	rBV4	2616	2925	0.11%	0.017%
6	6.351	551	555	557	rBV5	1915	2731	0.10%	0.016%
7	6.716	615	617	622	rBV6	1873	2942	0.11%	0.018%
8	7.063	669	676	687	rBV4	13669	34914	1.29%	0.208%
9	7.222	698	703	719	rBV	68829	127895	4.74%	0.762%
10	7.428	732	738	750	rBV	60173	111431	4.13%	0.664%
11	7.616	764	770	773	rBV6	4135	6116	0.23%	0.036%
12	7.822	803	805	808	rBV4	2058	3053	0.11%	0.018%
13	7.893	810	817	828	rVV	591597	992874	36.80%	5.916%
14	8.434	905	909	913	rBV4	4884	6677	0.25%	0.040%
15	8.610	933	939	949	rBV2	43646	86063	3.19%	0.513%
16	8.745	958	962	968	rVB9	3612	5311	0.20%	0.032%
17	9.057	1006	1015	1024	rBV2	80701	161562	5.99%	0.963%
18	9.198	1032	1039	1040	rBV7	2934	5008	0.19%	0.030%
19	9.363	1062	1067	1069	rBV6	2174	3709	0.14%	0.022%
20	9.498	1084	1090	1093	rBV8	3754	6527	0.24%	0.039%
21	9.781	1131	1138	1145	rBV2	58101	115809	4.29%	0.690%
22	10.328	1224	1231	1250	rBV2	64566	168870	6.26%	1.006%
23	10.469	1254	1255	1261	rVB5	2492	2756	0.10%	0.016%
24	10.692	1285	1293	1299	rBV	868567	1495131	55.42%	8.909%
25	10.739	1299	1301	1310	rVB	52994	89410	3.31%	0.533%
26	10.839	1312	1318	1331	rVV3	55195	154388	5.72%	0.920%
27	11.986	1509	1513	1519	rBV7	3249	6087	0.23%	0.036%
28	12.375	1575	1579	1583	rBV6	2678	5412	0.20%	0.032%
29	12.581	1610	1614	1619	rVB8	2389	3666	0.14%	0.022%
30	12.869	1657	1663	1665	rBV7	1812	3146	0.12%	0.019%
31	13.080	1697	1699	1703	rVB5	2101	2828	0.10%	0.017%
32	13.269	1727	1731	1732	rBV5	2686	3064	0.11%	0.018%
33	13.369	1743	1748	1750	rBV5	5093	6468	0.24%	0.039%
34	13.939	1839	1845	1857	rBV	214851	345986	12.82%	2.062%
35	14.216	1886	1892	1903	rBV	232090	363434	13.47%	2.166%
36	14.433	1925	1929	1934	rVB7	4289	7152	0.27%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
 Data File : BP010420.D
 Acq On : 20 May 2022 01:09
 Operator : CG/JU
 Sample : N2918-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	14.527	1938	1945	1953	rBV	1368784	2119571	78.56%	12.630%
38	14.927	2010	2013	2016	rBV5	2469	3241	0.12%	0.019%
39	15.174	2052	2055	2059	rVB6	2187	3197	0.12%	0.019%
40	15.522	2108	2114	2126	rBV	309051	496818	18.41%	2.960%
41	15.645	2130	2135	2145	rVV	47588	95930	3.56%	0.572%
42	15.763	2149	2155	2162	rVV	5460	9842	0.36%	0.059%
43	16.310	2243	2248	2251	rVB7	3567	5285	0.20%	0.031%
44	16.580	2293	2294	2300	rVB6	2549	2925	0.11%	0.017%
45	16.851	2338	2340	2343	rBV3	2804	2718	0.10%	0.016%
46	16.986	2357	2363	2367	rVB8	3325	6460	0.24%	0.038%
47	17.039	2370	2372	2374	rBV2	2618	2914	0.11%	0.017%
48	17.063	2374	2376	2381	rVB6	4074	5213	0.19%	0.031%
49	17.274	2405	2412	2424	rBV	1738065	2601275	96.42%	15.500%
50	17.380	2424	2430	2443	rVB2	345609	581058	21.54%	3.462%
51	17.851	2508	2510	2515	rBV6	2669	3719	0.14%	0.022%
52	17.951	2523	2527	2535	rVB6	9300	15774	0.58%	0.094%
53	18.163	2560	2563	2571	rBV7	20049	31923	1.18%	0.190%
54	18.239	2571	2576	2579	rBV7	4487	7764	0.29%	0.046%
55	19.257	2747	2749	2754	rBV6	6843	11194	0.41%	0.067%
56	19.610	2803	2809	2816	rBV	542096	767674	28.45%	4.574%
57	21.068	3053	3057	3061	rBV3	105725	146966	5.45%	0.876%
58	21.362	3101	3107	3120	rBV	1915582	2697923	100.00%	16.076%
59	23.627	3487	3492	3497	rBV	260062	479548	17.77%	2.857%
60	23.786	3512	3519	3531	rVB2	1056378	2282096	84.59%	13.598%




Sum of corrected areas: 16782602

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010420.D
Acq On : 20 May 2022 01:09
Operator : CG/JU
Sample : N2918-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

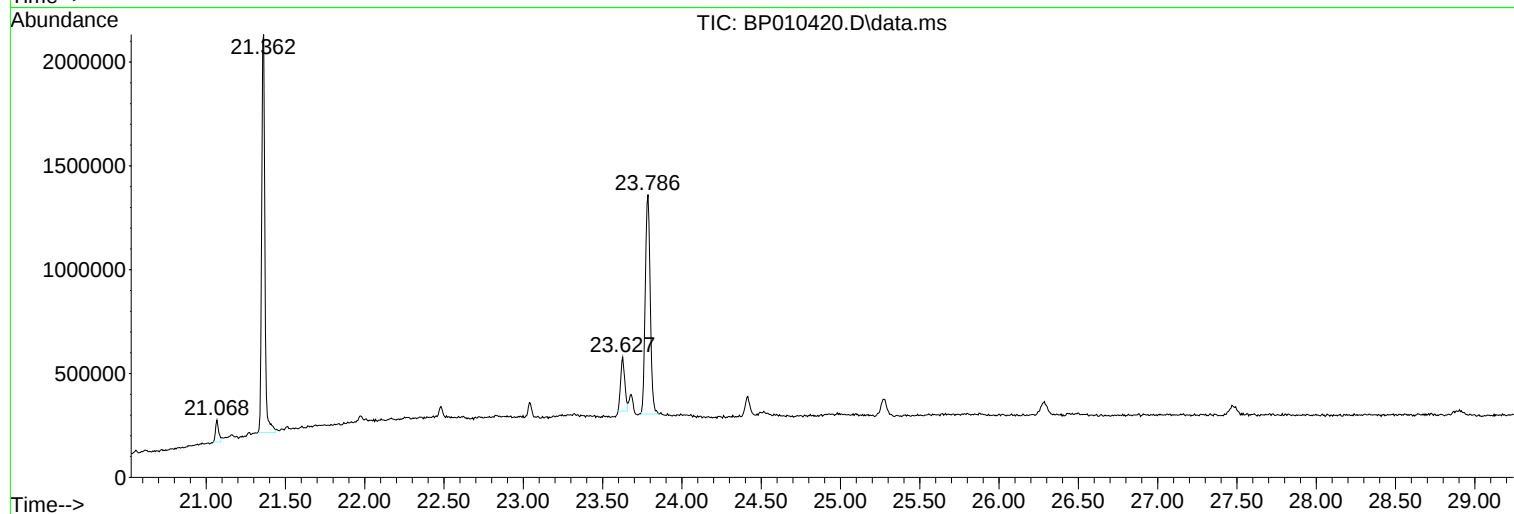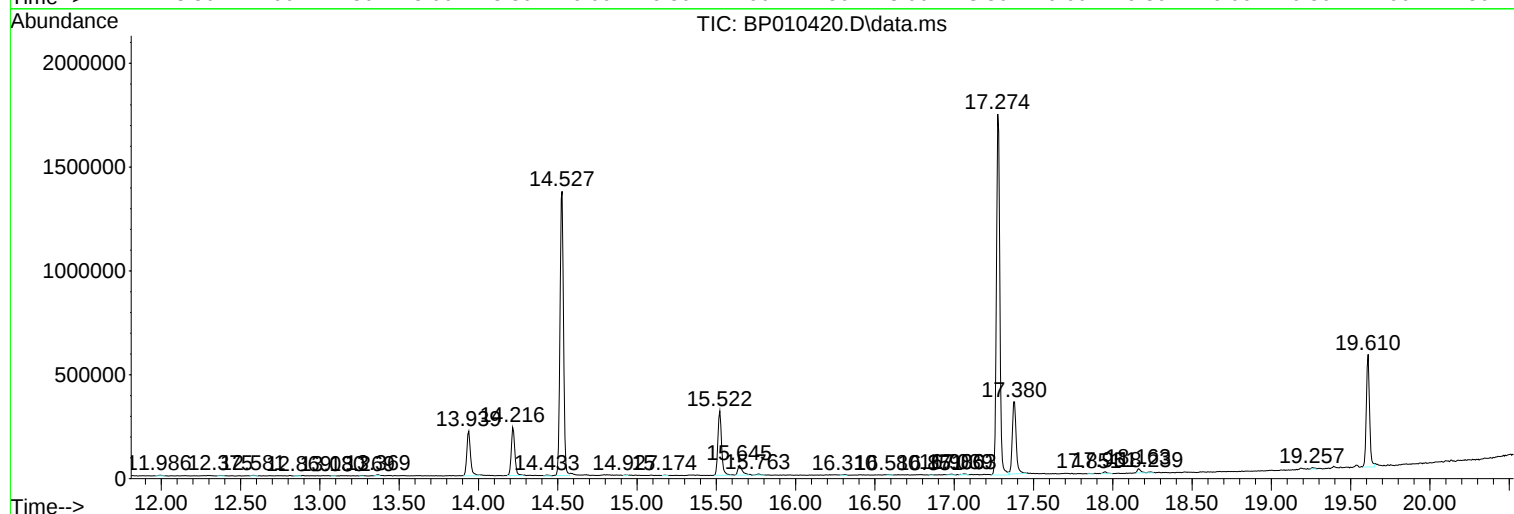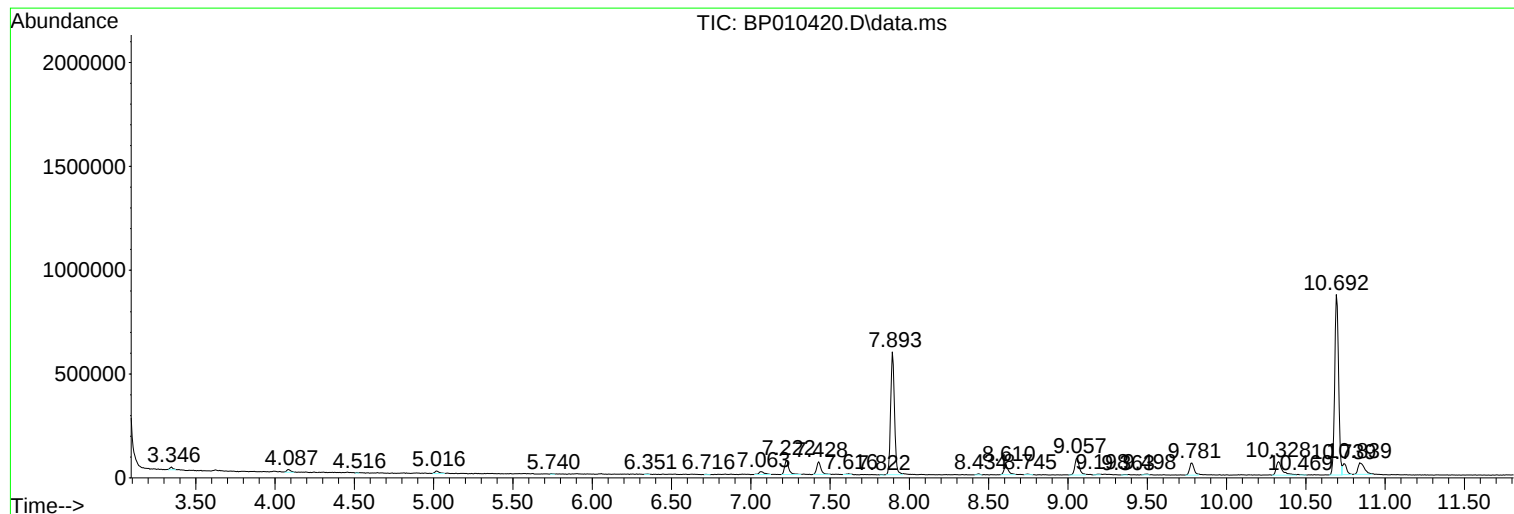

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010420.D
Acq On : 20 May 2022 01:09
Operator : CG/JU
Sample : N2918-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051922\
Data File : BP010420.D
Acq On : 20 May 2022 01:09
Operator : CG/JU
Sample : N2918-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc