

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015183.D
 Acq On : 19 May 2023 20:57
 Operator : CG/JU
 Sample : 02689-08MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREM0MSD

Quant Time: May 19 22:14:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	251233	20.000	ng/u1	0.00
20) Naphthalene-d8	10.957	136	1099653	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.763	164	701529	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.522	188	1510686	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	959633	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	1012857	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	22234	3.439	ng/uL	0.00
4) Pyridine-d5	3.875	84	251927	13.745	ng/u1	0.00
7) Phenol-d5	7.281	99	608909	26.104	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	371162	27.550	ng/u1	0.00
11) 2-Chlorophenol-d4	7.652	132	488484	28.482	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	503963	27.113	ng/u1	0.00
21) Nitrobenzene-d5	9.305	128	265286	30.701	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	298756	31.073	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	545507	31.442	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	650480	25.340	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	1744957	32.917	ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	1944903	32.078	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	283334	27.525	ng/u1	0.00
60) Fluorene-d10	15.757	176	1482492	33.142	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	239818	25.190	ng/u1	0.00
73) Anthracene-d10	17.616	188	2244650	32.449	ng/u1	0.00
81) Pyrene-d10	19.839	212	2391770	42.973	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	1762205	35.048	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.470	88	54994	7.915	ng/uL	96
5) Pyridine	3.893	79	342782	17.982	ng/u1	97
6) Benzaldehyde	7.258	77	302255	47.143	ng/u1	98
8) Phenol	7.310	94	602000	25.168	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.540	93	463656	24.228	ng/u1	98
12) 2-Chlorophenol	7.687	128	450501	24.833	ng/u1	98
13) 2-Methylphenol	8.575	108	426889	23.092	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.663	45	583297	24.328	ng/u1	99
16) Acetophenone	8.963	105	755291	26.036	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.946	70	382084	25.113	ng/u1	97
18) 4-Methylphenol	8.905	108	499586	24.553	ng/u1	98
19) Hexachloroethane	9.222	117	184651	24.928	ng/u1	87
22) Nitrobenzene	9.346	77	565755	26.510	ng/u1	99
23) Isophorone	9.875	82	1129320	25.744	ng/u1	99
25) 2-Nitrophenol	10.063	139	284580	26.991	ng/u1	93
26) 2,4-Dimethylphenol	10.116	107	256936	12.212	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.357	93	682582	25.574	ng/u1	98
29) 2,4-Dichlorophenol	10.599	162	486749	27.775	ng/u1	99
30) Naphthalene	11.010	128	1579611	26.422	ng/u1	100
32) 4-Chloroaniline	11.116	127	537458	20.371	ng/u1	99
33) Hexachlorobutadiene	11.287	225	314198	29.747	ng/u1	96
34) Caprolactam	11.904	113	136648	20.682	ng/u1	97
35) 4-Chloro-3-methylphenol	12.234	107	545119	27.548	ng/u1	97
36) 2-Methylnaphthalene	12.604	142	1084902	26.933	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015183.D
 Acq On : 19 May 2023 20:57
 Operator : CG/JU
 Sample : 02689-08MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREM0MSD

Quant Time: May 19 22:14:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.822	142	1118064	27.639	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.969	216	611698	29.155	ng/ul	99
40) Hexachlorocyclopentadiene	12.940	237	213168	15.681	ng/ul	99
41) 2,4,6-Trichlorophenol	13.204	196	414577	27.983	ng/ul	98
42) 2,4,5-Trichlorophenol	13.281	196	470266	29.275	ng/ul	99
43) 1,1'-Biphenyl	13.604	154	1498547	27.532	ng/ul	98
44) 2-Chloronaphthalene	13.645	162	1183930	27.853	ng/ul	99
45) 2-Nitroaniline	13.851	65	362680	29.820	ng/ul	95
47) Dimethylphthalate	14.216	163	1557905	28.219	ng/ul	100
48) 2,6-Dinitrotoluene	14.345	165	333574	30.498	ng/ul	96
50) Acenaphthylene	14.492	152	1821144	26.920	ng/ul	100
51) 3-Nitroaniline	14.675	138	330584	33.566	ng/ul	98
52) Acenaphthene	14.834	153	1255870	27.181	ng/ul	99
53) 2,4-Dinitrophenol	14.881	184	155994	21.480	ng/ul	97
55) 4-Nitrophenol	14.981	109	241958	31.958	ng/ul	88
56) Dibenzofuran	15.163	168	1790332	27.858	ng/ul	99
57) 2,4-Dinitrotoluene	15.128	165	488600	30.871	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.392	232	410321	30.266	ng/ul	93
59) Diethylphthalate	15.575	149	1643562	29.848	ng/ul	99
61) Fluorene	15.816	166	1450188	28.080	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.798	204	740423	29.342	ng/ul	96
63) 4-Nitroaniline	15.834	138	356623	41.931	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.892	198	248478	25.289	ng/ul	99
67) N-Nitrosodiphenylamine	16.016	169	1301858	29.308	ng/ul	99
68) 4-Bromophenyl-phenylether	16.698	248	501248	32.213	ng/ul	99
69) Hexachlorobenzene	16.822	284	592968	32.247	ng/ul	98
70) Atrazine	16.969	200	339046	20.650	ng/ul	99
71) Pentachlorophenol	17.163	266	310113	26.961	ng/ul	96
72) Phenanthrene	17.563	178	2438954	29.648	ng/ul	99
74) Anthracene	17.651	178	2342353	28.158	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.569	216	623912	29.129	ng/ul	99
76) Pentachlorobenzene	15.087	250	637818	29.657	ng/ul	100
77) Carbazole	17.922	167	2225552	30.511	ng/ul	99
78) Di-n-butylphthalate	18.445	149	3003224	31.971	ng/ul	99
80) Fluoranthene	19.510	202	2685389	39.586	ng/ul	98
82) Pyrene	19.869	202	2661096	37.987	ng/ul	96
83) Butylbenzylphthalate	20.716	149	1196306	38.521	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.498	252	458294	21.745	ng/ul	99
85) Benzo(a)anthracene	21.580	228	2121683	31.975	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.474	149	1681171	37.601	ng/ul	99
87) Chrysene	21.633	228	2017740	31.811	ng/ul	98
89) Di-n-octyl phthalate	22.445	149	2577173	37.152	ng/ul	100
90) Benzo(b)fluoranthene	23.368	252	2035653	31.703	ng/ul	99
91) Benzo(k)fluoranthene	23.416	252	1914552	31.052	ng/ul	99
93) Benzo(a)pyrene	24.039	252	1702842	30.003	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.868	276	2363814	32.167	ng/ul	97
95) Dibenzo(a,h)anthracene	26.886	278	1947710	32.287	ng/ul	98
96) Benzo(g,h,i)perylene	27.704	276	1781746	29.733	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015183.D
 Acq On : 19 May 2023 20:57
 Operator : CG/JU
 Sample : 02689-08MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREM0MSD

Quant Time: May 19 22:14:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration




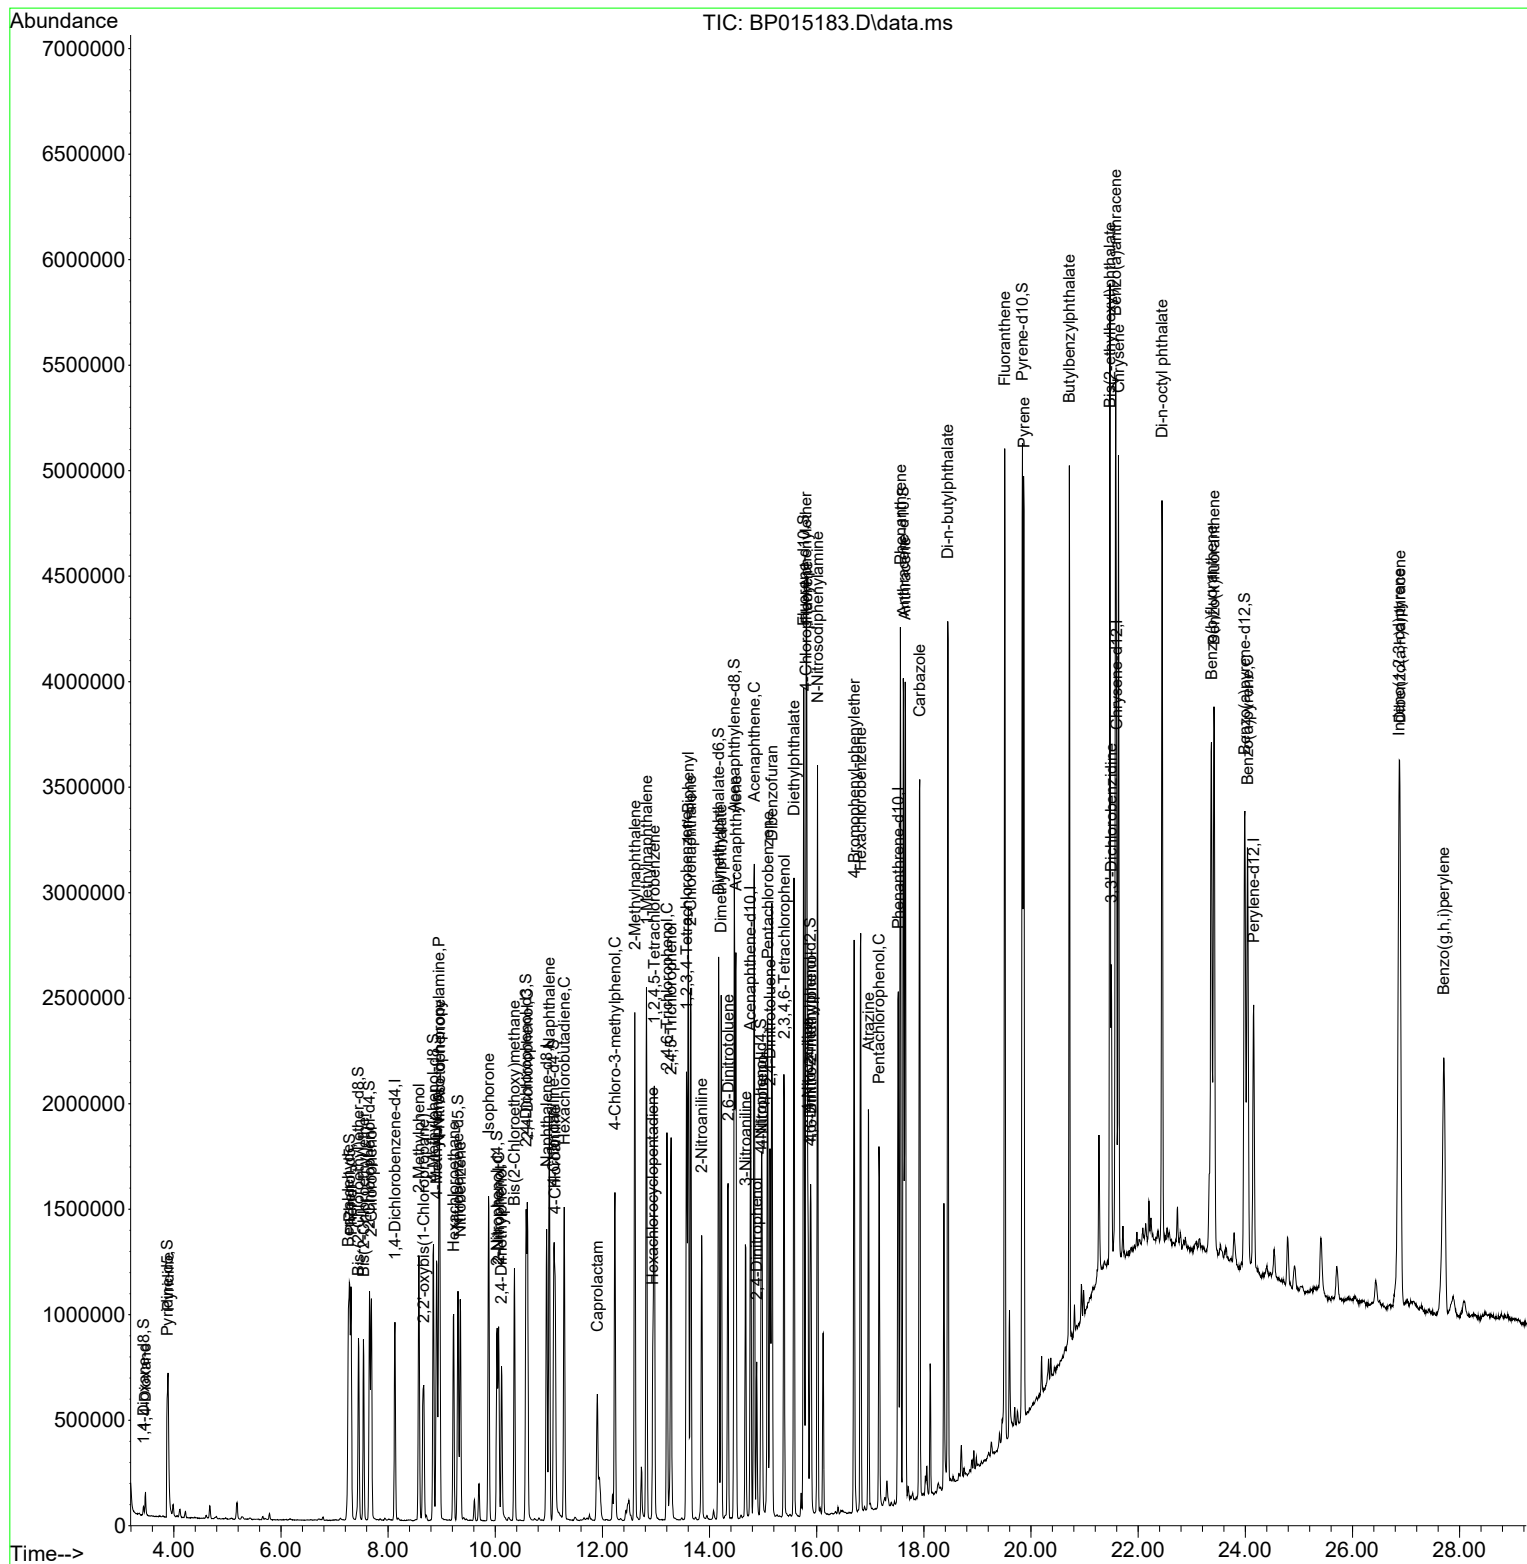




#2
1,4-Dioxane
Concen: 7.915 ng/uL
RT: 3.470 min Scan# 41
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion: 88	Resp: 54994
Ion Ratio	Lower Upper
88 100	
43 28.9	20.4 30.6
58 71.8	55.4 83.2



#5
Pyridine
Concen: 17.982 ng/uL
RT: 3.893 min Scan# 120
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion: 79	Resp: 342782
Ion Ratio	Lower Upper
79 100	
52 68.7	55.4 83.2
51 35.6	25.4 38.2









#6
Benzaldehyde
Concen: 47.143 ng/ul
RT: 7.258 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion: 77 Resp: 302255
Ion Ratio Lower Upper
77 100
105 99.4 76.9 115.3
106 93.8 75.0 112.6

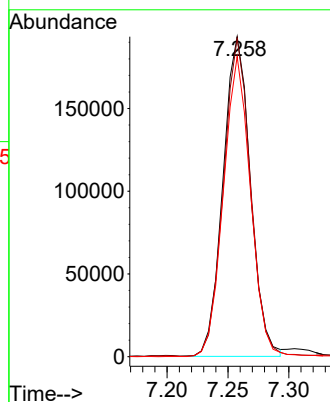

#8
Phenol
Concen: 25.168 ng/ul
RT: 7.310 min Scan# 701
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion: 94 Resp: 602000
Ion Ratio Lower Upper
94 100
65 27.6 20.6 31.0
66 36.7 26.1 39.1









#10
Bis(2-Chloroethyl)ether
Concen: 24.228 ng/ul
RT: 7.540 min Scan# 741
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion: 93 Resp: 463656
Ion Ratio Lower Upper
93 100
63 74.4 58.0 87.0
95 32.3 26.4 39.6



#12
2-Chlorophenol
Concen: 24.833 ng/ul
RT: 7.687 min Scan# 765
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:128 Resp: 450501
Ion Ratio Lower Upper
128 100
64 46.3 36.2 54.2
130 31.7 26.3 39.5





#13

2-Methylphenol

Concen: 23.092 ng/ul

RT: 8.575 min Scan# 91

Delta R.T. 0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :





JREM0MSD

Tgt Ion:108 Resp: 426889

Ion Ratio Lower Upper

108 100

107 89.8 71.8 107.6

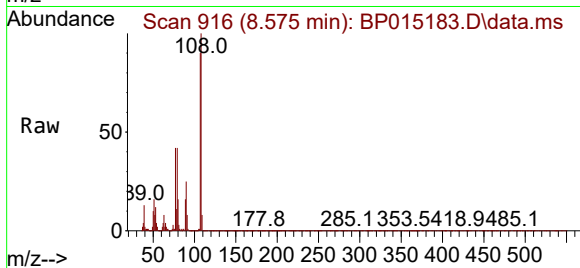

#14

2,2'-oxybis(1-Chloropropane)

Concen: 24.328 ng/ul

RT: 8.663 min Scan# 931

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion: 45 Resp: 583297


Ion Ratio Lower Upper

45 100

77 16.4 12.8 19.2

79 12.3 9.5 14.3



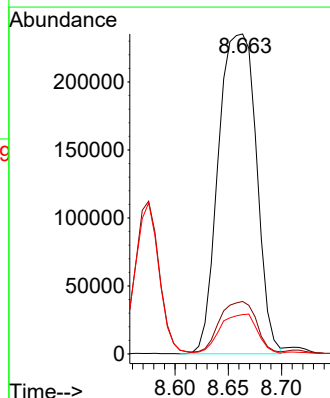
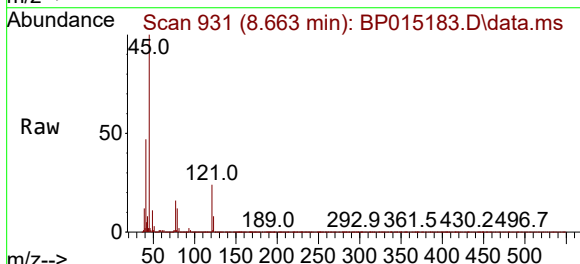




#16
Acetophenone
Concen: 26.036 ng/ul
RT: 8.963 min Scan# 948
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:105 Resp: 755291
Ion Ratio Lower Upper
105 100
77 77.5 59.4 89.2
51 25.8 19.2 28.8



#17
N-Nitroso-di-n-propylamine
Concen: 25.113 ng/ul
RT: 8.946 min Scan# 979
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion: 70 Resp: 382084
Ion Ratio Lower Upper
70 100
42 53.9 41.0 61.6
101 10.0 7.9 11.9
130 21.6 16.1 24.1









#18
4-Methylphenol
Concen: 24.553 ng/ul
RT: 8.905 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:108 Resp: 499586
Ion Ratio Lower Upper
108 100
107 112.9 88.5 132.7



#19
Hexachloroethane
Concen: 24.928 ng/ul
RT: 9.222 min Scan# 1026
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:117 Resp: 184651
Ion Ratio Lower Upper
117 100
201 108.0 75.8 113.8
199 66.4 46.5 69.7

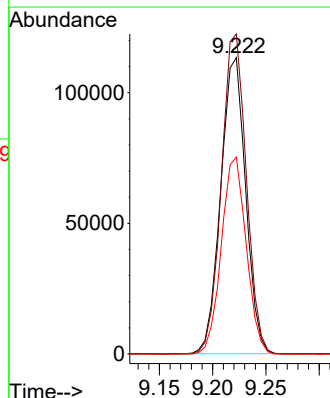



#22

Nitrobenzene

Concen: 26.510 ng/ul

RT: 9.346 min Scan# 1107

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion: 77 Resp: 565755

Ion Ratio Lower Upper

77 100

123 44.8 36.2 54.2

65 12.9 10.1 15.1



#23

Isophorone

Concen: 25.744 ng/ul

RT: 9.875 min Scan# 1137

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion: 82 Resp: 1129320


Ion Ratio Lower Upper

82 100

95 7.3 5.4 8.0

138 17.3 13.6 20.4



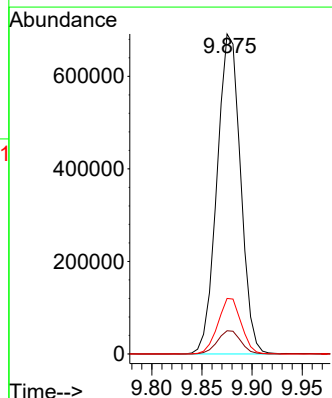





#25
2-Nitrophenol
Concen: 26.991 ng/ul
RT: 10.063 min Scan# 1135
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:139 Resp: 284580
Ion Ratio Lower Upper
139 100
65 51.3 38.4 57.6
109 32.6 22.2 33.2



#26
2,4-Dimethylphenol
Concen: 12.212 ng/ul
RT: 10.116 min Scan# 1178
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:107 Resp: 256936
Ion Ratio Lower Upper
107 100
121 49.4 41.0 61.6
122 83.5 69.5 104.3





#27

Bis(2-Chloroethoxy)methane

Concen: 25.574 ng/ul

RT: 10.357 min Scan# 1185

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion: 93 Resp: 682582

Ion Ratio Lower Upper

93 100

95 32.4 26.7 40.1

123 10.9 9.1 13.7



#29

2,4-Dichlorophenol

Concen: 27.775 ng/ul

RT: 10.599 min Scan# 1260

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:162 Resp: 486749


Ion Ratio Lower Upper

162 100

164 66.1 52.0 78.0

98 36.5 28.9 43.3









#30
Naphthalene
Concen: 26.422 ng/ul
RT: 11.010 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:128 Resp: 1579611
Ion Ratio Lower Upper
128 100
129 10.9 8.9 13.3
127 13.1 10.6 15.8

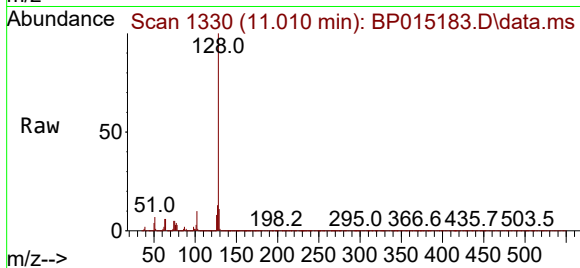

#32
4-Chloroaniline
Concen: 20.371 ng/ul
RT: 11.116 min Scan# 1348
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:127 Resp: 537458
Ion Ratio Lower Upper
127 100
129 31.7 25.8 38.8




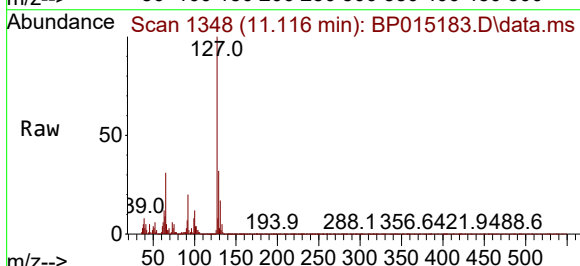




#33
Hexachlorobutadiene
Concen: 29.747 ng/ul
RT: 11.287 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:225 Resp: 314198
Ion Ratio Lower Upper
225 100
223 61.6 51.0 76.6
227 61.8 52.2 78.4

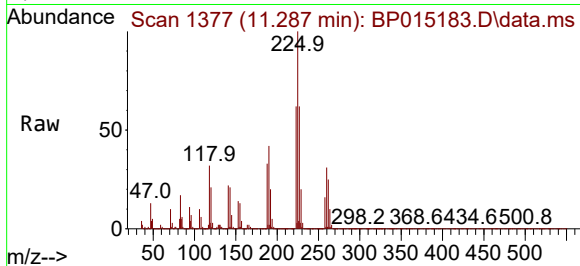

#34
Caprolactam
Concen: 20.682 ng/ul
RT: 11.904 min Scan# 1482
Delta R.T. 0.012 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:113 Resp: 136648
Ion Ratio Lower Upper
113 100
55 155.7 121.2 181.8
56 115.4 90.2 135.4




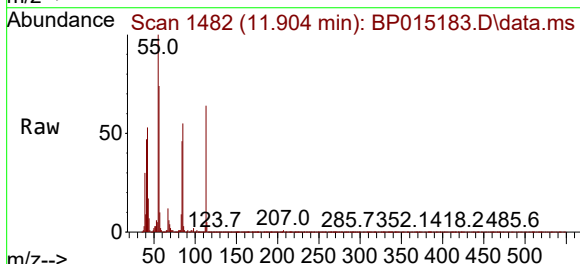




#35
4-Chloro-3-methylphenol
Concen: 27.548 ng/ul
RT: 12.234 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:107 Resp: 545119
Ion Ratio Lower Upper
107 100
144 24.9 20.3 30.5
142 76.4 63.2 94.8

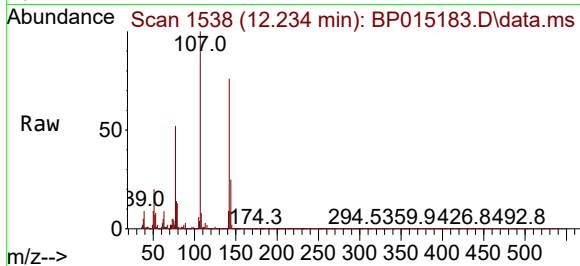

#36
2-Methylnaphthalene
Concen: 26.933 ng/ul
RT: 12.604 min Scan# 1601
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:142 Resp: 1084902
Ion Ratio Lower Upper
142 100
141 88.2 71.0 106.6



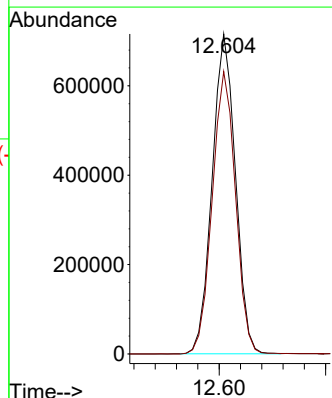
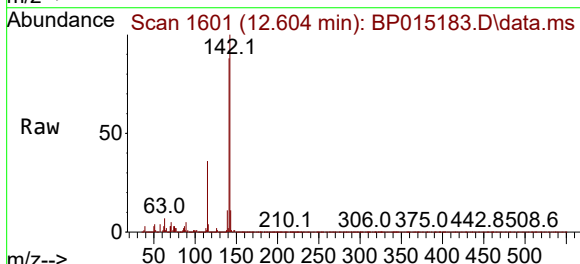




#37
1-Methylnaphthalene
Concen: 27.639 ng/ul
RT: 12.822 min Scan# 1604
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:142 Resp: 1118064
Ion Ratio Lower Upper
142 100
141 91.1 74.6 112.0
116 3.8 2.9 4.3

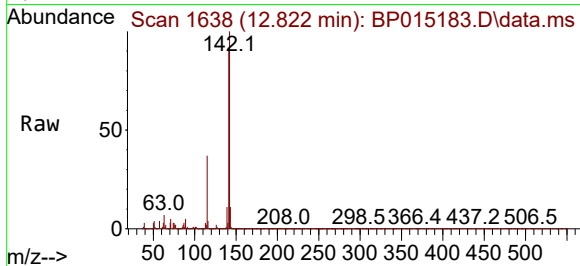

#39
1,2,4,5-Tetrachlorobenzene
Concen: 29.155 ng/ul
RT: 12.969 min Scan# 1663
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:216 Resp: 611698
Ion Ratio Lower Upper
216 100
214 77.9 61.4 92.0
179 20.7 15.9 23.9
108 16.6 13.7 20.5




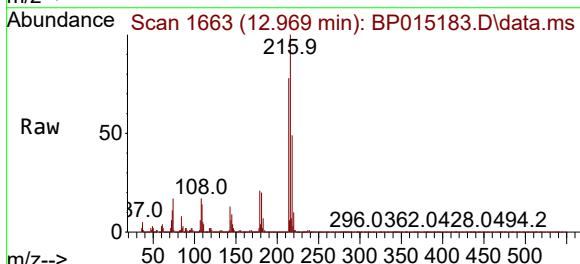




#40
Hexachlorocyclopentadiene
Concen: 15.681 ng/ul
RT: 12.940 min Scan# 1703
Delta R.T. -0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:237 Resp: 213168
Ion Ratio Lower Upper
237 100
235 61.4 49.4 74.0
272 12.0 10.4 15.6

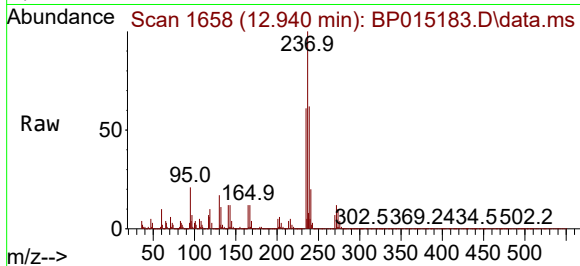

#41
2,4,6-Trichlorophenol
Concen: 27.983 ng/ul
RT: 13.204 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:196 Resp: 414577
Ion Ratio Lower Upper
196 100
198 96.2 75.5 113.3
200 30.0 23.6 35.4




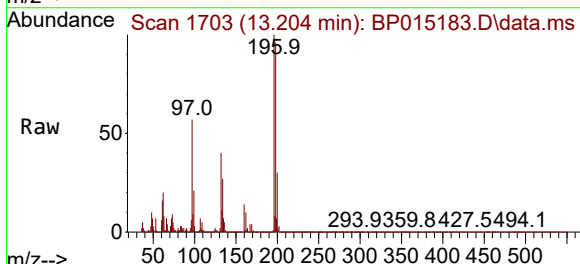




#42
2,4,5-Trichlorophenol
Concen: 29.275 ng/ul
RT: 13.281 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:196 Resp: 470266
Ion Ratio Lower Upper
196 100
198 95.4 77.0 115.4
200 30.8 24.3 36.5

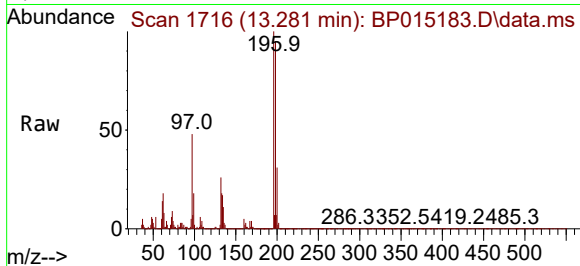

#43
1,1'-Biphenyl
Concen: 27.532 ng/ul
RT: 13.604 min Scan# 1771
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:154 Resp: 1498547
Ion Ratio Lower Upper
154 100
153 39.9 32.7 49.1
76 12.6 10.7 16.1

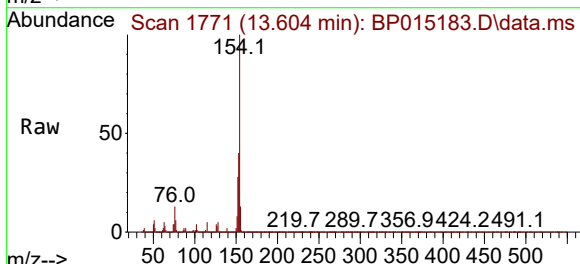



#44

2-Chloronaphthalene

Concen: 27.853 ng/ul

RT: 13.645 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:162 Resp: 1183930

Ion Ratio Lower Upper

162 100

164 32.6 25.9 38.9

127 39.8 30.8 46.2

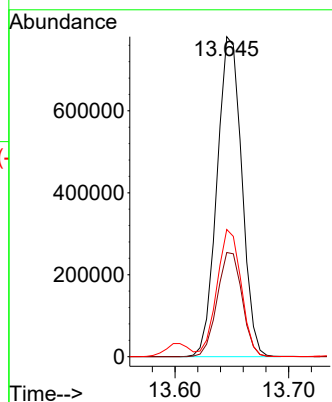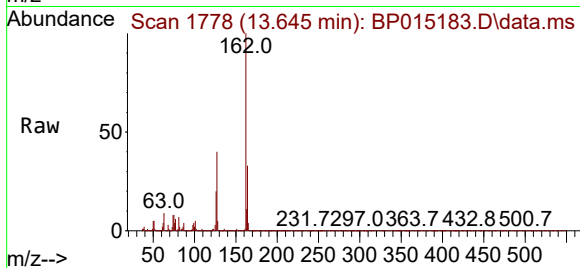

#45

2-Nitroaniline

Concen: 29.820 ng/ul

RT: 13.851 min Scan# 1813

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion: 65 Resp: 362680


Ion Ratio Lower Upper

65 100

92 71.6 59.8 89.8

138 108.9 92.3 138.5


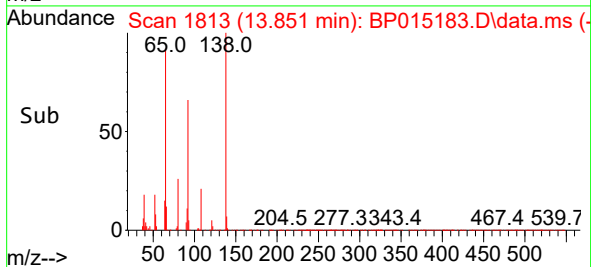

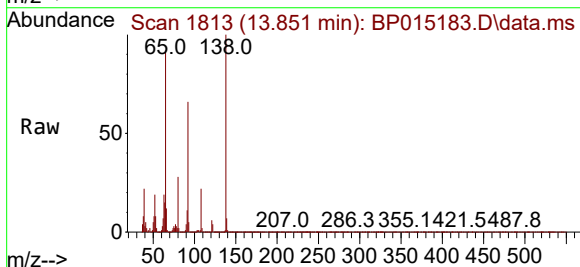




#47
Dimethylphthalate
Concen: 28.219 ng/ul
RT: 14.216 min Scan# 1875
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:163 Resp: 1557905
Ion Ratio Lower Upper
163 100
194 4.1 3.1 4.7
164 10.3 8.2 12.4

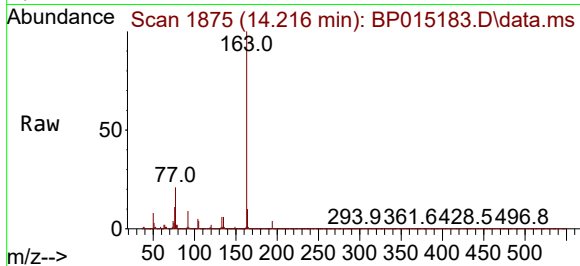

#48
2,6-Dinitrotoluene
Concen: 30.498 ng/ul
RT: 14.345 min Scan# 1897
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:165 Resp: 333574
Ion Ratio Lower Upper
165 100
89 56.0 48.0 72.0
121 20.7 17.5 26.3




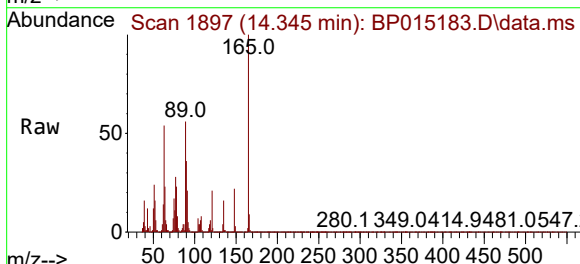




#50
Acenaphthylene
Concen: 26.920 ng/ul
RT: 14.492 min Scan# 1888
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:152 Resp: 1821144
Ion Ratio Lower Upper
152 100
151 20.1 16.1 24.1
153 12.8 10.3 15.5



#51
3-Nitroaniline
Concen: 33.566 ng/ul
RT: 14.675 min Scan# 1953
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:138 Resp: 330584
Ion Ratio Lower Upper
138 100
108 10.6 8.8 13.2
92 113.9 93.4 140.0

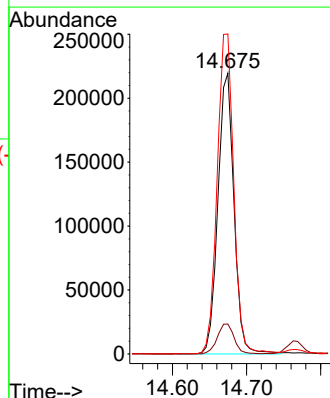



#52

Acenaphthene

Concen: 27.181 ng/ul

RT: 14.834 min Scan# 1946

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:153 Resp: 1255870

Ion Ratio Lower Upper

153 100

152 47.8 38.0 57.0

154 87.8 71.0 106.4

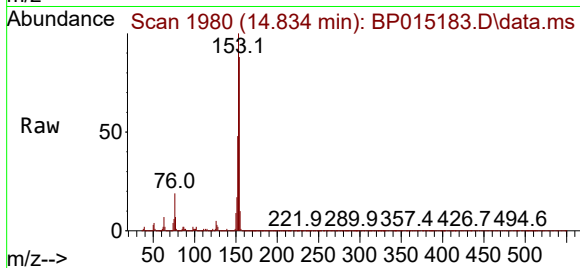

#53

2,4-Dinitrophenol

Concen: 21.480 ng/ul

RT: 14.881 min Scan# 1988

Delta R.T. 0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:184 Resp: 155994


Ion Ratio Lower Upper

184 100

63 62.3 49.7 74.5

154 64.5 47.5 71.3


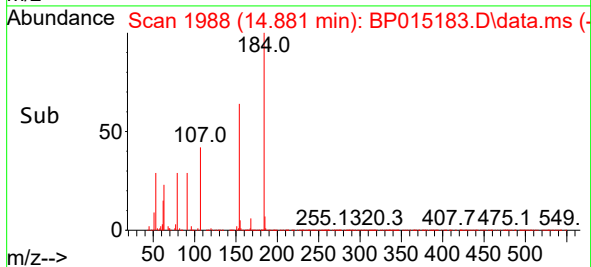

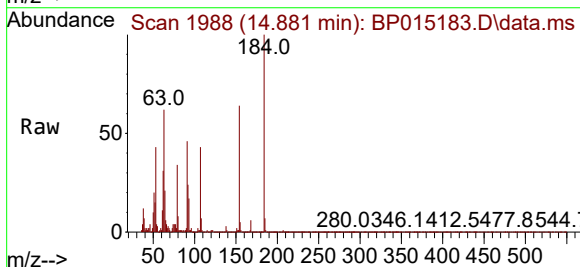




#55
4-Nitrophenol
Concen: 31.958 ng/ul
RT: 14.981 min Scan# 2005
Delta R.T. 0.012 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:109 Resp: 241958
Ion Ratio Lower Upper
109 100
139 130.4 115.3 172.9
65 119.0 107.9 161.9



#56
Dibenzofuran
Concen: 27.858 ng/ul
RT: 15.163 min Scan# 2036
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:168 Resp: 1790332
Ion Ratio Lower Upper
168 100
139 37.3 29.4 44.0









#57
2,4-Dinitrotoluene
Concen: 30.871 ng/ul
RT: 15.128 min Scan# 2075
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:165 Resp: 488600
Ion Ratio Lower Upper
165 100
63 43.1 33.1 49.7
182 2.6 2.1 3.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 30.266 ng/ul
RT: 15.392 min Scan# 2075
Delta R.T. 0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:232 Resp: 410321
Ion Ratio Lower Upper
232 100
131 40.0 36.8 55.2
130 2.1 1.9 2.9
166 28.7 24.6 37.0





#59

Diethylphthalate

Concen: 29.848 ng/ul

RT: 15.575 min Scan# 2106

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:149 Resp: 1643562

Ion Ratio Lower Upper

149 100

177 22.5 17.5 26.3

150 12.7 9.8 14.8

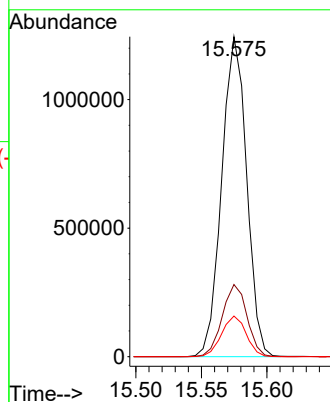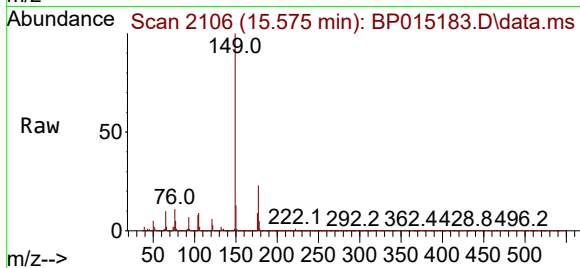

#61

Fluorene

Concen: 28.080 ng/ul

RT: 15.816 min Scan# 2147

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:166 Resp: 1450188


Ion Ratio Lower Upper

166 100

165 98.5 77.8 116.6

167 13.2 10.6 15.8



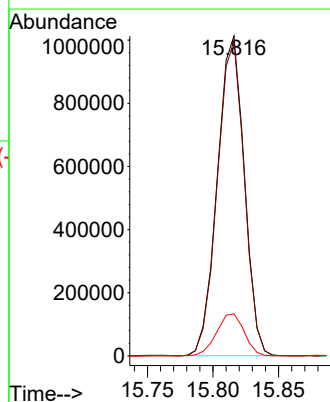
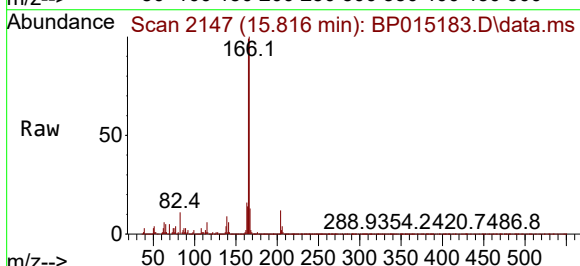




#62
4-Chlorophenyl-phenylether
Concen: 29.342 ng/ul
RT: 15.798 min Scan# 2111
Delta R.T. -0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:204 Resp: 740423
Ion Ratio Lower Upper
204 100
206 33.4 26.1 39.1
141 59.3 44.5 66.7

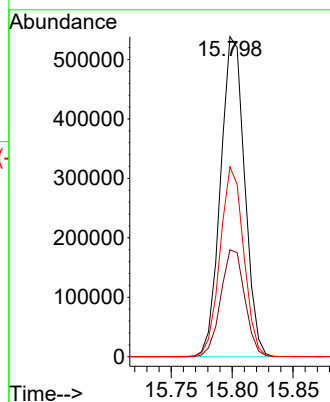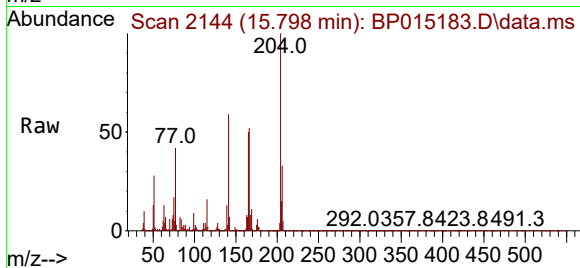

#63
4-Nitroaniline
Concen: 41.931 ng/ul
RT: 15.834 min Scan# 2150
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:138 Resp: 356623
Ion Ratio Lower Upper
138 100
92 52.6 41.2 61.8
108 83.8 60.1 90.1


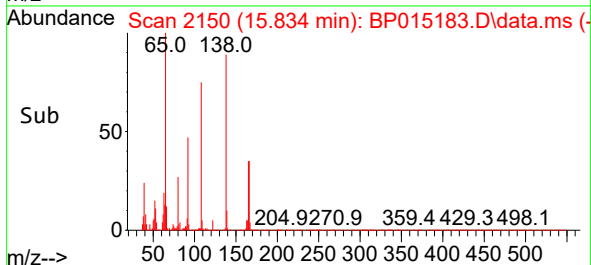

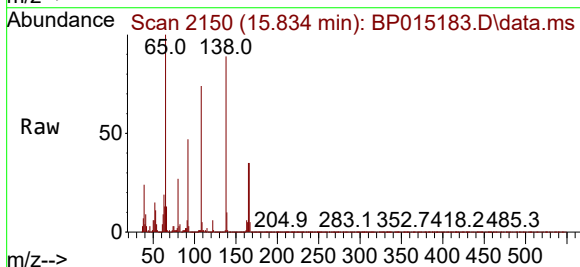




#66
4,6-Dinitro-2-methylphenol
Concen: 25.289 ng/ul
RT: 15.892 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:198 Resp: 248478
Ion Ratio Lower Upper
198 100
182 3.8 3.7 5.5
77 25.9 21.2 31.8

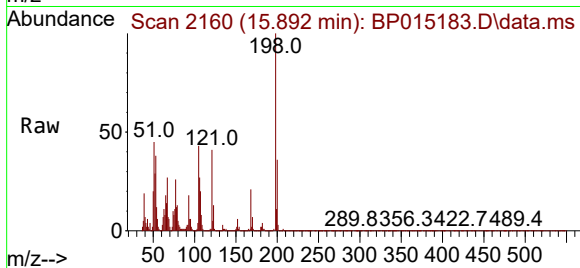

#67
N-Nitrosodiphenylamine
Concen: 29.308 ng/ul
RT: 16.016 min Scan# 2181
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:169 Resp: 1301858
Ion Ratio Lower Upper
169 100
168 66.1 53.5 80.3
167 36.3 28.9 43.3




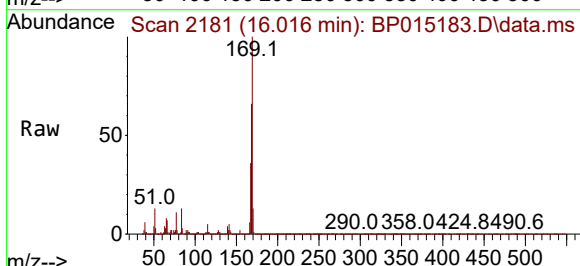




#68
4-Bromophenyl-phenylether
Concen: 32.213 ng/ul
RT: 16.698 min Scan# 2118
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:248 Resp: 501248
Ion Ratio Lower Upper
248 100
250 99.3 79.0 118.4
141 72.7 58.6 87.8



#69
Hexachlorobenzene
Concen: 32.247 ng/ul
RT: 16.822 min Scan# 2318
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:284 Resp: 592968
Ion Ratio Lower Upper
284 100
142 32.0 27.3 40.9
249 31.0 24.6 36.8





#70

Atrazine

Concen: 20.650 ng/ul

RT: 16.969 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:200 Resp: 339046

Ion Ratio Lower Upper

200 100

173 26.4 21.4 32.2

215 48.1 38.1 57.1

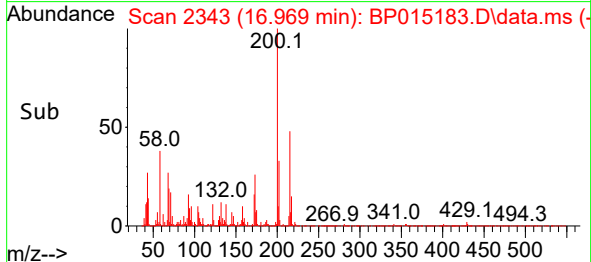

#71

Pentachlorophenol

Concen: 26.961 ng/ul

RT: 17.163 min Scan# 2376

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:266 Resp: 310113


Ion Ratio Lower Upper

266 100

264 61.5 51.0 76.4

268 60.9 51.8 77.6

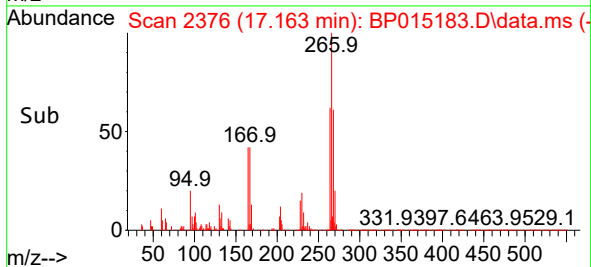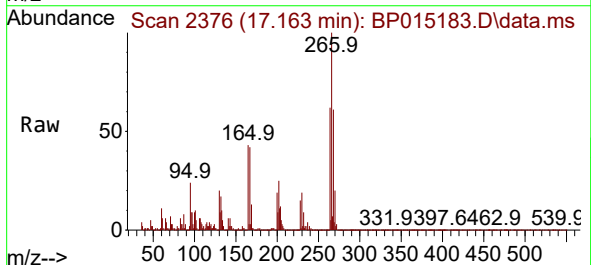



#72

Phenanthrene

Concen: 29.648 ng/ul

RT: 17.563 min Scan# 2410

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:178 Resp: 2438954

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.2

176 19.0 15.6 23.4

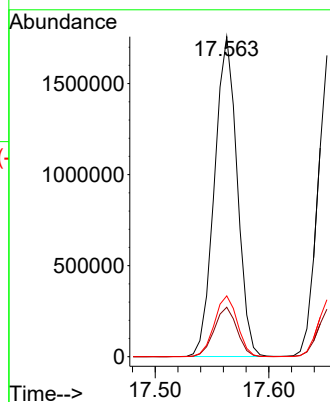

#74

Anthracene

Concen: 28.158 ng/ul

RT: 17.651 min Scan# 2459

Delta R.T. -0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:178 Resp: 2342353


Ion Ratio Lower Upper

178 100

179 15.8 12.2 18.2

176 18.9 15.2 22.8





#75

1,2,3,4-Tetrachlorobenzene

Concen: 29.129 ng/uL

RT: 13.569 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:216 Resp: 623912

Ion Ratio Lower Upper

216 100

214 79.3 62.2 93.4

218 48.2 38.2 57.2

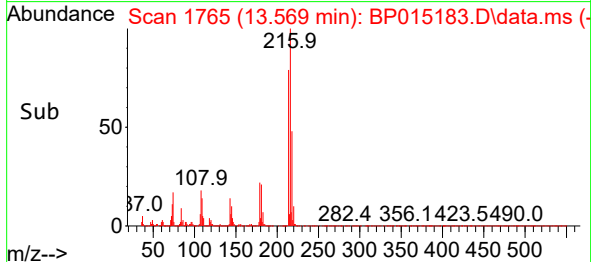

#76

Pentachlorobenzene

Concen: 29.657 ng/uL

RT: 15.087 min Scan# 2023

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:250 Resp: 637818


Ion Ratio Lower Upper

250 100

248 62.6 49.8 74.6

252 64.3 51.6 77.4


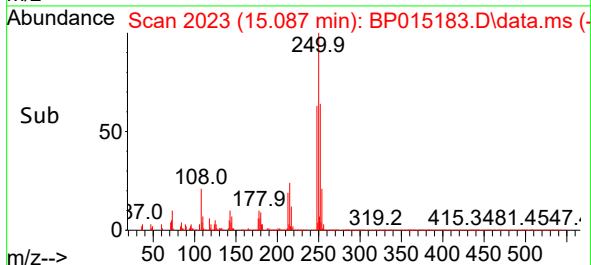
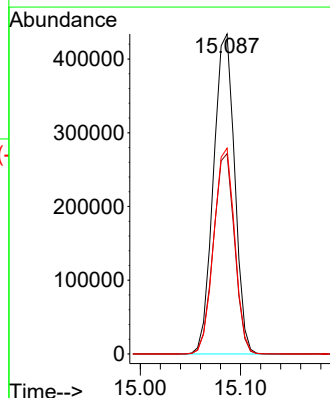
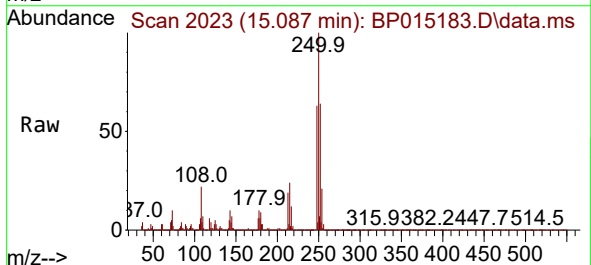




#77
 Carbazole
 Concen: 30.511 ng/ul
 RT: 17.922 min Scan# 2471
 Delta R.T. 0.006 min
 Lab File: BP015183.D
 Acq: 19 May 2023 20:57




Instrument :
 BNA_P
 ClientSampleId :
 JREM0MSD


Tgt Ion:167 Resp: 2225552
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.4 26.2
 139 12.4 10.2 15.4



#78
 Di-n-butylphthalate
 Concen: 31.971 ng/ul
 RT: 18.445 min Scan# 2594
 Delta R.T. -0.006 min
 Lab File: BP015183.D
 Acq: 19 May 2023 20:57

Tgt Ion:149 Resp: 3003224
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.3 10.9
 104 5.3 3.9 5.9

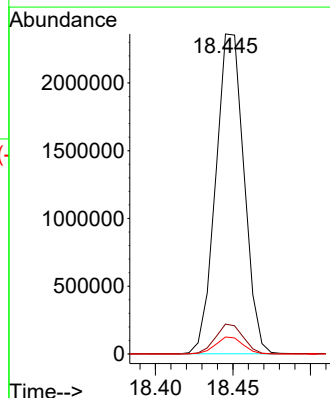



#80

Fluoranthene

Concen: 39.586 ng/ul

RT: 19.510 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:202 Resp: 2685389

Ion Ratio Lower Upper

202 100

101 11.2 9.5 14.3

100 8.6 7.3 10.9

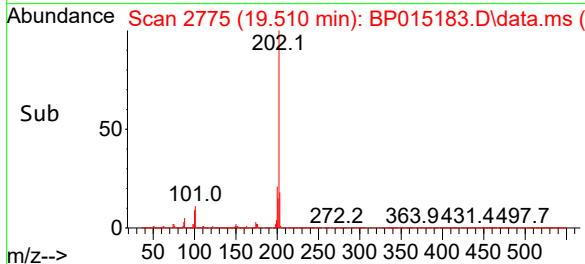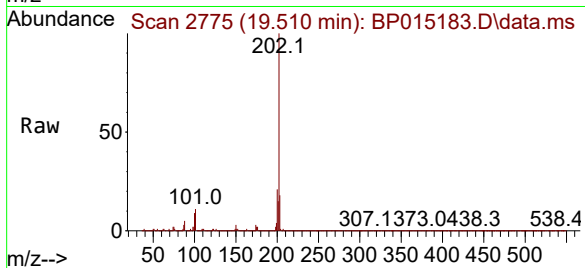

#82

Pyrene

Concen: 37.987 ng/ul

RT: 19.869 min Scan# 2836

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:202 Resp: 2661096


Ion Ratio Lower Upper

202 100

101 11.9 11.2 16.8

100 9.9 9.0 13.6

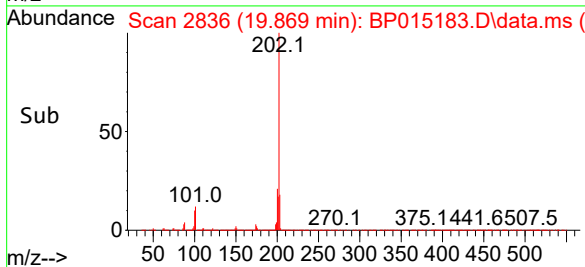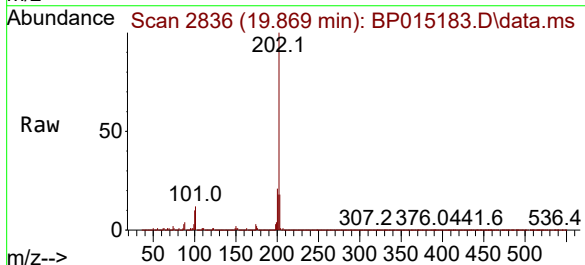



#83

Butylbenzylphthalate

Concen: 38.521 ng/ul

RT: 20.716 min Scan# 2947

Delta R.T. -0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:149 Resp: 1196306

Ion Ratio Lower Upper

149 100

91 71.6 57.4 86.2

206 21.3 16.6 25.0

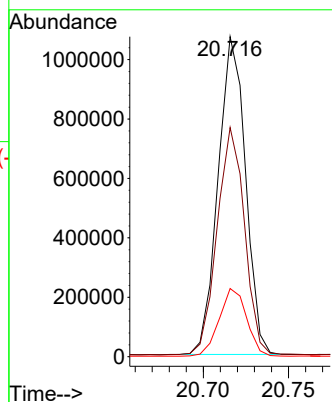

#84

3,3'-Dichlorobenzidine

Concen: 21.745 ng/ul

RT: 21.498 min Scan# 3113

Delta R.T. -0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:252 Resp: 458294


Ion Ratio Lower Upper

252 100

254 64.4 50.8 76.2

126 11.6 9.8 14.8





#85

Benzo(a)anthracene

Concen: 31.975 ng/ul

RT: 21.580 min Scan# 3109

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:228 Resp: 2121683

Ion Ratio Lower Upper

228 100

229 19.7 16.1 24.1

226 27.1 21.9 32.9

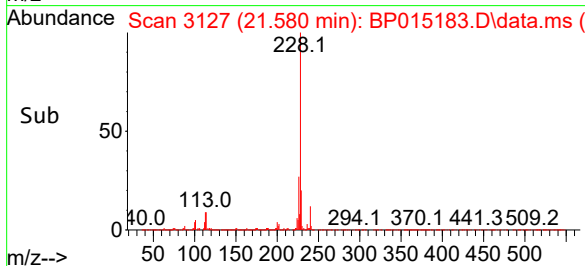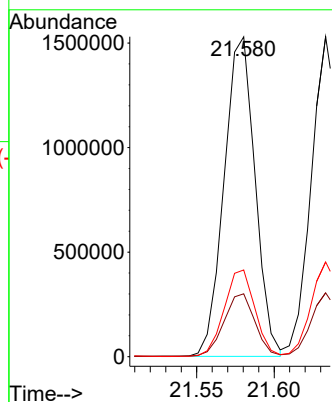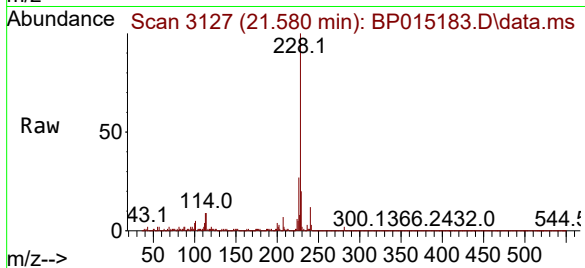

#86

Bis(2-ethylhexyl)phthalate

Concen: 37.601 ng/ul

RT: 21.474 min Scan# 3109

Delta R.T. -0.006 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57




Tgt Ion:149 Resp: 1681171


Ion Ratio Lower Upper

149 100

167 27.8 21.8 32.6

279 4.7 3.2 4.8


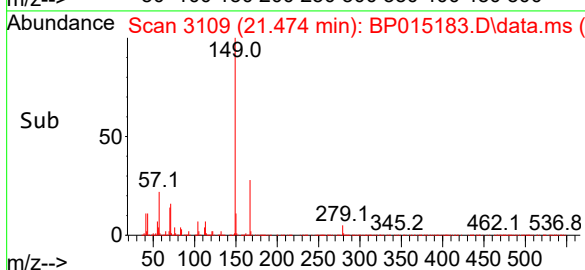

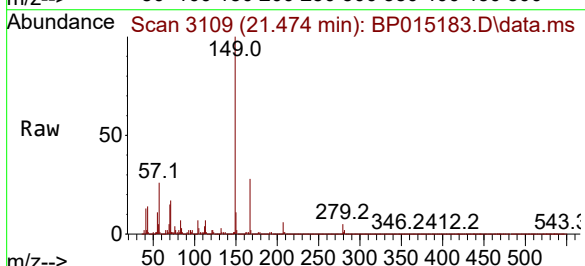


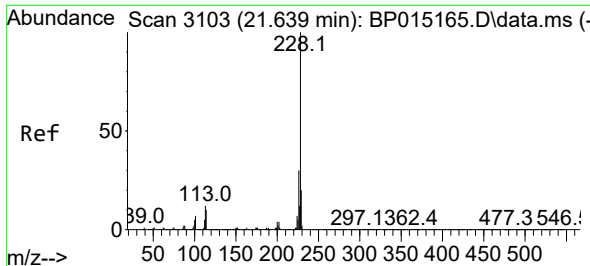

#87
 Chrysene
 Concen: 31.811 ng/ul
 RT: 21.633 min Scan# 3103
 Delta R.T. 0.000 min
 Lab File: BP015183.D
 Acq: 19 May 2023 20:57




Instrument :
 BNA_P
 ClientSampleId :
 JREM0MSD


Tgt Ion:228 Resp: 2017740
 Ion Ratio Lower Upper
 228 100
 226 29.6 25.0 37.6
 229 19.9 16.1 24.1

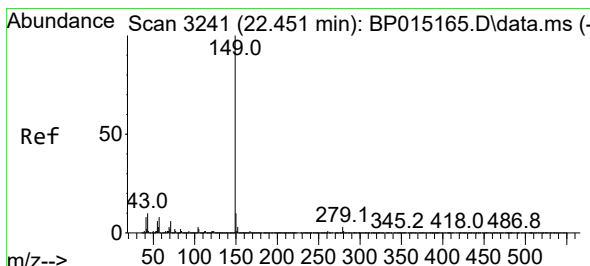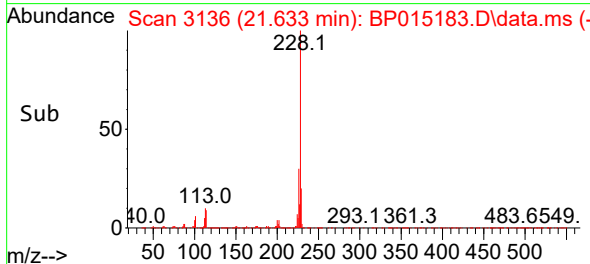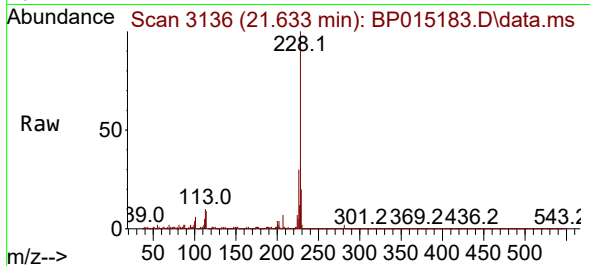

#89
 Di-n-octyl phthalate
 Concen: 37.152 ng/ul
 RT: 22.445 min Scan# 3274
 Delta R.T. -0.006 min
 Lab File: BP015183.D
 Acq: 19 May 2023 20:57

Tgt Ion:149 Resp: 2577173


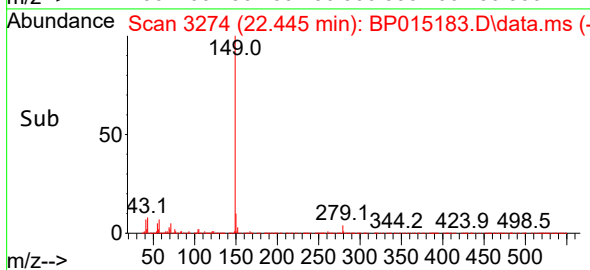

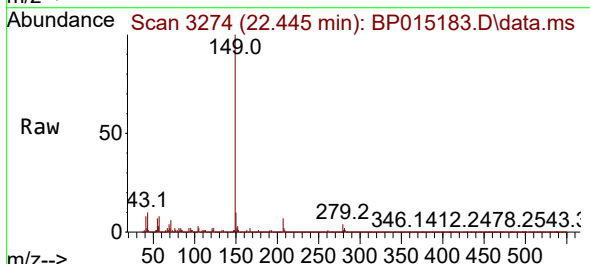




#90
Benzo(b)fluoranthene
Concen: 31.703 ng/ul
RT: 23.368 min Scan# 3431
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:252 Resp: 2035653
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.2
125 9.6 8.3 12.5



#91
Benzo(k)fluoranthene
Concen: 31.052 ng/ul
RT: 23.416 min Scan# 3439
Delta R.T. -0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:252 Resp: 1914552
Ion Ratio Lower Upper
252 100
253 21.7 17.5 26.3
125 10.0 8.5 12.7









#93
Benzo(a)pyrene
Concen: 30.003 ng/ul
RT: 24.039 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57




Instrument :
BNA_P
ClientSampleId :
JREM0MSD


Tgt Ion:252 Resp: 1702842
Ion Ratio Lower Upper
252 100
253 22.0 17.2 25.8
125 11.3 9.1 13.7

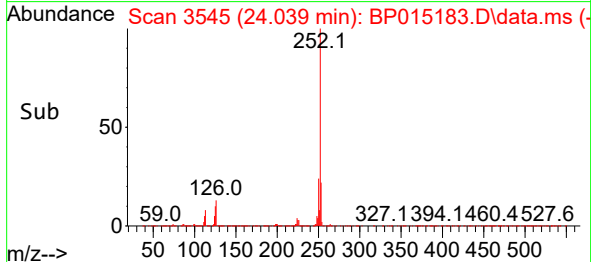

#94
Indeno(1,2,3-cd)pyrene
Concen: 32.167 ng/ul
RT: 26.868 min Scan# 4026
Delta R.T. 0.000 min
Lab File: BP015183.D
Acq: 19 May 2023 20:57

Tgt Ion:276 Resp: 2363814
Ion Ratio Lower Upper
276 100
138 21.9 20.1 30.1
277 24.8 19.8 29.8





#95

Dibenzo(a,h)anthracene

Concen: 32.287 ng/ul

RT: 26.886 min Scan# 4029

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Instrument :

BNA_P

ClientSampleId :

JREM0MSD





Tgt Ion:278 Resp: 1947710

Ion Ratio Lower Upper

278 100

139 15.3 13.3 19.9

279 24.2 19.1 28.7

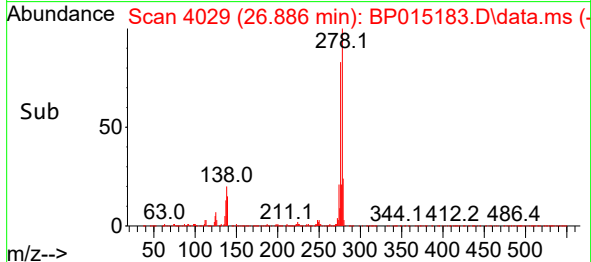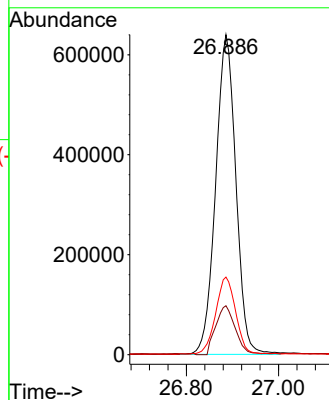

#96

Benzo(g,h,i)perylene

Concen: 29.733 ng/ul

RT: 27.704 min Scan# 4168

Delta R.T. 0.000 min

Lab File: BP015183.D

Acq: 19 May 2023 20:57

Tgt Ion:276 Resp: 1781746

Ion Ratio Lower Upper

276 100

138 19.7 17.7 26.5

277 24.1 18.8 28.2

