

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP05184.D
 Acq On : 19 May 2023 21:31
 Operator : CG/JU
 Sample : 02689-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREP1

Quant Time: May 19 23:14:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	231150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1023059	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	662089	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1442002	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	944937	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1005359	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	17176	2.887	ng/uL	0.00
4) Pyridine-d5	3.893	84	23618	1.401	ng/ul	0.02
7) Phenol-d5	7.275	99	476516	22.203	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	291114	23.486	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	378678	23.998	ng/ul	0.00
15) 4-Methylphenol-d8	8.840	113	406813	23.788	ng/ul	0.00
21) Nitrobenzene-d5	9.305	128	200170	24.899	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	233757	26.133	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	411224	25.477	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	521177	21.823	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1425919	28.501	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	1578065	27.578	ng/ul	0.00
54) 4-Nitrophenol-d4	14.957	143	202570	20.851	ng/ul	0.00
60) Fluorene-d10	15.757	176	1208841	28.634	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	177102	19.488	ng/ul	0.00
73) Anthracene-d10	17.616	188	1922117	29.110	ng/ul	0.00
81) Pyrene-d10	19.833	212	2072305	37.813	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1562217	31.303	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.958	105	71404	2.675	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP05184.D
Acq On : 19 May 2023 21:31
Operator : CG/JU
Sample : 02689-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREP1

Quant Time: May 19 23:14:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

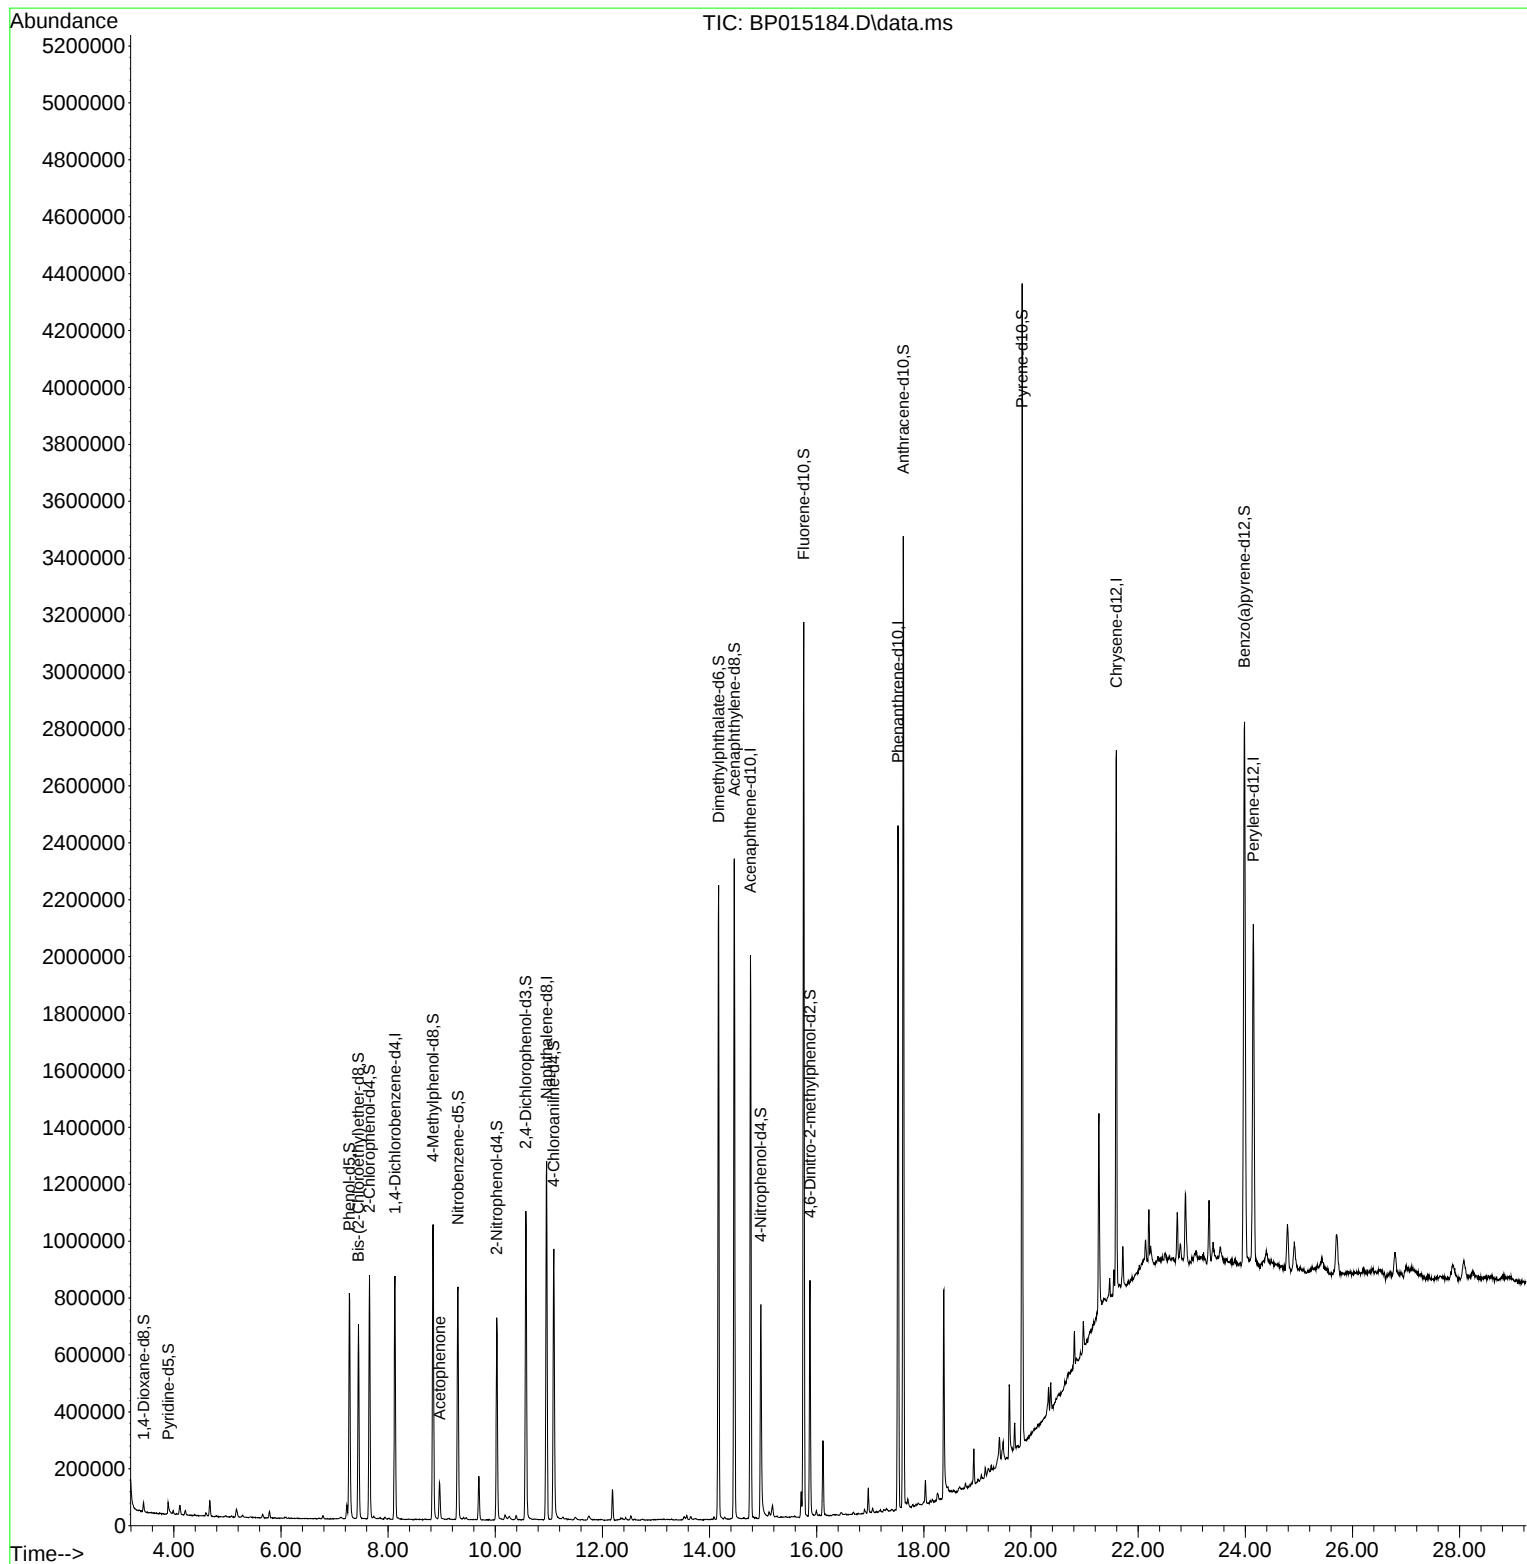

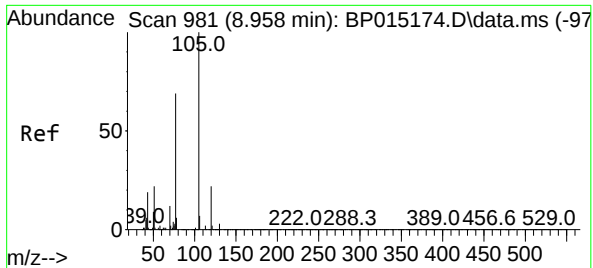

#16
 Acetophenone
 Concen: 2.675 ng/ul
 RT: 8.958 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP015184.D
 Acq: 19 May 2023 21:31

Instrument :
 BNA_P
 ClientSampleId :
 JREP1

Tgt Ion:	105	Resp:	71404
Ion	Ratio	Lower	Upper
105	100		
77	79.7	59.4	89.2
51	25.5	19.2	28.8

