

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP05186.D
 Acq On : 19 May 2023 22:38
 Operator : CG/JU
 Sample : 02689-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREQ0

Quant Time: May 19 23:19:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	270101	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1203287	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	772417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1647464	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1114651	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1119579	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	8658	1.245	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.275	99	336204	13.406	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	209104	14.437	ng/ul	0.00
11) 2-Chlorophenol-d4	7.651	132	266322	14.443	ng/ul	0.00
15) 4-Methylphenol-d8	8.840	113	263249	13.173	ng/ul	0.00
21) Nitrobenzene-d5	9.304	128	142367	15.057	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	160154	15.223	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	282876	14.900	ng/ul	0.00
31) 4-Chloroaniline-d4	11.092	131	321514	11.446	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	999435	17.123	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1114843	16.700	ng/ul	0.00
54) 4-Nitrophenol-d4	14.957	143	115164	10.161	ng/ul	0.00
60) Fluorene-d10	15.751	176	853930	17.338	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	102797	9.901	ng/ul	0.00
73) Anthracene-d10	17.616	188	1317534	17.465	ng/ul	0.00
81) Pyrene-d10	19.833	212	1432847	22.164	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1001095	18.013	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.957	105	108959	3.494	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015186.D
Acq On : 19 May 2023 22:38
Operator : CG/JU
Sample : 02689-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREQ0

Quant Time: May 19 23:19:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration

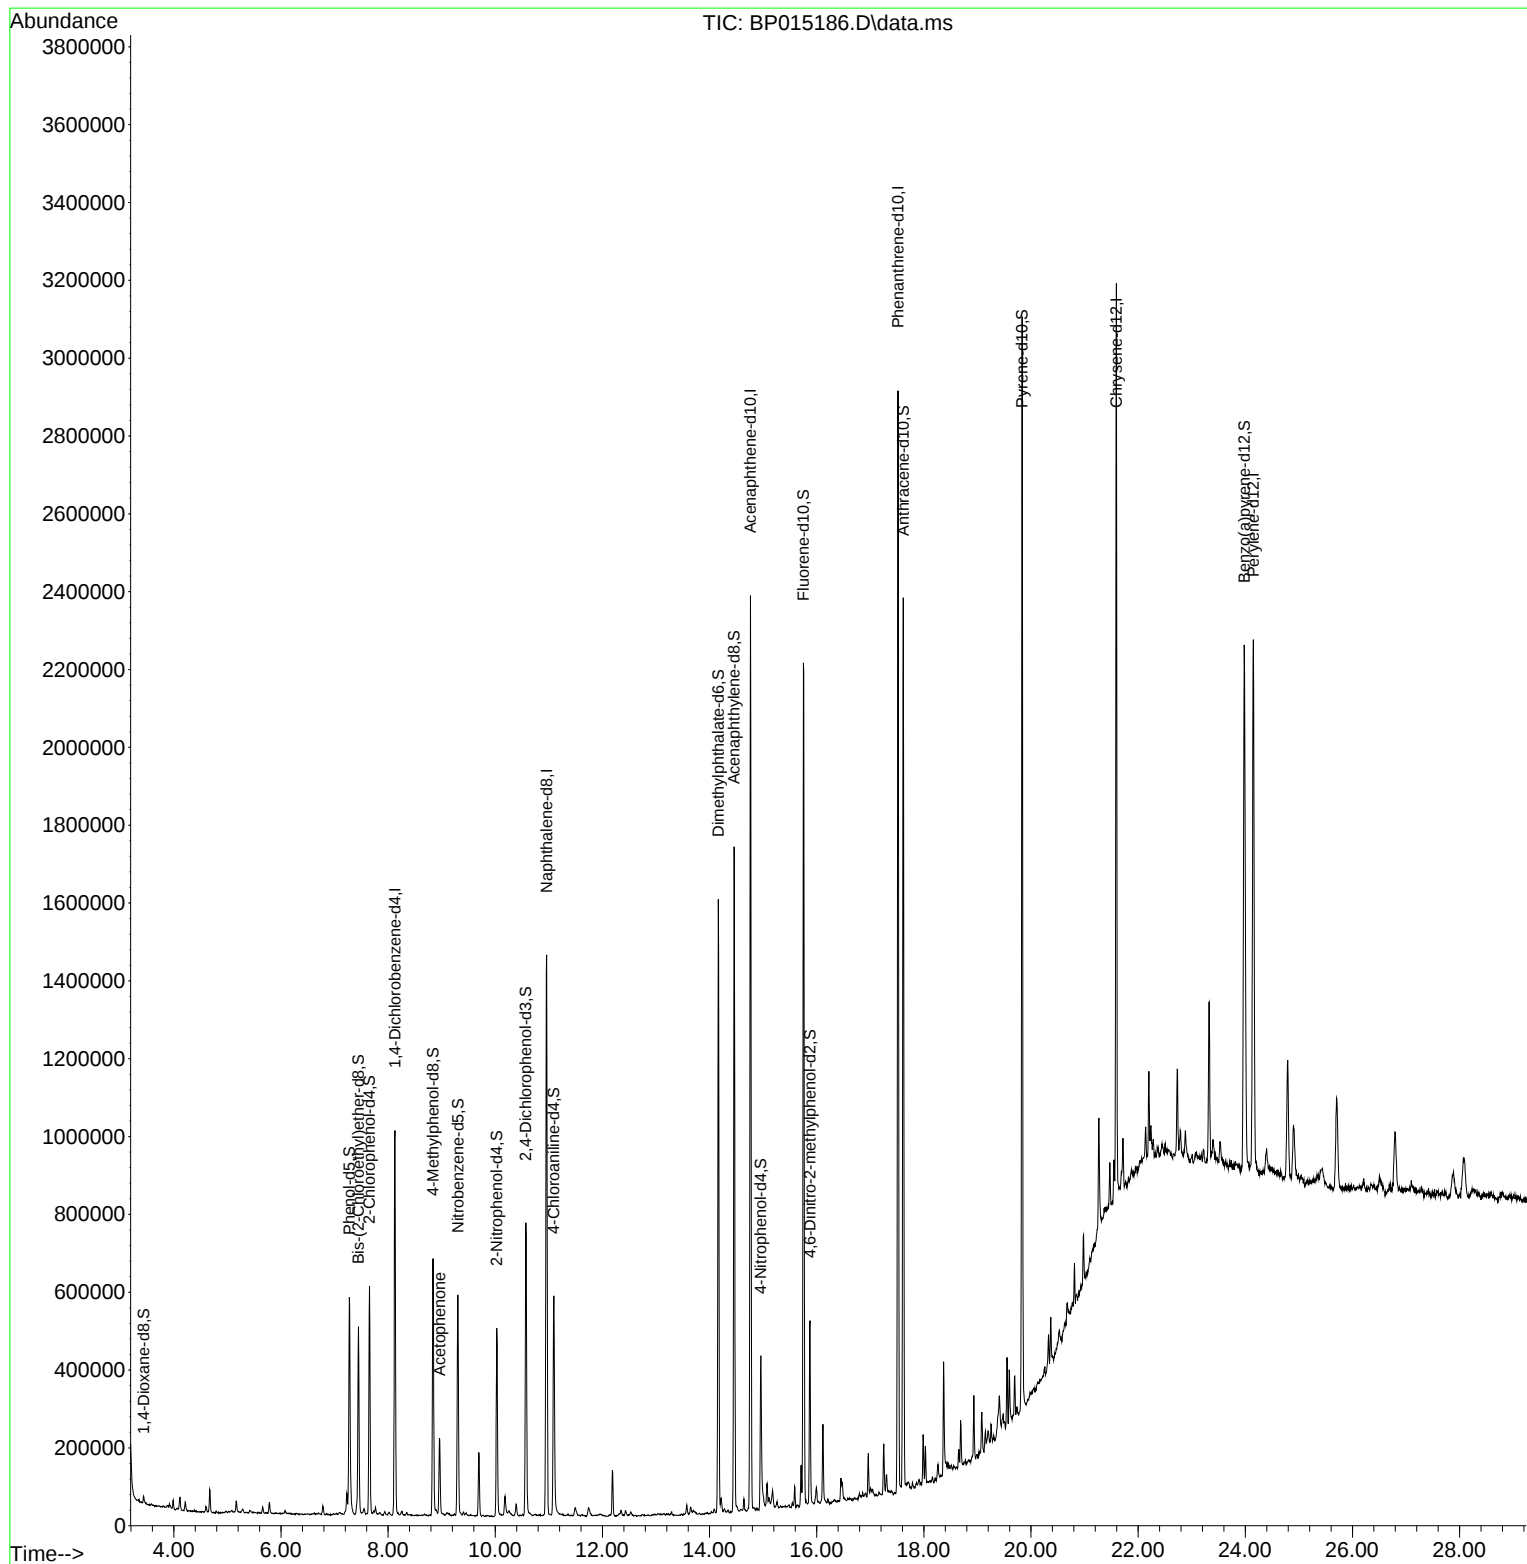

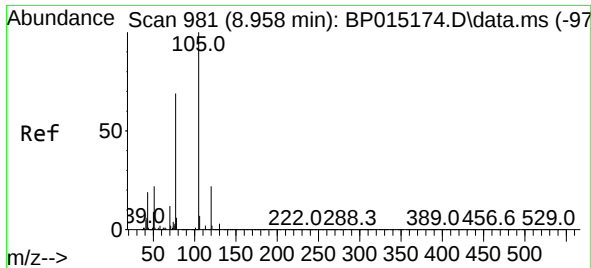

#16
 Acetophenone
 Concen: 3.494 ng/ul
 RT: 8.957 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP015186.D
 Acq: 19 May 2023 22:38

Instrument :
 BNA_P
 ClientSampleId :
 JREQ0

Tgt Ion:105 Resp: 108959
 Ion Ratio Lower Upper
 105 100
 77 79.1 59.4 89.2
 51 26.5 19.2 28.8

