

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP05190.D
 Acq On : 20 May 2023 00:52
 Operator : CG/JU
 Sample : 02689-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREM4

Quant Time: May 20 01:36:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	262114	20.000	ng/u1	0.00
20) Naphthalene-d8	10.951	136	1139697	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.763	164	756287	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.516	188	1682761	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1202813	20.000	ng/u1	-0.01
88) Perylene-d12	24.145	264	1279547	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	35959	5.330	ng/uL	0.00
4) Pyridine-d5	3.875	84	291891	15.264	ng/u1	0.00
7) Phenol-d5	7.275	99	630120	25.892	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	382862	27.239	ng/u1	0.00
11) 2-Chlorophenol-d4	7.652	132	496809	27.764	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	521585	26.896	ng/u1	0.00
21) Nitrobenzene-d5	9.305	128	264215	29.503	ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	303571	30.464	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	534093	29.703	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	680004	25.560	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	1838316	32.167	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	2025574	30.990	ng/u1	0.00
54) 4-Nitrophenol-d4	14.957	143	269319	24.269	ng/u1	0.00
60) Fluorene-d10	15.751	176	1540602	31.947	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	223957	21.118	ng/u1	0.00
73) Anthracene-d10	17.616	188	2429206	31.526	ng/u1	0.00
81) Pyrene-d10	19.833	212	2693990	38.617	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	2152769	33.892	ng/u1	-0.01
Target Compounds						
8) Phenol	7.305	94	27103	1.086	ng/u1#	90
18) 4-Methylphenol	8.893	108	79314	3.736	ng/u1	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015190.D
Acq On : 20 May 2023 00:52
Operator : CG/JU
Sample : 02689-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREM4

Quant Time: May 20 01:36:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration




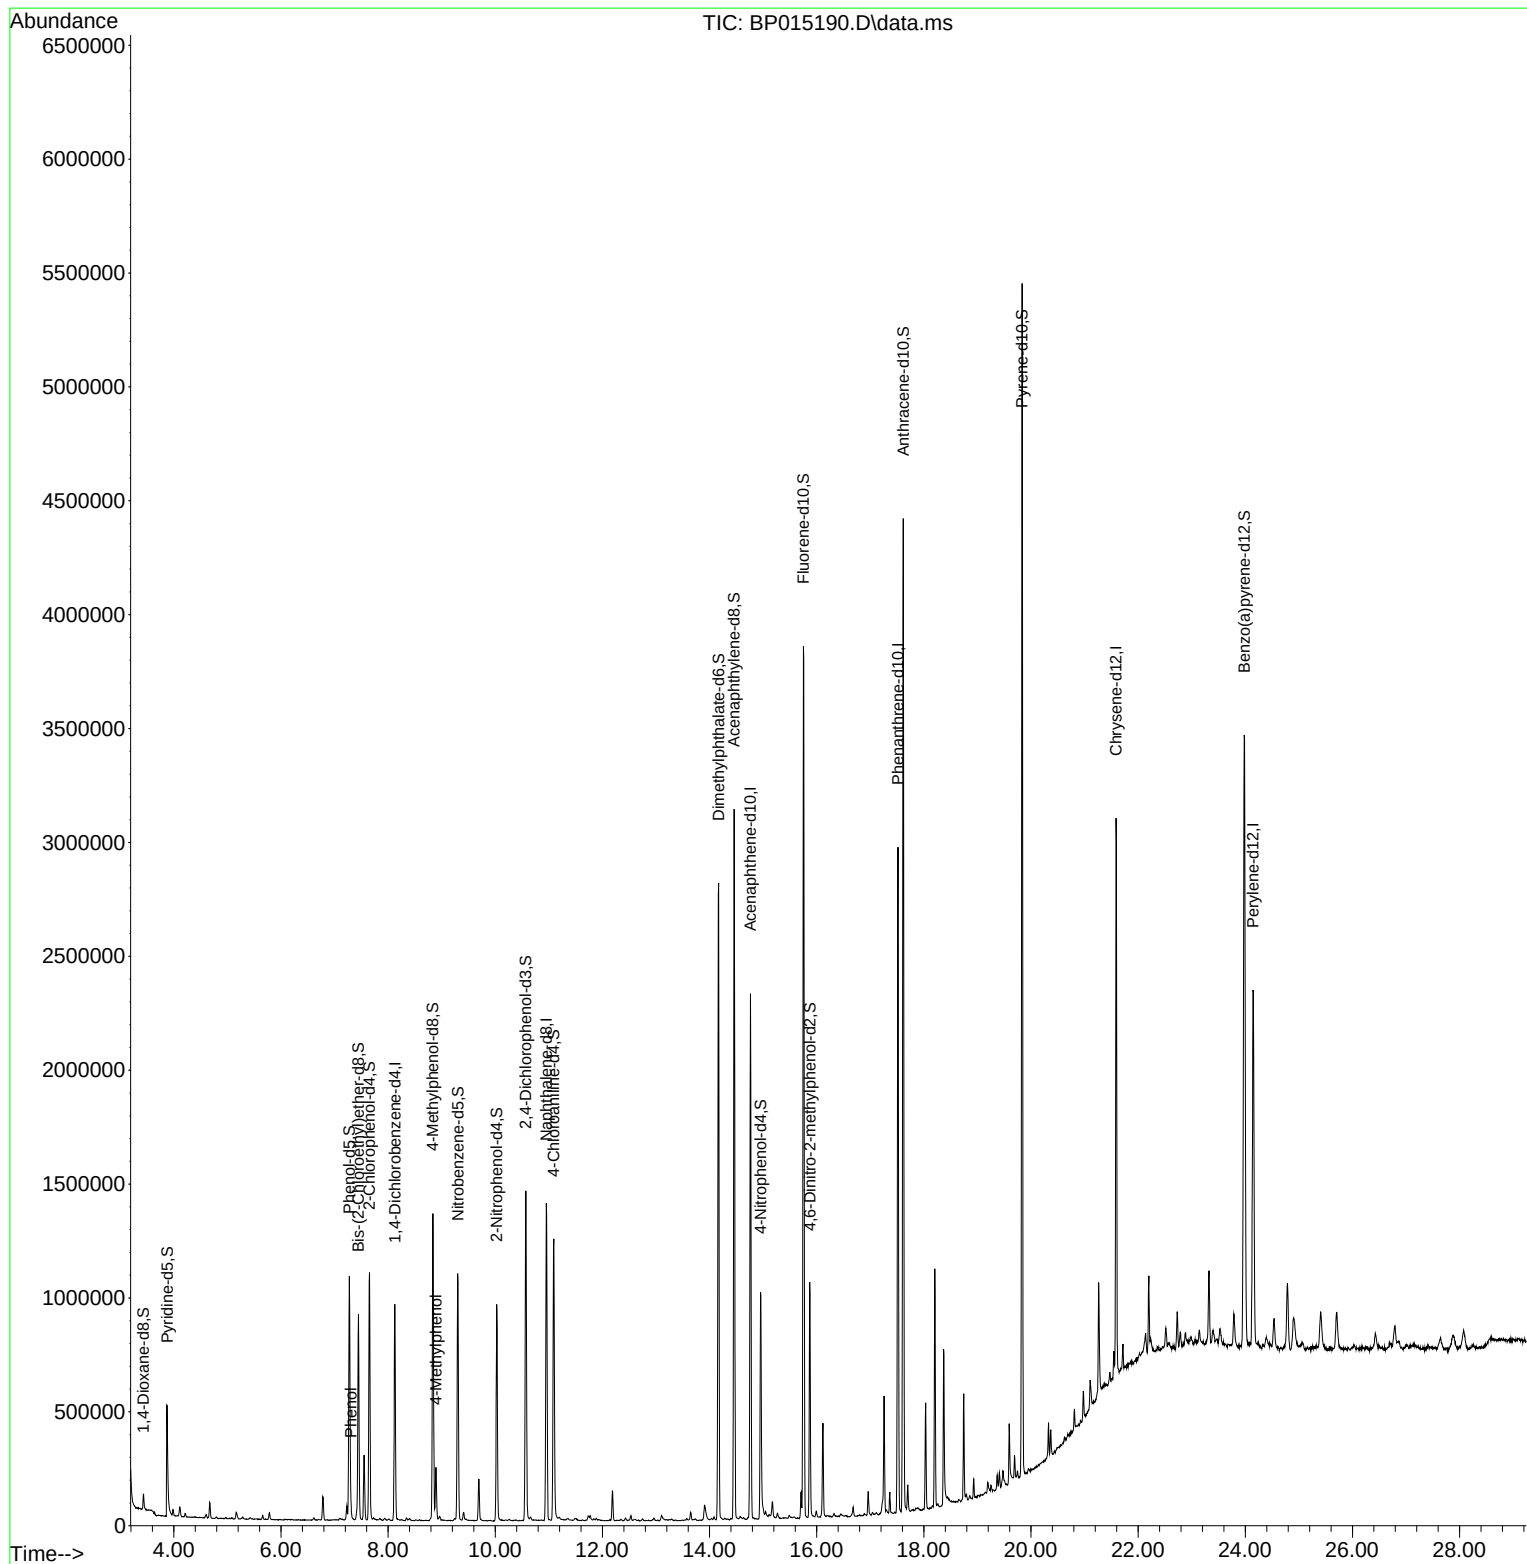


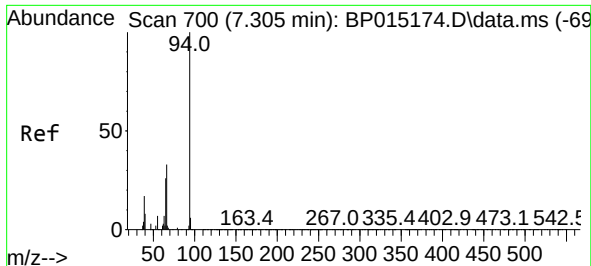

#8
Phenol
Concen: 1.086 ng/ul
RT: 7.305 min Scan# 700
Delta R.T. 0.000 min
Lab File: BP015190.D
Acq: 20 May 2023 00:52

Instrument :
BNA_P
ClientSampleId :
JREM4

Tgt Ion: 94 Resp: 27103
Ion Ratio Lower Upper
94 100
65 27.5 20.6 31.0
66 41.5 26.1 39.1#

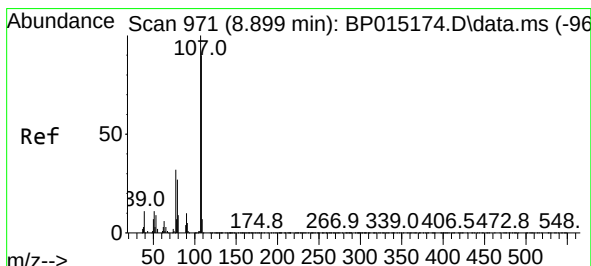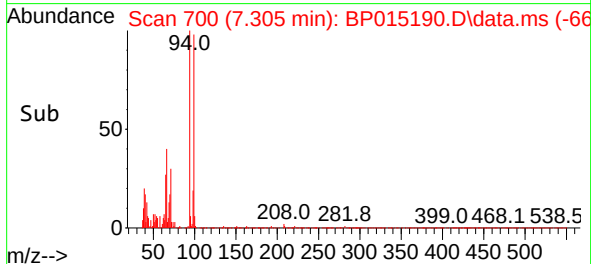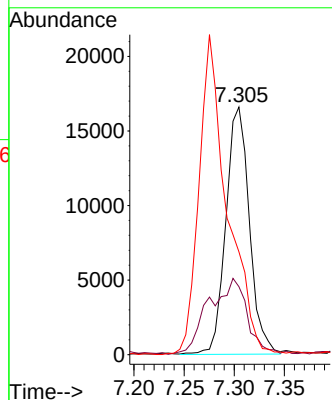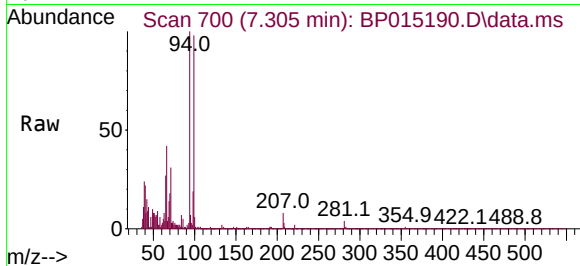

#18
4-Methylphenol
Concen: 3.736 ng/ul
RT: 8.893 min Scan# 970
Delta R.T. -0.012 min
Lab File: BP015190.D
Acq: 20 May 2023 00:52

Tgt Ion: 108 Resp: 79314
Ion Ratio Lower Upper
108 100
107 126.6 88.5 132.7

