

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015195.D
 Acq On : 20 May 2023 04:13
 Operator : CG/JU
 Sample : 02689-22
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREP4

Quant Time: May 20 04:55:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	227889	20.000	ng/u1	0.00
20) Naphthalene-d8	10.952	136	990243	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.763	164	653724	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.516	188	1430168	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1038592	20.000	ng/u1	-0.01
88) Perylene-d12	24.145	264	1030530	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	12643	2.156	ng/uL	0.00
4) Pyridine-d5	3.893	84	19233	1.157	ng/u1	0.02
7) Phenol-d5	7.275	99	341536	16.141	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	210869	17.256	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	275702	17.722	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	243573	14.447	ng/u1	0.00
21) Nitrobenzene-d5	9.299	128	146455	18.821	ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	167099	19.300	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	299439	19.166	ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	323535	13.996	ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	1048727	21.230	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	1133010	20.054	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	141268	14.727	ng/u1	0.00
60) Fluorene-d10	15.751	176	913480	21.915	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	134875	14.964	ng/u1	0.00
73) Anthracene-d10	17.610	188	1440056	21.990	ng/u1	0.00
81) Pyrene-d10	19.828	212	1683148	27.942	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.980	264	1218609	23.821	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.958	105	62276	2.367	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.469	149	57270	1.184	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015195.D
Acq On : 20 May 2023 04:13
Operator : CG/JU
Sample : 02689-22
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREP4

Quant Time: May 20 04:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration




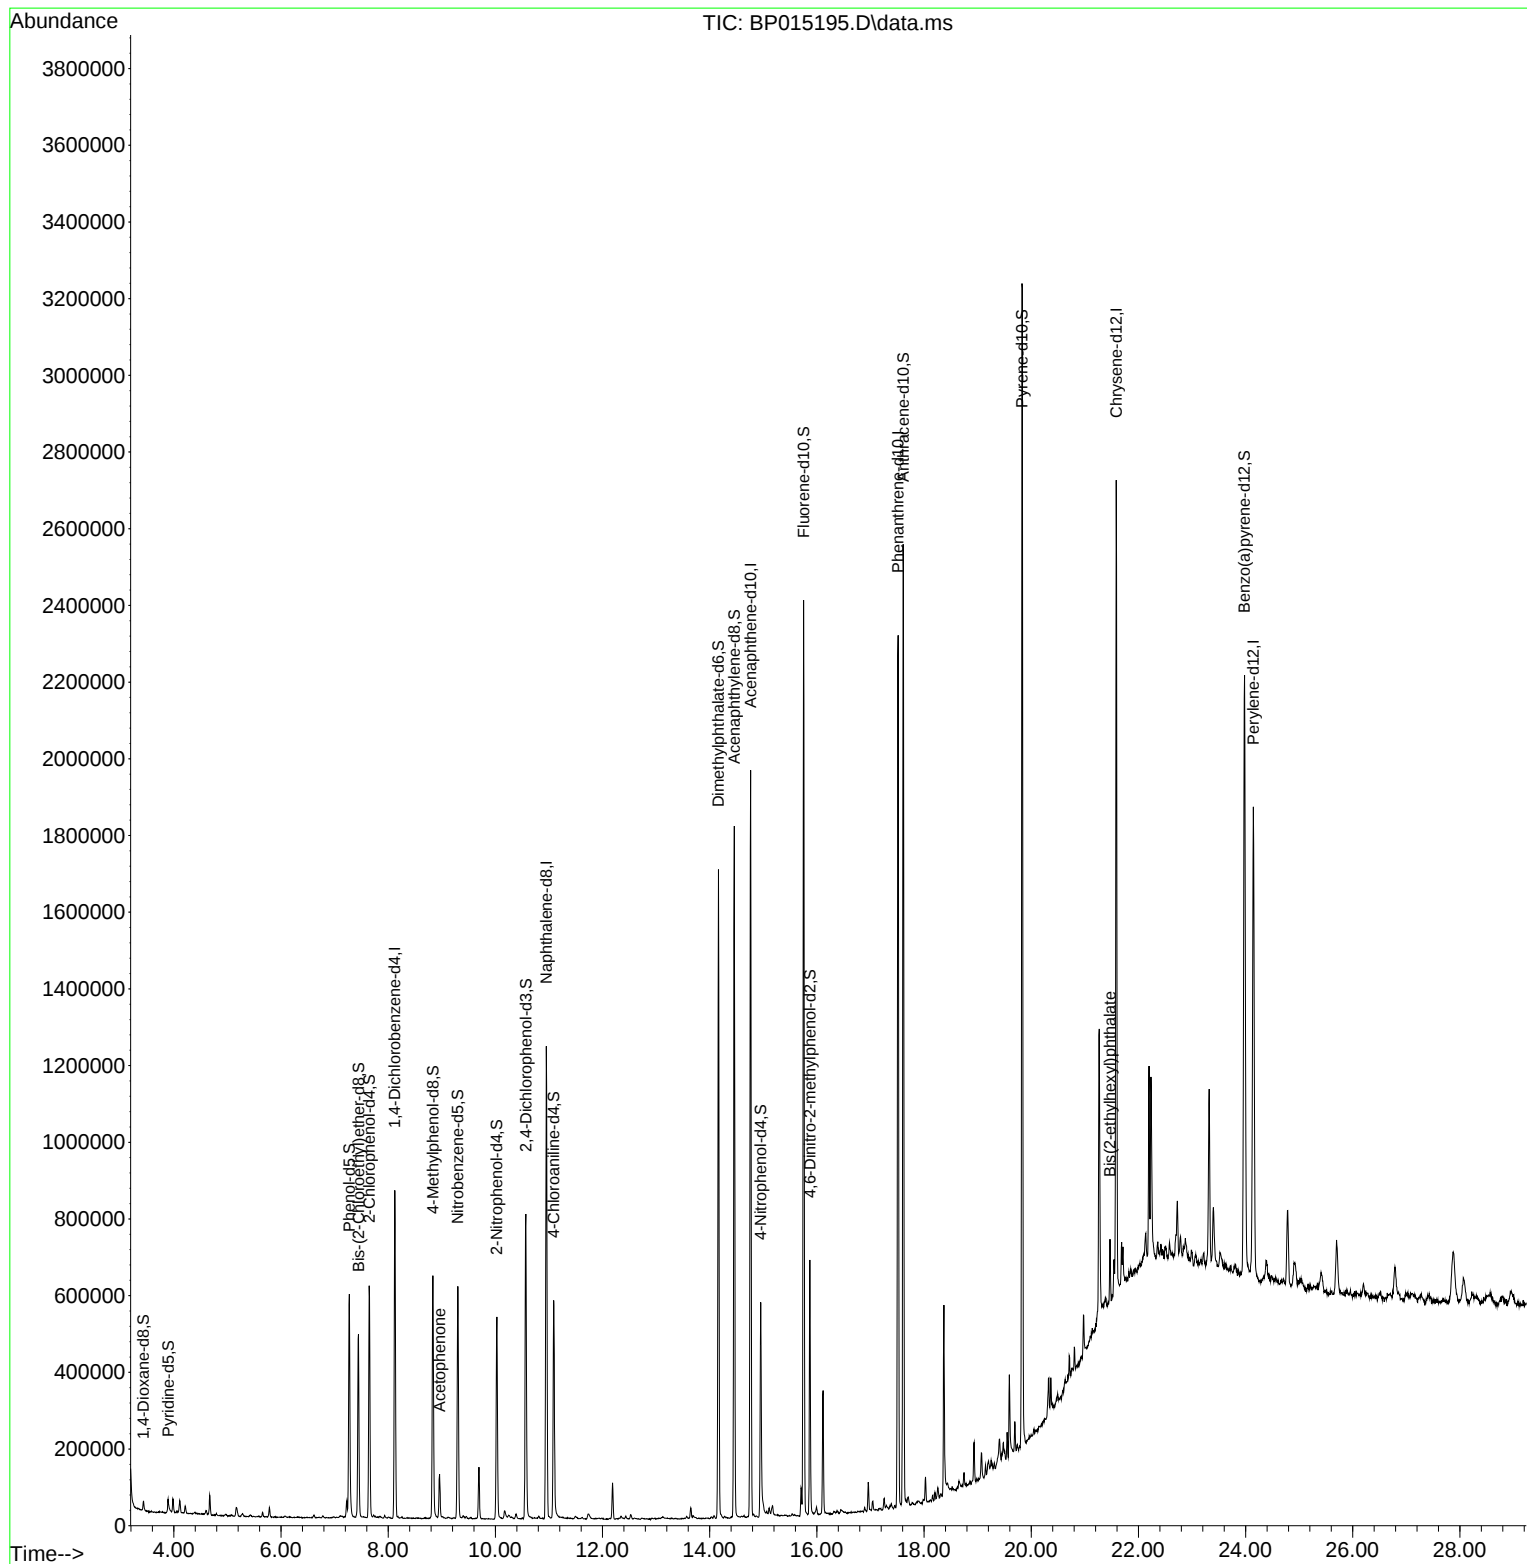


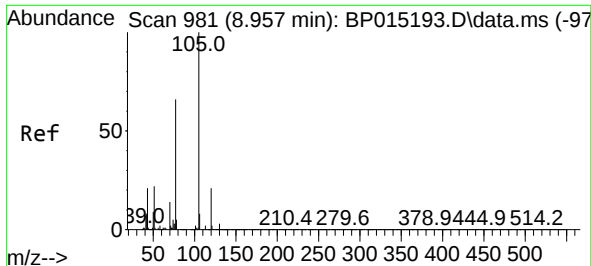

#16
Acetophenone
Concen: 2.367 ng/ul
RT: 8.958 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP015195.D
Acq: 20 May 2023 04:13

Instrument :
BNA_P
ClientSampleId :
JREP4

Tgt Ion:105 Resp: 62276
Ion Ratio Lower Upper
105 100
77 71.9 59.4 89.2
51 26.9 19.2 28.8

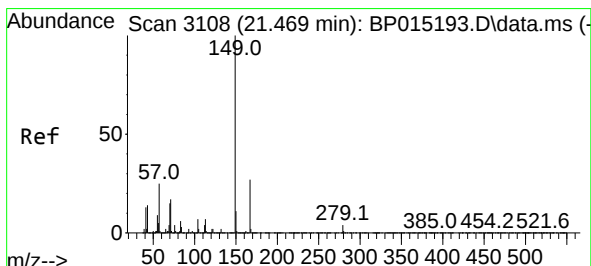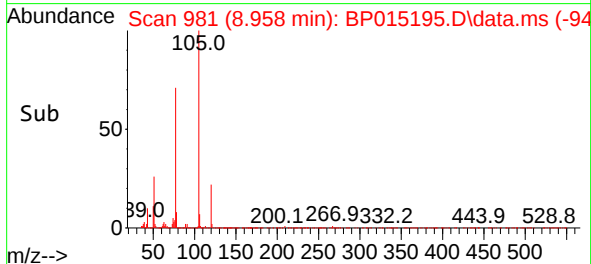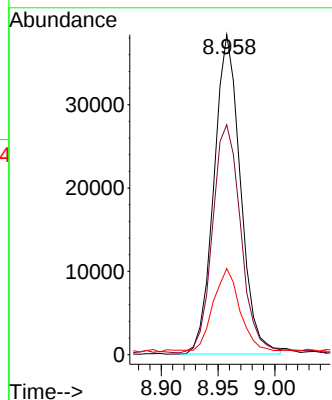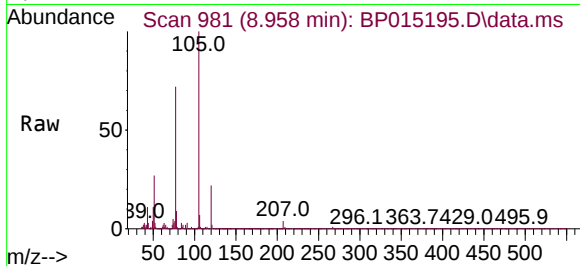

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.184 ng/ul
RT: 21.469 min Scan# 3108
Delta R.T. -0.012 min
Lab File: BP015195.D
Acq: 20 May 2023 04:13

Tgt Ion:149 Resp: 57270
Ion Ratio Lower Upper
149 100
167 27.3 21.8 32.6
279 4.5 3.2 4.8

