

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015196.D
 Acq On : 20 May 2023 04:46
 Operator : CG/JU
 Sample : 02689-25
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREK7

Quant Time: May 20 05:23:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	227785	20.000	ng/ul	0.00
20) Naphthalene-d8	10.951	136	991663	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	635395	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1386824	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	919059	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	943840	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	11432	1.950	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.275	99	355548	16.811	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	219747	17.990	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	287287	18.475	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	253369	15.034	ng/ul	0.00
21) Nitrobenzene-d5	9.298	128	153996	19.762	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	173449	20.004	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	307445	19.650	ng/ul	0.00
31) 4-Chloroaniline-d4	11.087	131	304100	13.137	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	1051587	21.902	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1172083	21.344	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	151646	16.265	ng/ul	0.00
60) Fluorene-d10	15.751	176	917719	22.651	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	133920	15.323	ng/ul	0.00
73) Anthracene-d10	17.616	188	1424703	22.435	ng/ul	0.00
81) Pyrene-d10	19.833	212	1518806	28.493	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1087902	23.219	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.957	105	85562	3.253	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	21.468	149	97020	2.266	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP05196.D
Acq On : 20 May 2023 04:46
Operator : CG/JU
Sample : 02689-25
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREK7

Quant Time: May 20 05:23:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration




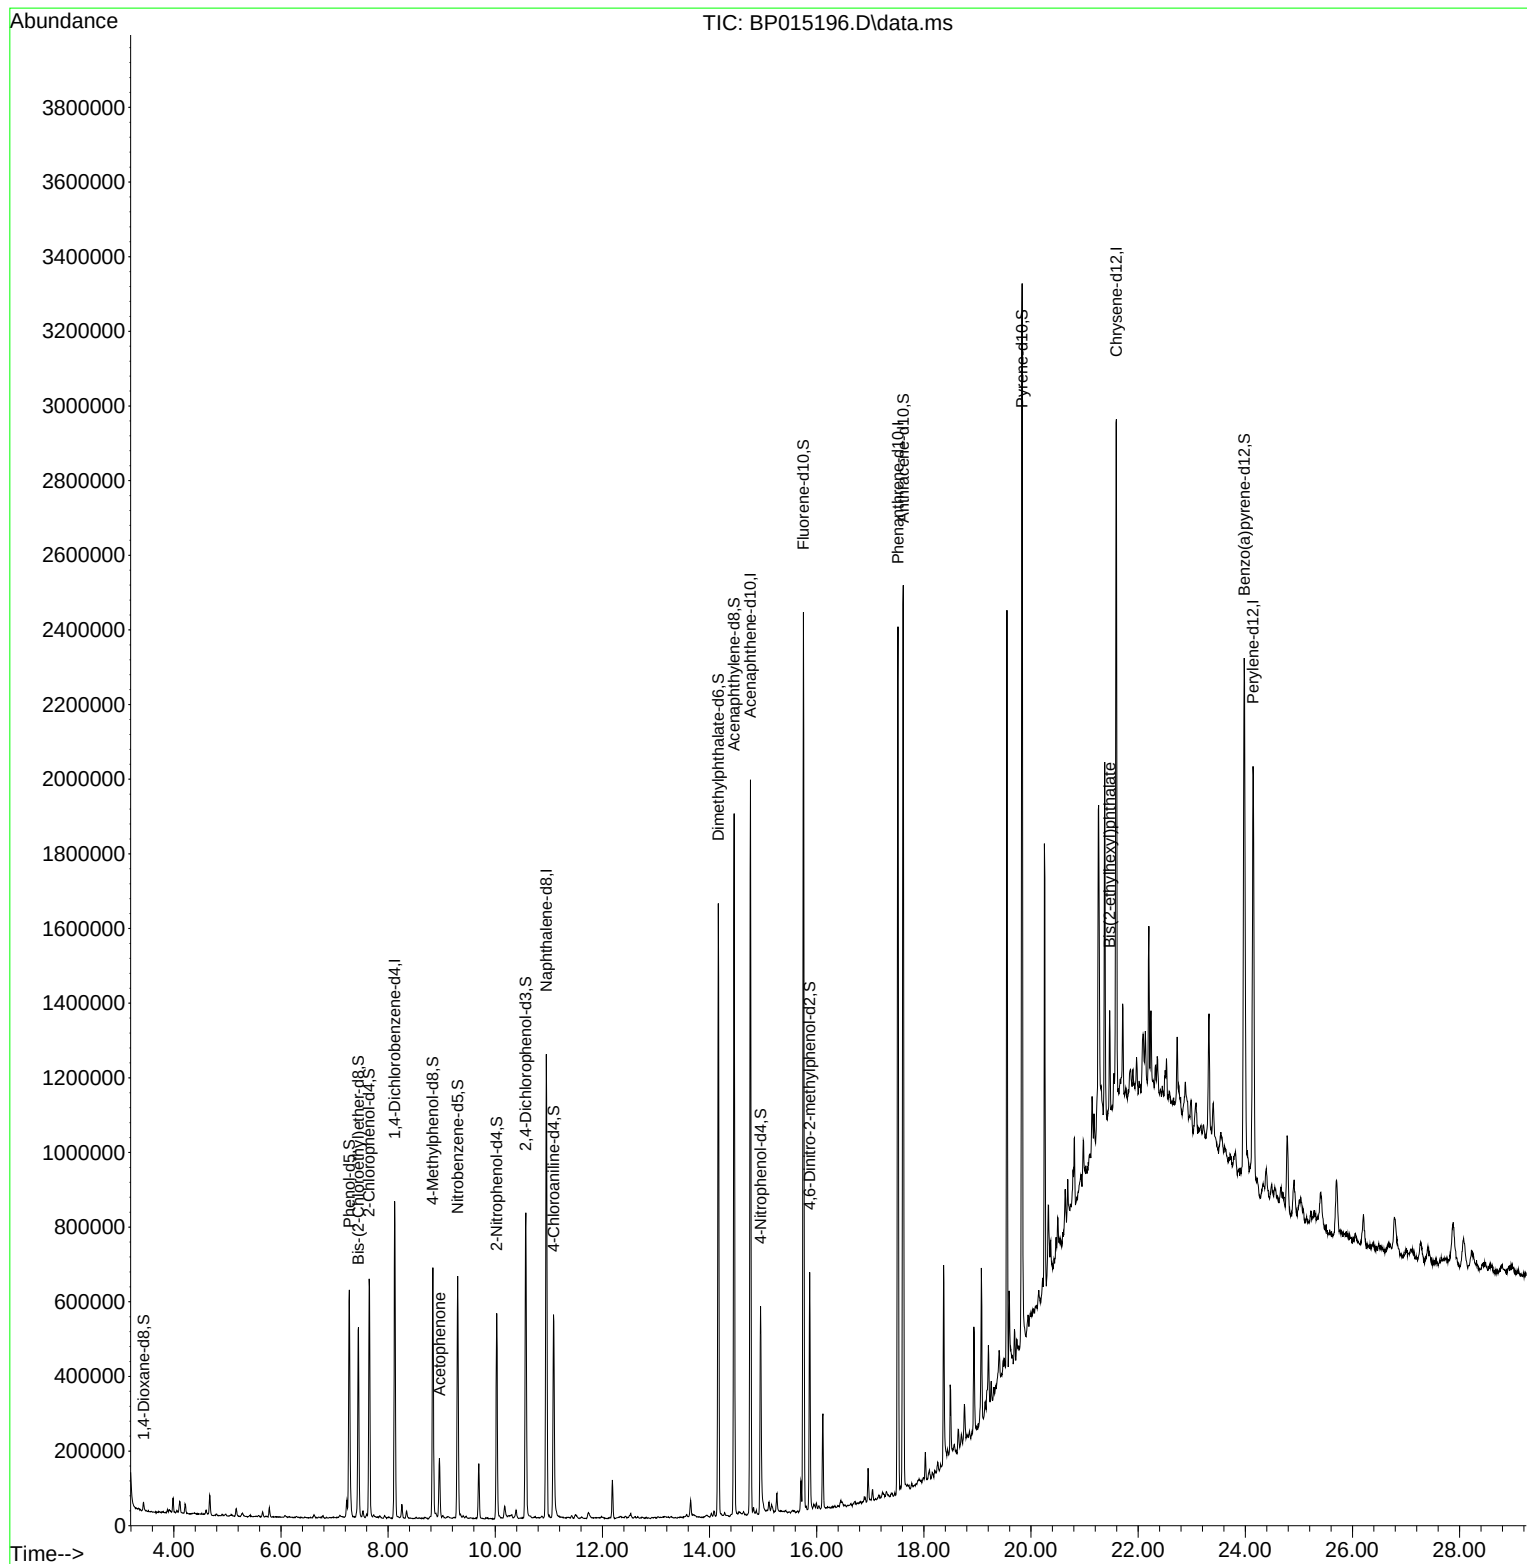


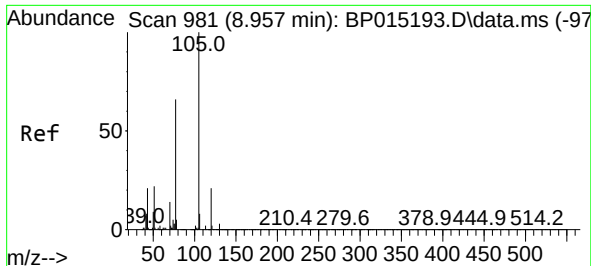

#16
 Acetophenone
 Concen: 3.253 ng/ul
 RT: 8.957 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP015196.D
 Acq: 20 May 2023 04:46

Instrument :
 BNA_P
 ClientSampleId :
 JREK7

Tgt Ion:105 Resp: 85562
 Ion Ratio Lower Upper
 105 100
 77 77.3 59.4 89.2
 51 26.6 19.2 28.8

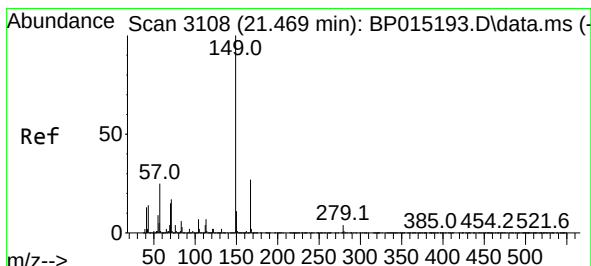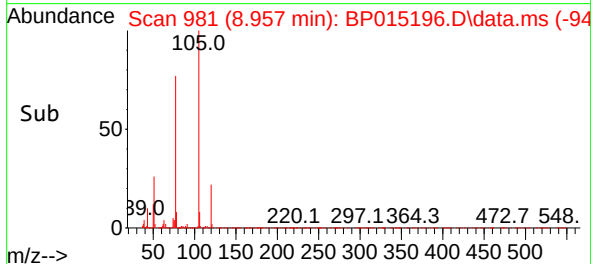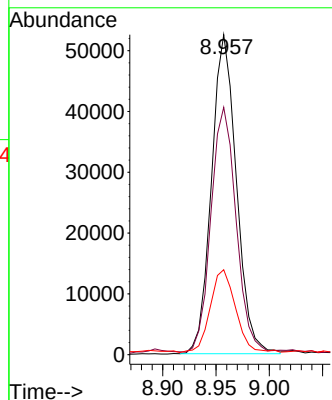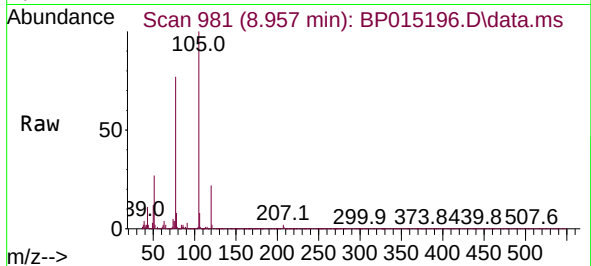

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.266 ng/ul
 RT: 21.468 min Scan# 3108
 Delta R.T. -0.012 min
 Lab File: BP015196.D
 Acq: 20 May 2023 04:46

Tgt Ion:149 Resp: 97020
 Ion Ratio Lower Upper
 149 100
 167 28.6 21.8 32.6
 279 4.9 3.2 4.8#

