

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015197.D
 Acq On : 20 May 2023 05:20
 Operator : CG/JU
 Sample : 02689-20
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREP2

Quant Time: May 20 05:50:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 01:07:51 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	223155	20.000	ng/u1	0.00
20) Naphthalene-d8	10.952	136	984849	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.763	164	637875	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.516	188	1395257	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	954904	20.000	ng/u1	-0.01
88) Perylene-d12	24.145	264	970807	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	16499	2.873	ng/uL	0.00
4) Pyridine-d5	3.893	84	22563	1.386	ng/u1	0.02
7) Phenol-d5	7.275	99	502594	24.257	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	310878	25.979	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	402369	26.412	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	332032	20.111	ng/u1	0.00
21) Nitrobenzene-d5	9.299	128	216231	27.941	ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	253083	29.391	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	440554	28.353	ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	443575	19.294	ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	1524111	31.620	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	1680134	30.477	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	208256	22.250	ng/u1	0.00
60) Fluorene-d10	15.751	176	1276335	31.380	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	197926	22.509	ng/u1	0.00
73) Anthracene-d10	17.610	188	1961443	30.700	ng/u1	0.00
81) Pyrene-d10	19.834	212	2154066	38.894	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	1580500	32.796	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.958	105	71837	2.788	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.486	149	94907	2.133	ng/u1#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015197.D
Acq On : 20 May 2023 05:20
Operator : CG/JU
Sample : 02689-20
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREP2

Quant Time: May 20 05:50:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 01:07:51 2023
Response via : Initial Calibration




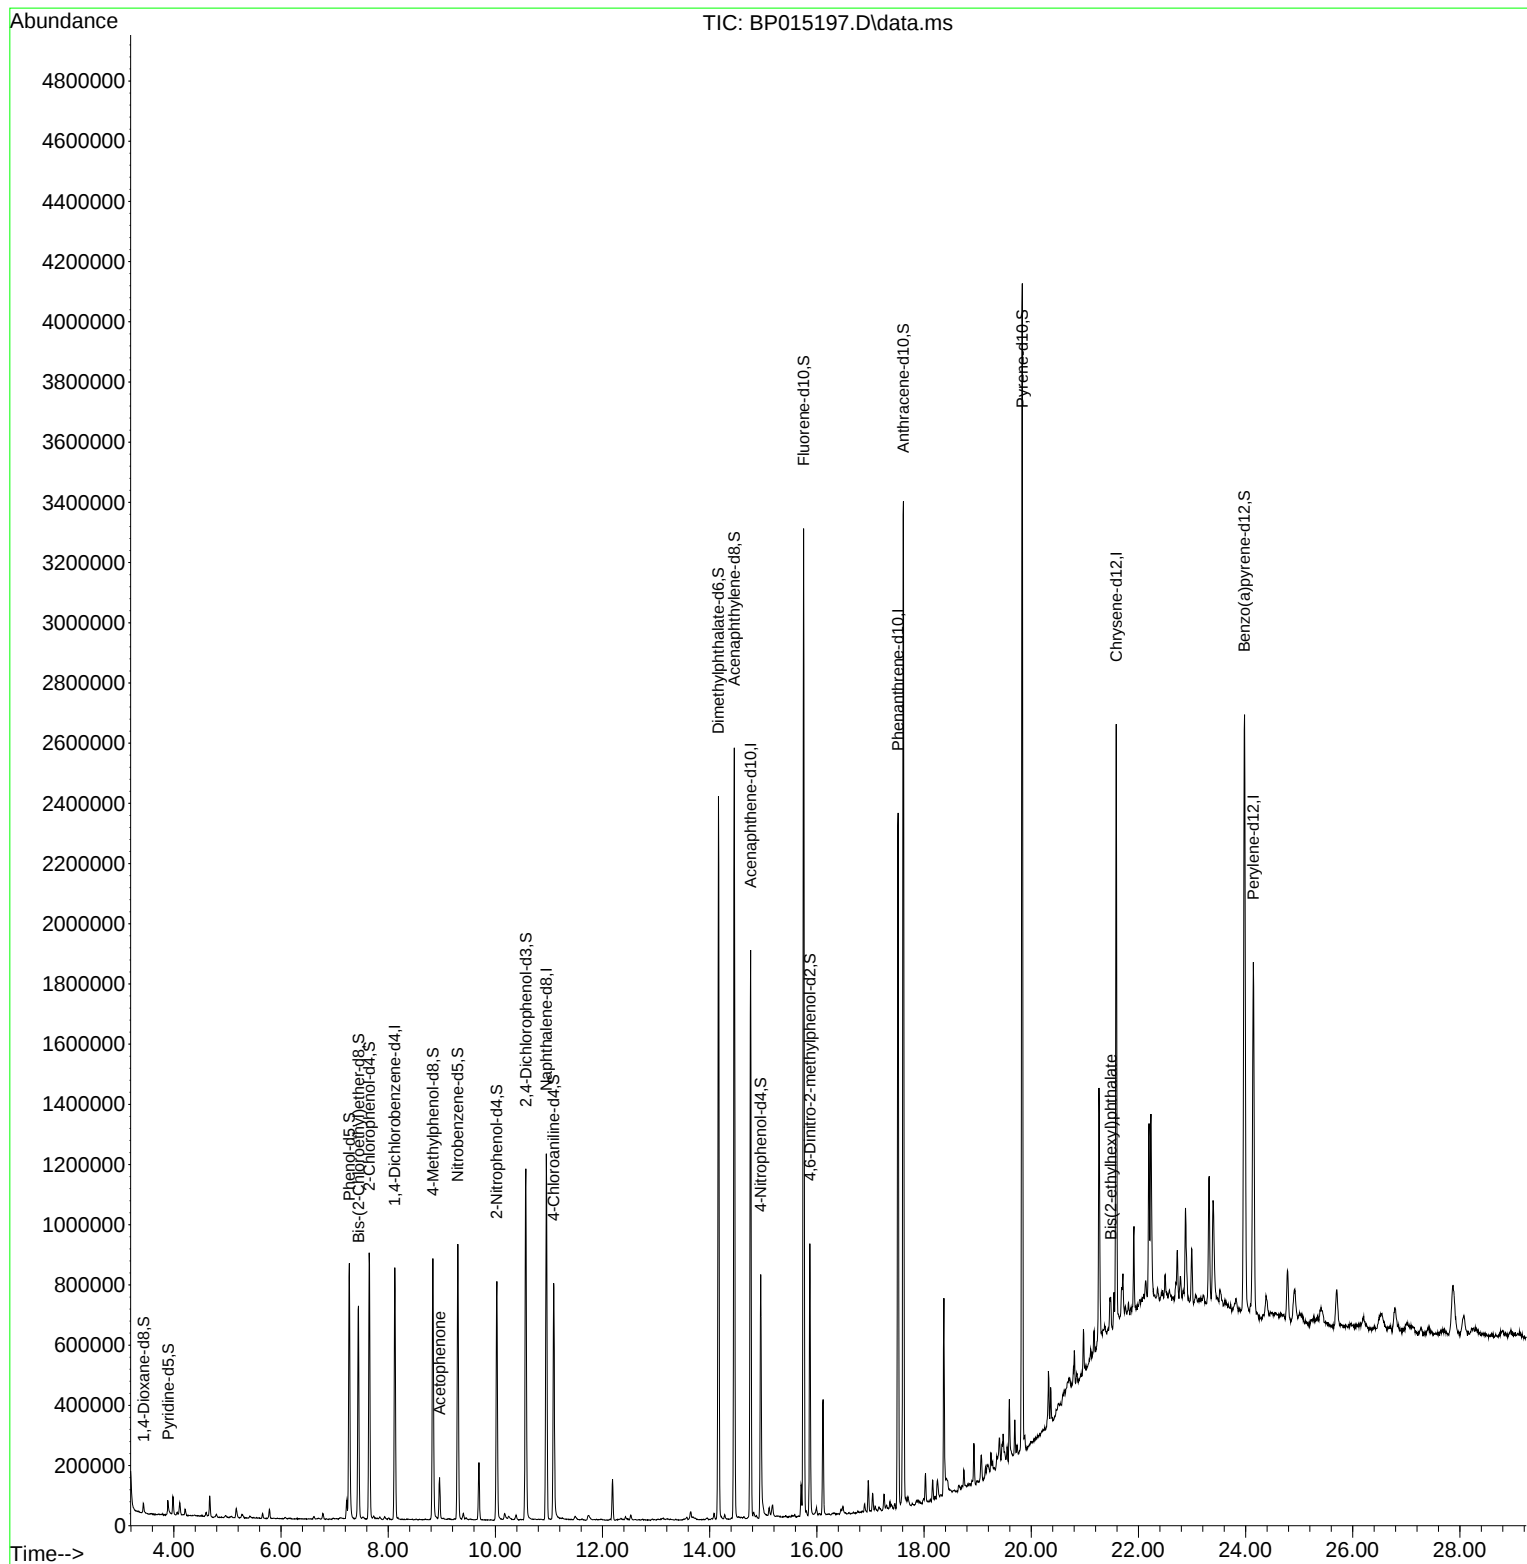


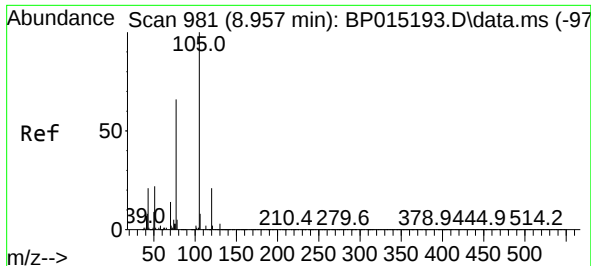

#16
Acetophenone
Concen: 2.788 ng/ul
RT: 8.958 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP015197.D
Acq: 20 May 2023 05:20

Instrument :
BNA_P
ClientSampleId :
JREP2

Tgt Ion:105 Resp: 71837
Ion Ratio Lower Upper
105 100
77 77.0 59.4 89.2
51 27.3 19.2 28.8

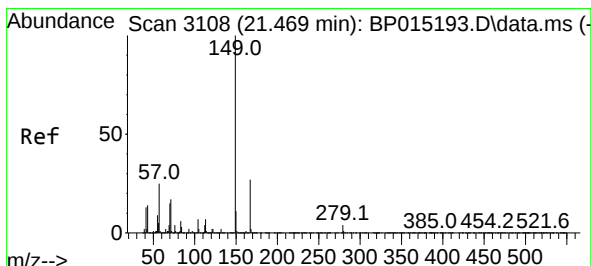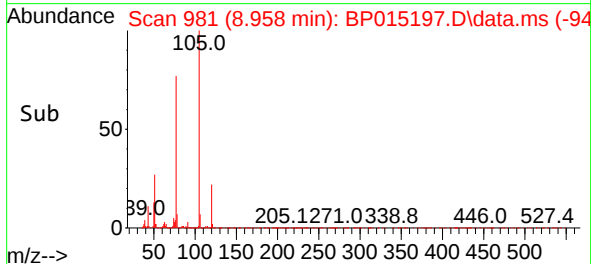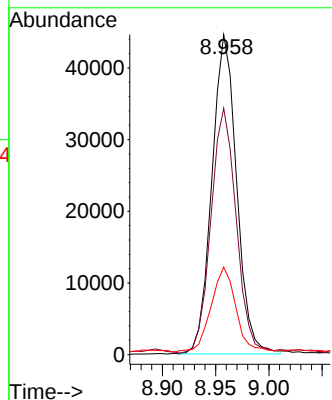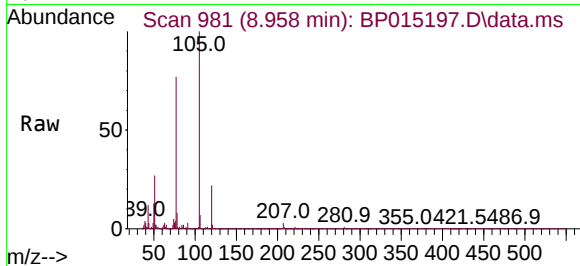

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.133 ng/ul
RT: 21.486 min Scan# 3111
Delta R.T. 0.006 min
Lab File: BP015197.D
Acq: 20 May 2023 05:20

Tgt Ion:149 Resp: 94907
Ion Ratio Lower Upper
149 100
167 3.4 21.8 32.6#
279 0.8 3.2 4.8#

