

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015166.D
 Acq On : 19 May 2023 09:44
 Operator : CG/JU
 Sample : PB152814BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	3	7	19	rBV	83132	128834	1.50%	0.153%
2	3.869	79	82	102	rBV	1097695	1708904	19.94%	2.029%
3	4.211	137	140	146	rBV	16861	23431	0.27%	0.028%
4	7.275	653	661	675	rBV	1253632	2049825	23.92%	2.434%
5	7.446	683	690	705	rVB	1172673	1857731	21.68%	2.206%
6	7.652	717	725	737	rBV	1368319	2195546	25.62%	2.607%
7	8.128	799	806	817	rVB	908765	1476181	17.23%	1.753%
8	8.834	917	926	943	rBV	1700852	2818983	32.90%	3.347%
9	9.304	997	1006	1016	rBV	1312411	2201867	25.70%	2.614%
10	10.028	1122	1129	1141	rBV	1065903	1797663	20.98%	2.134%
11	10.569	1213	1221	1243	rBV	1613273	2780658	32.45%	3.301%
12	10.957	1279	1287	1298	rVB	1399531	2323068	27.11%	2.758%
13	11.093	1302	1310	1327	rBV	1728429	3042577	35.51%	3.612%
14	12.545	1550	1557	1566	rBV2	17788	42789	0.50%	0.051%
15	13.651	1737	1745	1751	rBV7	8693	15281	0.18%	0.018%
16	14.169	1825	1833	1845	rBV	3117183	4401185	51.36%	5.225%
17	14.463	1875	1883	1897	rBV	3744478	5544246	64.70%	6.583%
18	14.763	1926	1934	1944	rBV	2251132	3246859	37.89%	3.855%
19	14.951	1959	1966	1984	rBV	1350429	2168496	25.31%	2.575%
20	15.169	2001	2003	2008	rVB5	8782	10613	0.12%	0.013%
21	15.757	2096	2103	2116	rBV	4790114	6805014	79.42%	8.079%
22	15.869	2116	2122	2139	rVV	1368465	2006961	23.42%	2.383%
23	15.998	2139	2144	2152	rVB3	21823	40828	0.48%	0.048%
24	17.192	2342	2347	2352	rVB8	6515	10660	0.12%	0.013%
25	17.516	2396	2402	2412	rBV	2881096	3916586	45.71%	4.650%
26	17.616	2412	2419	2438	rVV2	5102192	7472559	87.21%	8.872%
27	19.416	2720	2725	2731	rBV2	55405	84218	0.98%	0.100%
28	19.480	2733	2736	2744	rVB	52089	73823	0.86%	0.088%
29	19.833	2790	2796	2810	rBV	6434805	8568823	100.00%	10.174%
30	21.592	3090	3095	3105	rBV	2845843	3864474	45.10%	4.588%
31	23.986	3494	3502	3516	rBV2	3609433	7778917	90.78%	9.236%
32	24.151	3523	3530	3547	rVB	1705090	3768412	43.98%	4.474%




Sum of corrected areas: 84226012

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015166.D
Acq On : 19 May 2023 09:44
Operator : CG/JU
Sample : PB152814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

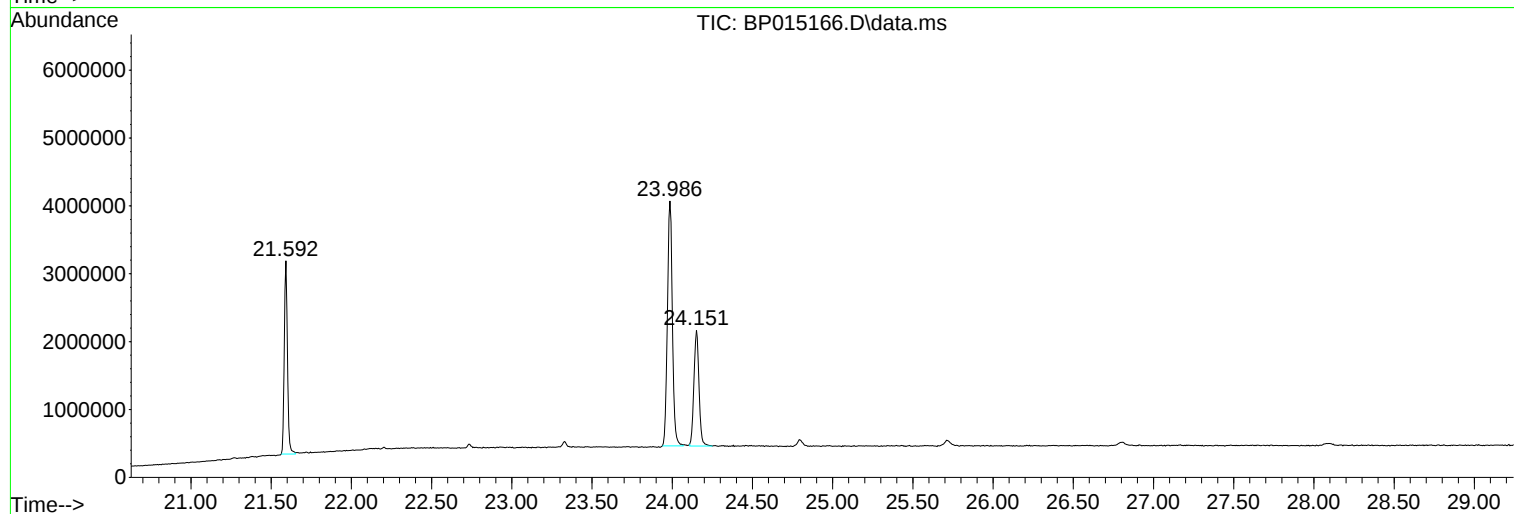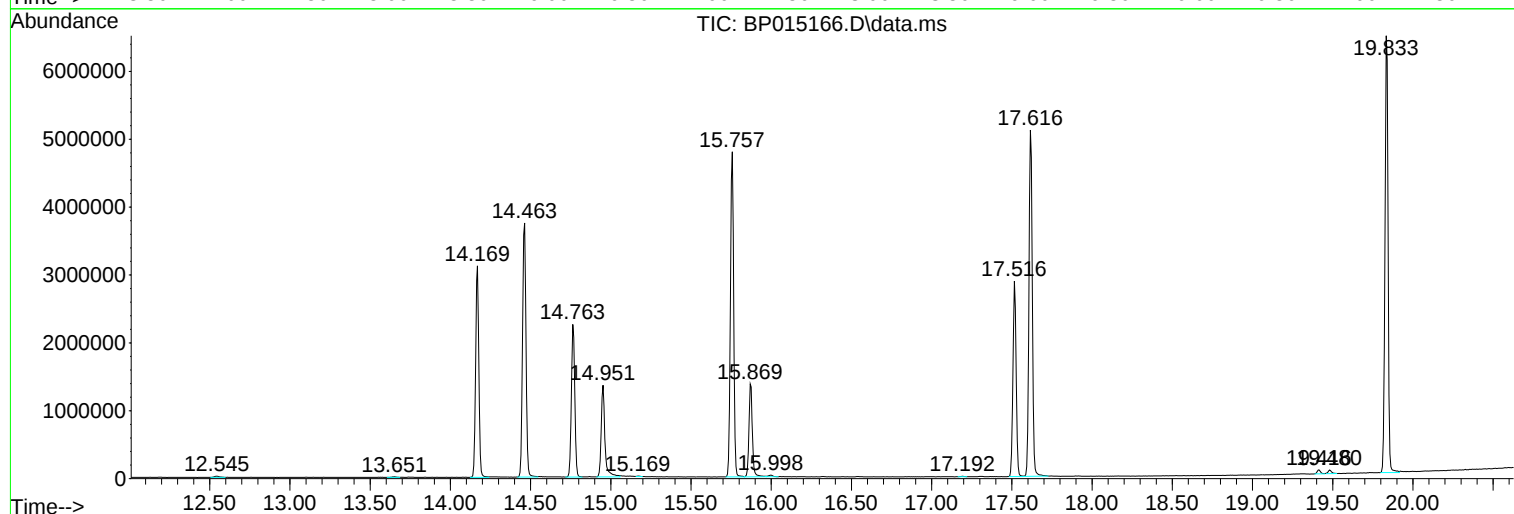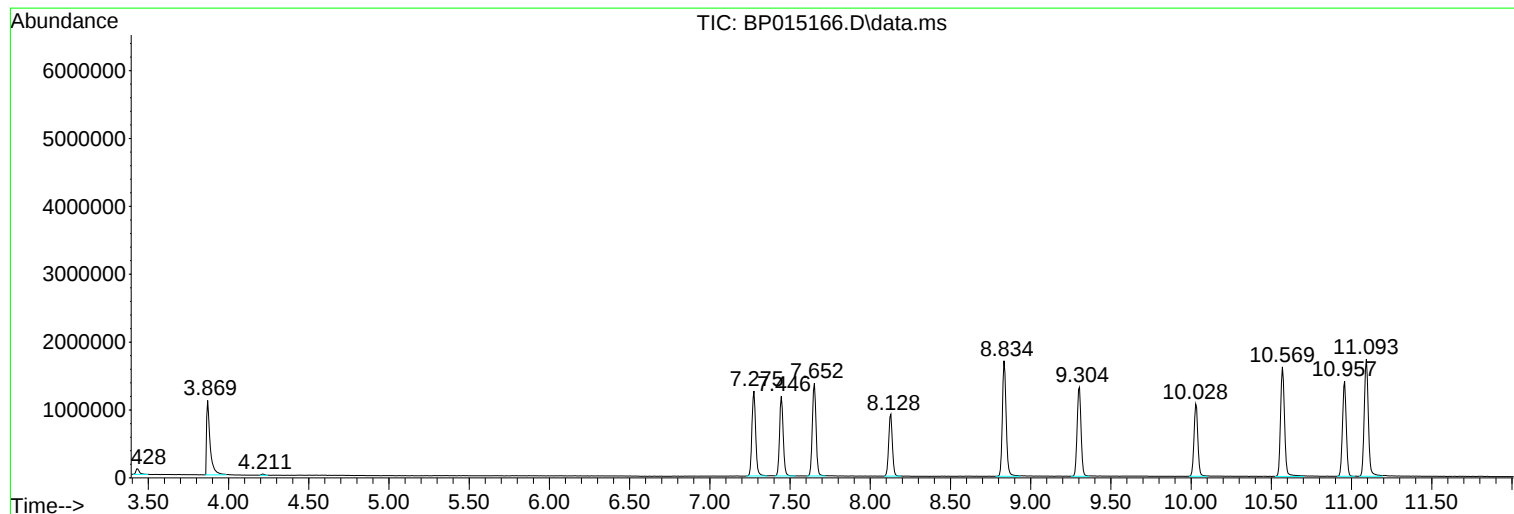

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015166.D
Acq On : 19 May 2023 09:44
Operator : CG/JU
Sample : PB152814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015166.D
Acq On : 19 May 2023 09:44
Operator : CG/JU
Sample : PB152814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------