

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
 Data File : BP015194.D
 Acq On : 20 May 2023 03:39
 Operator : CG/JU
 Sample : PB152787BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK787

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	49	rVB	25351	33042	0.45%	0.053%
2	3.875	114	117	133	rBV	315988	506938	6.84%	0.812%
3	4.211	170	174	178	rBV	11793	16562	0.22%	0.027%
4	7.275	687	695	709	rVB	366517	612677	8.26%	0.981%
5	7.446	717	724	735	rBV	292958	468959	6.32%	0.751%
6	7.646	752	758	768	rBV	366587	609534	8.22%	0.976%
7	8.122	828	839	850	rBV	830356	1326468	17.89%	2.124%
8	8.834	953	960	972	rBV	652043	1090656	14.71%	1.746%
9	9.299	1031	1039	1050	rBV	444081	736467	9.93%	1.179%
10	10.028	1155	1163	1174	rBV	438342	727012	9.80%	1.164%
11	10.569	1246	1255	1269	rBV	741760	1286465	17.35%	2.060%
12	10.951	1312	1320	1329	rBV	1200003	2031416	27.39%	3.252%
13	11.087	1336	1343	1361	rBV	1001968	1793278	24.18%	2.871%
14	12.534	1582	1589	1596	rBV2	11830	24009	0.32%	0.038%
15	13.645	1773	1778	1785	rVB2	14899	22345	0.30%	0.036%
16	14.163	1855	1866	1876	rBV	2950357	4280808	57.73%	6.854%
17	14.457	1909	1916	1929	rBV2	2853223	4209640	56.77%	6.740%
18	14.763	1961	1968	1980	rBV	1952546	2859703	38.56%	4.579%
19	14.857	1980	1984	1993	rVB	4228	8289	0.11%	0.013%
20	14.951	1993	2000	2027	rBV	1321117	2153774	29.04%	3.448%
21	15.169	2035	2037	2043	rVB7	6500	10395	0.14%	0.017%
22	15.751	2129	2136	2150	rBV	3923992	5839386	78.75%	9.349%
23	15.869	2150	2156	2171	rVV	1354554	1904591	25.68%	3.049%
24	15.992	2172	2177	2183	rVB2	22082	37060	0.50%	0.059%
25	17.181	2375	2379	2384	rVB8	7006	12345	0.17%	0.020%
26	17.298	2397	2399	2406	rVB5	6555	11650	0.16%	0.019%
27	17.516	2429	2436	2446	rBV	2408617	3457916	46.63%	5.536%
28	17.616	2446	2453	2467	rVV	4809709	6902464	93.08%	11.051%
29	17.804	2482	2485	2492	rVB9	9260	15009	0.20%	0.024%
30	17.892	2496	2500	2506	rBV7	7006	14098	0.19%	0.023%
31	19.410	2754	2758	2764	rVB2	67241	88039	1.19%	0.141%
32	19.475	2765	2769	2775	rBV	59107	87227	1.18%	0.140%
33	19.833	2824	2830	2840	rBV	5647112	7415503	100.00%	11.873%
34	21.586	3123	3128	3138	rBV	2014069	2850490	38.44%	4.564%
35	23.980	3527	3535	3547	rBV2	2865467	6315090	85.16%	10.111%
36	24.145	3557	3563	3575	rVB	1239930	2698922	36.40%	4.321%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015194.D
Acq On : 20 May 2023 03:39
Operator : CG/JU
Sample : PB152787BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 62458227

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015194.D
Acq On : 20 May 2023 03:39
Operator : CG/JU
Sample : PB152787BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

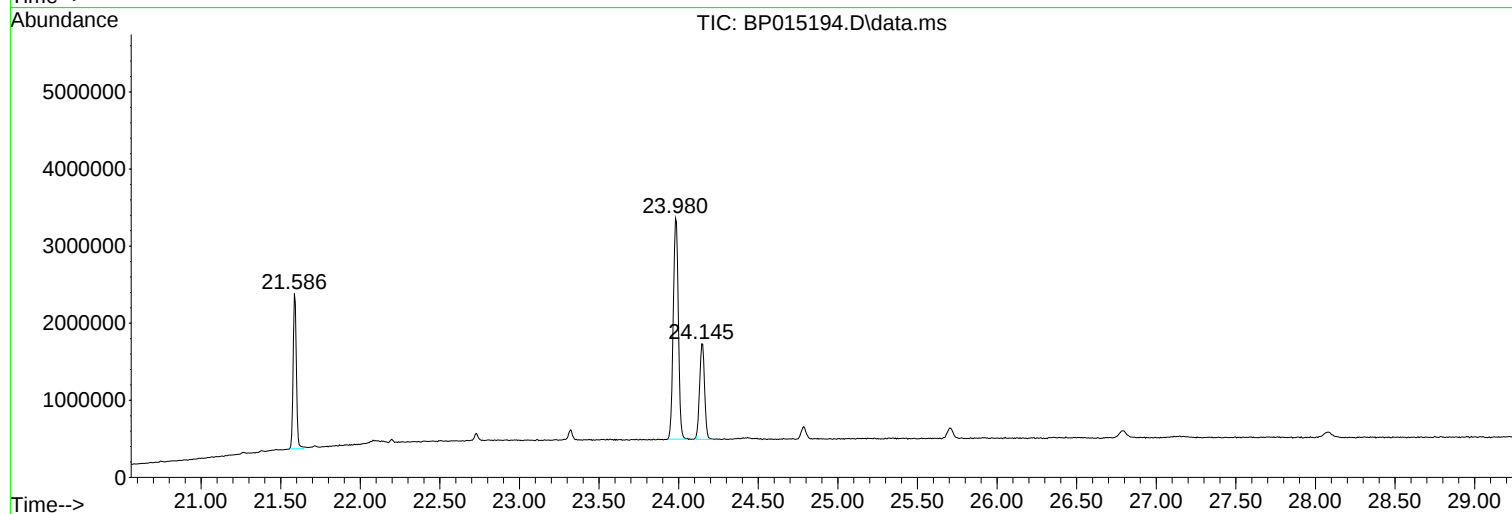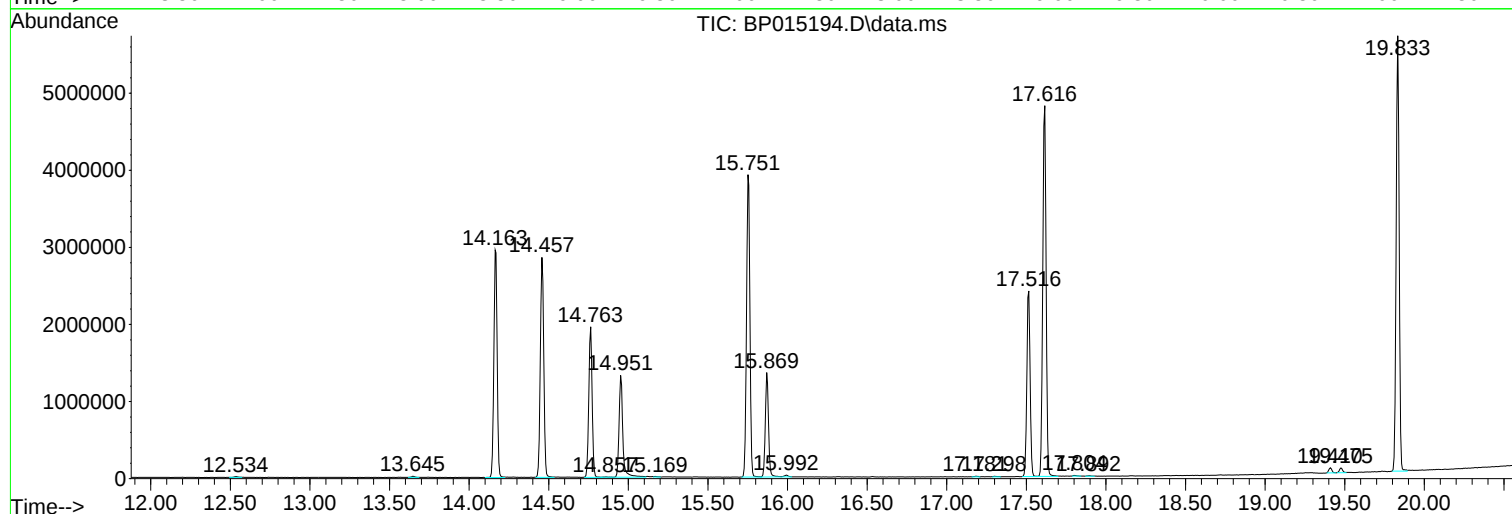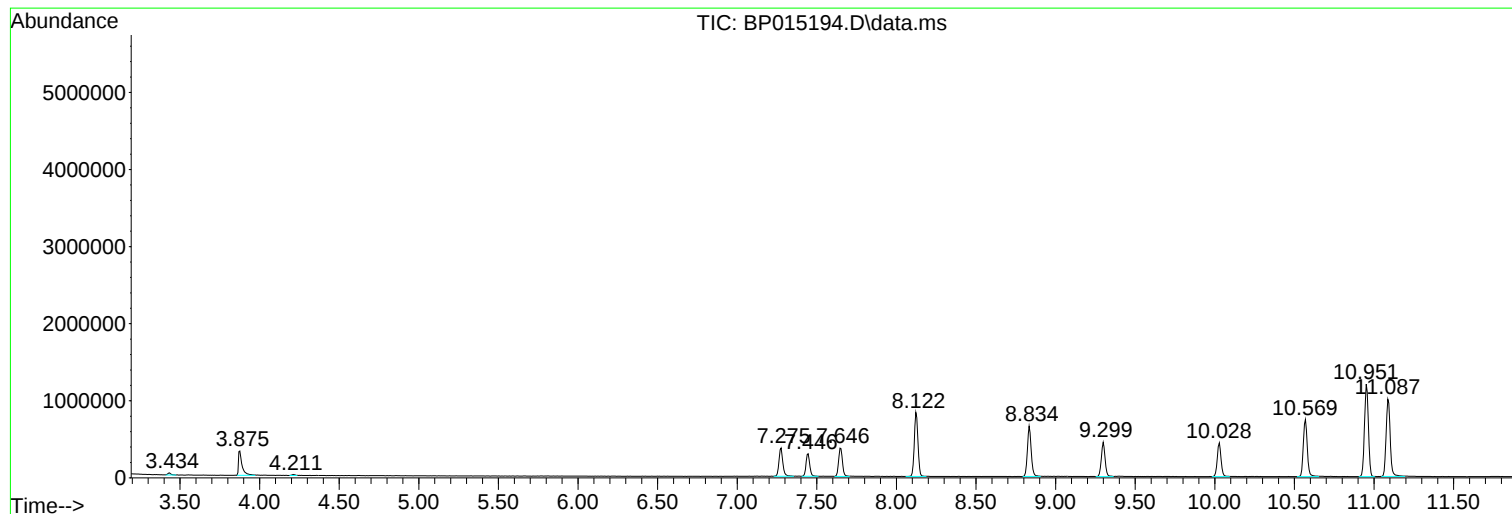

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP05194.D
Acq On : 20 May 2023 03:39
Operator : CG/JU
Sample : PB152787BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051923\
Data File : BP015194.D
Acq On : 20 May 2023 03:39
Operator : CG/JU
Sample : PB152787BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------