
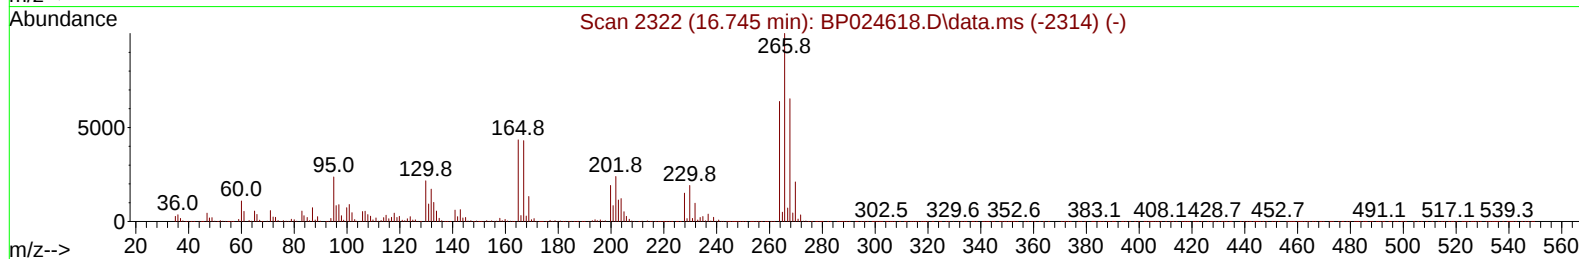
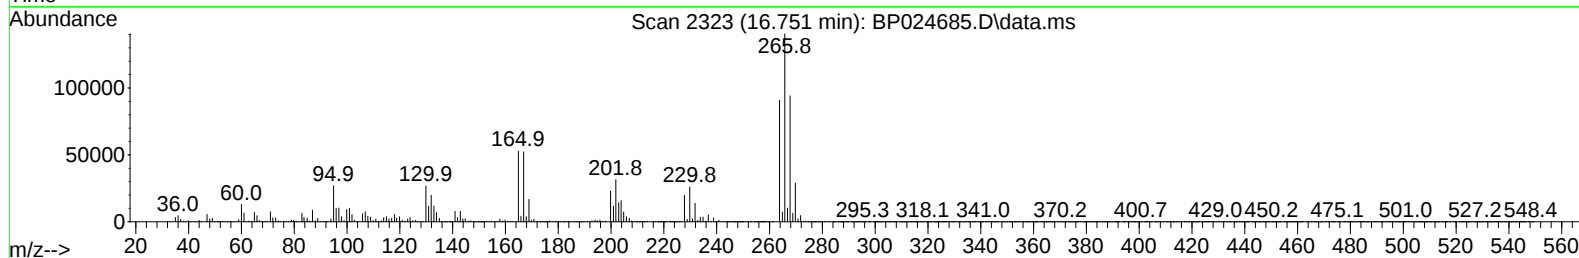


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051925\
Data File : BP024685.D
Acq On : 19 May 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 14:36:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

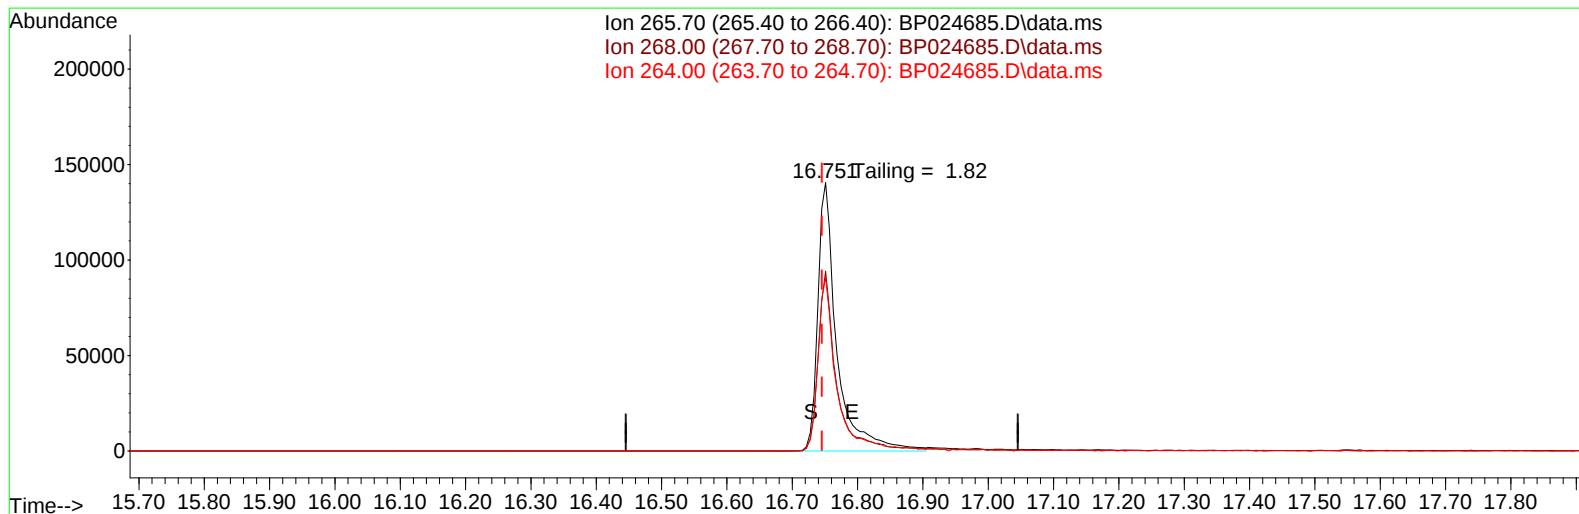

TIC: BP024685.D\data.ms

(70) Pentachlorophenol (C)




16.751min (+ 0.006) 677862.06 ng

response 284874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	67.02
264.00	63.90	64.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051925\
Data File : BP024685.D
Acq On : 19 May 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 14:36:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

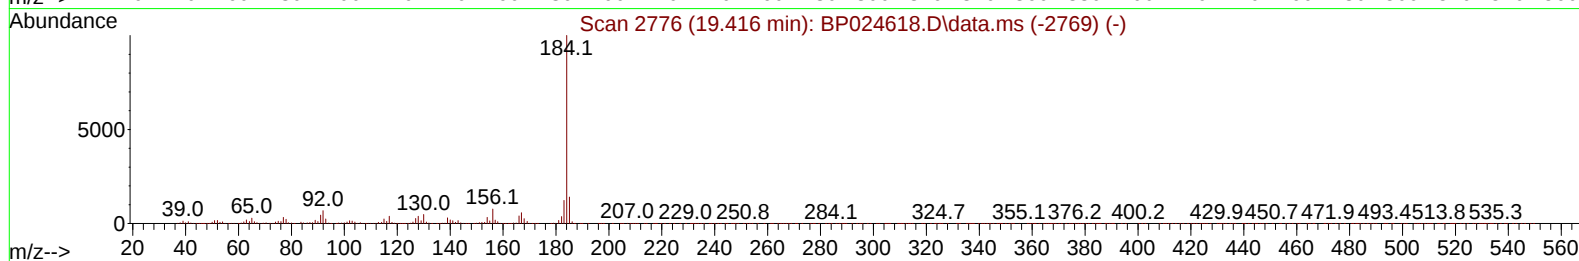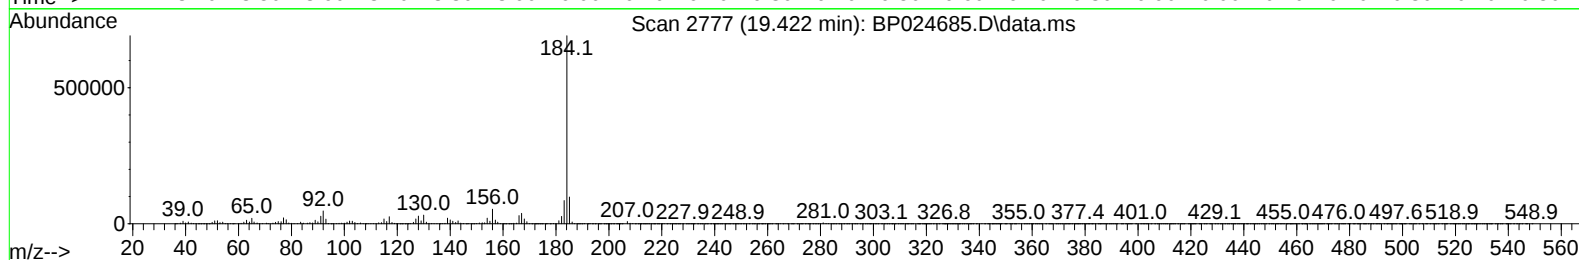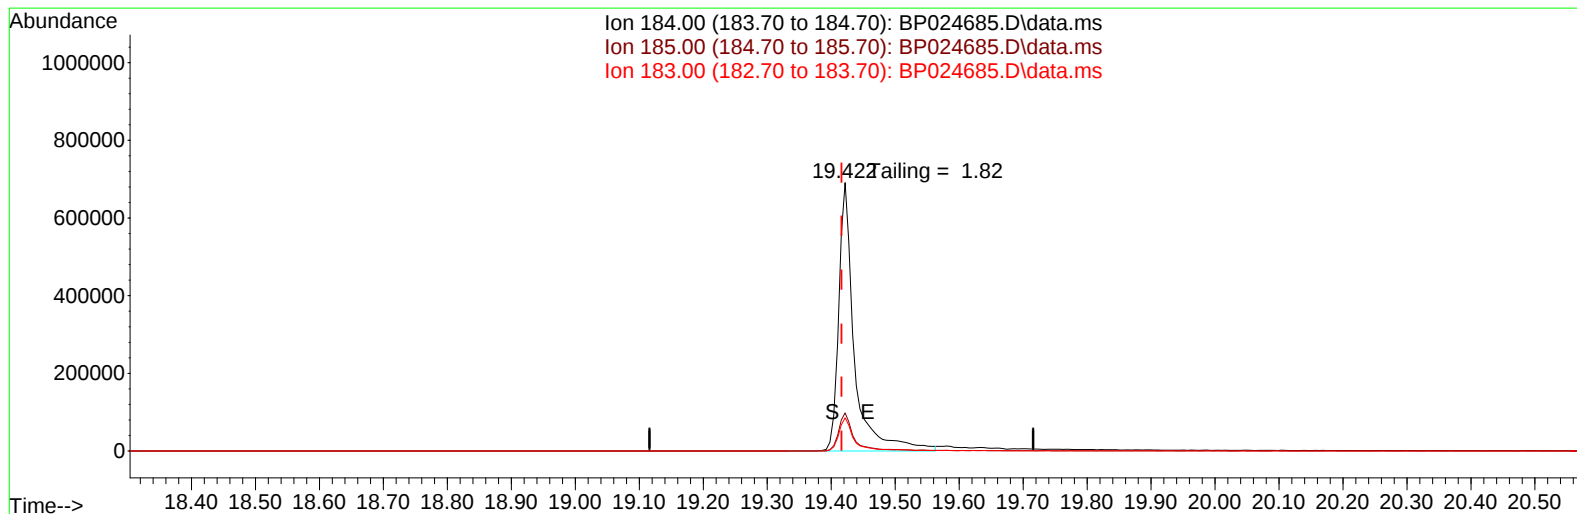

TIC: BP024685.D\data.ms

(77) Benzidine**19.422min (+ 0.006) 78779.38 ng****response 1186534**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.18
183.00	12.30	12.34
0.00	0.00	0.00