

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052021\
 Data File : BP005621.D
 Acq On : 20 May 2021 13:42
 Operator : CG/JU
 Sample : PB136538TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136538TB

Quant Time: May 20 14:36:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 20 14:18:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	7732	20.00	ng	0.00
21) Naphthalene-d8	10.451	136	22555	20.00	ng	# 0.00
39) Acenaphthene-d10	14.316	164	17458	20.00	ng	0.00
64) Phenanthrene-d10	17.068	188	45237	20.00	ng	# 0.00
76) Chrysene-d12	21.174	240	69019	20.00	ng	# 0.00
86) Perylene-d12	23.462	264	79403	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.251	112	58052	144.09	ng	0.00
7) Phenol-d6	6.863	99	56785	113.03	ng	0.00
23) Nitrobenzene-d5	8.828	82	49794	86.89	ng	0.00
42) 2,4,6-Tribromophenol	15.816	330	55471	111.97	ng	0.00
45) 2-Fluorobiphenyl	12.927	172	121358	78.42	ng	0.00
79) Terphenyl-d14	19.639	244	340202	83.71	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052021\
Data File : BP005621.D
Acq On : 20 May 2021 13:42
Operator : CG/JU
Sample : PB136538TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136538TB

Quant Time: May 20 14:36:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 20 14:18:01 2021
Response via : Initial Calibration




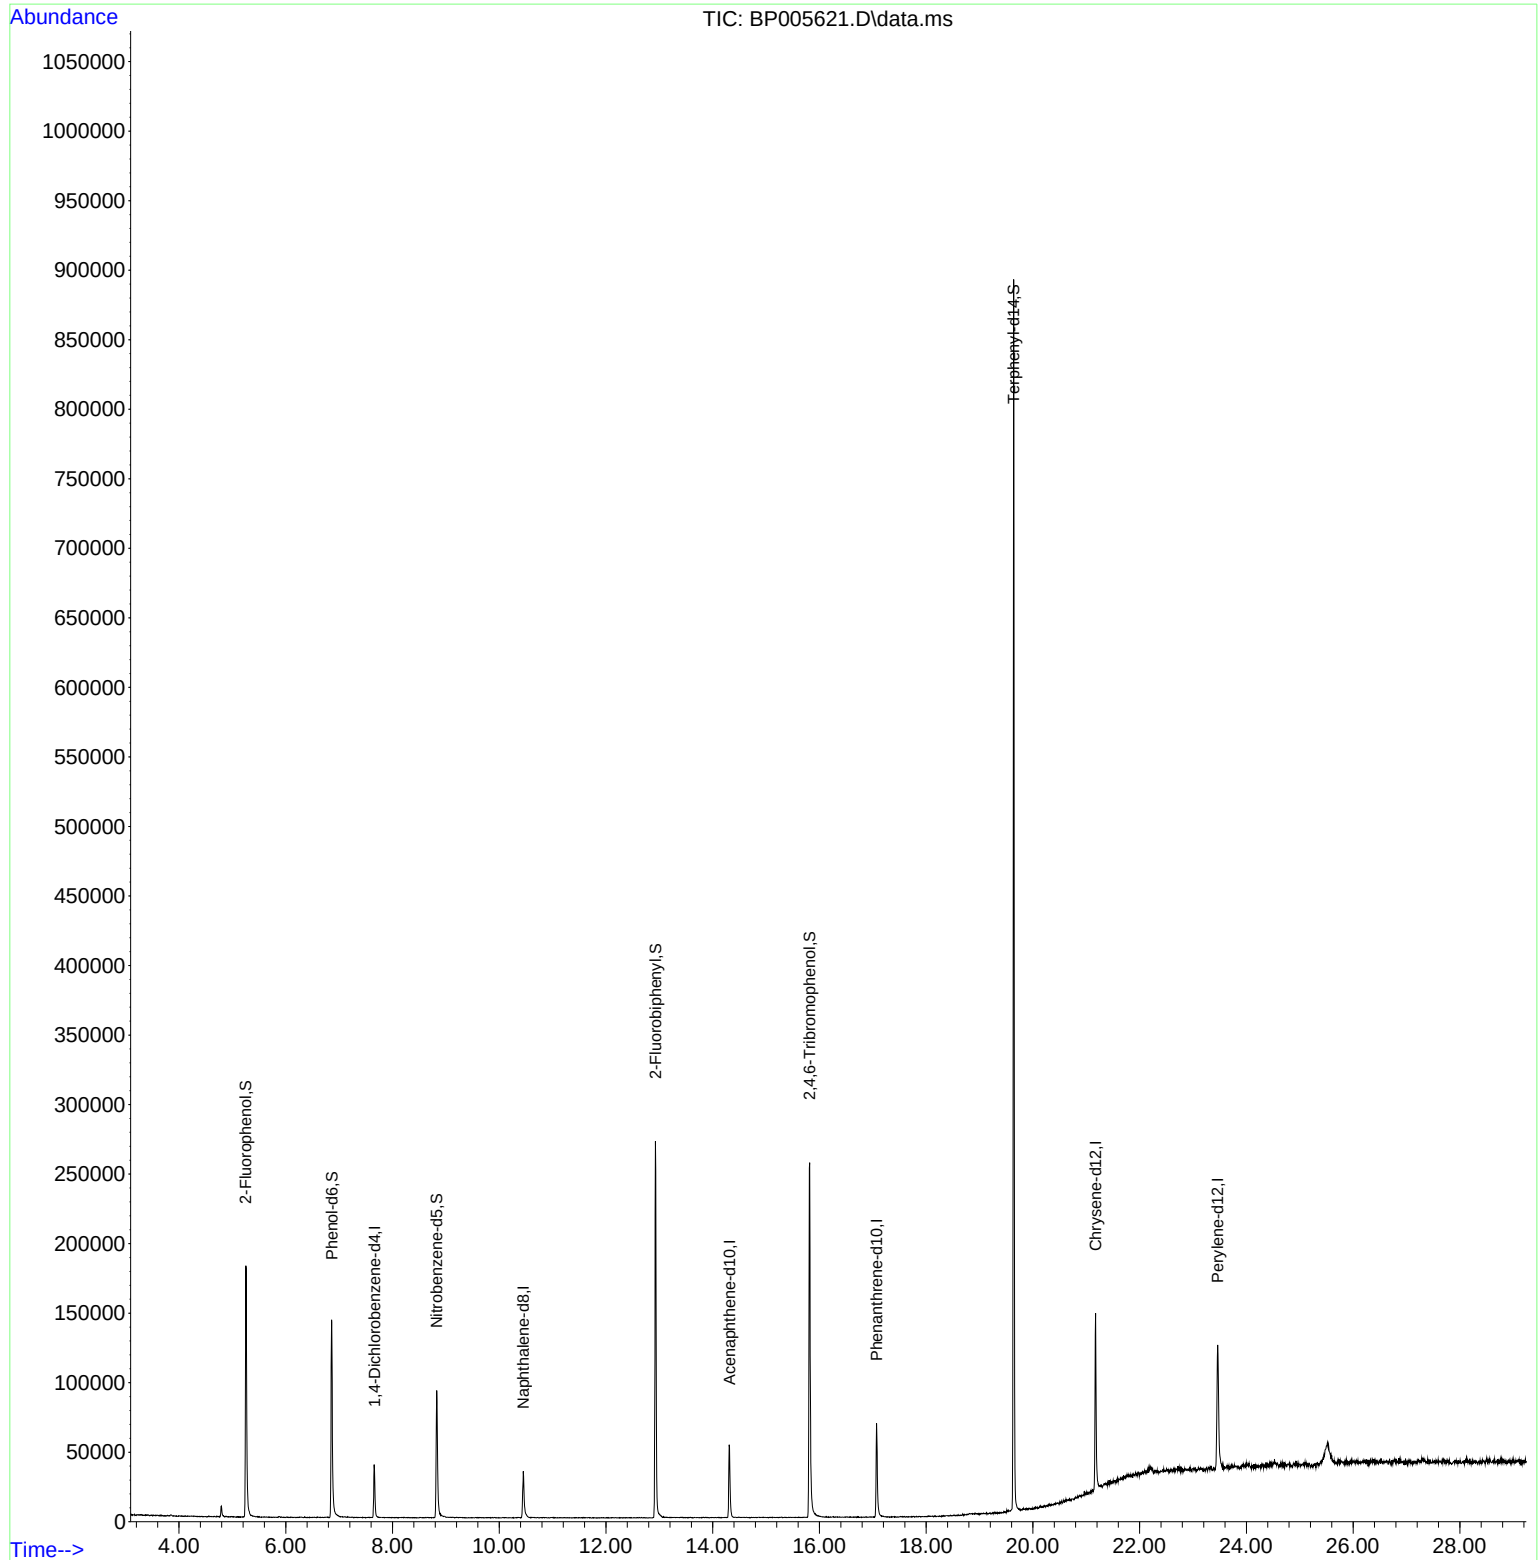


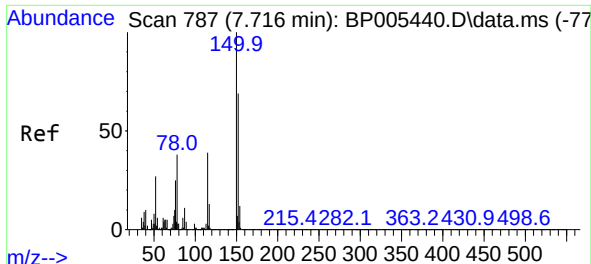

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.663 min Scan# 778
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42




Instrument :
BNA_P
ClientSampleId :
PB136538TB


Tgt Ion:152 Resp: 7732
Ion Ratio Lower Upper
152 100
150 151.7 119.8 179.8
115 59.5 49.0 73.4

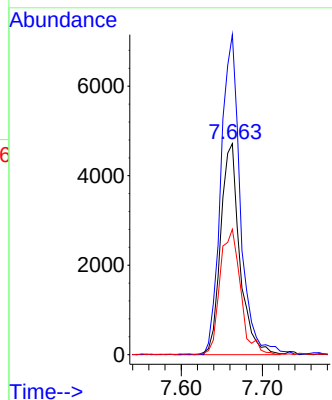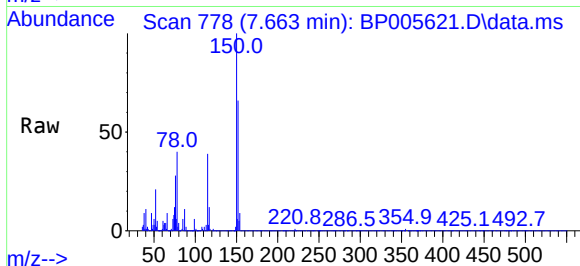

#5
2-Fluorophenol
Concen: 144.09 ng
RT: 5.251 min Scan# 368
Delta R.T. -0.000 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion:112 Resp: 58052
Ion Ratio Lower Upper
112 100
64 53.2 33.6 50.4#
63 47.0 18.6 27.8#


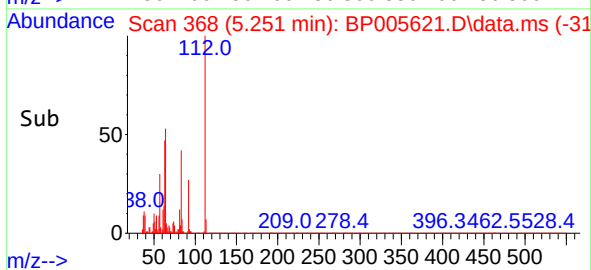
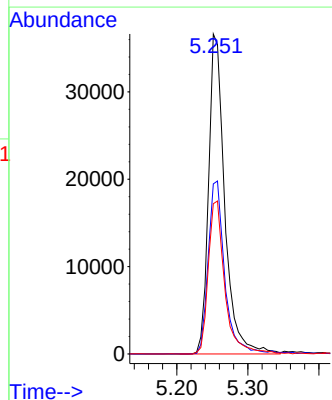
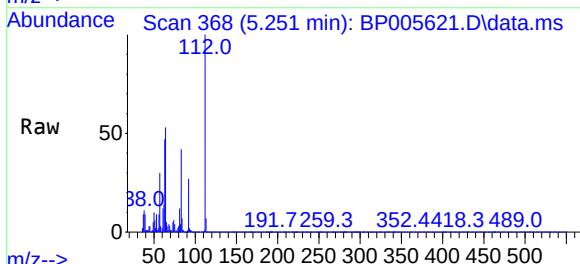


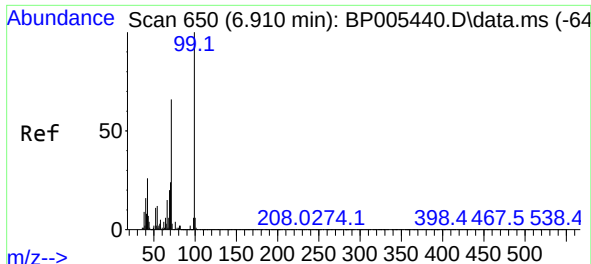

#7
Phenol-d6
Concen: 113.03 ng
RT: 6.863 min Scan# 642
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42




Instrument :
BNA_P
ClientSampleId :
PB136538TB


Tgt Ion:	99	Resp:	56785
Ion	Ratio	Lower	Upper
99	100		
42	34.0	12.9	19.3#
71	77.5	26.7	40.1#

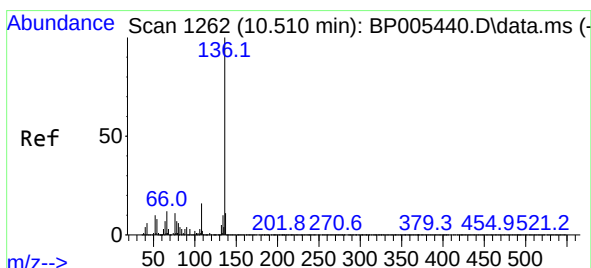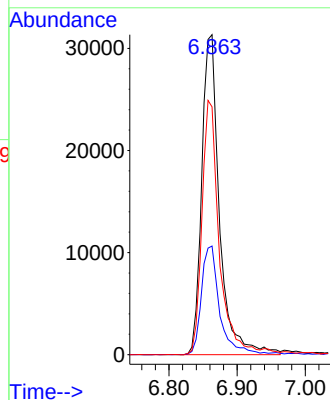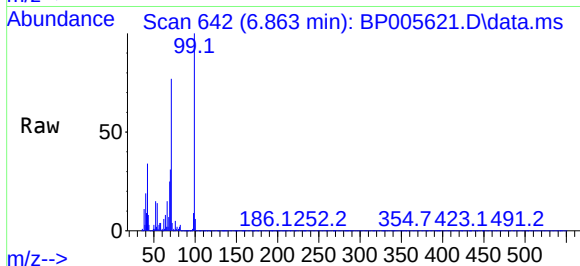

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.451 min Scan# 1252
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion:	136	Resp:	22555
Ion	Ratio	Lower	Upper
136	100		
137	7.6	8.9	13.3#
54	10.4	5.0	7.4#
68	2.8	3.7	5.5#


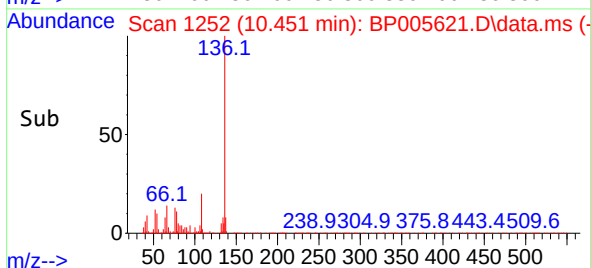
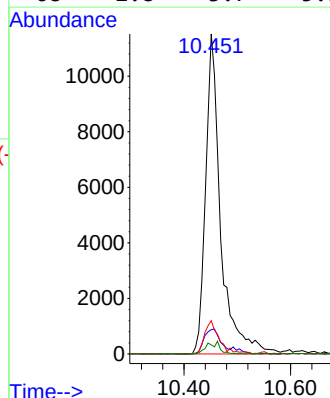
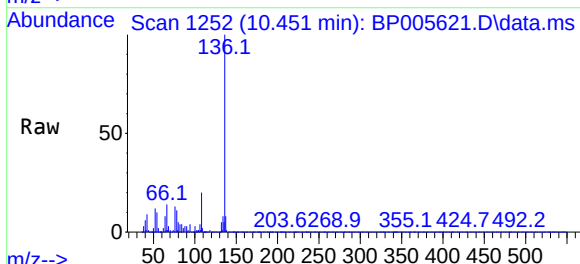


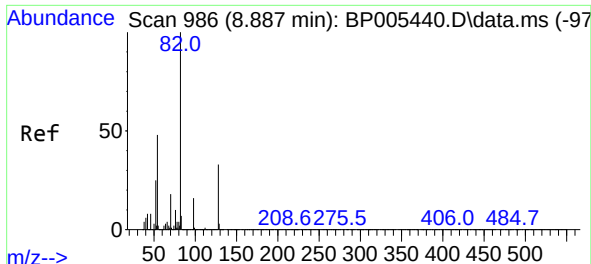

#23
Nitrobenzene-d5
Concen: 86.89 ng
RT: 8.828 min Scan# 976
Delta R.T. -0.000 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42




Instrument :
BNA_P
ClientSampleId :
PB136538TB


Tgt Ion: 82 Resp: 49794
Ion Ratio Lower Upper
82 100
128 31.9 30.5 45.7
54 56.1 33.9 50.9#

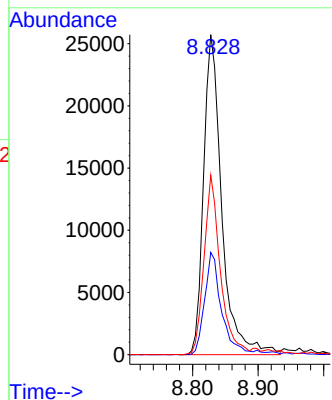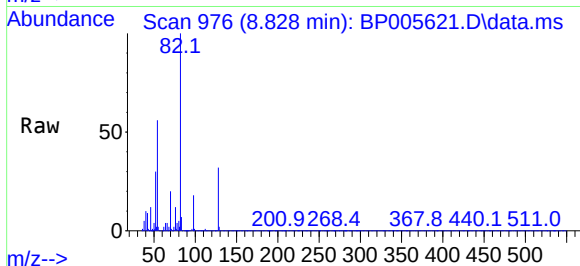

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.316 min Scan# 1909
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion: 164 Resp: 17458
Ion Ratio Lower Upper
164 100
162 95.2 73.5 110.3
160 41.7 40.6 61.0


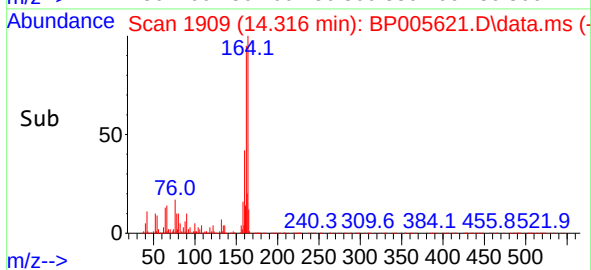
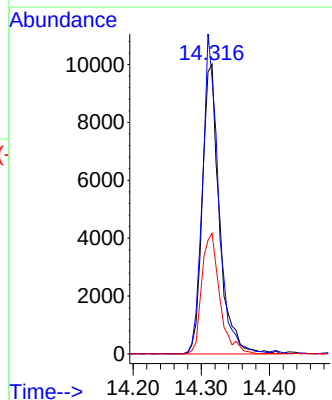
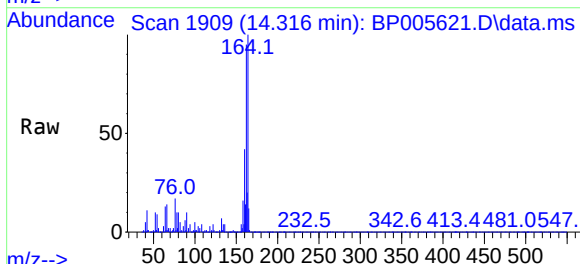


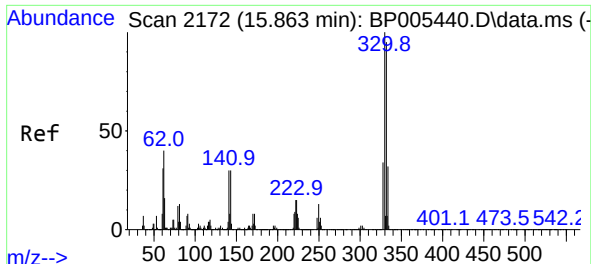

#42
2,4,6-Tribromophenol
Concen: 111.97 ng
RT: 15.816 min Scan# 2164
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42




Instrument :
BNA_P
ClientSampleId :
PB136538TB


Tgt Ion:	330	Resp:	55471
Ion Ratio	Lower	Upper	
330	100		
332	99.3	76.3	114.5
141	31.3	22.8	34.2

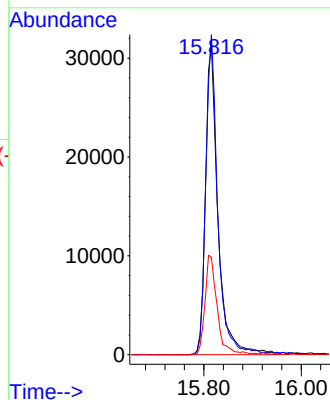

#45
2-Fluorobiphenyl
Concen: 78.42 ng
RT: 12.927 min Scan# 1673
Delta R.T. -0.000 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion:	172	Resp:	121358
Ion Ratio	Lower	Upper	
172	100		
171	35.6	28.1	42.1
170	22.9	19.6	29.4


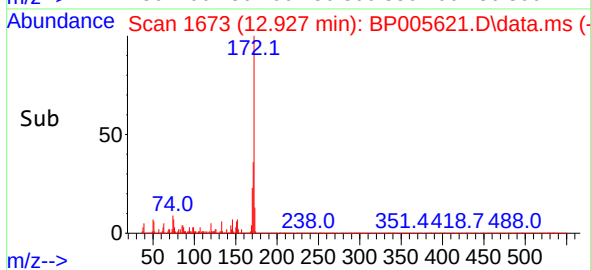
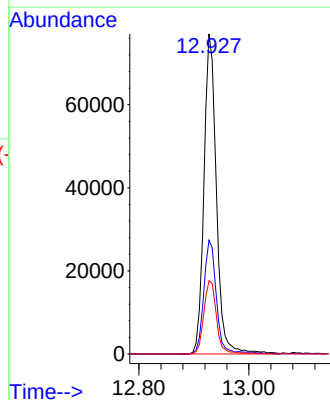
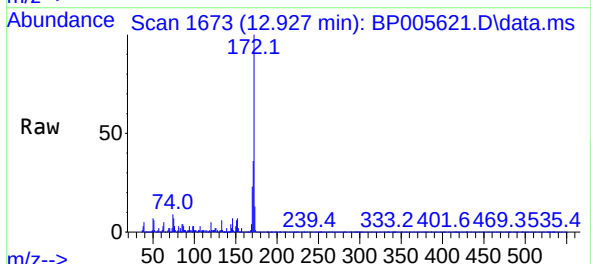


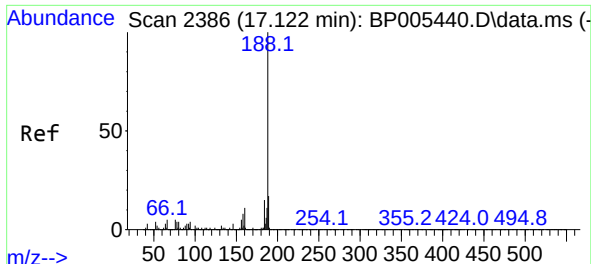

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.068 min Scan# 2377
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42




Instrument :
BNA_P
ClientSampleId :
PB136538TB


Tgt Ion:188	Resp:	45237
Ion Ratio	Lower	Upper
188	100	
94	4.6	5.0 7.6#
80	4.6	5.9 8.9#

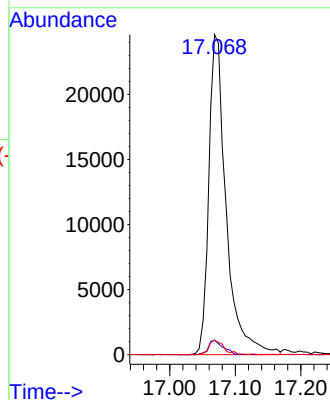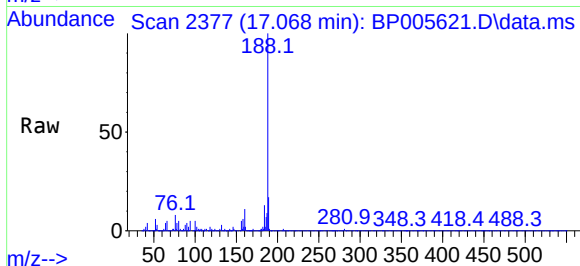

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.174 min Scan# 3075
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion:240	Resp:	69019
Ion Ratio	Lower	Upper
240	100	
120	1.3	4.2 6.2#
236	27.1	20.2 30.2

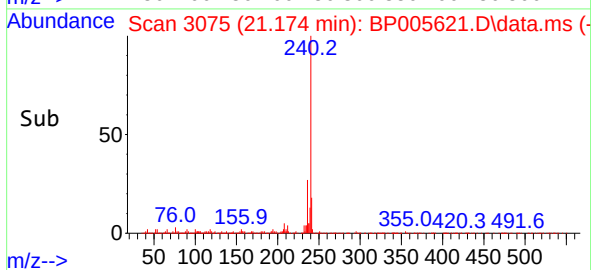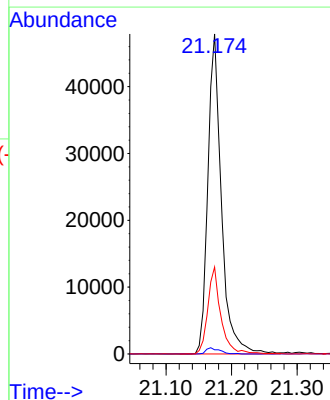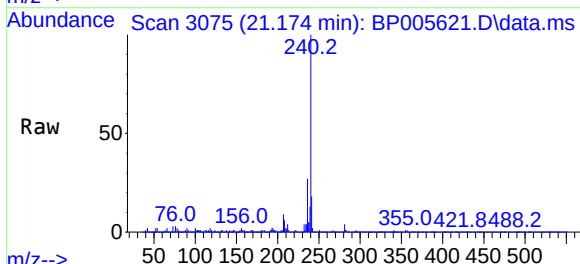







#79
Terphenyl-d14
Concen: 83.71 ng
RT: 19.639 min Scan# 2814
Delta R.T. -0.000 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Instrument :
BNA_P
ClientSampleId :
PB136538TB

Tgt Ion:244 Resp: 340202

Ion	Ratio	Lower	Upper
244	100		
212	8.4	5.8	8.6
122	4.2	5.2	7.8#

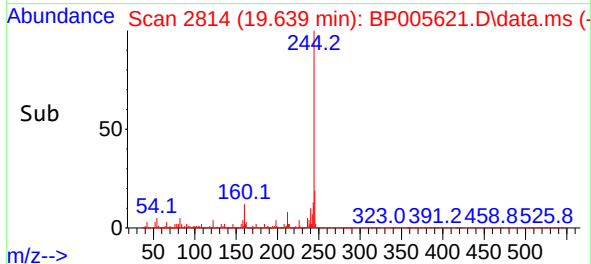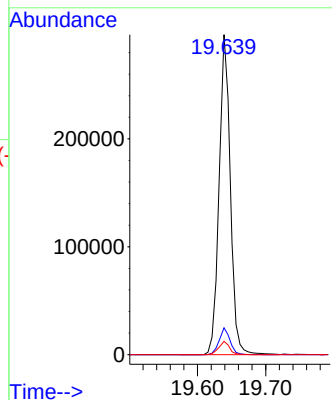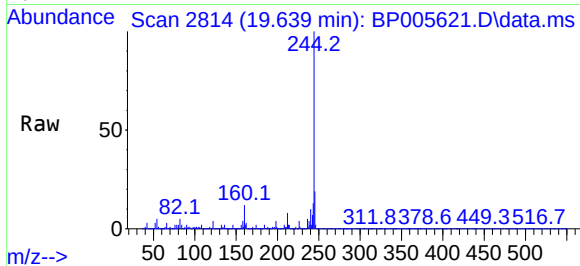

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.462 min Scan# 3464
Delta R.T. 0.005 min
Lab File: BP005621.D
Acq: 20 May 2021 13:42

Tgt Ion:264 Resp: 79403

Ion	Ratio	Lower	Upper
264	100		
260	25.2	20.6	30.8
265	21.7	19.0	28.6

