
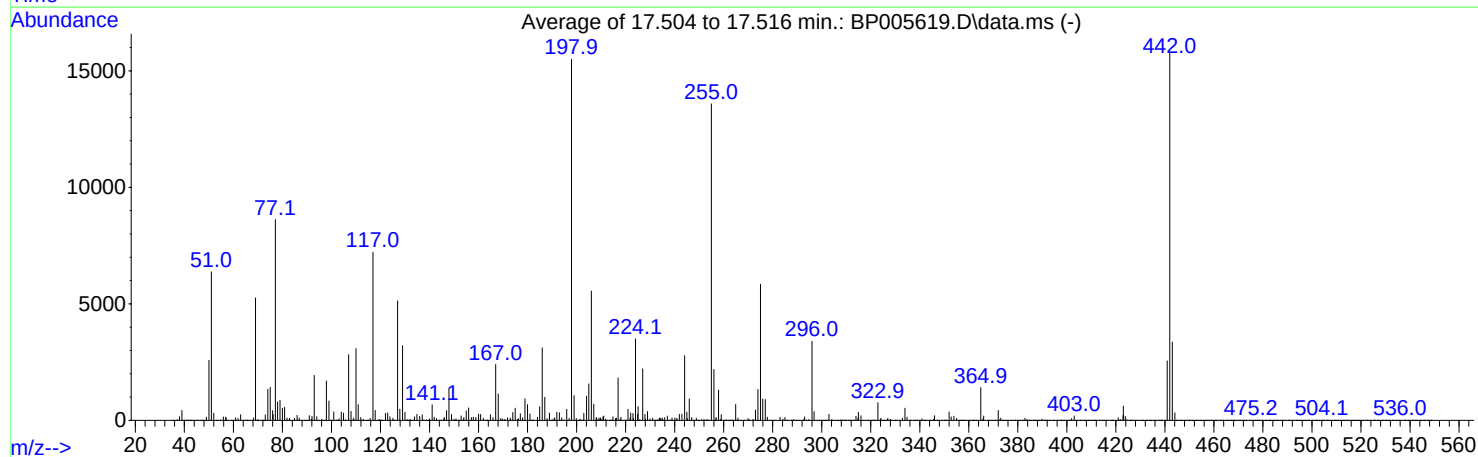


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052021\  
 Data File : BP005619.D  
 Acq On : 20 May 2021 12:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP050521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu May 20 14:18:01 2021

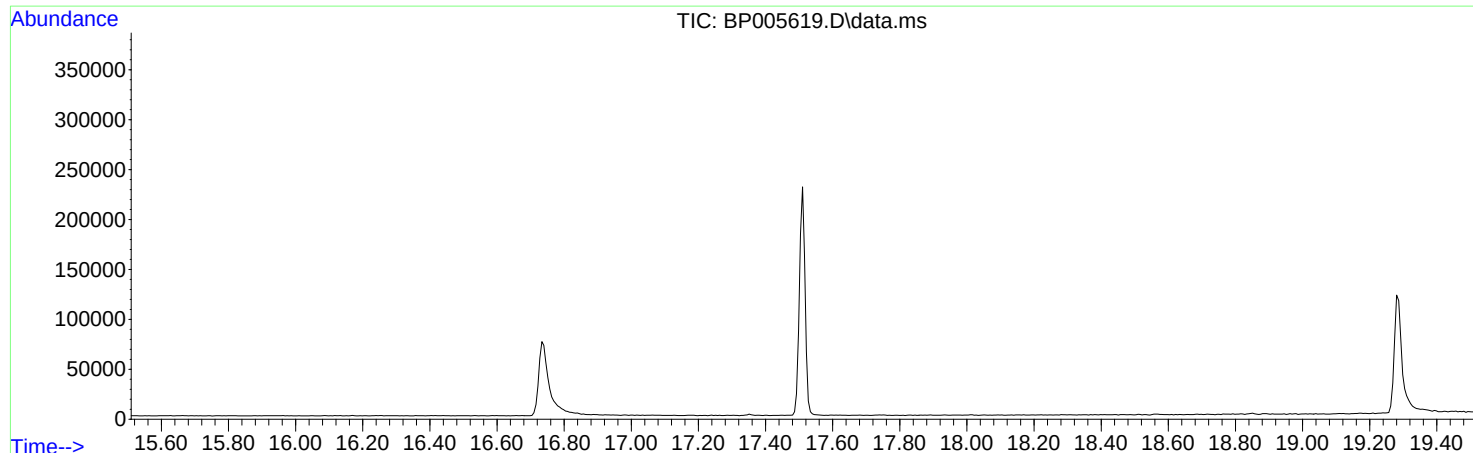




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2440

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.1         | 6374       | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 104        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.9         | 5253       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 41         | PASS                |
| 127            | 198             | 10              | 80              | 33.1         | 5131       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 80         | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 15499      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 1067       | PASS                |
| 275            | 198             | 10              | 60              | 37.7         | 5845       | PASS                |
| 365            | 198             | 1               | 100             | 9.1          | 1405       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.5         | 2555       | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 15787      | PASS                |
| 443            | 442             | 15              | 24              | 21.3         | 3357       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052021\  
 Data File : BP005619.D  
 Acq On : 20 May 2021 12:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: May 20 13:55:50 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP050521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon May 17 15:35:47 2021  
 Response via : Initial Calibration

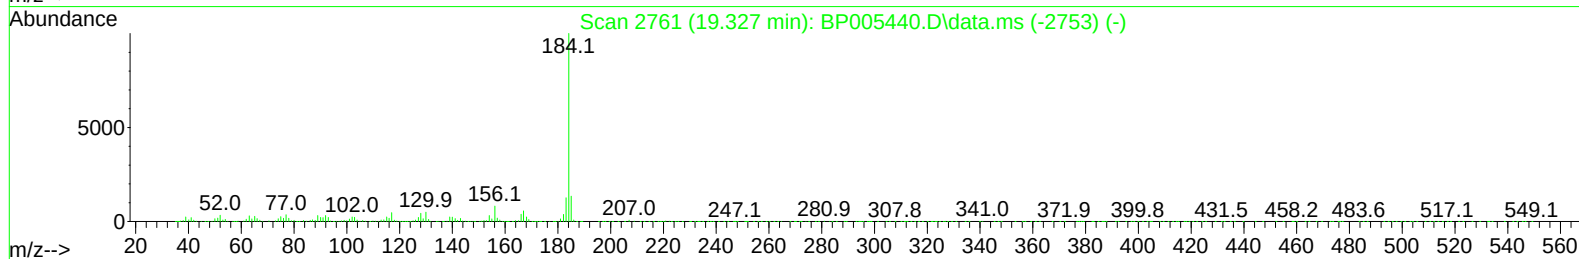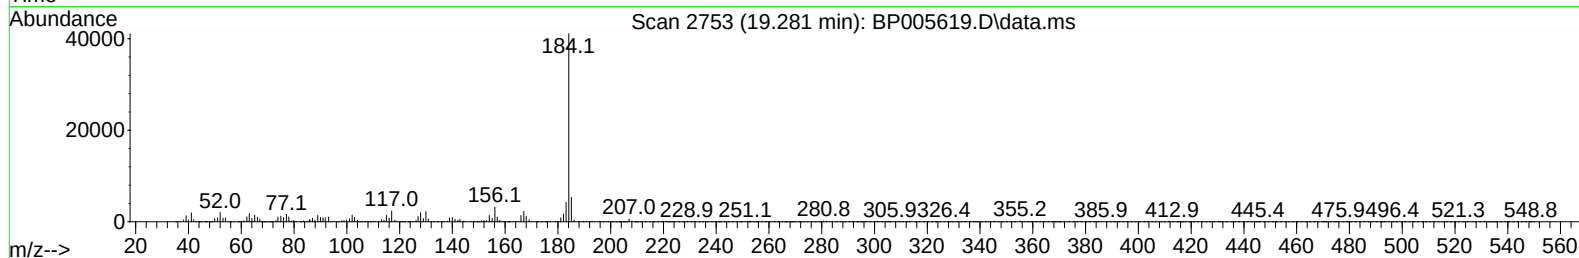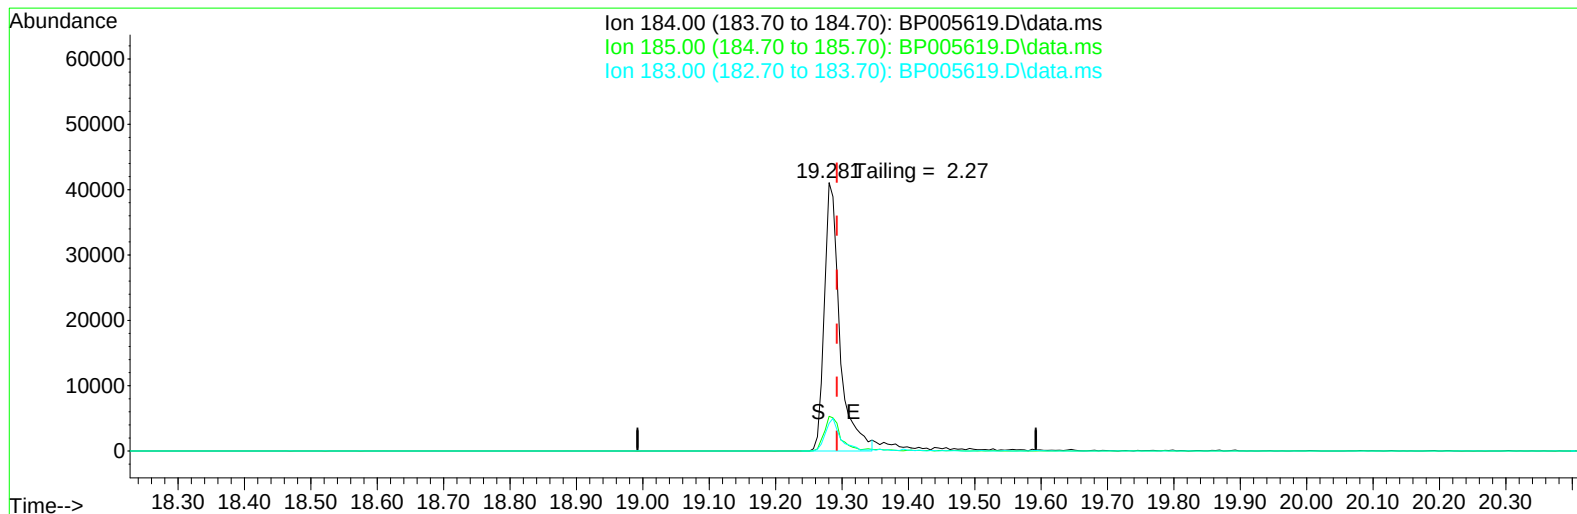

TIC: BP005619.D\data.ms

**(77) Benzidine**

19.281min (-0.012) 187520.07 ng




response 69662

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 12.98  |
| 183.00 | 12.30  | 10.34  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052021\  
 Data File : BP005619.D  
 Acq On : 20 May 2021 12:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: May 20 13:55:50 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP050521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon May 17 15:35:47 2021  
 Response via : Initial Calibration

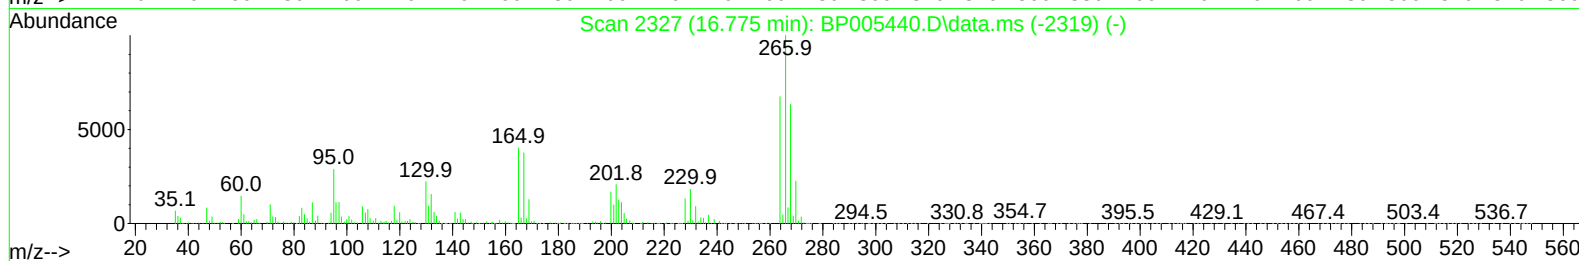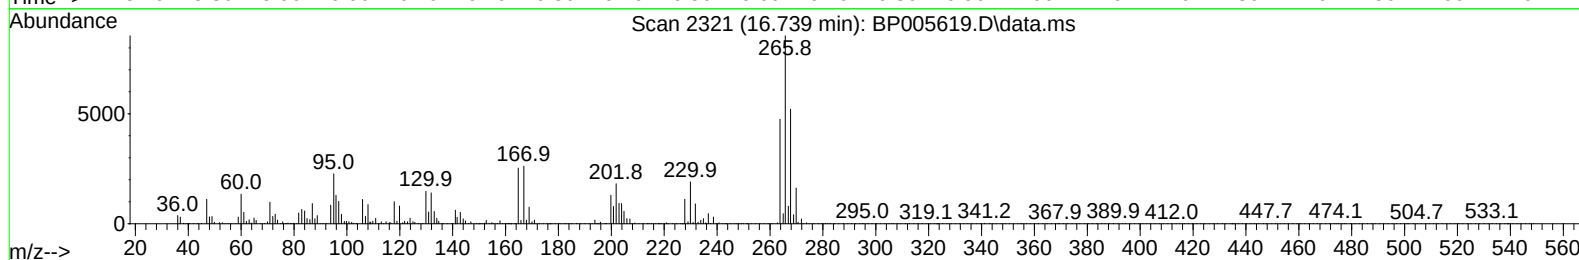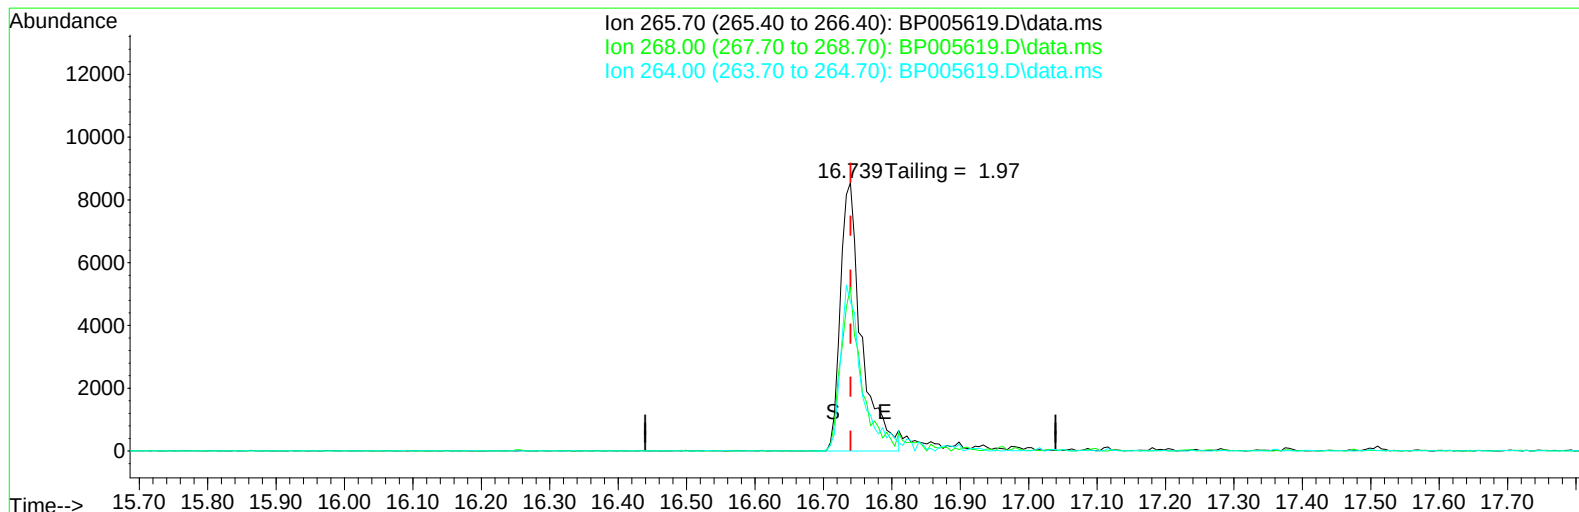

TIC: BP005619.D\data.ms

**(70) Pentachlorophenol (C)**

16.739min (+ 0.000) 122965.24 ng

response 18082

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.70  | 60.91  |
| 264.00 | 67.10  | 55.61  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/20/2021     | BNA_P            | <u>BP005619.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 57711            | 20.46              |
| DDD           | 3254             | 20.04              |
| DDE           | 349              | 19.54              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3603          | 61314            | 5.88               |
|               |                  |                    |