




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

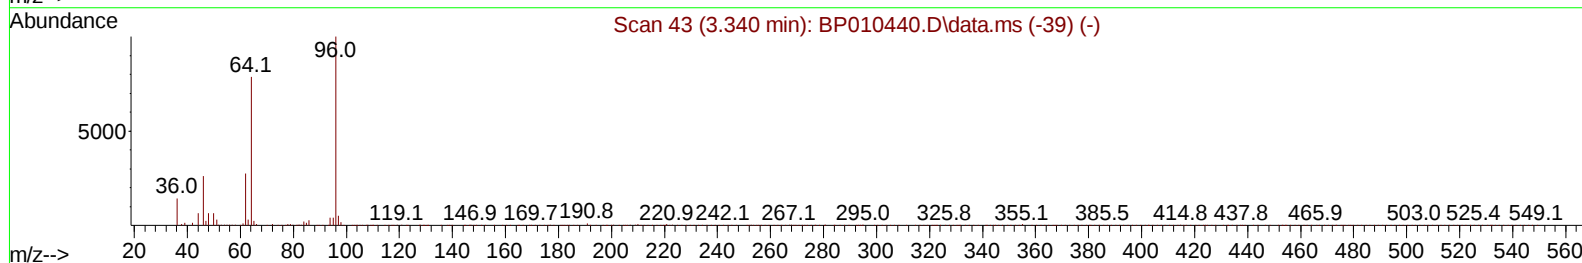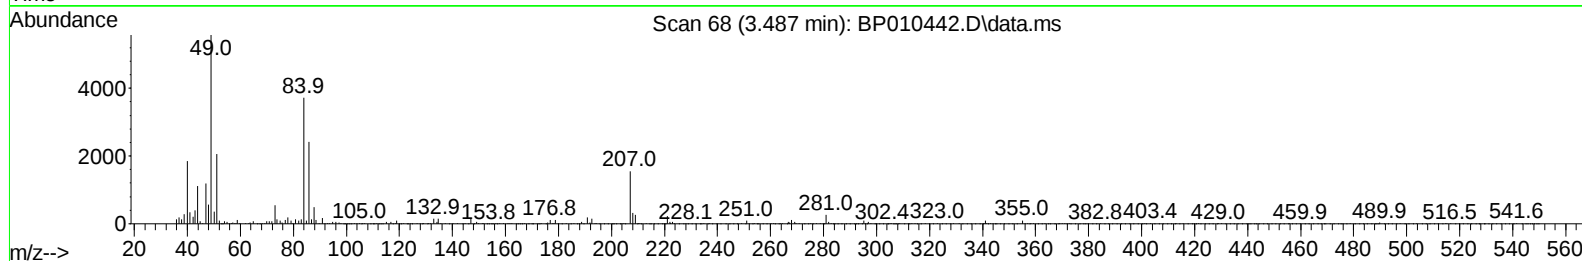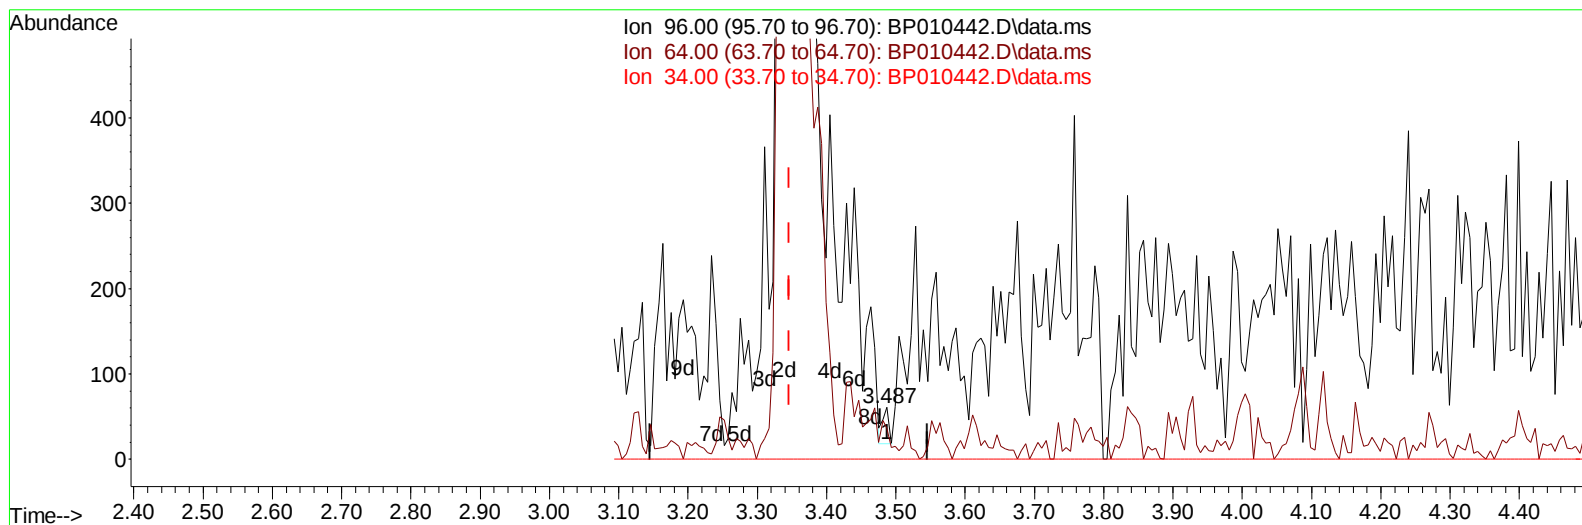

TIC: BP010442.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.487min (+ 0.141) 0.01 ng/uL

response 25

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	59.02
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

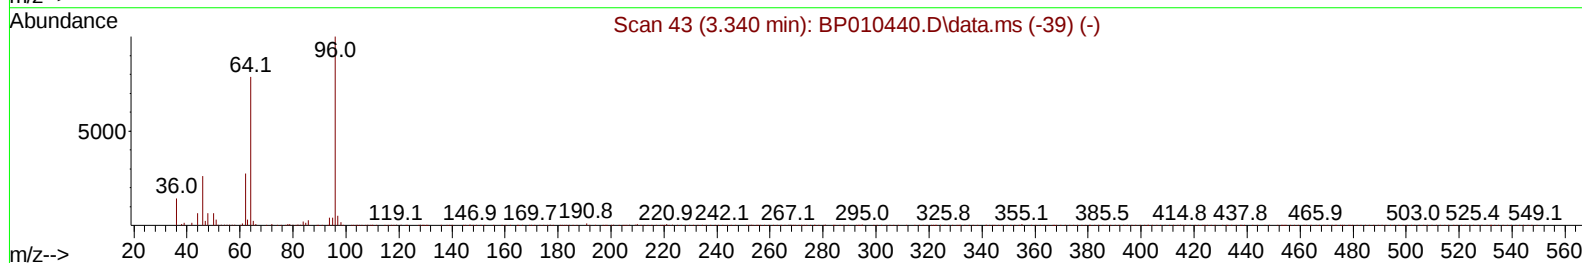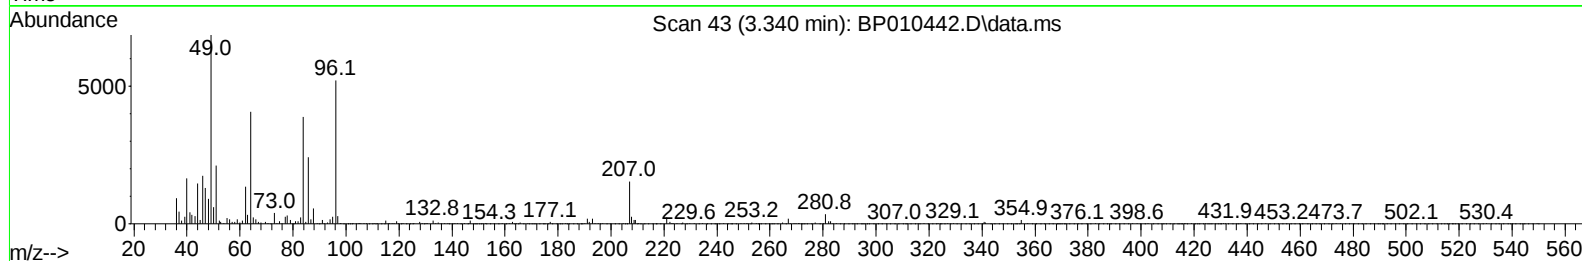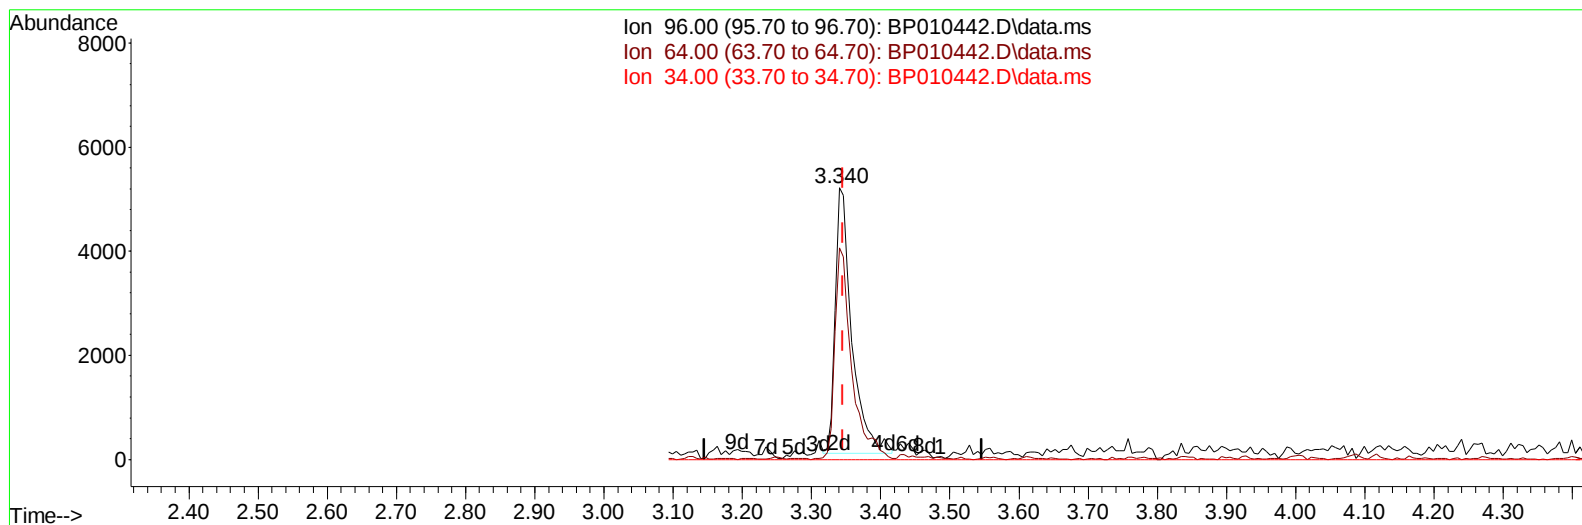

TIC: BP010442.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 2.96 ng/uL m

response 8480

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.95#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

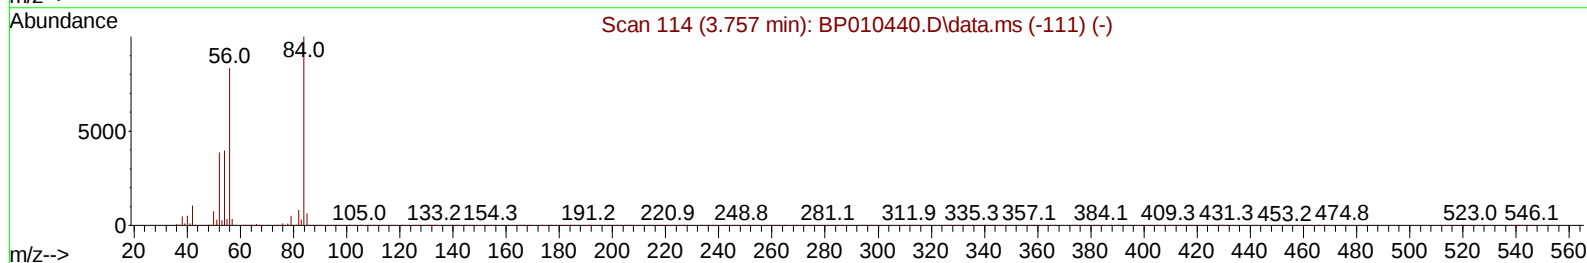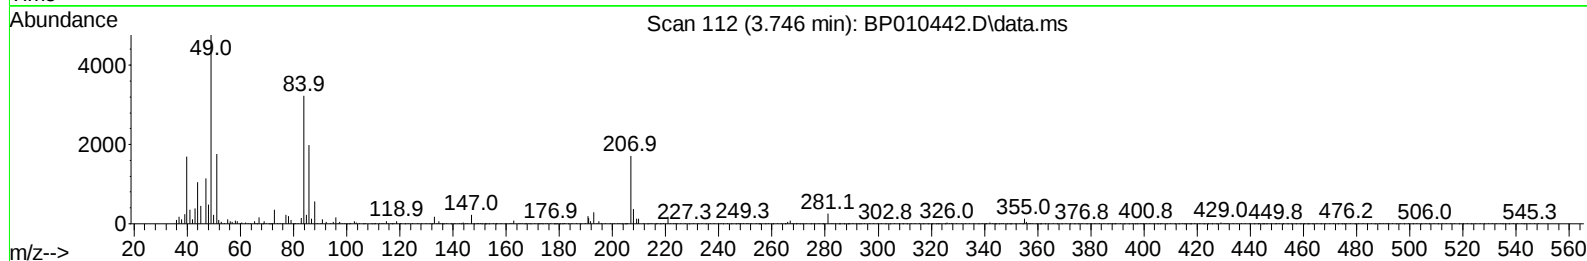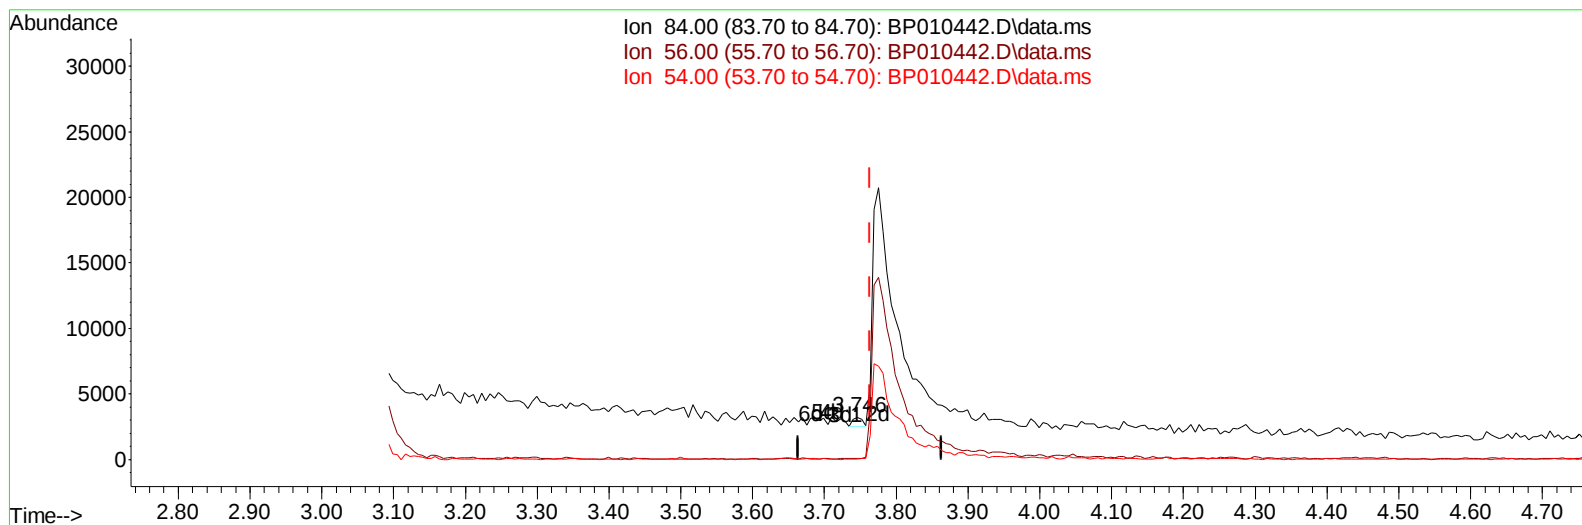

TIC: BP010442.D\data.ms

(4) Pyridine-d5 (S)

3.746min (-0.018) 0.08 ng/u1

response 648

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	2.23#
54.00	24.80	0.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

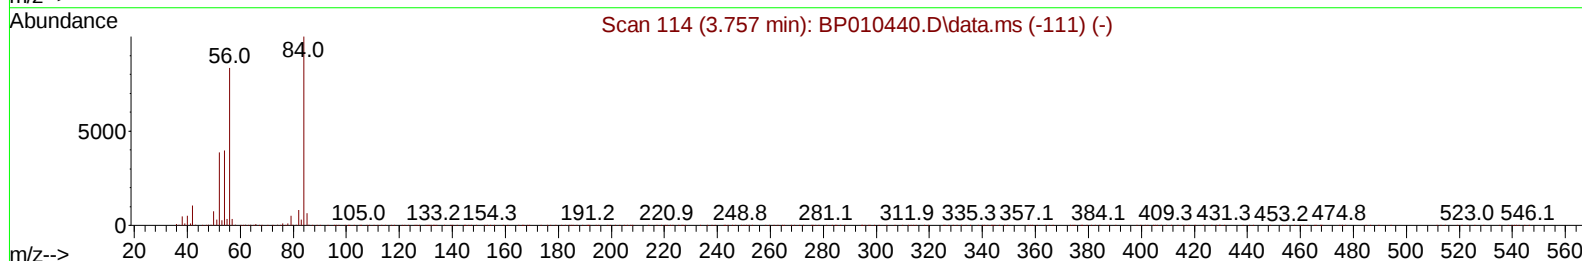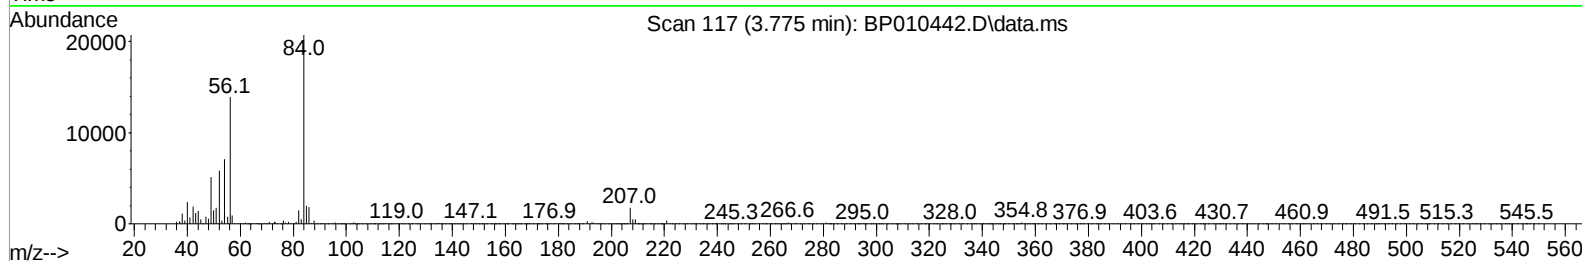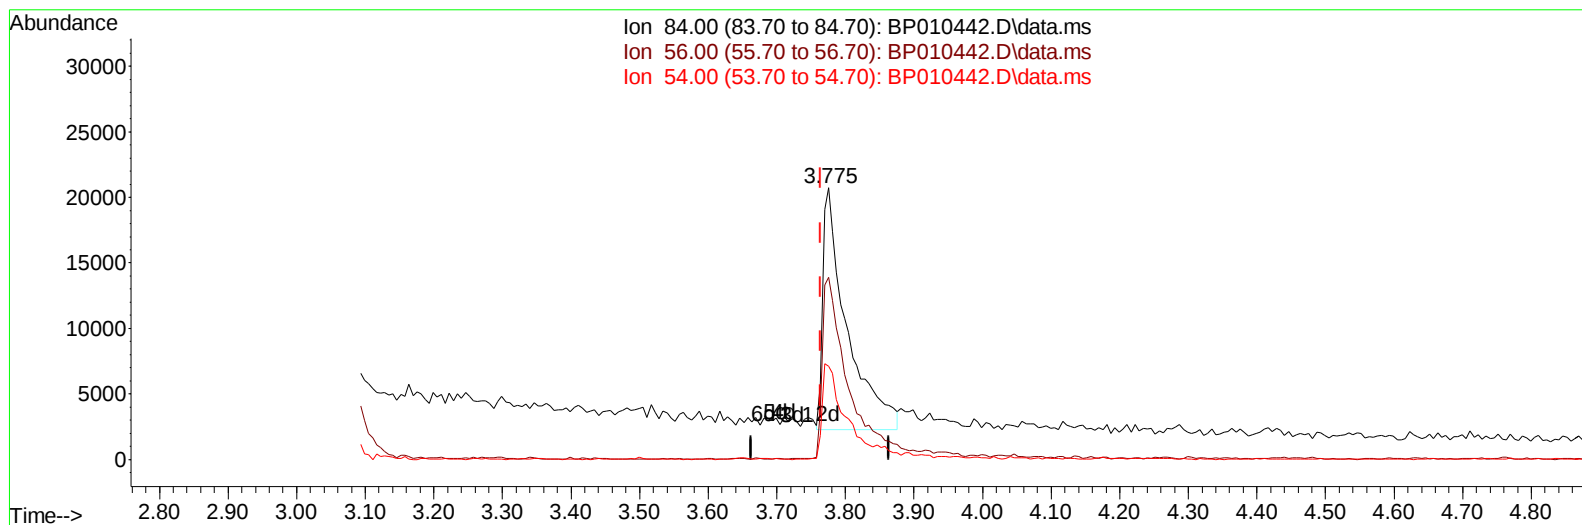

TIC: BP010442.D\data.ms

(4) Pyridine-d5 (S)

3.775min (+ 0.012) 5.54 ng/ul m

response 45030

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	67.04#
54.00	24.80	34.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

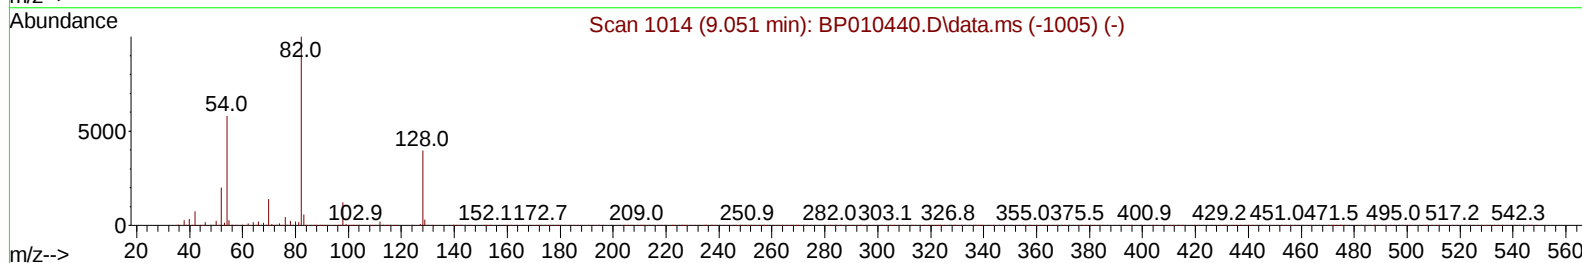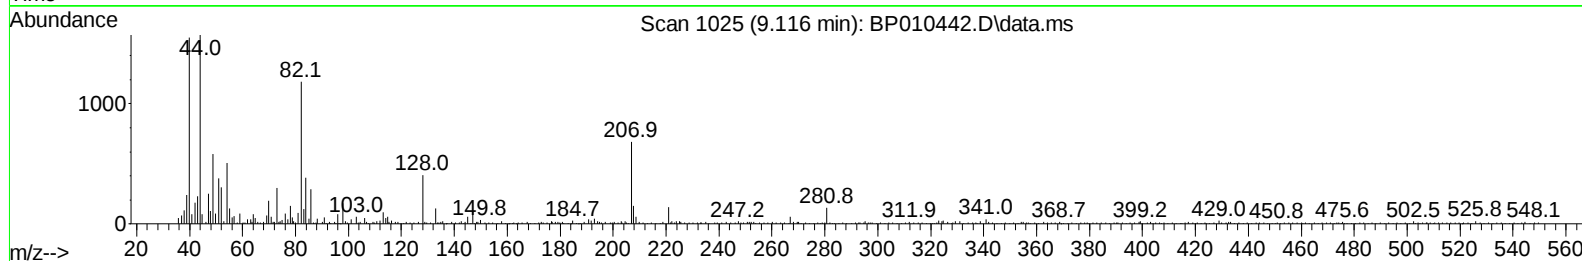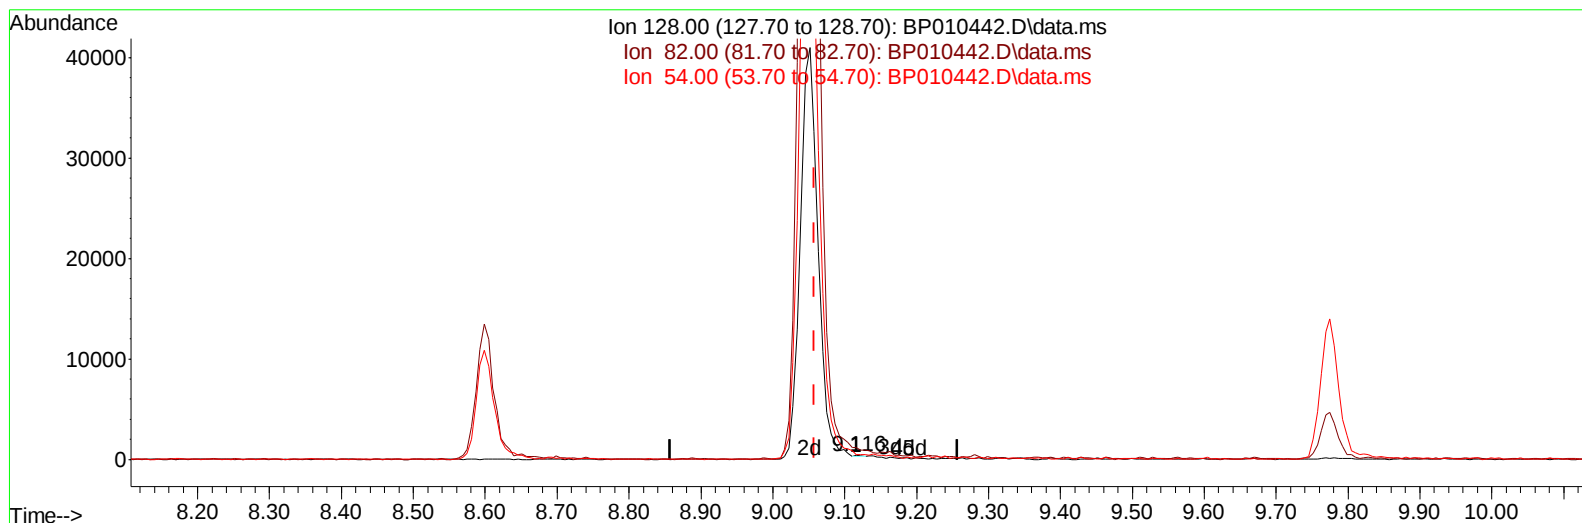

TIC: BP010442.D\data.ms

(21) Nitrobenzene-d5 (S)

9.116min (+ 0.059) 0.02 ng/u1

response 90

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	291.87
54.00	120.20	124.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

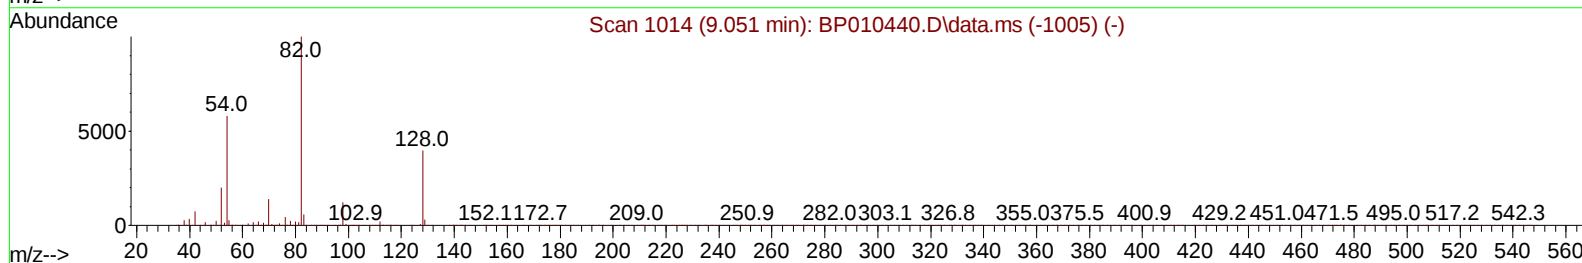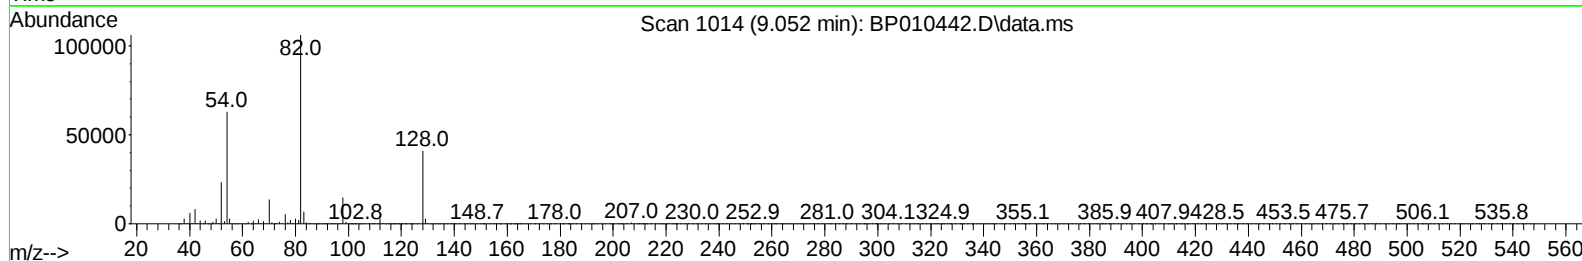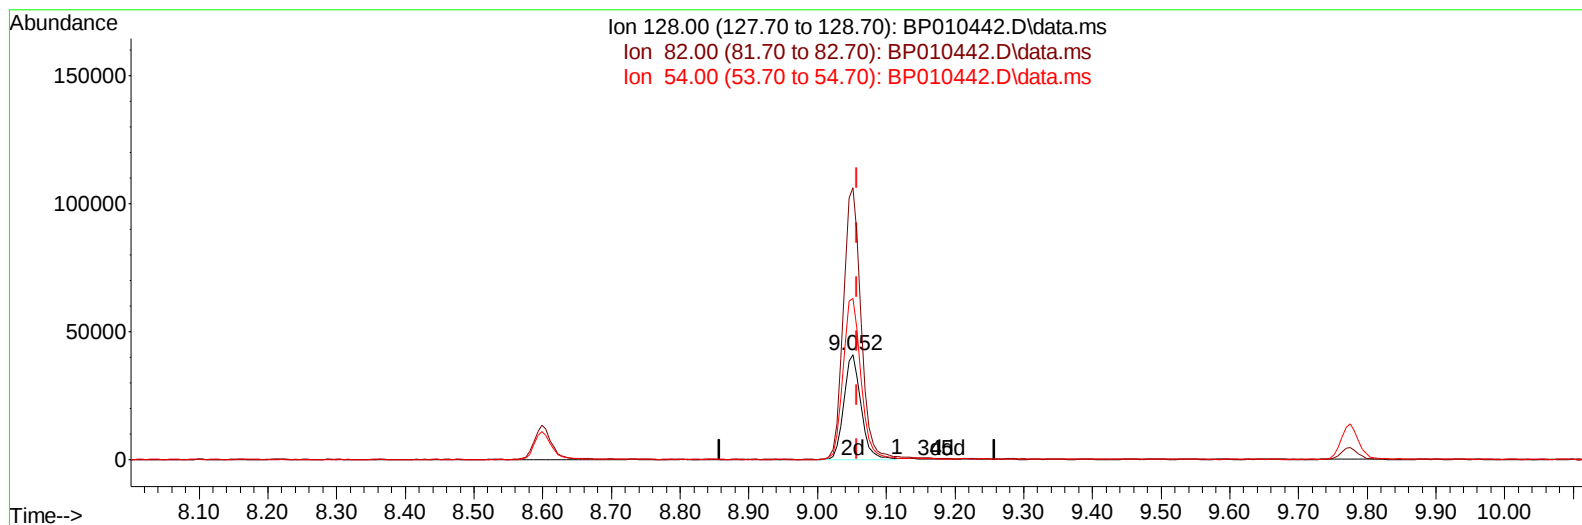

TIC: BP010442.D\data.ms

(21) Nitrobenzene-d5 (S)

9.052min (-0.006) 16.86 ng/ul m

response 71282

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	258.87
54.00	120.20	153.37#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	121924	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.693	136	546242	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	377363	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188	834388	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240	822482	20.000	ng/ul	# 0.00
88) Perylene-d12	23.780	264	839925	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	8480m	2.965	ng/uL	0.00
4) Pyridine-d5	3.775	84	45030m	5.544	ng/ul	0.01
7) Phenol-d5	7.058	99	159275	15.564	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	119655	17.403	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132	133545	17.054	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113	105167	12.093	ng/ul	-0.01
21) Nitrobenzene-d5	9.052	128	71282m	16.861	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	72279	16.133	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	138406	16.338	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	171280	13.598	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	502195	18.063	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	559957	17.461	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	44859	9.065	ng/ul	0.00
60) Fluorene-d10	15.516	176	461300	19.071	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	40703	8.341	ng/ul	0.00
73) Anthracene-d10	17.375	188	713301	18.879	ng/ul	0.00
81) Pyrene-d10	19.604	212	966720	22.132	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264	870072	20.630	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.716	105	14120	1.033	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010442.D
 Acq On : 20 May 2022 19:10
 Operator : CG/JU
 Sample : N2843-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 20 23:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

