




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010445.D
 Acq On : 20 May 2022 20:51
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

Manual IntegrationsAPPROVED

Quant Time: May 20 23:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

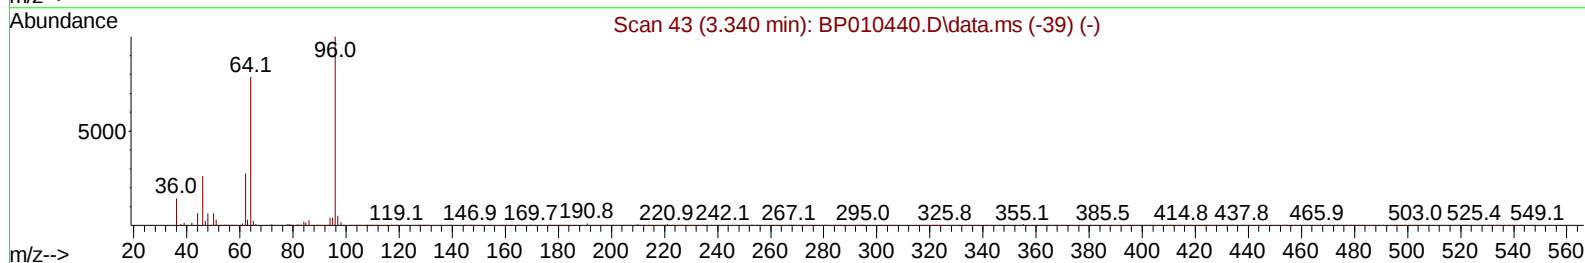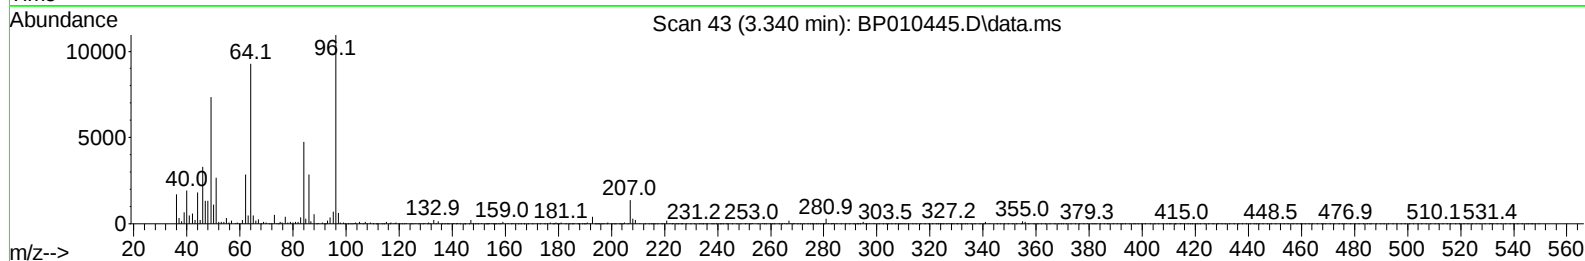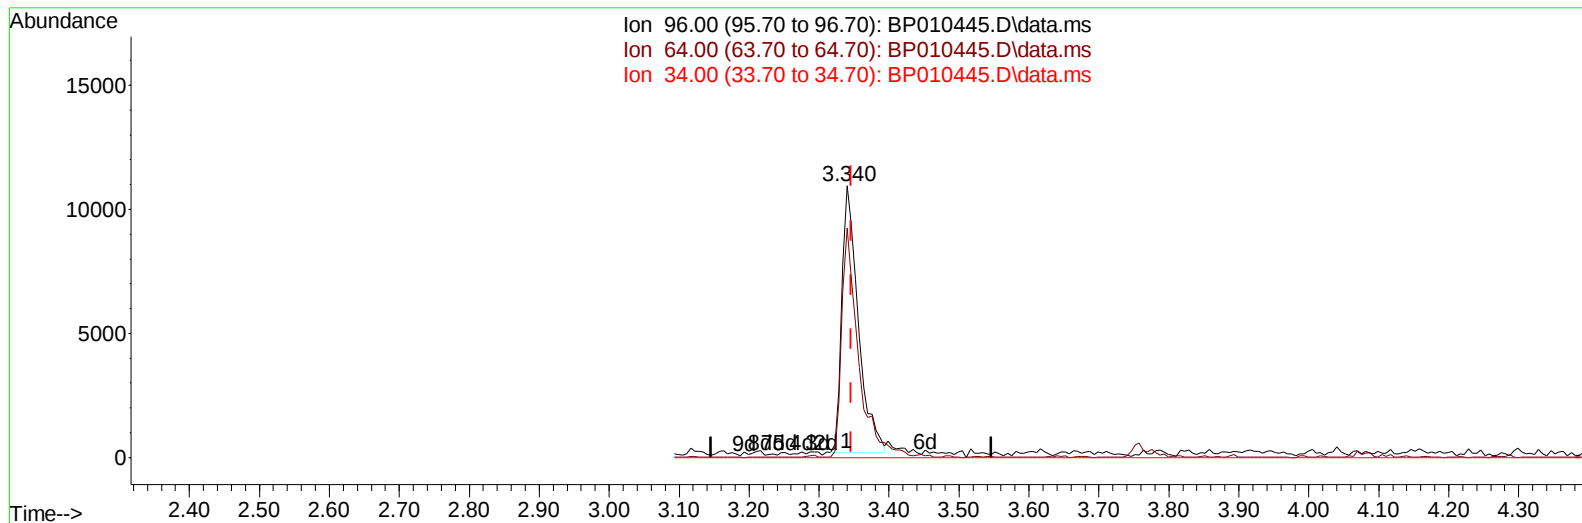

TIC: BP010445.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 5.46 ng/uL

response 17512

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	84.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010445.D
 Acq On : 20 May 2022 20:51
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

Manual IntegrationsAPPROVED

Quant Time: May 20 23:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

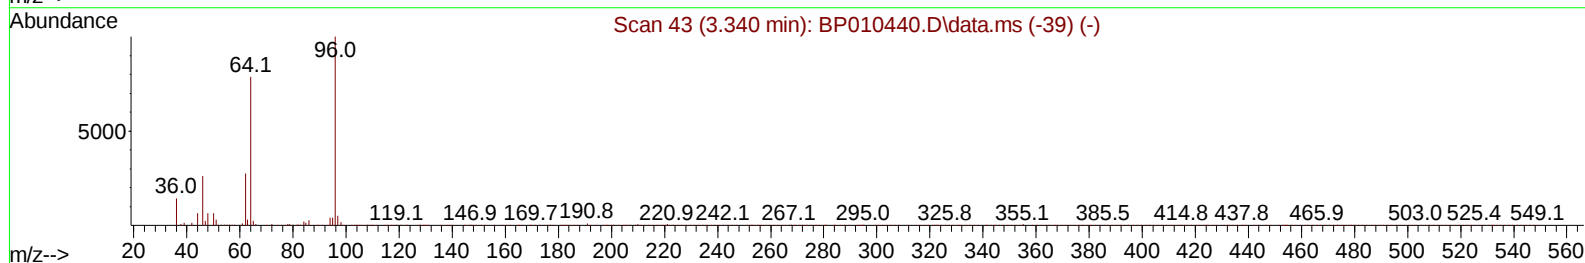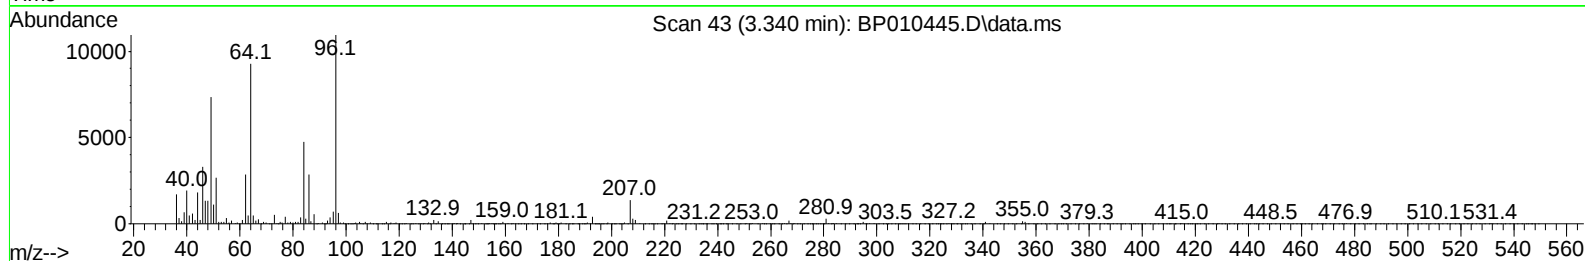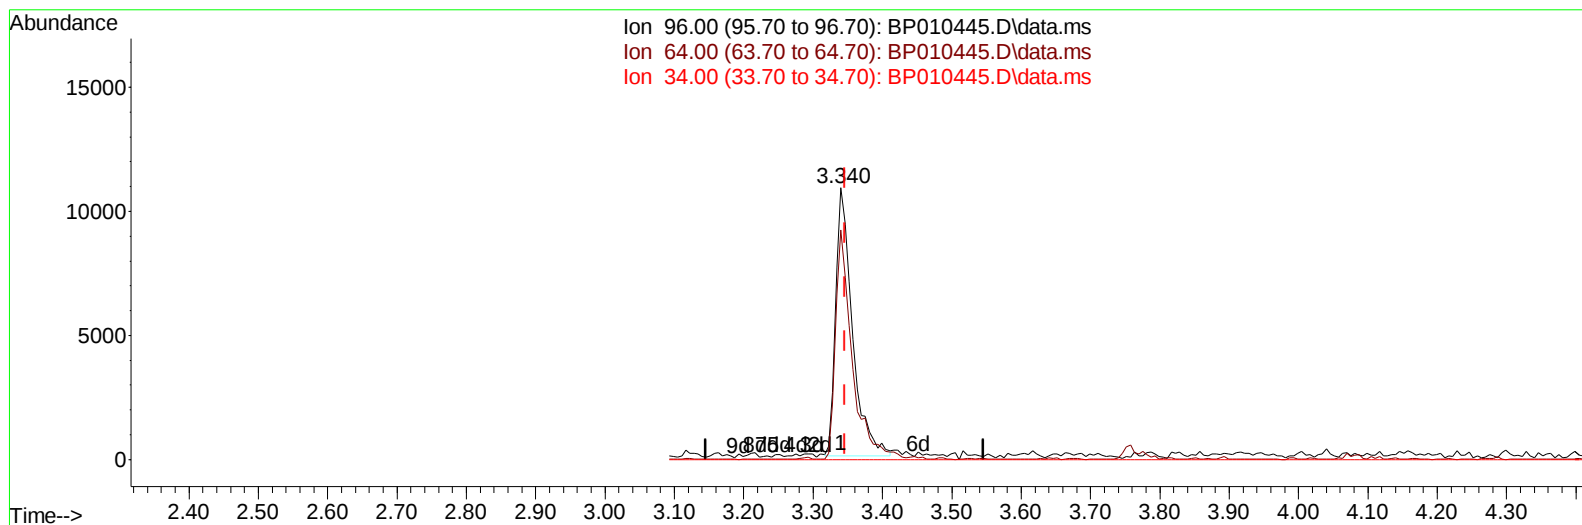

TIC: BP010445.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 5.62 ng/uL m

response 18025

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	84.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010445.D
 Acq On : 20 May 2022 20:51
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

Manual IntegrationsAPPROVED

Quant Time: May 20 23:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

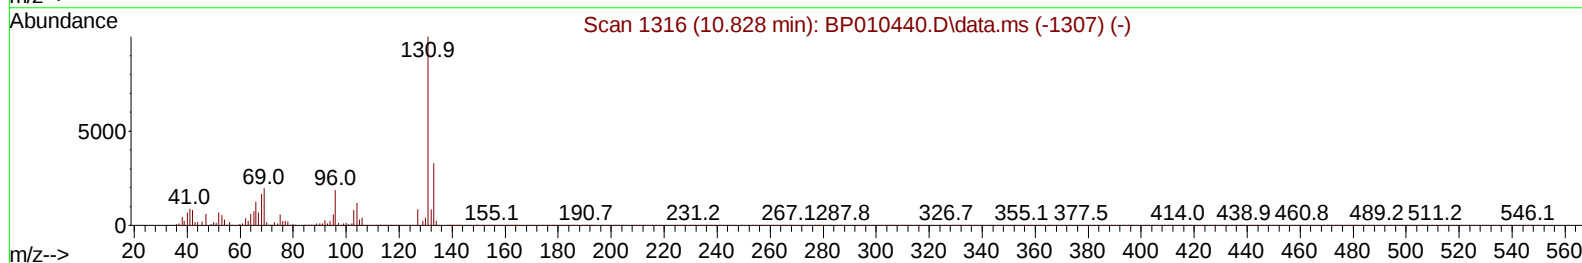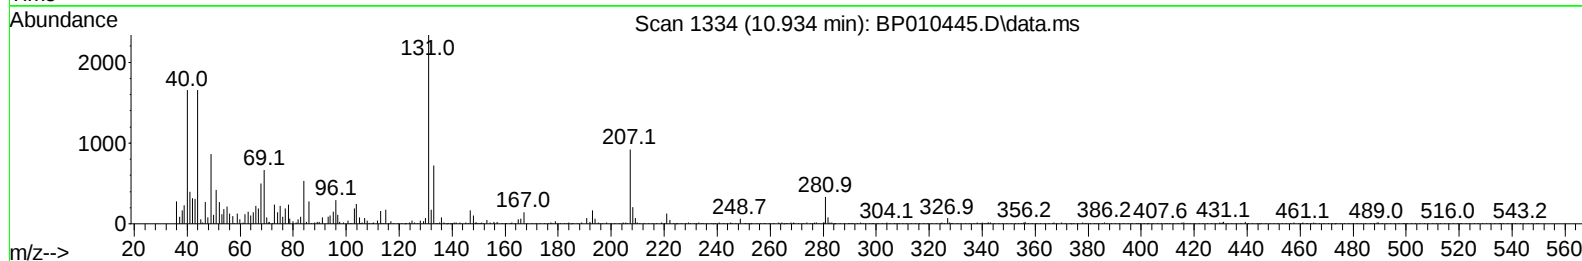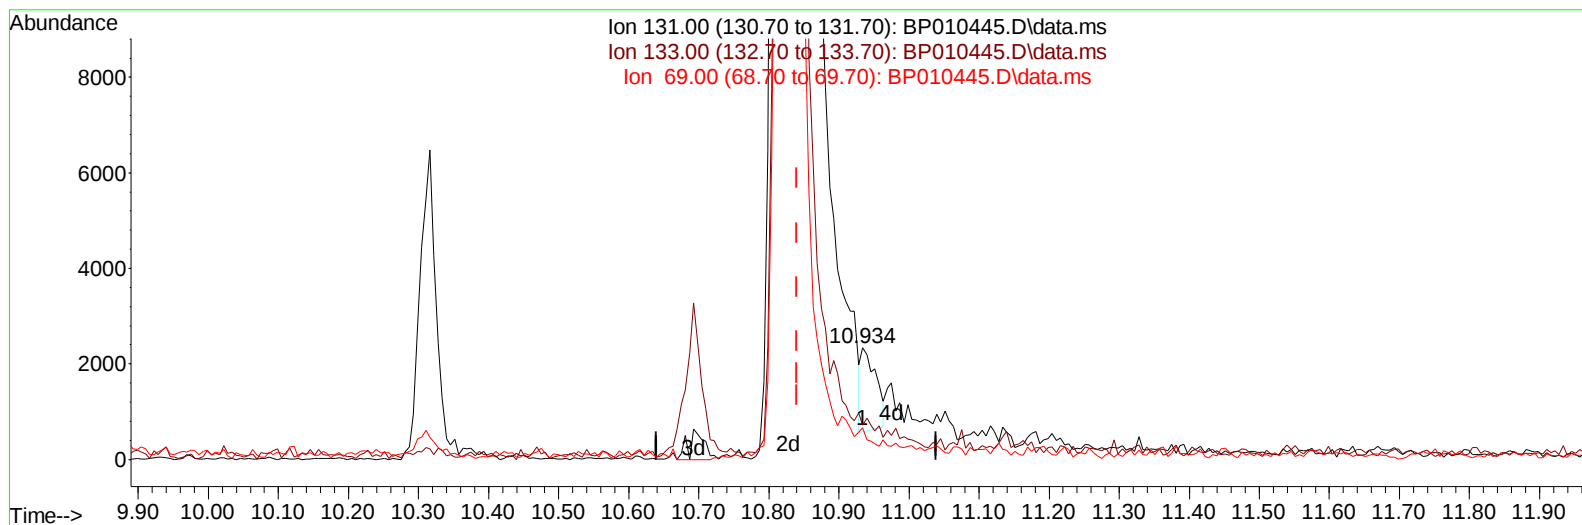

TIC: BP010445.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.934min (+ 0.094) 0.18 ng/ul

response 2592

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	30.98
69.00	26.10	28.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010445.D
Acq On : 20 May 2022 20:51
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4H9

Manual IntegrationsAPPROVED

Quant Time: May 20 23:04:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

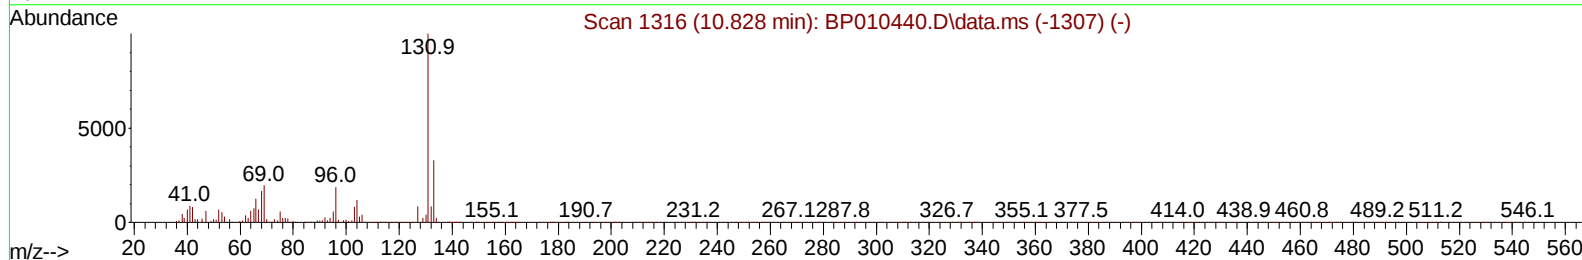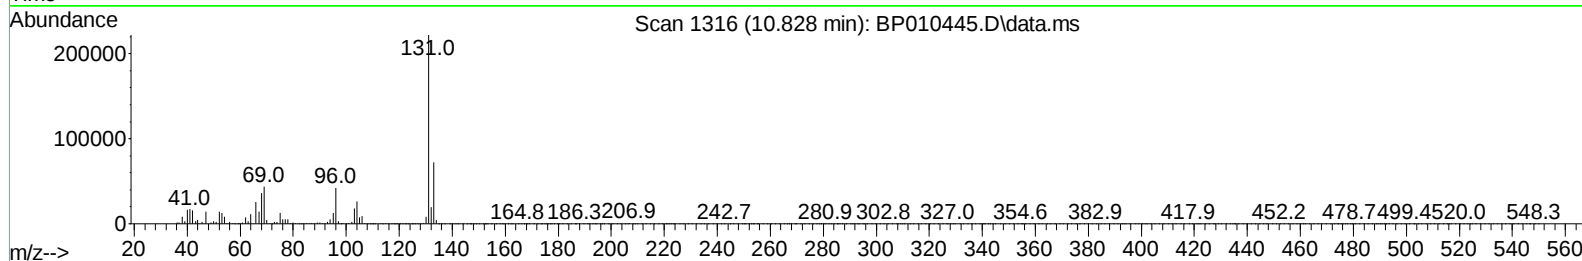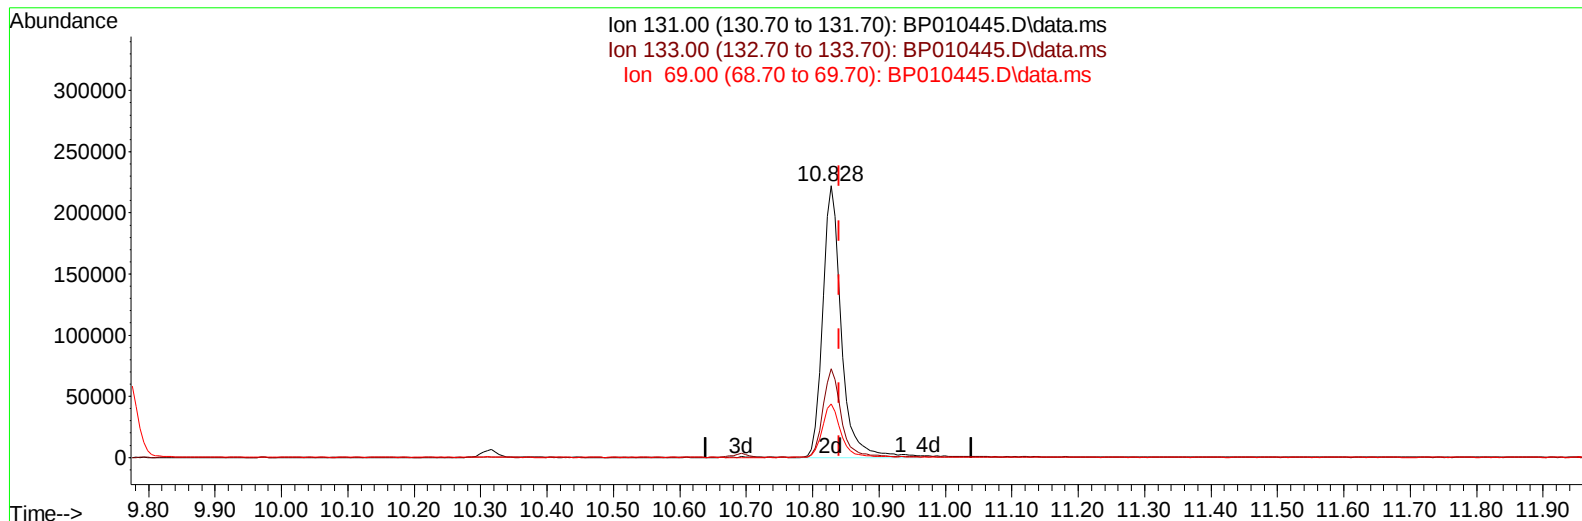

TIC: BP010445.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.828min (-0.012) 30.82 ng/ul m

response 435205

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	32.58
69.00	26.10	19.75#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010445.D
 Acq On : 20 May 2022 20:51
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 20 23:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.893	152		136618	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136		612292	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164		426431	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188		923549	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240		879197	20.000	ng/ul	# 0.00
88) Perylene-d12	23.780	264		815919	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.340	96		18025m	5.624	ng/uL	0.00
4) Pyridine-d5	3.758	84		268438	29.497	ng/ul	0.00
7) Phenol-d5	7.058	99		361877	31.559	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67		249132	32.338	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132		288845	32.920	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113		313894	32.211	ng/ul	-0.01
21) Nitrobenzene-d5	9.052	128		156194	32.961	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143		170728	33.996	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165		300671	31.664	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.828	131		435205m	30.824	ng/ul	-0.01
46) Dimethylphthalate-d6	13.934	166		1042654	33.186	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160		1205521	33.265	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143		137680	24.620	ng/ul	0.00
60) Fluorene-d10	15.516	176		903958	33.072	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200		121421	22.480	ng/ul	-0.01
73) Anthracene-d10	17.375	188		1391053	33.263	ng/ul	0.00
81) Pyrene-d10	19.604	212		1689374	36.182	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264		1408518	34.379	ng/ul	-0.01
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.269	149		666883	20.071	ng/ul#	Qvalue 81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010445.D
Acq On : 20 May 2022 20:51
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4H9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 20 23:04:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

