




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010449.D
 Acq On : 20 May 2022 23:07
 Operator : CG/JU
 Sample : N2843-22
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K2

Manual IntegrationsAPPROVED

Quant Time: May 21 01:20:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

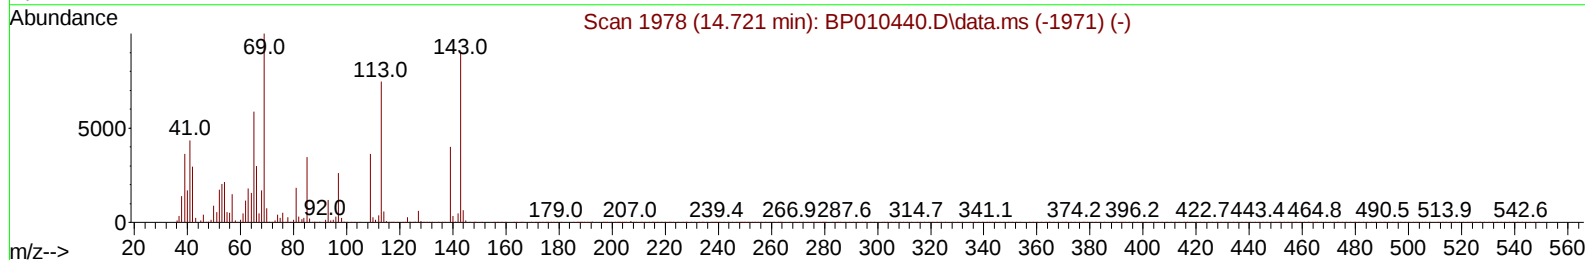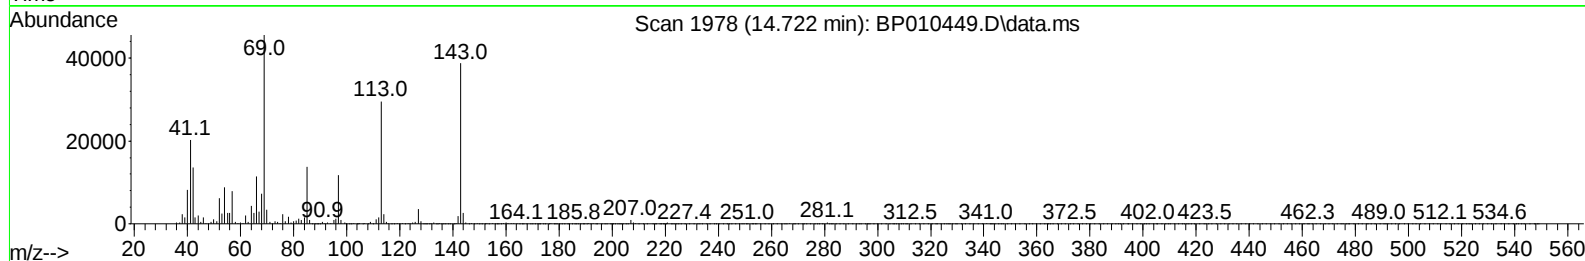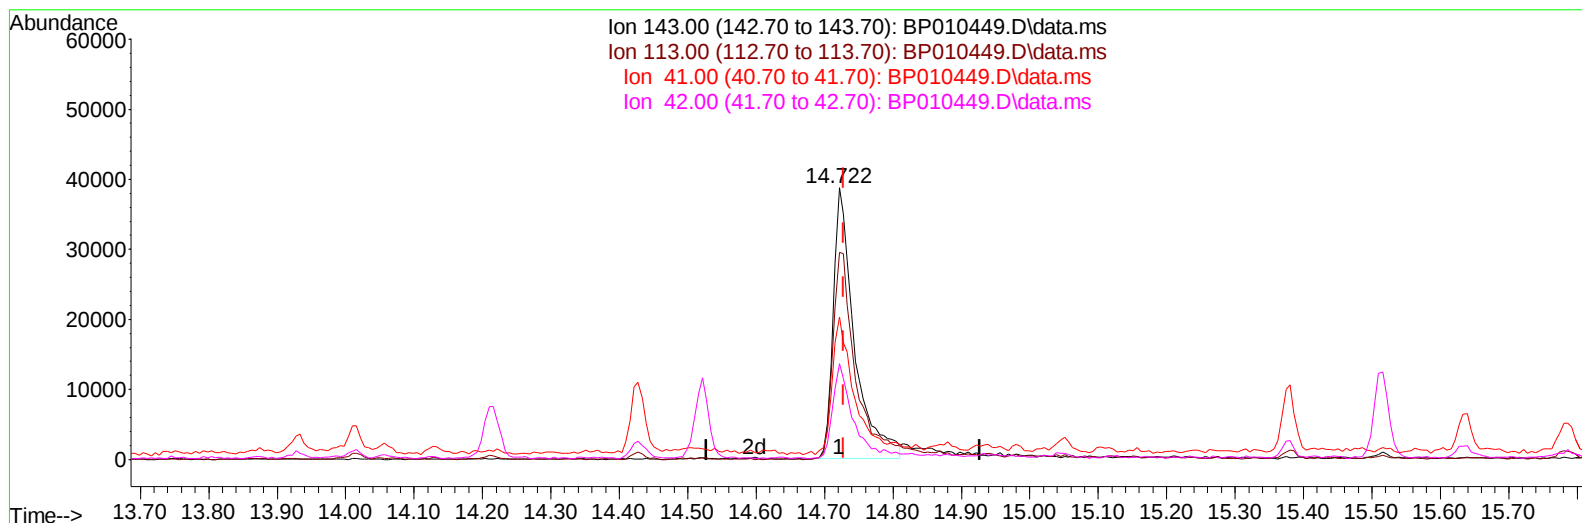

TIC: BP010449.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (-0.006) 14.93 ng/u1

response 83308

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.21#
41.00	23.20	52.36#
42.00	18.00	35.20#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010449.D
Acq On : 20 May 2022 23:07
Operator : CG/JU
Sample : N2843-22
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4K2

Manual IntegrationsAPPROVED

Quant Time: May 21 01:20:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

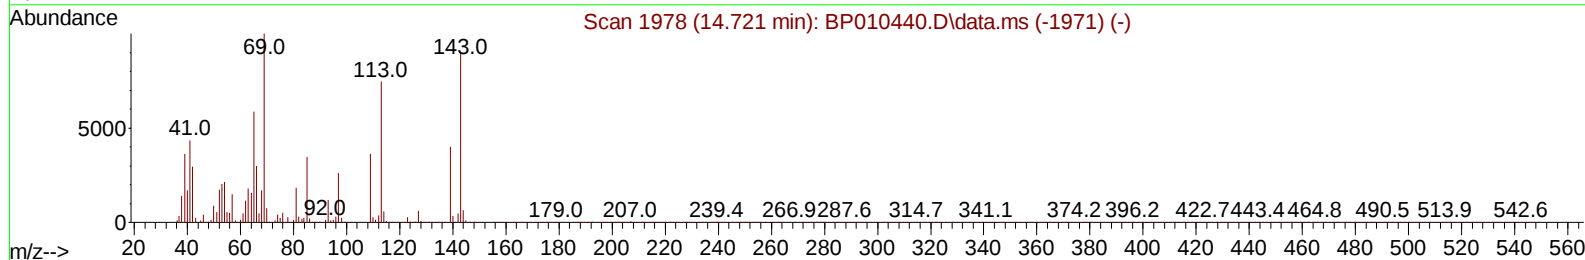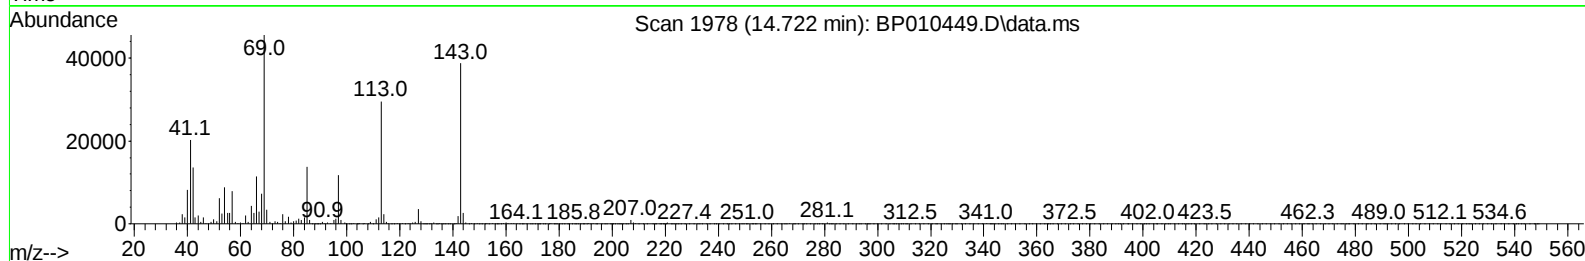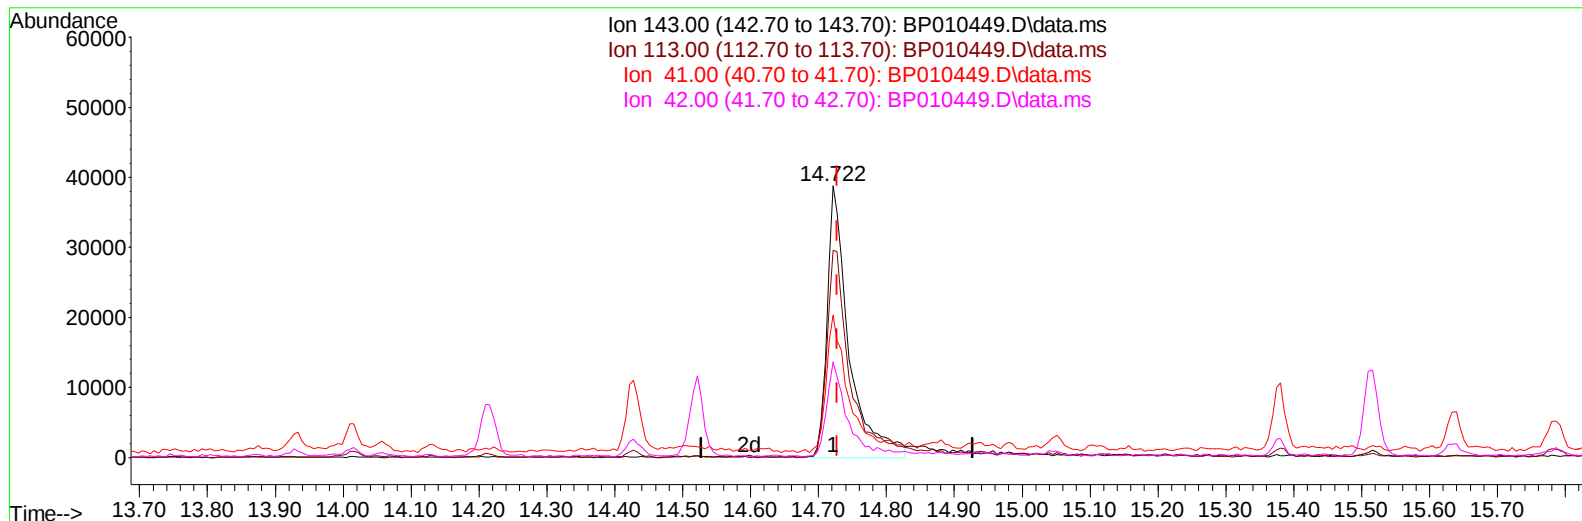

TIC: BP010449.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (-0.006) 15.45 ng/ul m

response 86200

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.21#
41.00	23.20	52.36#
42.00	18.00	35.20#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010449.D
 Acq On : 20 May 2022 23:07
 Operator : CG/JU
 Sample : N2843-22
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4K2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 01:20:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	139540	20.000	ng/ul	0.00
20) Naphthalene-d8	10.692	136	623846	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	425484	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.274	188	916300	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240	886481	20.000	ng/ul	0.00
88) Perylene-d12	23.774	264	812763	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	13017	3.976	ng/uL	0.00
4) Pyridine-d5	3.769	84	70504	7.585	ng/ul	0.00
7) Phenol-d5	7.057	99	250303	21.372	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	174666	22.197	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	204700	22.841	ng/ul	-0.01
15) 4-Methylphenol-d8	8.598	113	208219	20.920	ng/ul	-0.01
21) Nitrobenzene-d5	9.051	128	109841	22.750	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	113210	22.126	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	202625	20.943	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	274510	19.083	ng/ul	-0.01
46) Dimethylphthalate-d6	13.933	166	709742	22.641	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	828352	22.908	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	86200m	15.449	ng/ul	0.00
60) Fluorene-d10	15.516	176	624570	22.901	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	78445	14.638	ng/ul	0.00
73) Anthracene-d10	17.374	188	993574	23.946	ng/ul	0.00
81) Pyrene-d10	19.604	212	1258799	26.738	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264	1056819	25.895	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010449.D
Acq On : 20 May 2022 23:07
Operator : CG/JU
Sample : N2843-22
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4K2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 01:20:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

