




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010451.D
Acq On : 21 May 2022 00:14
Operator : CG/JU
Sample : N2843-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

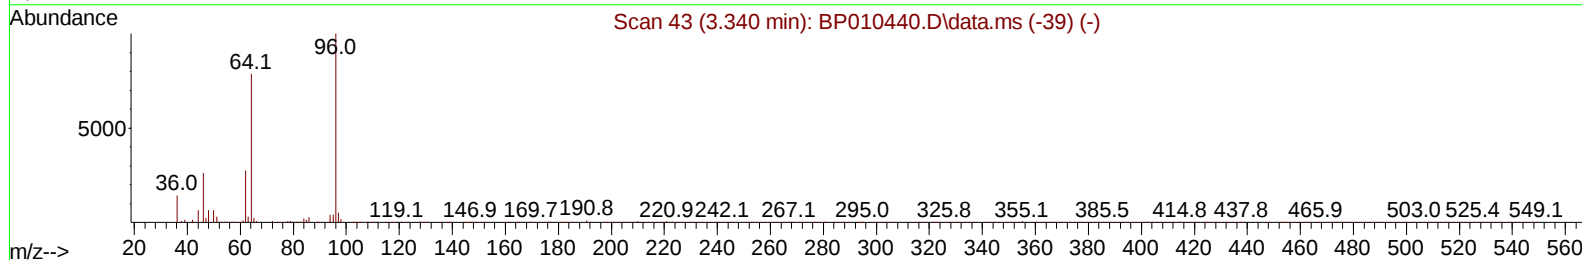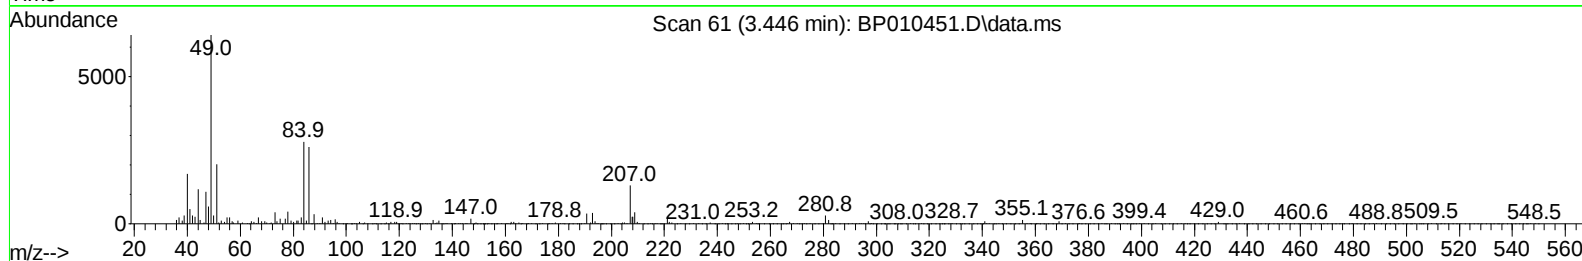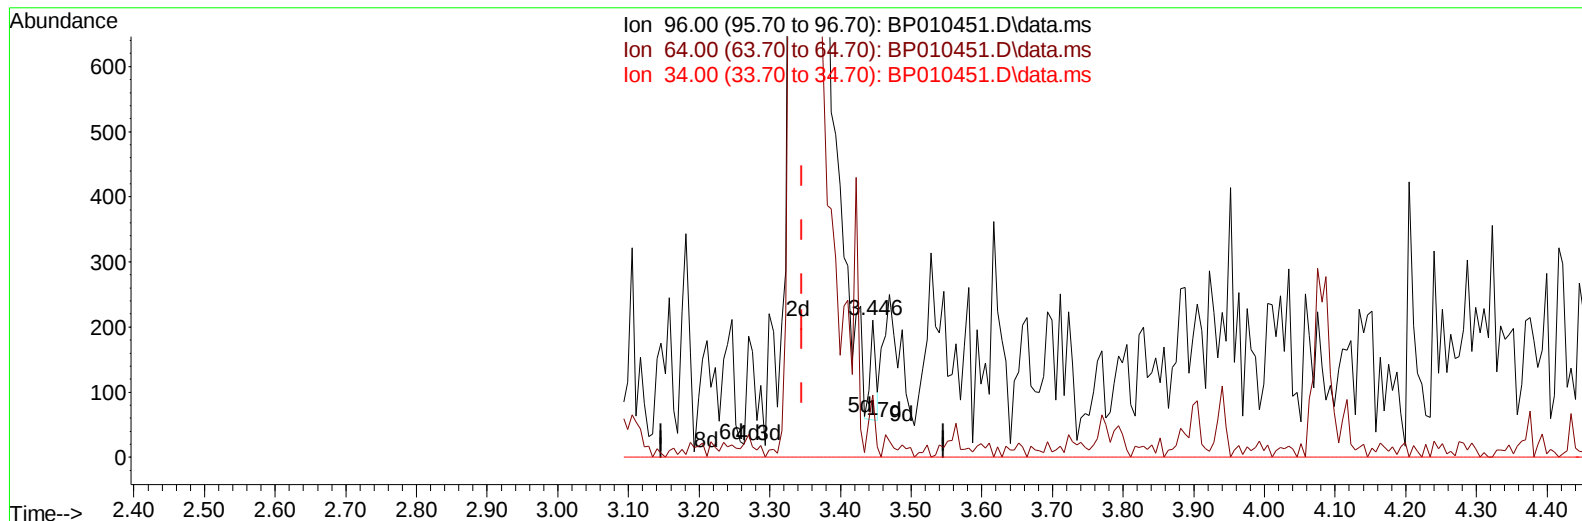

TIC: BP010451.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.446min (+ 0.100) 0.03 ng/uL

response	85	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	45.50
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010451.D
 Acq On : 21 May 2022 00:14
 Operator : CG/JU
 Sample : N2843-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

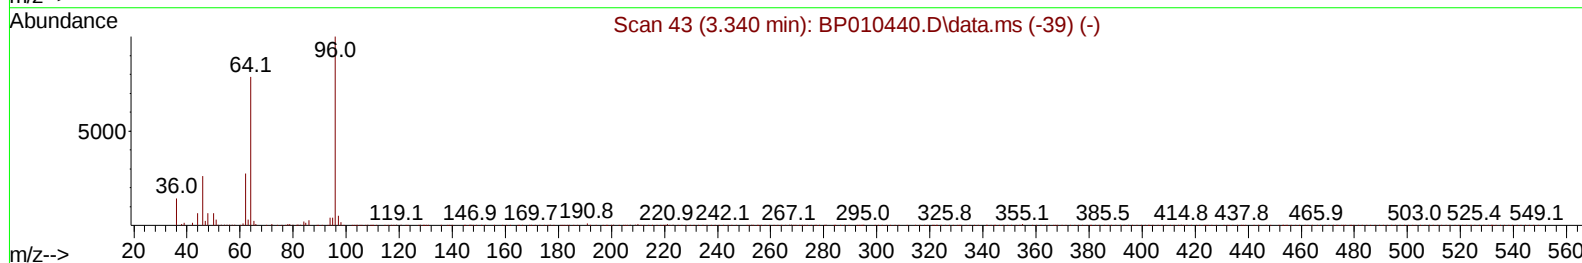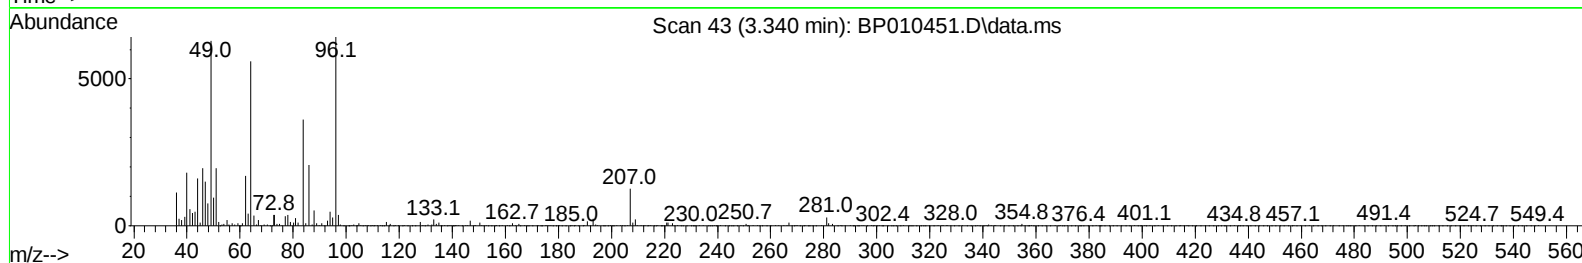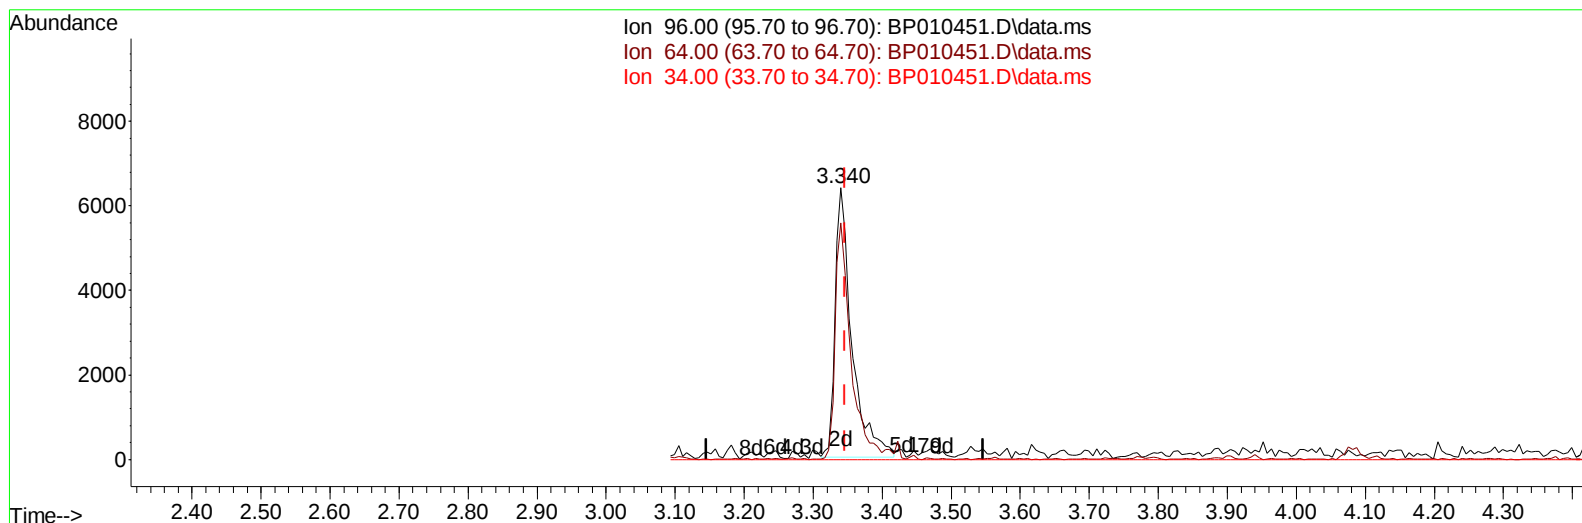

TIC: BP010451.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 3.66 ng/uL m

response 10752

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	87.22#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010451.D
Acq On : 21 May 2022 00:14
Operator : CG/JU
Sample : N2843-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

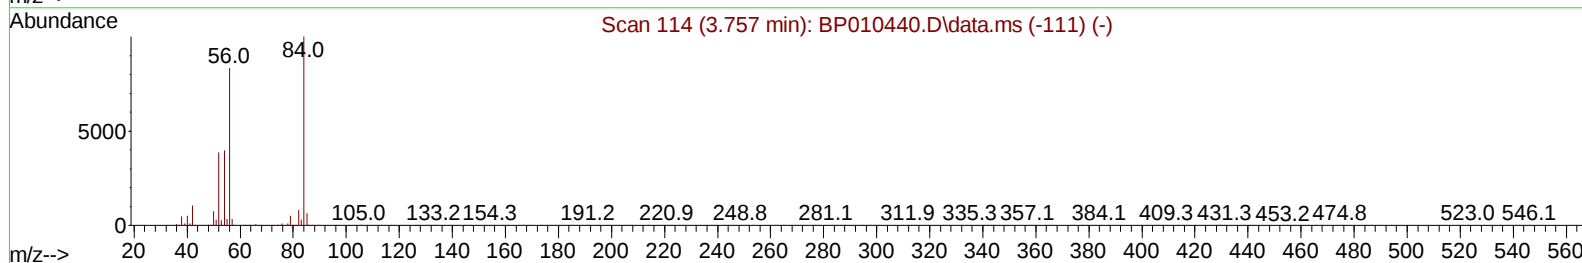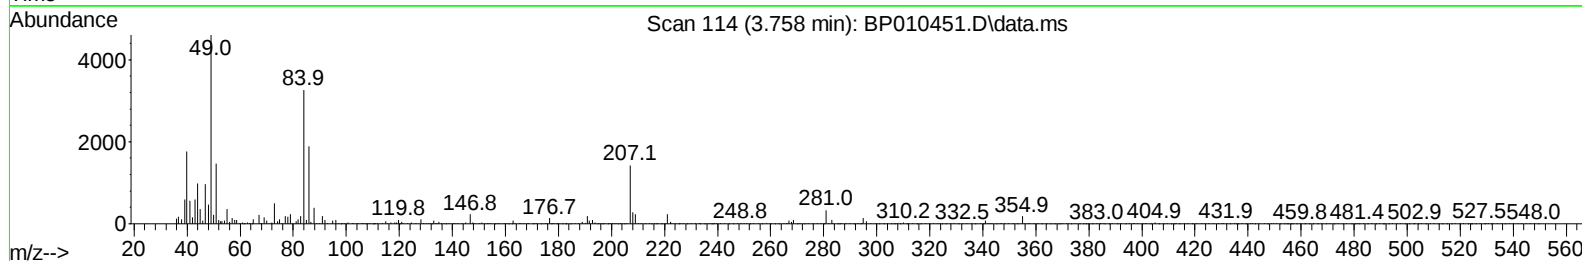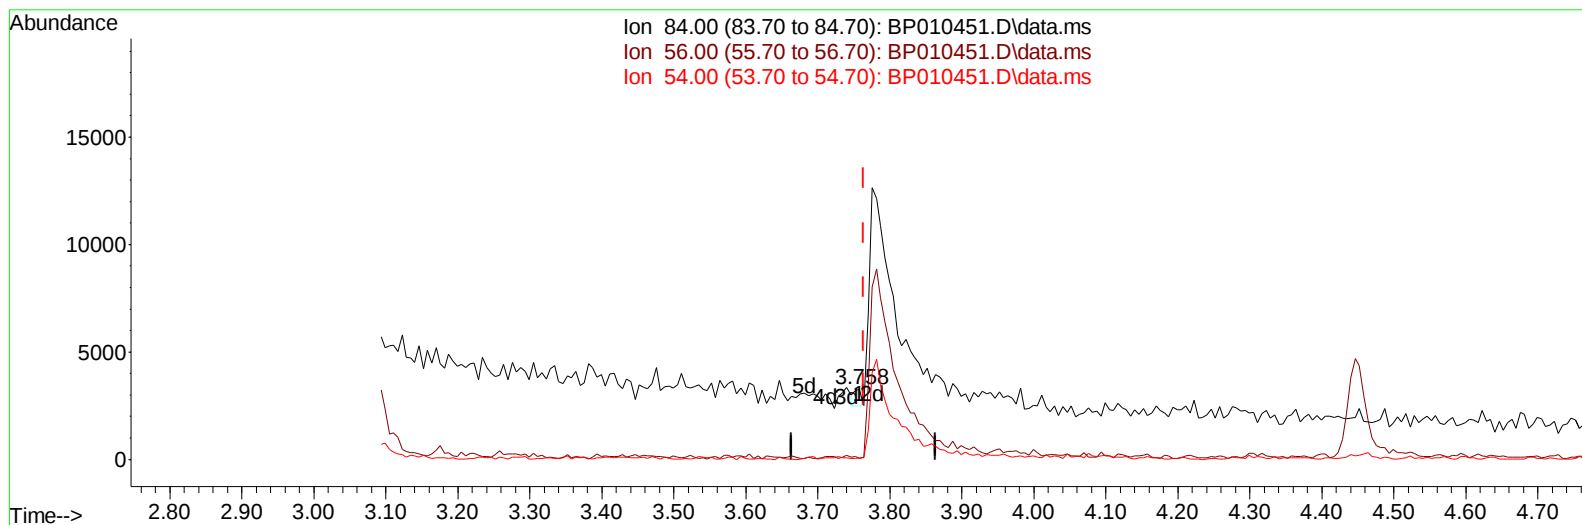

TIC: BP010451.D\data.ms

(4) Pyridine-d5 (S)

3.758min (-0.006) 0.06 ng/u1

response 522

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	1.53#
54.00	24.80	2.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010451.D
 Acq On : 21 May 2022 00:14
 Operator : CG/JU
 Sample : N2843-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

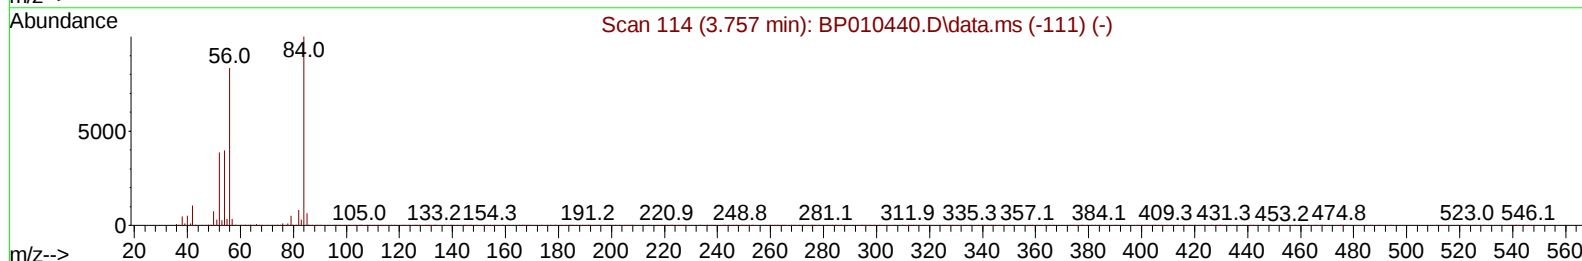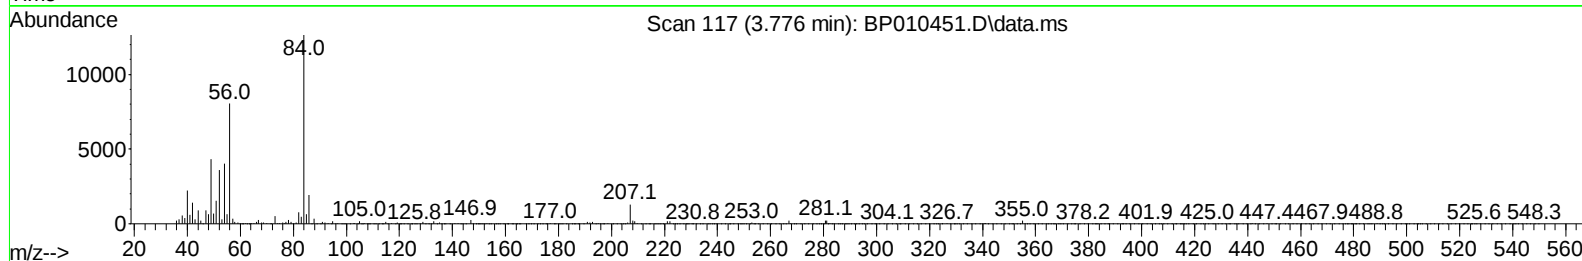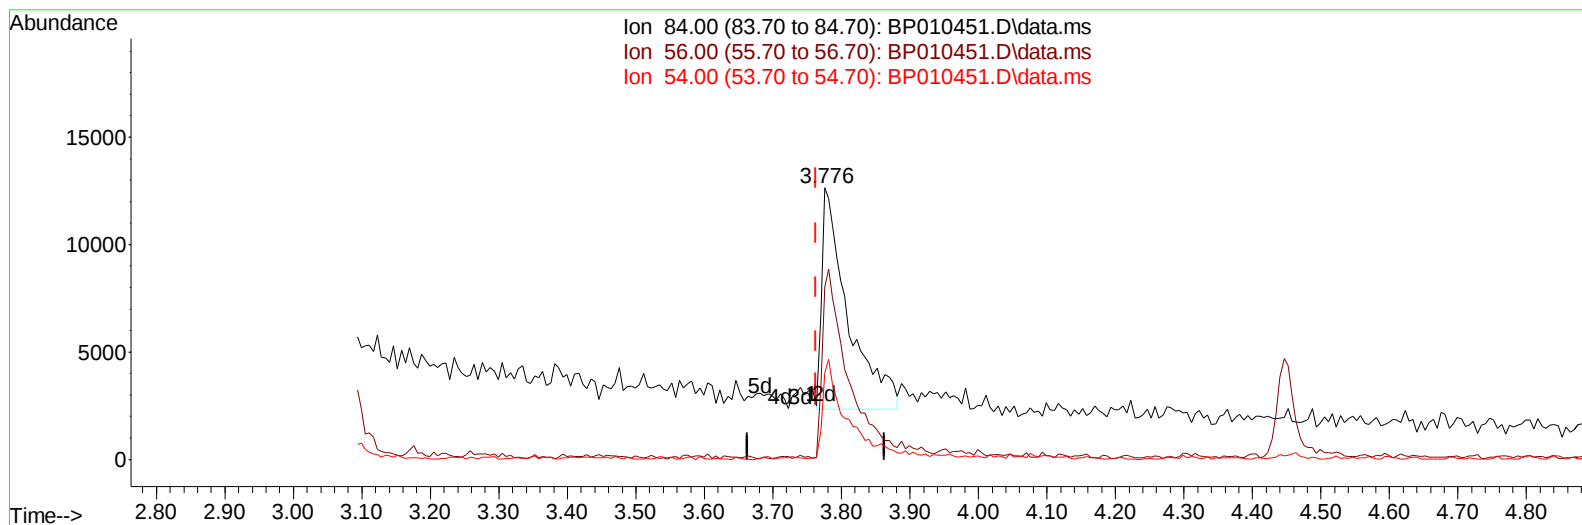

TIC: BP010451.D\data.ms

(4) Pyridine-d5 (S)

3.776min (+ 0.012) 3.31 ng/ul m

response 27589

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	63.62#
54.00	24.80	31.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010451.D
 Acq On : 21 May 2022 00:14
 Operator : CG/JU
 Sample : N2843-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

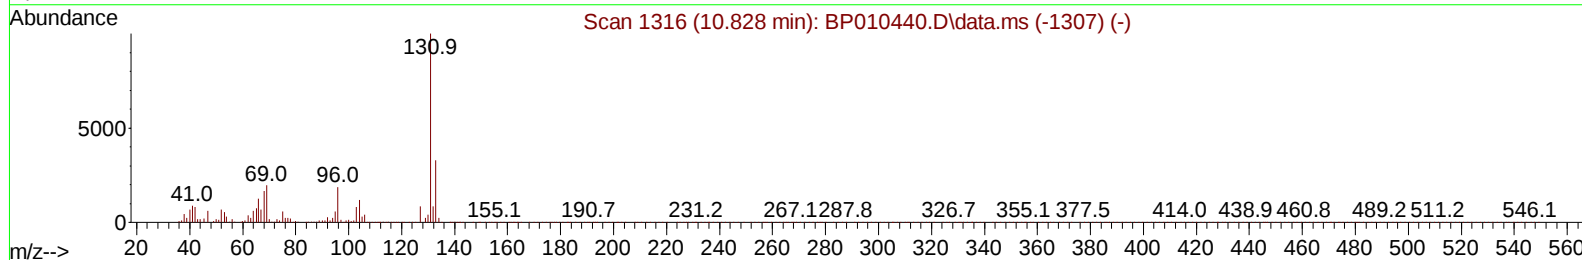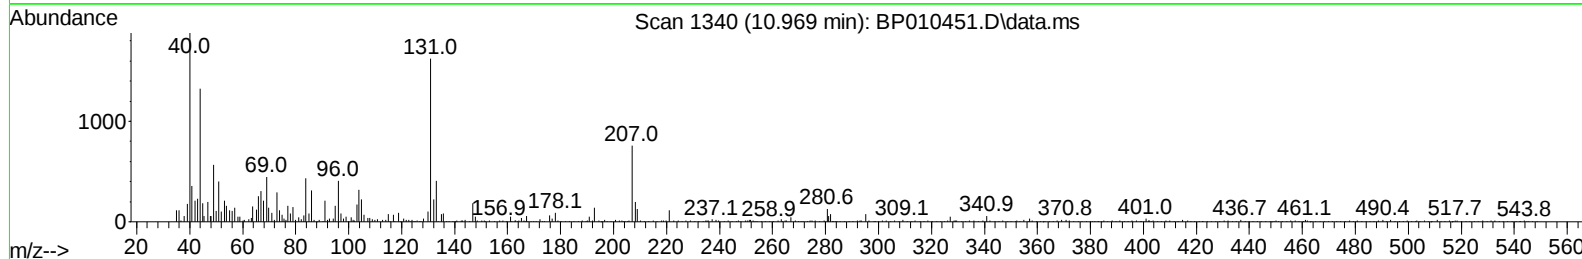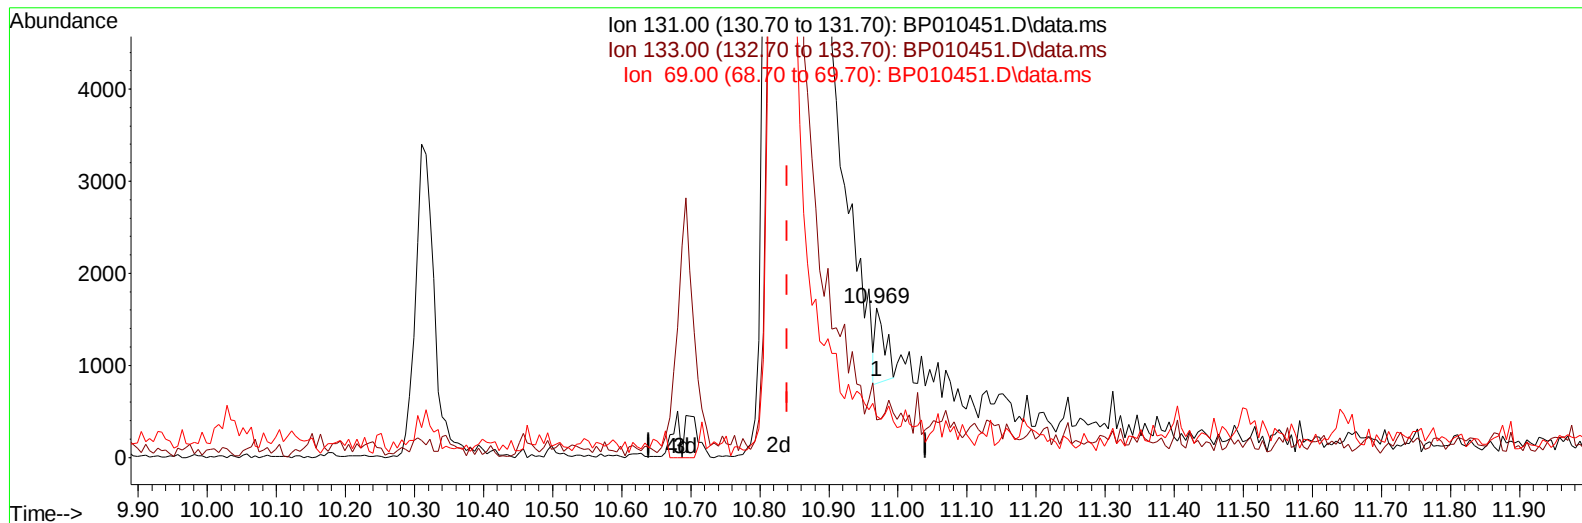

TIC: BP010451.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.130) 0.06 ng/u1

response 792

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	24.98
69.00	26.10	27.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010451.D
 Acq On : 21 May 2022 00:14
 Operator : CG/JU
 Sample : N2843-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J0

Manual IntegrationsAPPROVED

Quant Time: May 21 01:21:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

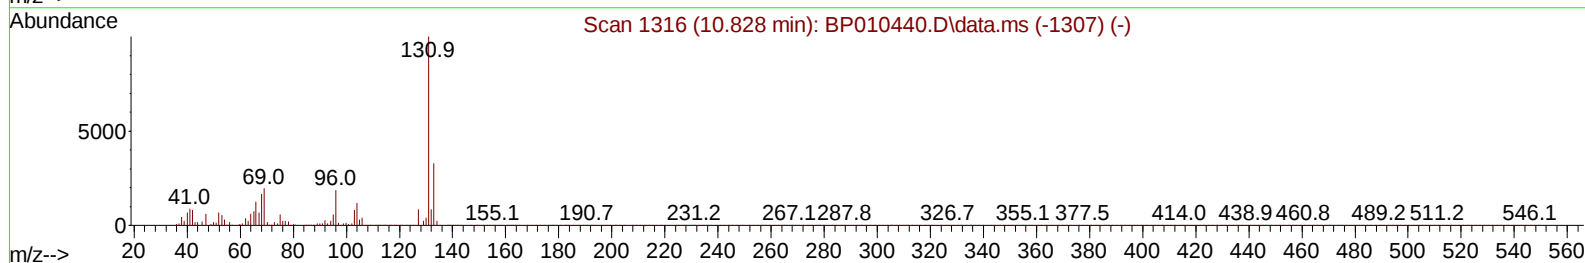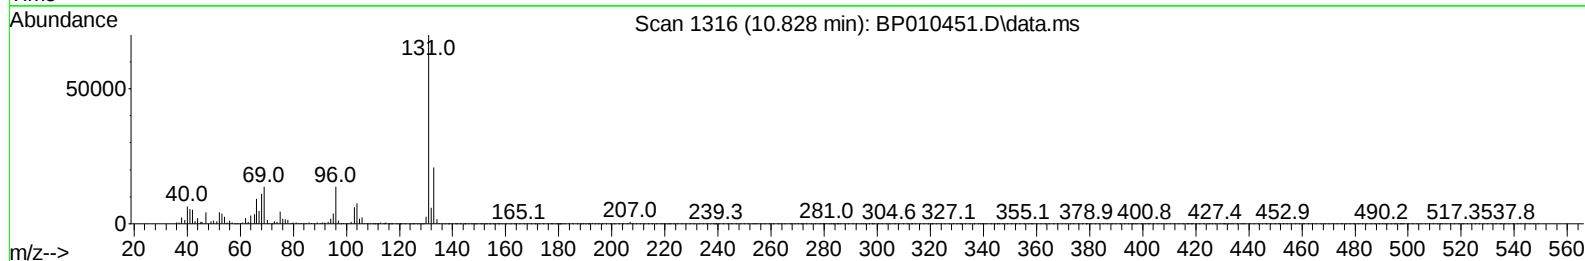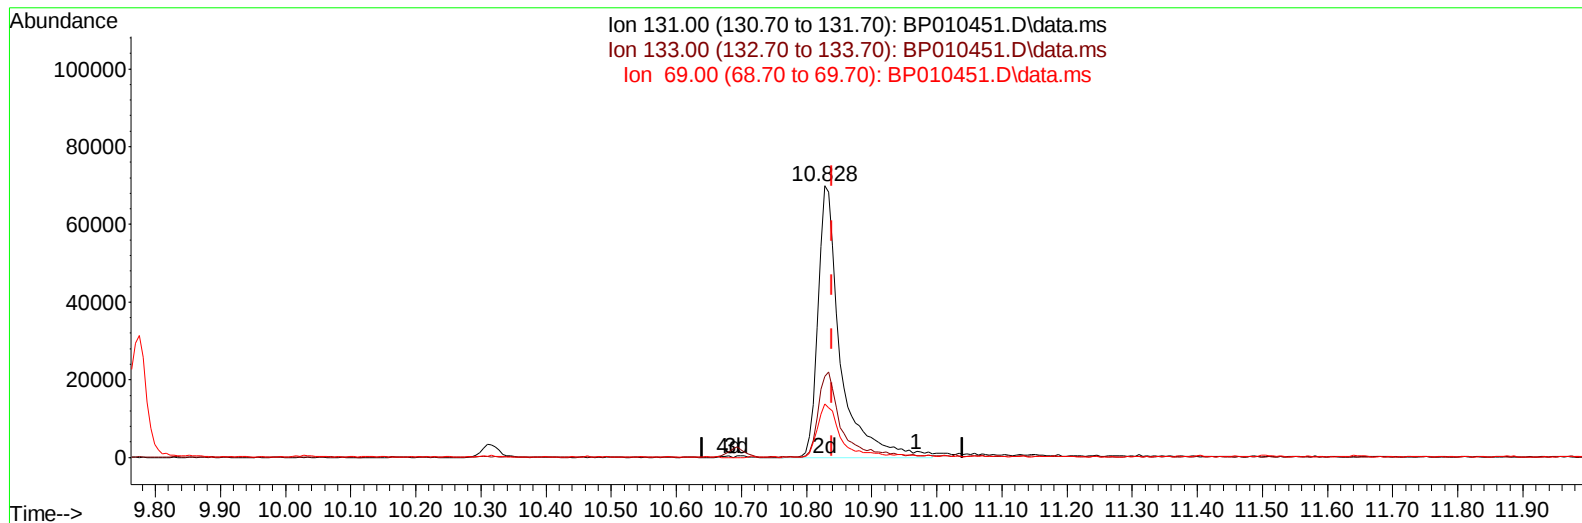

TIC: BP010451.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.828min (-0.011) 13.07 ng/ul m

response 166842

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	29.74
69.00	26.10	19.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010451.D
 Acq On : 21 May 2022 00:14
 Operator : CG/JU
 Sample : N2843-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 01:21:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	125121	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136	553670	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	381988	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188	840334	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240	824152	20.000	ng/ul	# 0.00
88) Perylene-d12	23.774	264	756924	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	10752m	3.663	ng/uL	0.00
4) Pyridine-d5	3.776	84	27589m	3.310	ng/ul	0.01
7) Phenol-d5	7.058	99	213089	20.291	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	147081	20.846	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132	169773	21.127	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113	178062	19.951	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	90803	21.191	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.775	143	93548	20.600	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	173223	20.174	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	166842m	13.068	ng/ul	-0.01
46) Dimethylphthalate-d6	13.934	166	617395	21.937	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	695759	21.432	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	76979	15.367	ng/ul	0.00
60) Fluorene-d10	15.516	176	548144	22.387	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	61078	12.428	ng/ul	-0.01
73) Anthracene-d10	17.369	188	844223	22.186	ng/ul	-0.01
81) Pyrene-d10	19.604	212	1091502	24.938	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.622	264	890198	23.421	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010451.D
Acq On : 21 May 2022 00:14
Operator : CG/JU
Sample : N2843-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 01:21:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

