




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010456.D
 Acq On : 21 May 2022 03:03
 Operator : CG/JU
 Sample : N2843-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J6

Manual IntegrationsAPPROVED

Quant Time: May 21 04:33:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

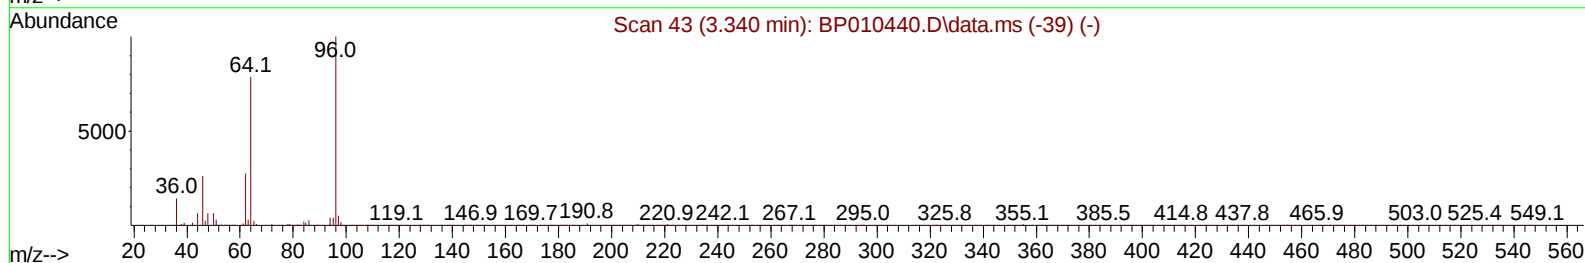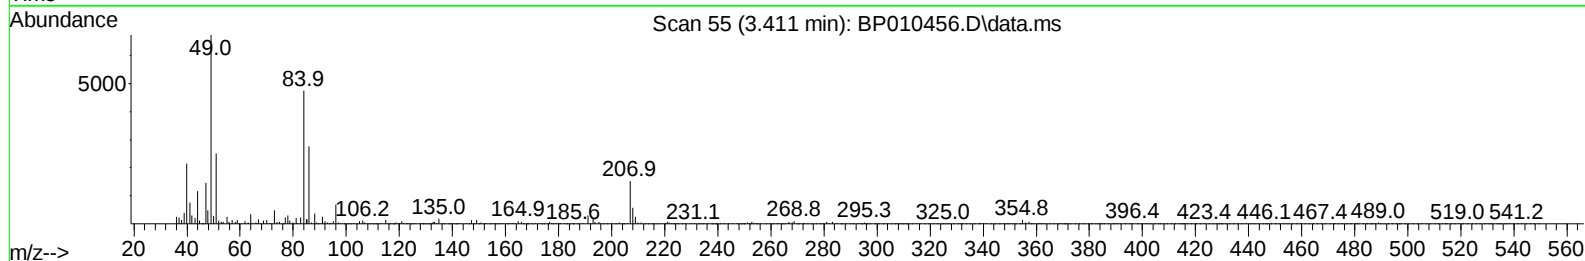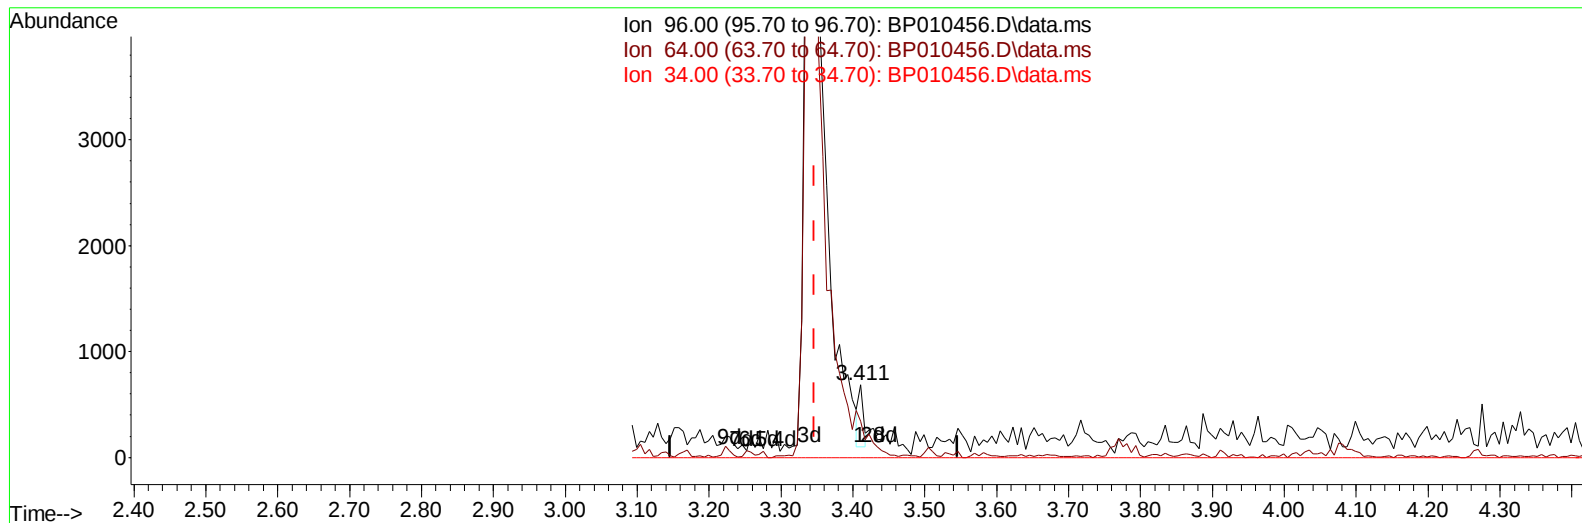

TIC: BP010456.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.411min (+ 0.065) 0.07 ng/uL

response 252

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	49.93
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010456.D
Acq On : 21 May 2022 03:03
Operator : CG/JU
Sample : N2843-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J6

Manual IntegrationsAPPROVED

Quant Time: May 21 04:33:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

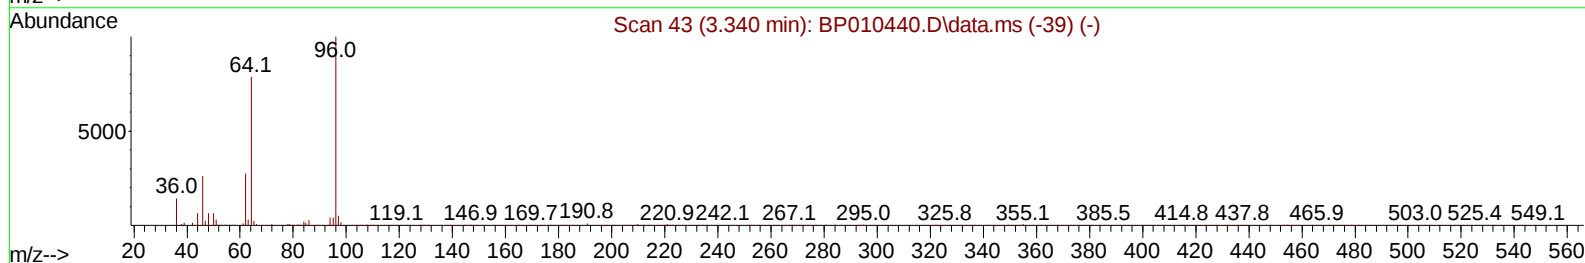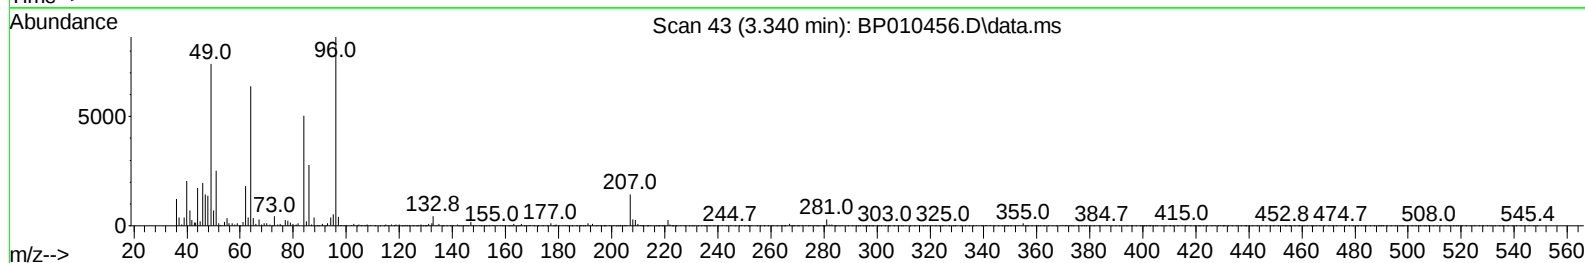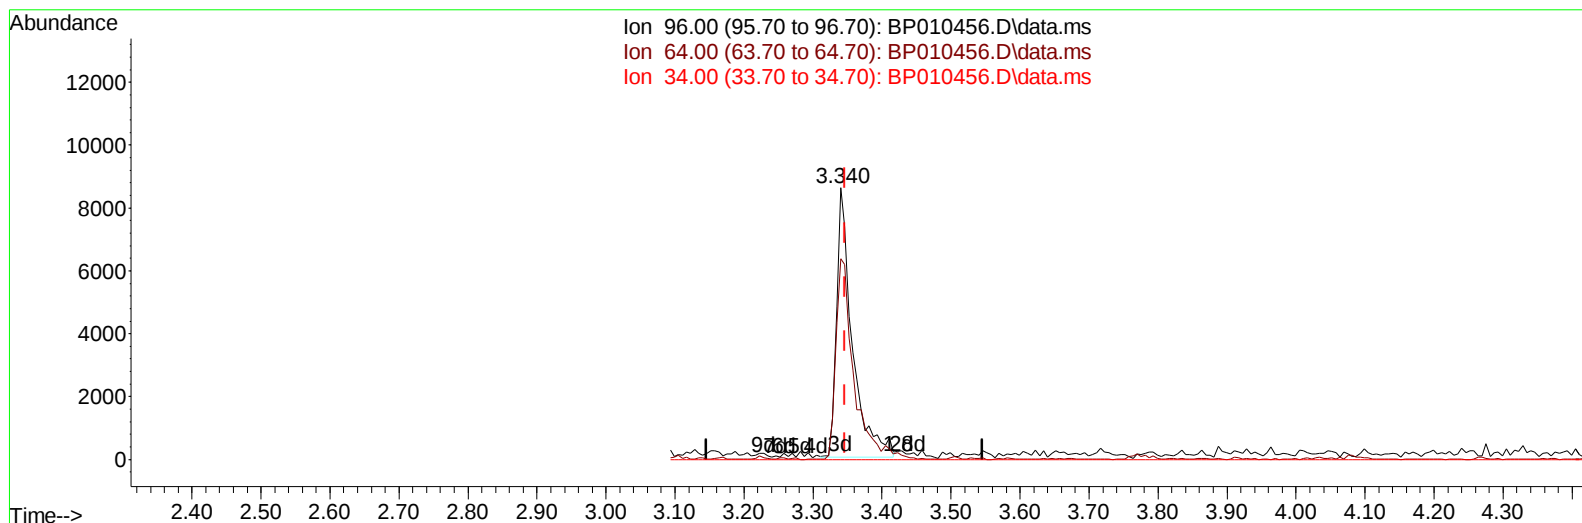

TIC: BP010456.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 3.98 ng/uL m

response 13589

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	73.85#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010456.D
 Acq On : 21 May 2022 03:03
 Operator : CG/JU
 Sample : N2843-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J6

Manual IntegrationsAPPROVED

Quant Time: May 21 04:33:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

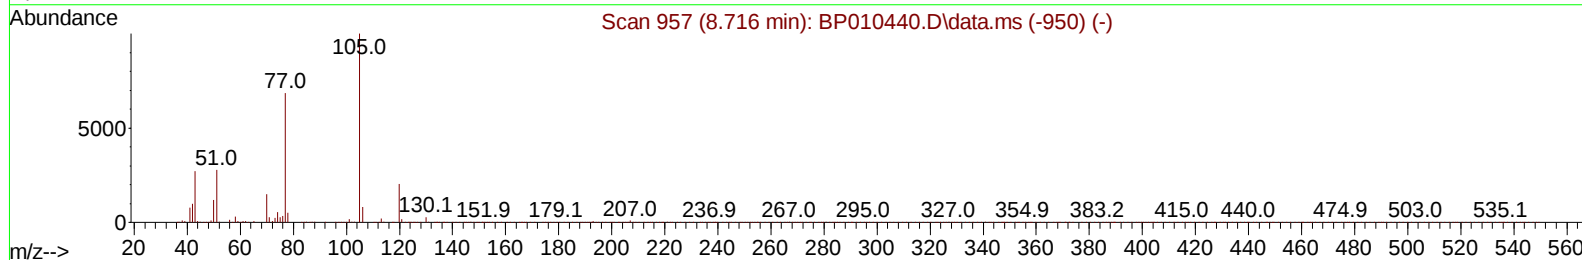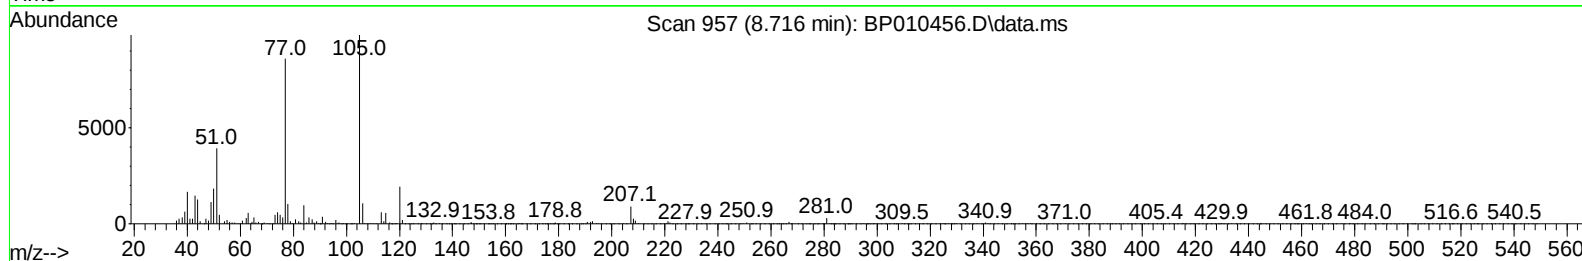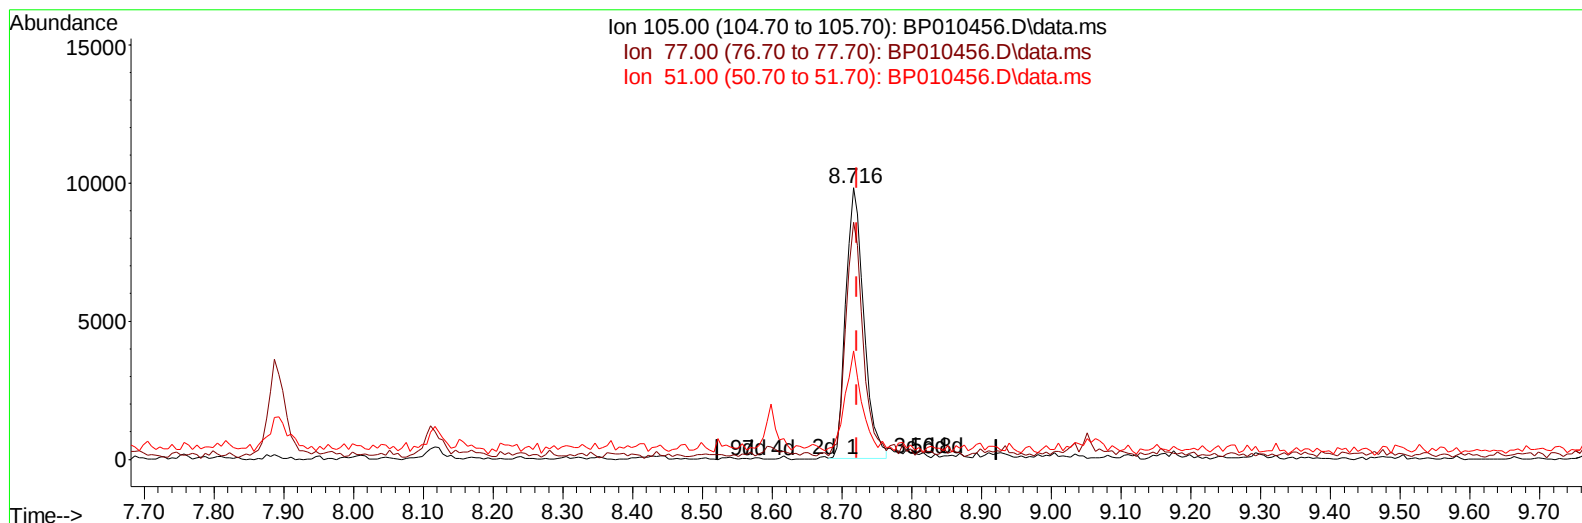

TIC: BP010456.D\data.ms

(16) Acetophenone

8.716min (-0.006) 1.08 ng/u1

response 17667

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	66.80	87.43#
51.00	17.30	39.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010456.D
Acq On : 21 May 2022 03:03
Operator : CG/JU
Sample : N2843-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 04:33:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

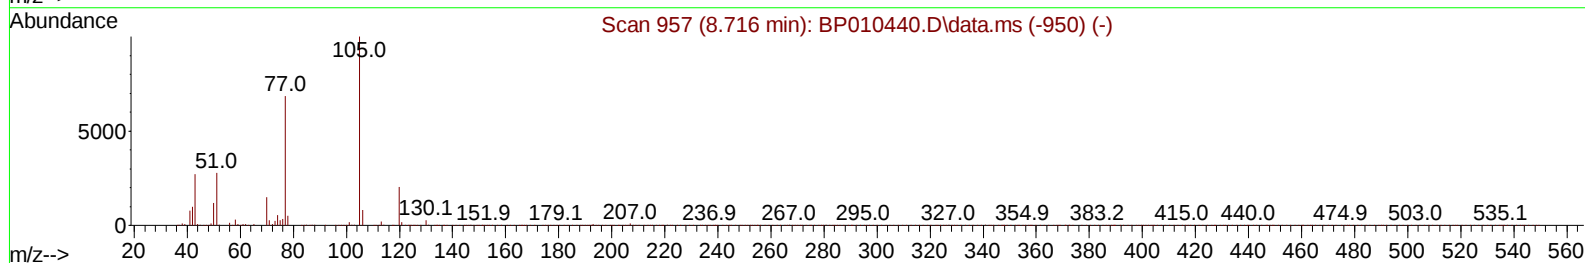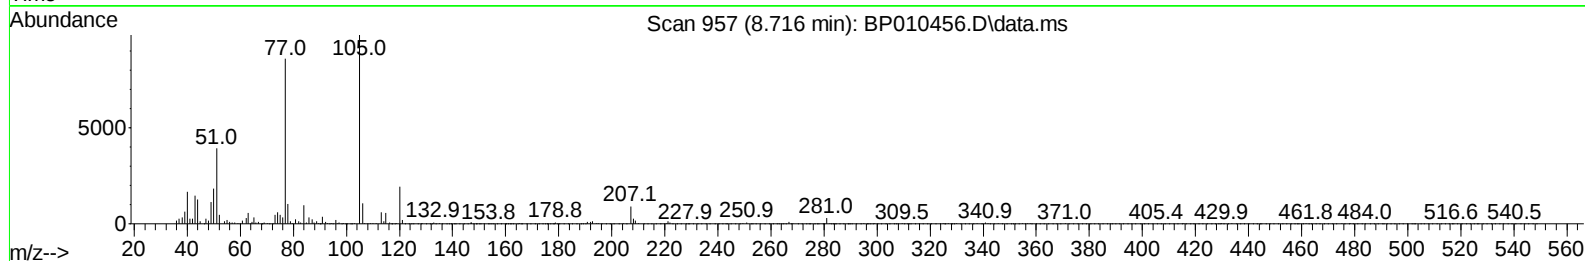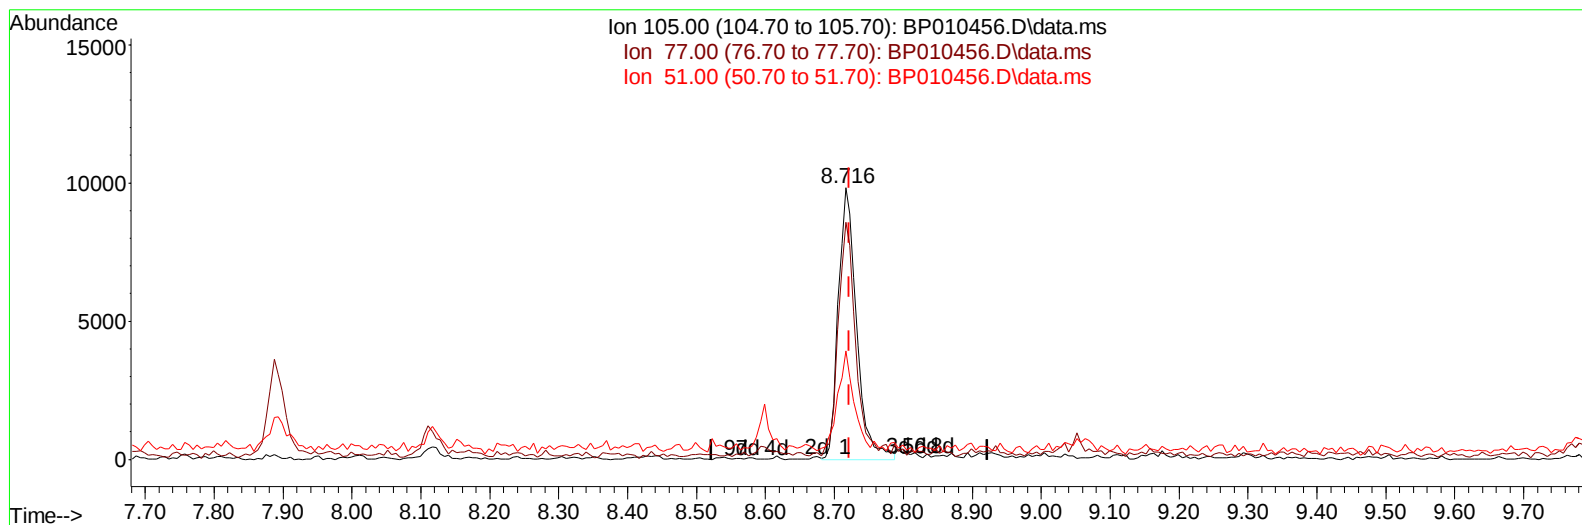

TIC: BP010456.D\data.ms

(16) Acetophenone

8.716min (-0.006) 1.12 ng/ul m

response 18242

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	66.80	87.43#
51.00	17.30	39.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010456.D
Acq On : 21 May 2022 03:03
Operator : CG/JU
Sample : N2843-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J6

Manual IntegrationsAPPROVED

Quant Time: May 21 04:33:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

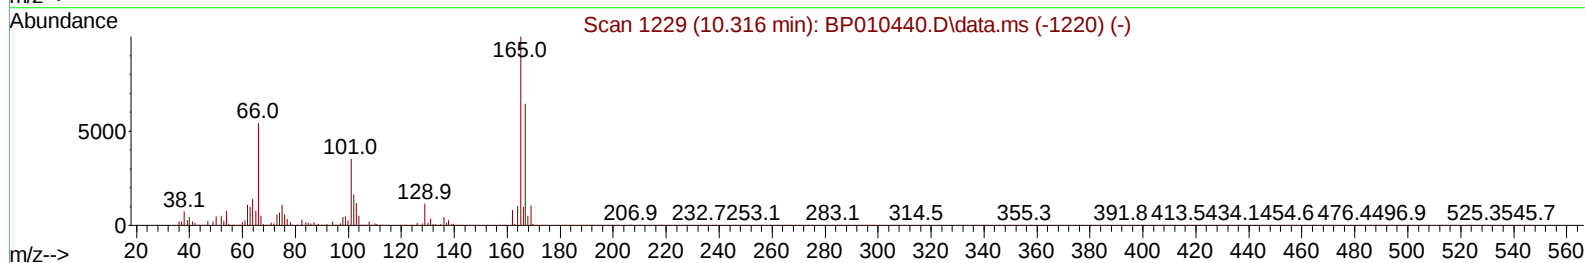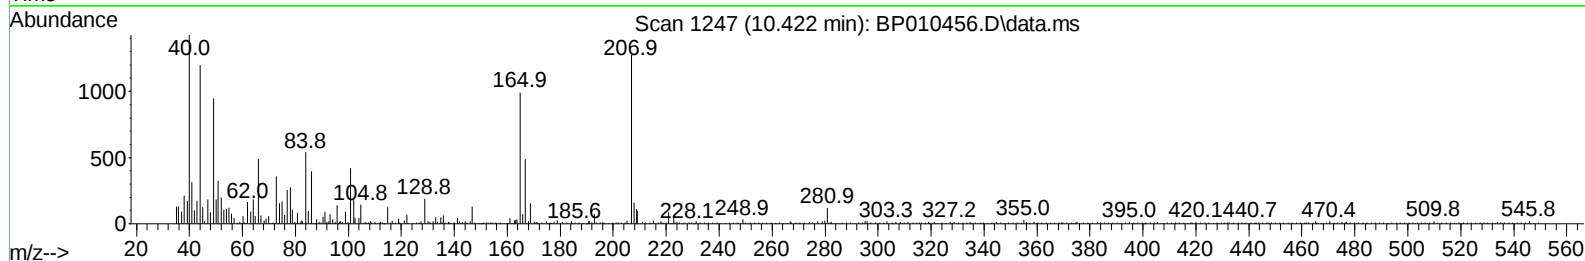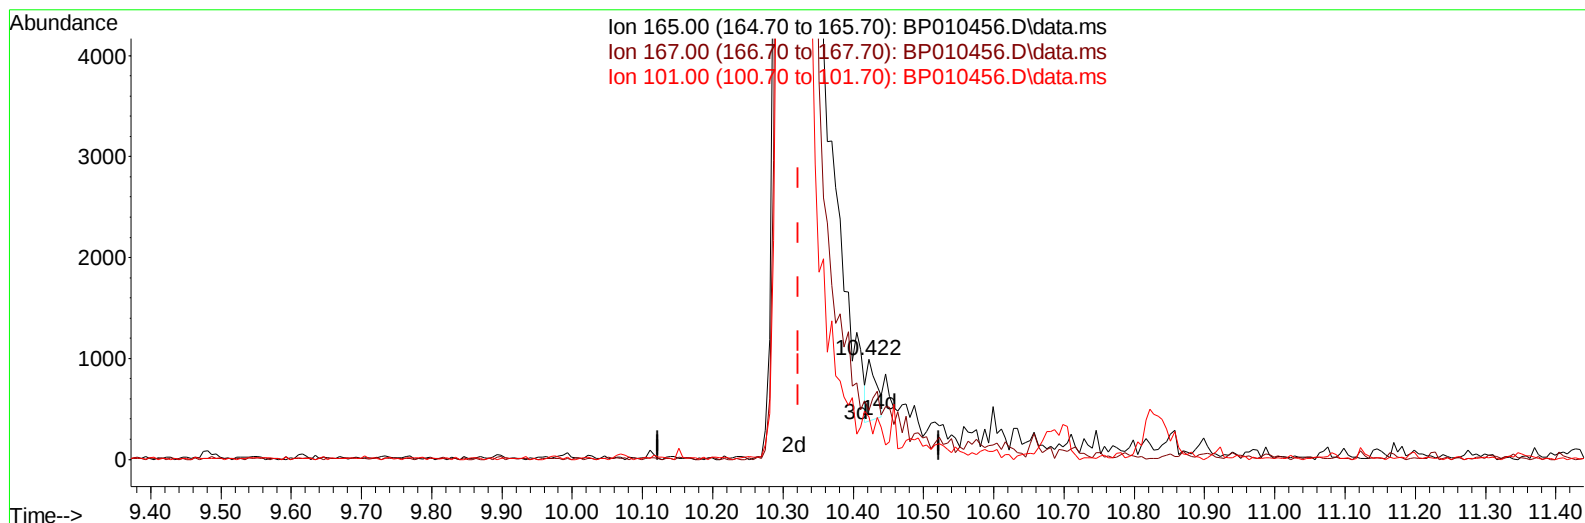

TIC: BP010456.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.422min (+ 0.100) 0.06 ng/u1

response 569

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	49.14
101.00	49.80	42.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010456.D
 Acq On : 21 May 2022 03:03
 Operator : CG/JU
 Sample : N2843-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J6

Manual IntegrationsAPPROVED

Quant Time: May 21 04:33:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

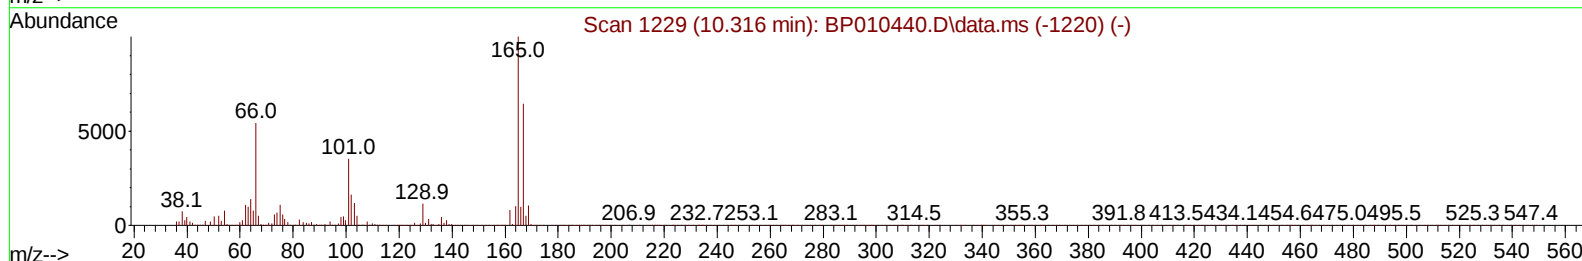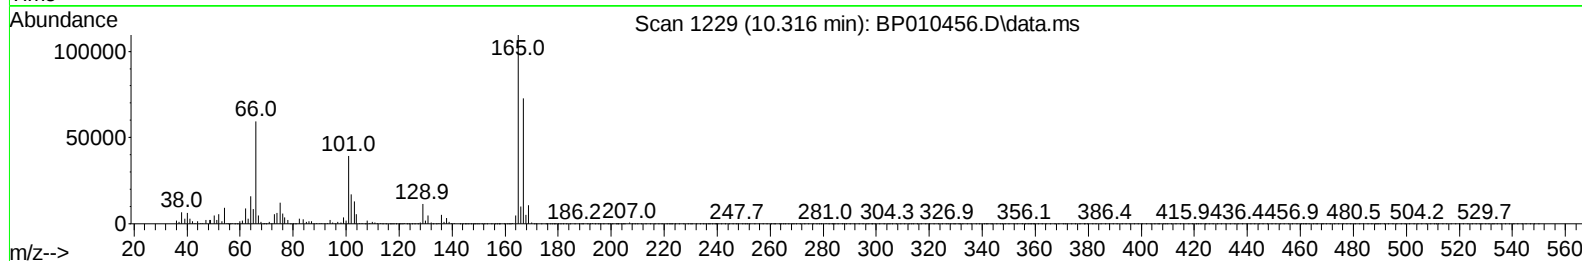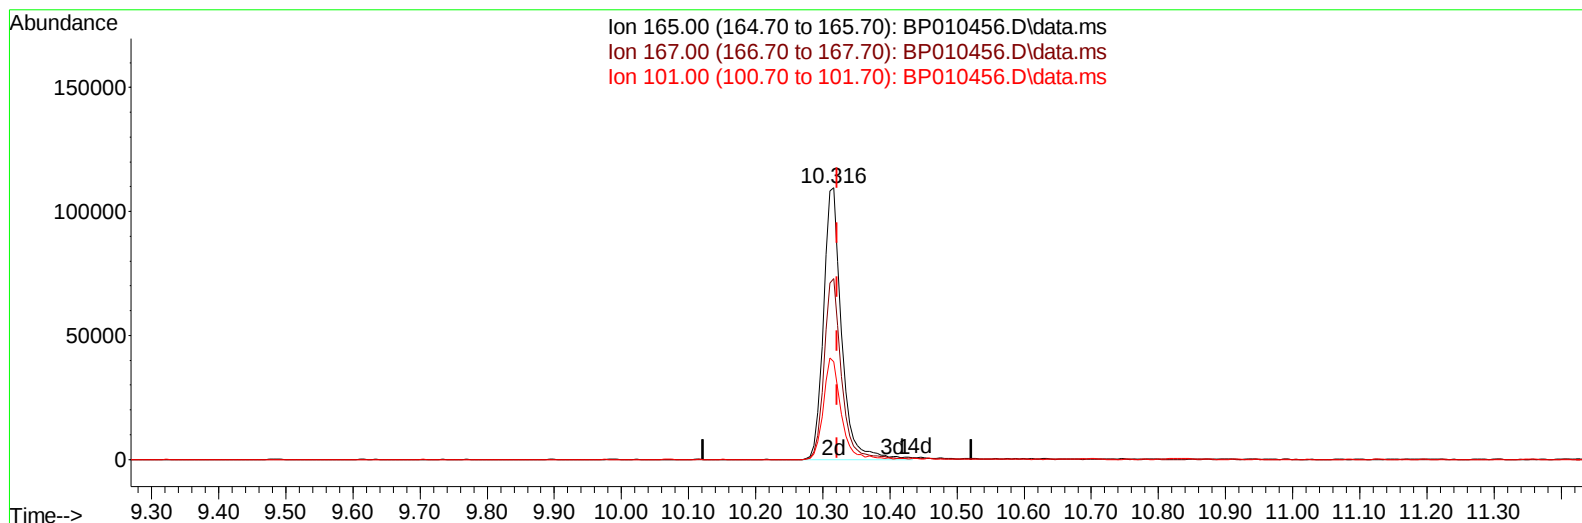

TIC: BP010456.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.316min (-0.006) 20.26 ng/ul m

response 206156

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	66.57
101.00	49.80	35.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010456.D
 Acq On : 21 May 2022 03:03
 Operator : CG/JU
 Sample : N2843-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 04:33:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	145631	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.687	136	656029	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.522	164	455728	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188	984198	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240	955808	20.000	ng/ul	# 0.00
88) Perylene-d12	23.774	264	858103	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	13589m	3.977	ng/uL	0.00
4) Pyridine-d5	3.764	84	95574	9.852	ng/ul	0.00
7) Phenol-d5	7.058	99	246133	20.137	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	179149	21.815	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132	203004	21.705	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113	202156	19.461	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	110554	21.774	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.775	143	114576	21.294	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	206156m	20.263	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	280168	18.520	ng/ul	-0.01
46) Dimethylphthalate-d6	13.934	166	733786	21.854	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	856023	22.103	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.728	143	78122	13.072	ng/ul	0.00
60) Fluorene-d10	15.516	176	651023	22.287	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	75624	13.138	ng/ul	-0.01
73) Anthracene-d10	17.375	188	1053325	23.635	ng/ul	0.00
81) Pyrene-d10	19.604	212	1289678	25.407	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264	1036162	24.047	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.716	105	18242m	1.118	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010456.D
Acq On : 21 May 2022 03:03
Operator : CG/JU
Sample : N2843-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 04:33:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

